

Data File : BM018139.D
Acq On : 13 Dec 2018 21:18
Operator : JU/SJ
Sample : J6271-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9E31

Quant Time: Dec 14 01:55:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 14 01:52:41 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	115801	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	512202	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.17	164	315000	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.93	188	744749	20.00	ng/ul	0.00
77) Chrysene-d12	21.14	240	914093	20.00	ng/ul	0.00
85) Perylene-d12	23.31	264	1059694	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	8037	3.31	ng/uL	0.00
5) Phenol-d5	6.70	99	190092	17.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	112340	18.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	170168	19.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	159172	17.63	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	81640	19.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	91848	18.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.92	165	149416	17.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	9929	1.31	ng/ul	0.04
43) Dimethylphthalate-d6	13.59	166	546302	19.60	ng/ul	0.00
46) Acenaphthylene-d8	13.86	160	673904	19.85	ng/ul	0.00
51) 4-Nitrophenol-d4	14.42	143	70705	14.06	ng/ul	0.00
57) Fluorene-d10	15.17	176	505114	21.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.32	200	89838	15.83	ng/ul	0.00
70) Anthracene-d10	17.03	188	810431	21.53	ng/ul	0.00
78) Pyrene-d10	19.34	212	944014	21.54	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.17	264	1220735	20.80	ng/ul	0.00


Target Compounds				Qvalue		
6) Phenol	6.73	94	35683	3.261	ng/ul	94
44) Dimethylphthalate	13.64	163	152999	5.767	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM018139.D
Acq On : 13 Dec 2018 21:18
Operator : JU/SJ
Sample : J6271-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9E31

Quant Time: Dec 14 01:55:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 14 01:52:41 2018
Response via : Initial Calibration

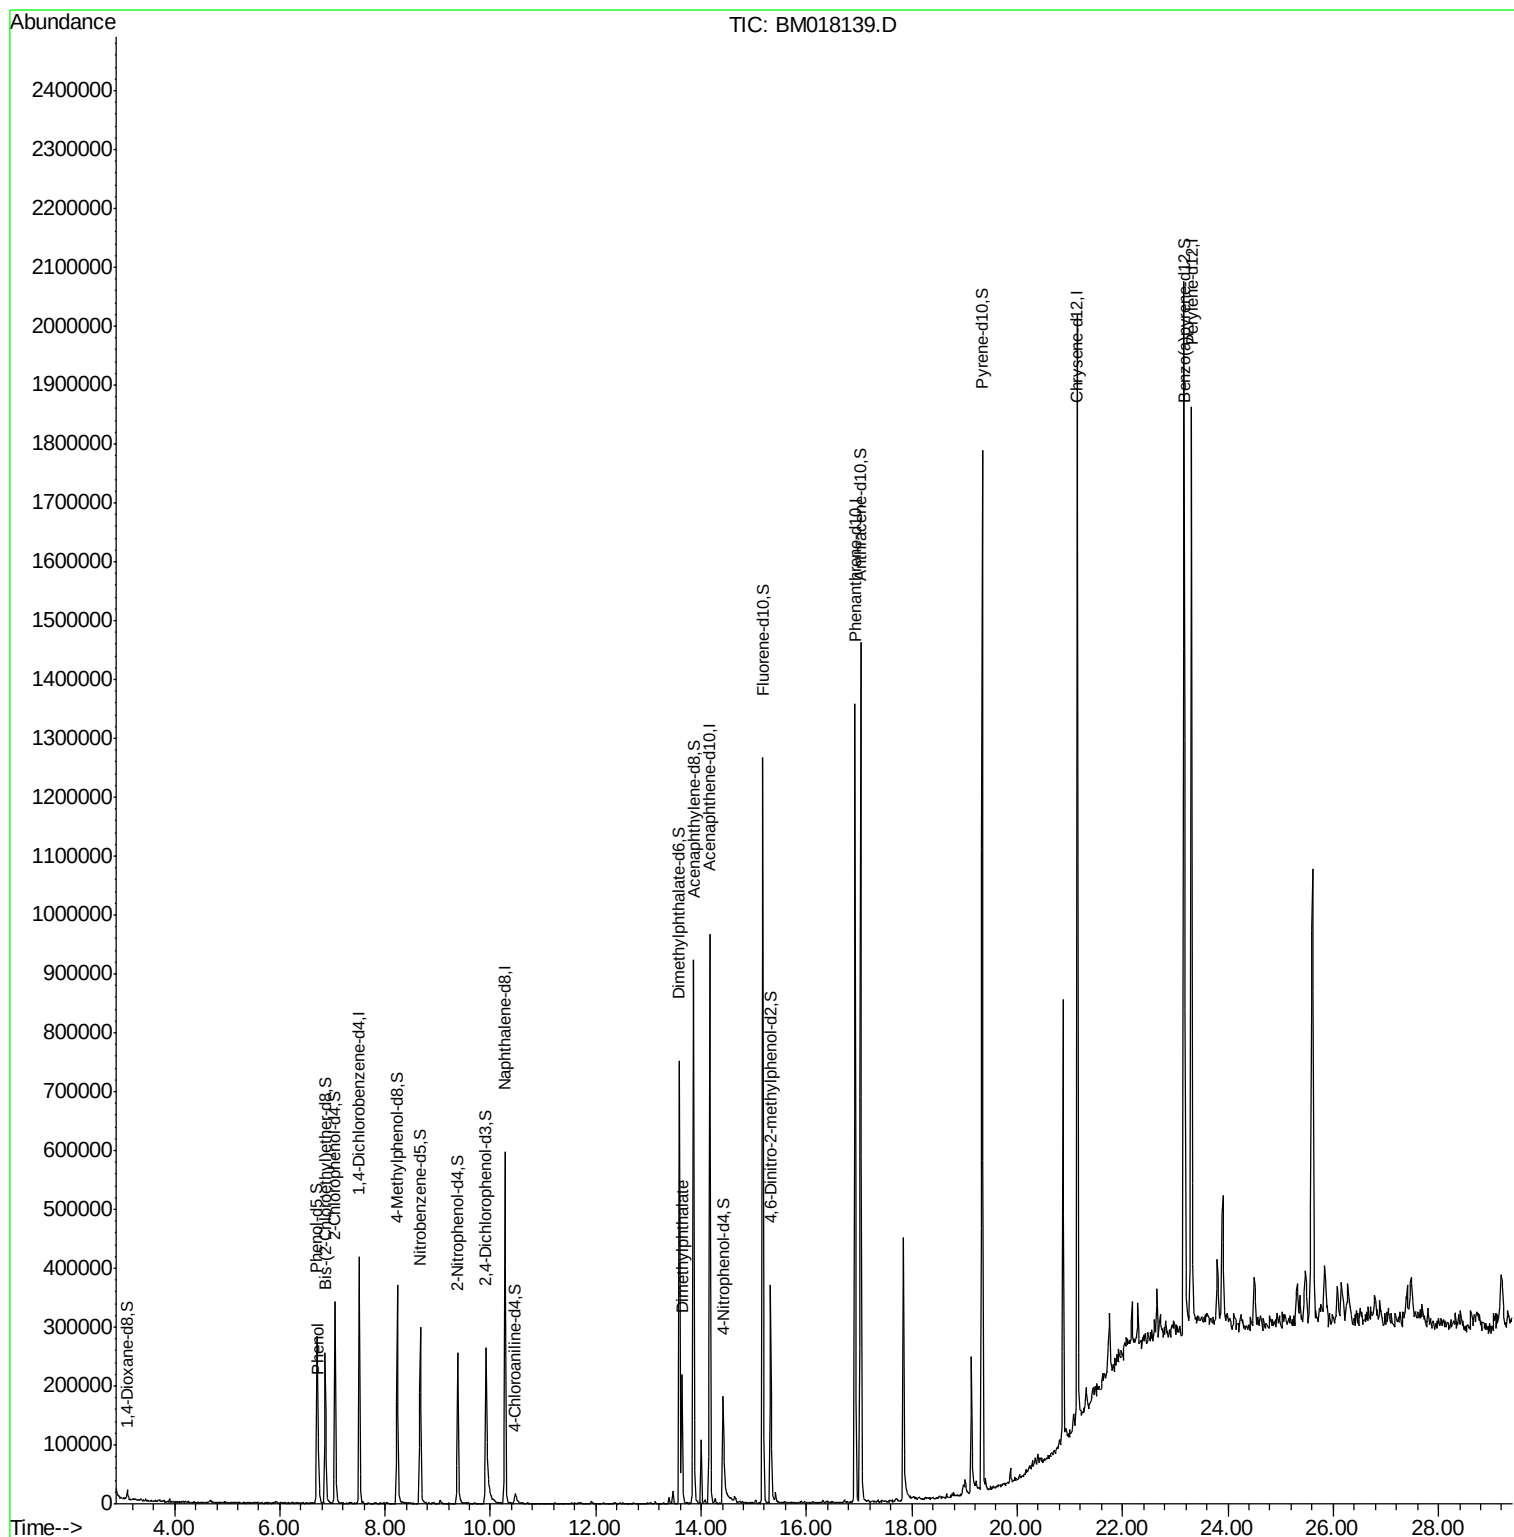

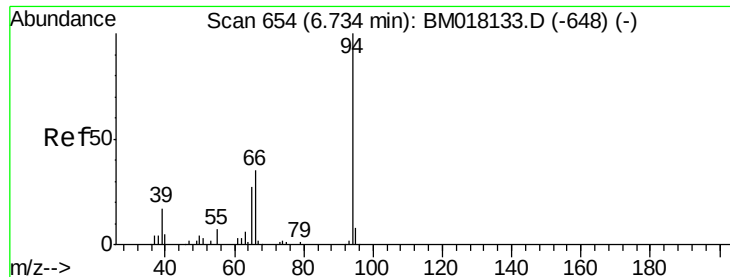

#6

Phenol

Concen: 3.261 ng/ul

RT: 6.73 min Scan# 654

Delta R.T. 0.00 min

Lab File: BM018139.D

Acq: 13 Dec 2018 21:18

Instrument :

BNA_M

ClientSampleId :

F9E31


Tgt Ion: 94 Resp: 35683

Ion Ratio Lower Upper

94 100

65 23.9 22.0 33.0

66 40.9 30.3 45.5



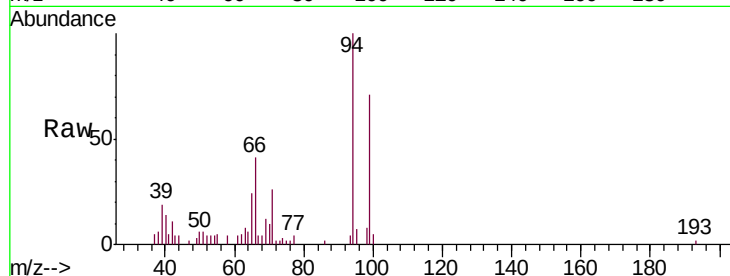


Abundance

Ion 94.00 (93.70 to 94.70): BM018139.D (-620) (-)

Ion 65.00 (64.70 to 65.70): BM018139.D (-620) (-)

Ion 66.00 (65.70 to 66.70): BM018139.D (-620) (-)

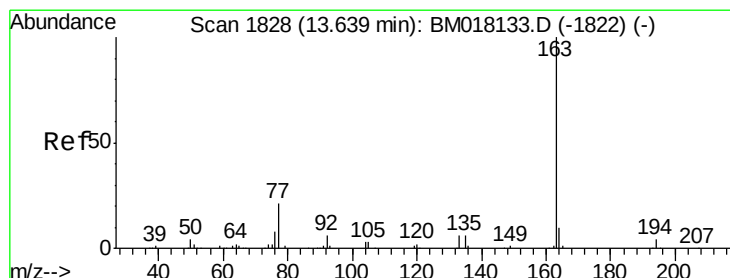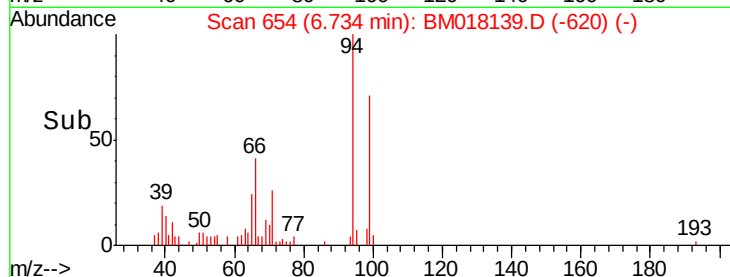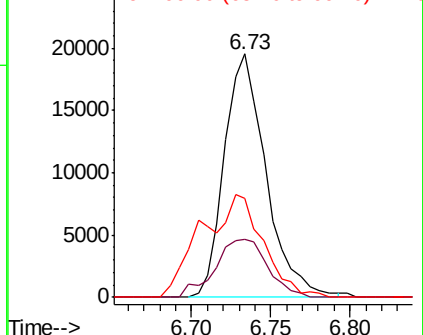

#44

Dimethylphthalate

Concen: 5.767 ng/ul

RT: 13.64 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BM018139.D

Acq: 13 Dec 2018 21:18


Tgt Ion:163 Resp: 152999

Ion Ratio Lower Upper

163 100

194 4.6 3.7 5.5

164 9.9 8.2 12.4

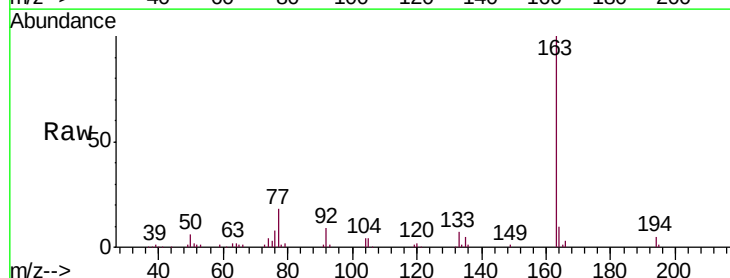

Abundance

Ion 163.00 (162.70 to 163.70): BM018139.D (-1794) (-)

Ion 194.00 (193.70 to 194.70): BM018139.D (-1794) (-)

Ion 164.00 (163.70 to 164.70): BM018139.D (-1794) (-)

