

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043307.D
 Acq On : 13 Dec 2023 18:37
 Operator : MA/JU
 Sample : PB157727BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	46	rVB	108859	165098	1.67%	0.149%
2	3.816	103	107	121	rBV	1573505	2620558	26.52%	2.363%
3	4.146	160	163	168	rVB	23018	31881	0.32%	0.029%
4	7.157	668	675	692	rVB	2207464	3460363	35.02%	3.121%
5	7.334	699	705	715	rVB	1566117	2523861	25.54%	2.276%
6	7.528	730	738	748	rBV	1981642	3221605	32.61%	2.906%
7	7.998	811	818	826	rBV	1499108	2379933	24.09%	2.146%
8	8.710	931	939	949	rBV	2567722	4232958	42.84%	3.818%
9	9.169	1009	1017	1030	rBV	2029590	3288590	33.28%	2.966%
10	9.886	1128	1139	1154	rBV	1540970	2612694	26.44%	2.356%
11	10.422	1222	1230	1242	rBV	2490530	4199214	42.50%	3.787%
12	10.804	1287	1295	1304	rBV	2268493	3868194	39.15%	3.489%
13	10.951	1309	1320	1335	rBV	2584419	4506464	45.61%	4.064%
14	11.792	1457	1463	1466	rVB8	7427	11077	0.11%	0.010%
15	12.386	1556	1564	1571	rVB3	44566	77417	0.78%	0.070%
16	13.527	1753	1758	1766	rVB2	40540	65822	0.67%	0.059%
17	13.604	1766	1771	1778	rBV6	9000	19173	0.19%	0.017%
18	14.045	1837	1846	1855	rBV	4419452	6103956	61.78%	5.505%
19	14.322	1884	1893	1904	rBV	4960615	7244836	73.32%	6.534%
20	14.622	1937	1944	1954	rBV	3407065	5040708	51.02%	4.546%
21	14.821	1970	1978	1994	rBV	2453731	3490179	35.32%	3.148%
22	15.033	2010	2014	2022	rVB	10002	21938	0.22%	0.020%
23	15.280	2052	2056	2060	rBV5	15079	23880	0.24%	0.022%
24	15.616	2105	2113	2121	rBV	6322642	8671438	87.76%	7.821%
25	15.727	2126	2132	2145	rBV	607370	856369	8.67%	0.772%
26	15.851	2149	2153	2160	rVB2	28021	47170	0.48%	0.043%
27	16.180	2203	2209	2216	rBV2	9686	24035	0.24%	0.022%
28	16.398	2242	2246	2250	rBV6	6516	12399	0.13%	0.011%
29	17.039	2350	2355	2358	rBV6	9794	15039	0.15%	0.014%
30	17.151	2371	2374	2379	rVB4	9609	14731	0.15%	0.013%
31	17.362	2403	2410	2418	rBV	3928806	5487275	55.54%	4.949%
32	17.462	2420	2427	2441	rBV	7143056	9605207	97.21%	8.663%
33	17.610	2447	2452	2465	rVB7	21995	55357	0.56%	0.050%
34	18.262	2558	2563	2569	rBV9	17866	31200	0.32%	0.028%
35	19.062	2695	2699	2702	rBV6	6669	10187	0.10%	0.009%
36	19.145	2710	2713	2719	rVB7	13096	19674	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043307.D
Acq On : 13 Dec 2023 18:37
Operator : MA/JU
Sample : PB157727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Title : SVOA CALIBRATION

37	19.315	2737	2742	2747	rBV	67370	97325	0.99%	0.088%
38	19.386	2748	2754	2757	rBV	83599	147329	1.49%	0.133%
39	19.427	2757	2761	2762	rBV4	25627	31639	0.32%	0.029%
40	19.533	2777	2779	2784	rVB5	19234	22551	0.23%	0.020%
41	19.686	2798	2805	2809	rBV6	94189	208752	2.11%	0.188%
42	19.745	2809	2815	2823	rVB	7452797	9880674	100.00%	8.911%
43	19.898	2837	2841	2854	rBV3	105760	189380	1.92%	0.171%
44	21.533	3113	3119	3129	rVB	3704859	4607640	46.63%	4.156%
45	23.797	3496	3504	3514	rVB2	3871675	7524020	76.15%	6.786%
46	23.950	3523	3530	3544	rVB	2028816	4109574	41.59%	3.706%



Sum of corrected areas: 110879364

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043307.D
Acq On : 13 Dec 2023 18:37
Operator : MA/JU
Sample : PB157727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

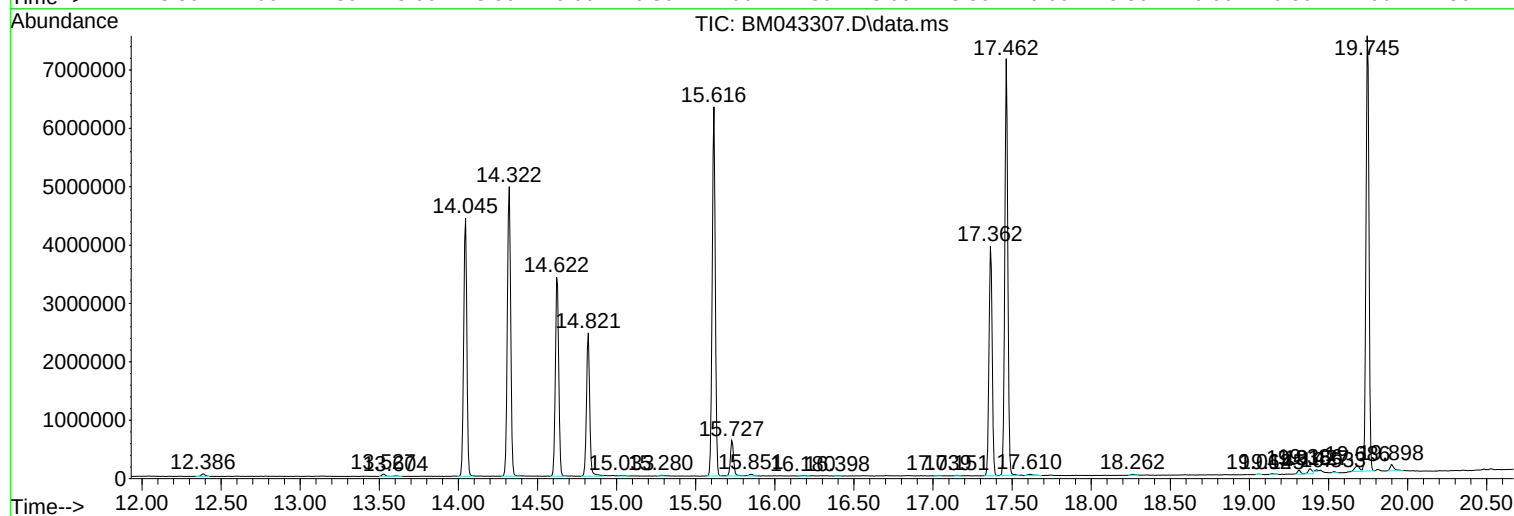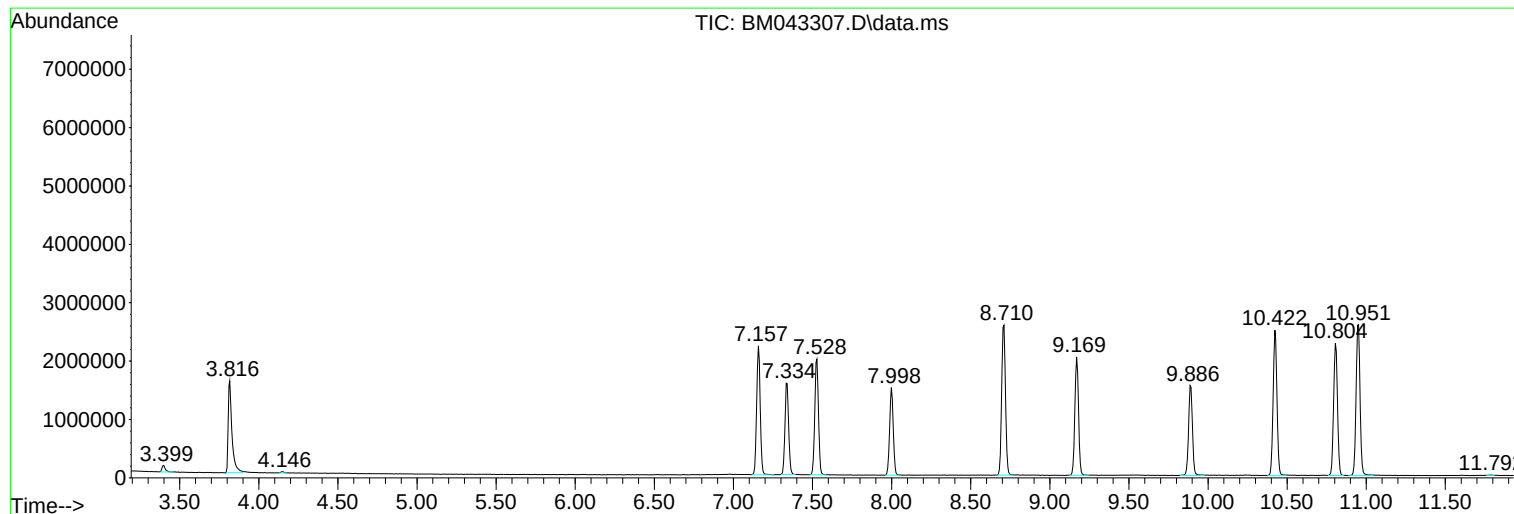

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043307.D
Acq On : 13 Dec 2023 18:37
Operator : MA/JU
Sample : PB157727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043307.D
Acq On : 13 Dec 2023 18:37
Operator : MA/JU
Sample : PB157727BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK727

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------