

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043308.D
 Acq On : 13 Dec 2023 19:13
 Operator : MA/JU
 Sample : PB157638BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK638

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	42	rVB	96471	140452	1.67%	0.141%
2	3.816	103	107	131	rBV	1436121	2474840	29.50%	2.481%
3	4.146	160	163	169	rVB3	27332	41524	0.49%	0.042%
4	7.157	668	675	683	rBV	2033139	3128669	37.29%	3.137%
5	7.334	699	705	719	rVB	1437266	2321549	27.67%	2.328%
6	7.528	730	738	748	rVB	1818828	2931116	34.94%	2.939%
7	7.998	811	818	831	rVB	1367091	2155054	25.69%	2.161%
8	8.710	929	939	951	rBV	2396850	3885715	46.32%	3.896%
9	9.169	1010	1017	1026	rBV	1850006	3004494	35.81%	3.012%
10	9.887	1132	1139	1153	rBV	1376107	2341924	27.92%	2.348%
11	10.422	1222	1230	1241	rBV	2290302	3823984	45.58%	3.834%
12	10.804	1288	1295	1303	rVB	2075311	3489366	41.59%	3.499%
13	10.951	1311	1320	1333	rBV	2335737	4149396	49.46%	4.160%
14	11.763	1454	1458	1461	rBV6	6542	11491	0.14%	0.012%
15	12.033	1501	1504	1510	rVB7	4437	8939	0.11%	0.009%
16	12.386	1559	1564	1571	rBV	40840	67219	0.80%	0.067%
17	13.139	1687	1692	1695	rBV6	6509	11676	0.14%	0.012%
18	13.527	1751	1758	1765	rBV	42404	72036	0.86%	0.072%
19	13.598	1765	1770	1774	rBV7	6012	11121	0.13%	0.011%
20	13.969	1827	1833	1838	rBV8	7188	13396	0.16%	0.013%
21	14.045	1838	1846	1857	rBV	3740491	5307969	63.27%	5.322%
22	14.322	1882	1893	1907	rBV2	4417582	6697444	79.84%	6.715%
23	14.622	1934	1944	1953	rBV	3063795	4616144	55.03%	4.628%
24	14.821	1970	1978	1992	rBV	1928704	2971019	35.42%	2.979%
25	15.039	2009	2015	2020	rBV10	11597	19934	0.24%	0.020%
26	15.286	2052	2057	2060	rBV5	12777	20787	0.25%	0.021%
27	15.616	2102	2113	2121	rBV	5454773	7858916	93.68%	7.880%
28	15.727	2127	2132	2139	rBV	444244	618076	7.37%	0.620%
29	15.851	2146	2153	2158	rBV3	24270	42169	0.50%	0.042%
30	16.180	2206	2209	2214	rBV7	7247	13095	0.16%	0.013%
31	17.151	2370	2374	2377	rVB3	7658	9331	0.11%	0.009%
32	17.363	2403	2410	2420	rBV	3682425	5075095	60.50%	5.089%
33	17.463	2420	2427	2437	rBV	6165388	8231738	98.13%	8.254%
34	17.615	2449	2453	2457	rBV5	17613	24741	0.29%	0.025%
35	17.739	2472	2474	2481	rVB5	6597	10434	0.12%	0.010%
36	18.262	2558	2563	2566	rBV6	15735	27412	0.33%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043308.D
 Acq On : 13 Dec 2023 19:13
 Operator : MA/JU
 Sample : PB157638BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK638

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	19.139	2710	2712	2718	rBV7	8440	15373	0.18%	0.015%
38	19.315	2737	2742	2746	rBV2	58478	80161	0.96%	0.080%
39	19.380	2748	2753	2756	rBV	66067	107306	1.28%	0.108%
40	19.533	2777	2779	2784	rVB6	15158	16869	0.20%	0.017%
41	19.745	2809	2815	2823	rVB	6463291	8389023	100.00%	8.411%
42	19.898	2837	2841	2848	rBV3	75857	119915	1.43%	0.120%
43	21.533	3113	3119	3131	rVB	3448329	4392138	52.36%	4.404%
44	23.250	3408	3411	3420	rVB	116204	191640	2.28%	0.192%
45	23.797	3496	3504	3515	rBV2	3362021	6608588	78.78%	6.626%
46	23.891	3517	3520	3523	rVV	144265	244362	2.91%	0.245%
47	23.950	3523	3530	3539	rVB	1908884	3940813	46.98%	3.951%




Sum of corrected areas: 99734453

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043308.D
Acq On : 13 Dec 2023 19:13
Operator : MA/JU
Sample : PB157638BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

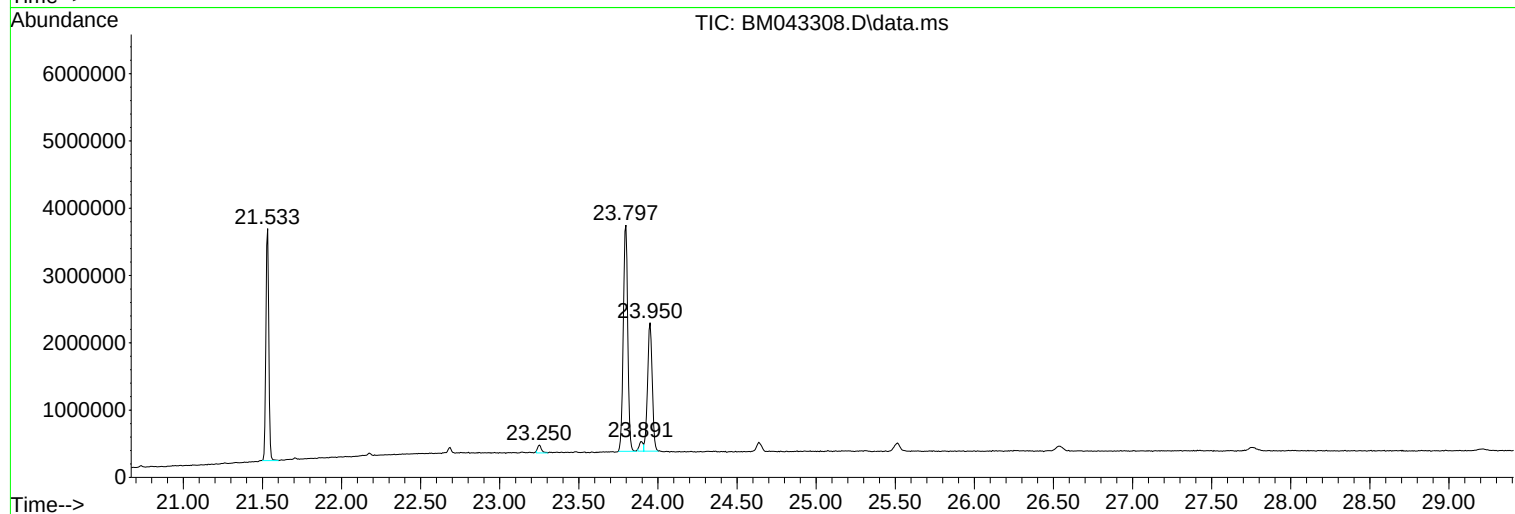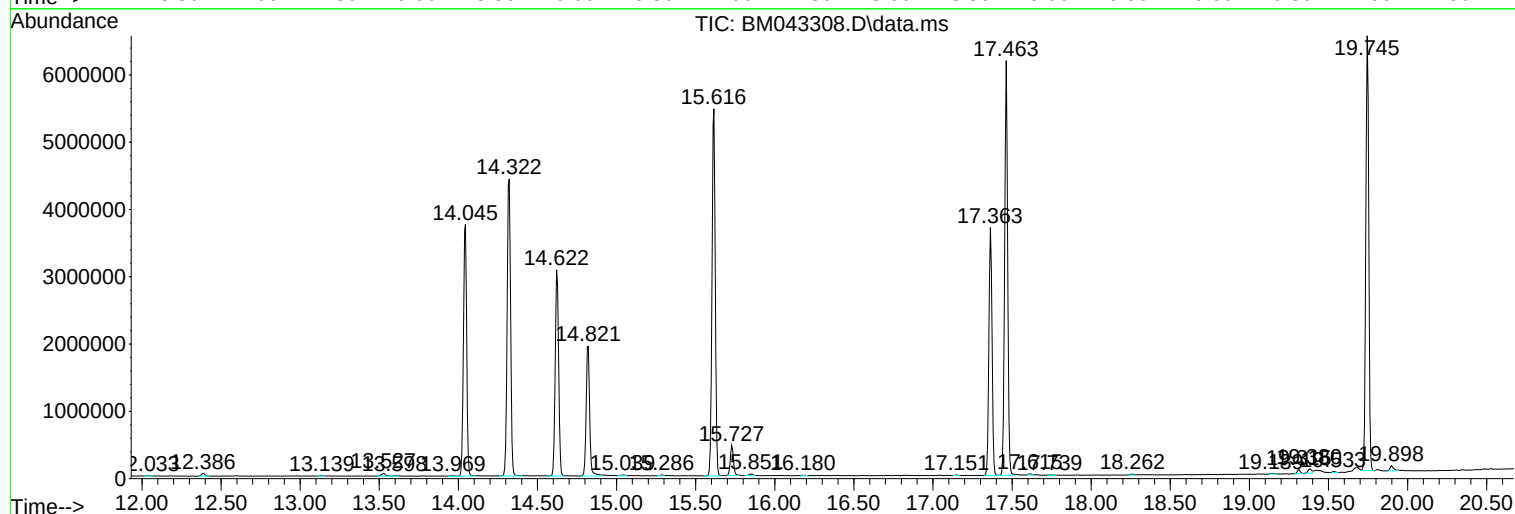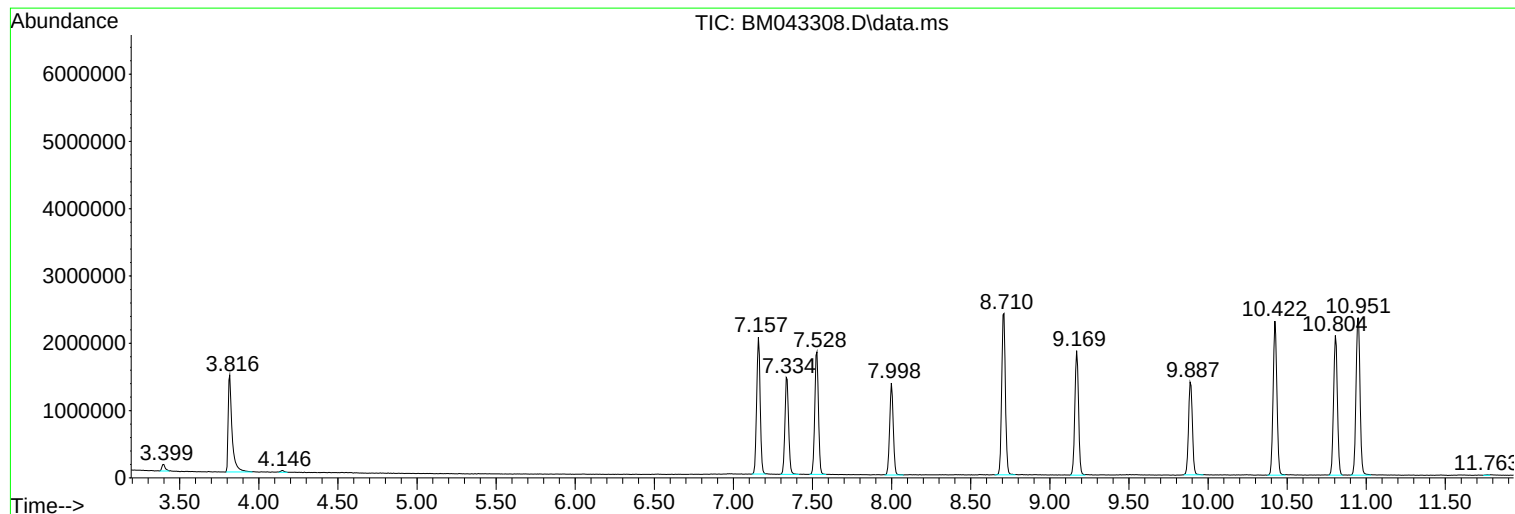

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043308.D
Acq On : 13 Dec 2023 19:13
Operator : MA/JU
Sample : PB157638BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043308.D
Acq On : 13 Dec 2023 19:13
Operator : MA/JU
Sample : PB157638BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK638

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc