

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043323.D
 Acq On : 14 Dec 2023 04:48
 Operator : MA/JU
 Sample : PB157724BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK724

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	45	rVB	112259	172401	1.68%	0.147%
2	3.816	103	107	130	rBV	1648320	2784387	27.13%	2.367%
3	4.146	160	163	171	rVB2	25252	38503	0.38%	0.033%
4	7.157	668	675	690	rVB	2266372	3598299	35.06%	3.059%
5	7.334	699	705	717	rVB	1724435	2726182	26.57%	2.317%
6	7.522	730	737	747	rBV	2093390	3436799	33.49%	2.921%
7	7.998	811	818	826	rBV	1661108	2605876	25.39%	2.215%
8	8.704	930	938	948	rBV	2756142	4468215	43.54%	3.798%
9	9.169	1009	1017	1029	rBV	2196861	3587172	34.96%	3.049%
10	9.886	1128	1139	1156	rBV	1717163	2942497	28.67%	2.501%
11	10.422	1223	1230	1242	rBV	2724105	4486079	43.72%	3.813%
12	10.804	1286	1295	1304	rBV	2499488	4235465	41.27%	3.600%
13	10.951	1312	1320	1333	rBV	2718972	4839767	47.16%	4.114%
14	11.598	1423	1430	1434	rBV8	7940	19810	0.19%	0.017%
15	12.386	1559	1564	1570	rVB2	47540	77879	0.76%	0.066%
16	13.521	1751	1757	1766	rVB	59705	104420	1.02%	0.089%
17	13.598	1766	1770	1776	rBV6	10079	17951	0.17%	0.015%
18	14.045	1839	1846	1854	rBV	4799331	6594522	64.26%	5.605%
19	14.321	1884	1893	1905	rBV	5360700	7909829	77.08%	6.723%
20	14.621	1937	1944	1952	rBV	3660411	5482010	53.42%	4.660%
21	14.821	1969	1978	1989	rBV	2326633	3577221	34.86%	3.041%
22	15.045	2010	2016	2019	rVB7	9486	18438	0.18%	0.016%
23	15.286	2053	2057	2063	rVB9	9570	16511	0.16%	0.014%
24	15.615	2104	2113	2121	rBV	6615108	9353633	91.15%	7.951%
25	15.733	2126	2133	2147	rVV	1112368	1584290	15.44%	1.347%
26	15.851	2149	2153	2161	rVB3	30260	61367	0.60%	0.052%
27	15.939	2161	2168	2170	rBV7	5404	10707	0.10%	0.009%
28	16.398	2242	2246	2250	rVB6	8108	11141	0.11%	0.009%
29	17.045	2353	2356	2360	rVB5	10956	14740	0.14%	0.013%
30	17.151	2369	2374	2379	rBV3	9780	15148	0.15%	0.013%
31	17.362	2402	2410	2420	rBV	4075988	5911605	57.61%	5.025%
32	17.462	2420	2427	2441	rVV2	7210093	10209961	99.49%	8.679%
33	17.615	2447	2453	2459	rBV4	30707	62950	0.61%	0.054%
34	17.739	2469	2474	2479	rBV3	13029	24263	0.24%	0.021%
35	18.262	2558	2563	2565	rBV6	10572	12974	0.13%	0.011%
36	19.315	2736	2742	2748	rBV2	76447	113450	1.11%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043323.D
Acq On : 14 Dec 2023 04:48
Operator : MA/JU
Sample : PB157724BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK724

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Title : SVOA CALIBRATION

37	19.380	2748	2753	2758	rBV	77816	114352	1.11%	0.097%
38	19.450	2761	2765	2770	rVV8	13054	19799	0.19%	0.017%
39	19.686	2803	2805	2809	rVB4	25551	25334	0.25%	0.022%
40	19.750	2809	2816	2822	rBV	7697825	10261905	100.00%	8.723%
41	20.733	2980	2983	2988	rBV3	37579	42533	0.41%	0.036%
42	21.533	3114	3119	3128	rVB	3703116	4650004	45.31%	3.953%
43	23.797	3496	3504	3514	rVB2	3771008	7360260	71.72%	6.256%
44	23.950	3523	3530	3540	rVB	2014394	4043976	39.41%	3.437%




Sum of corrected areas: 117644625

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043323.D
Acq On : 14 Dec 2023 04:48
Operator : MA/JU
Sample : PB157724BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

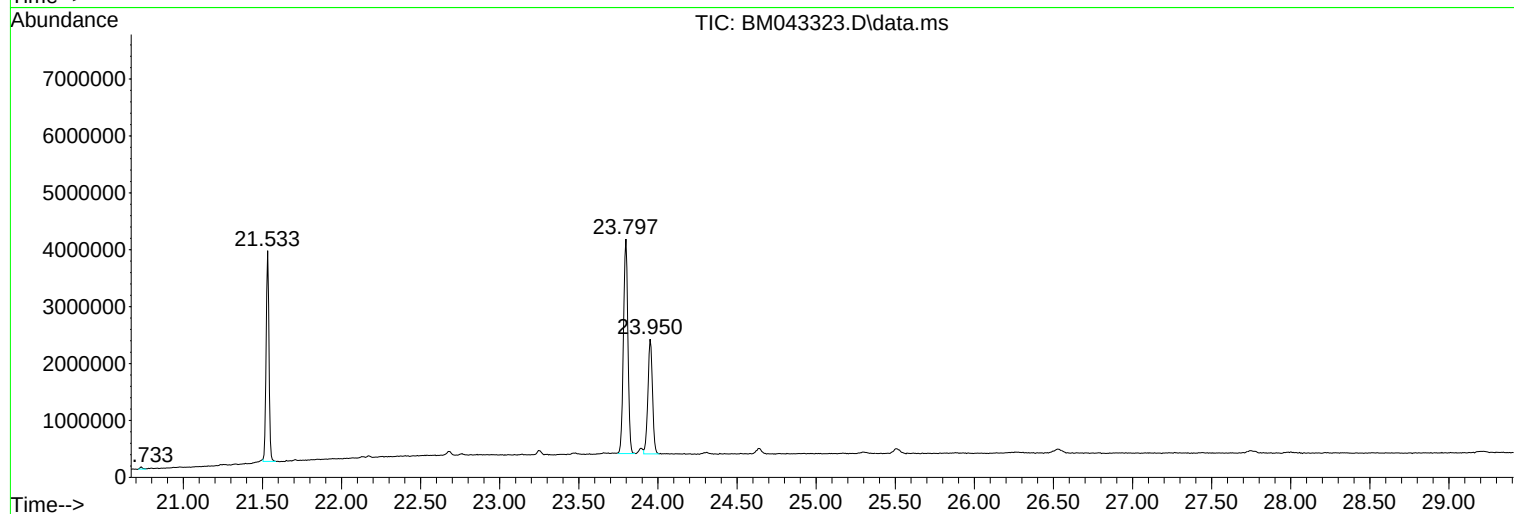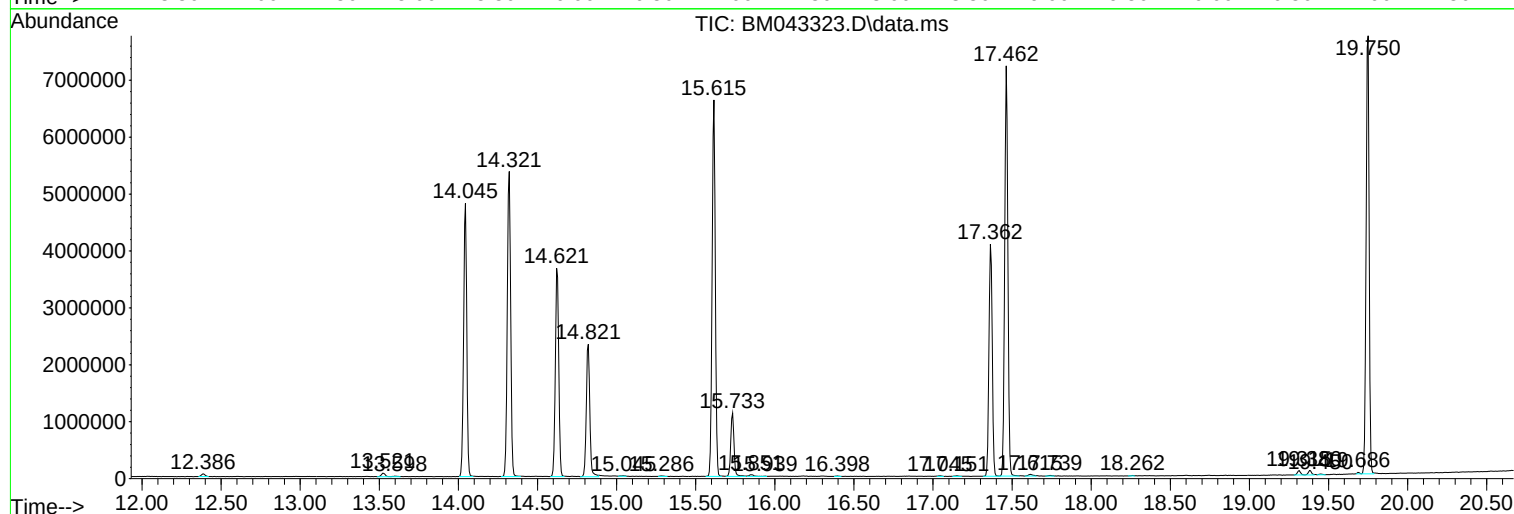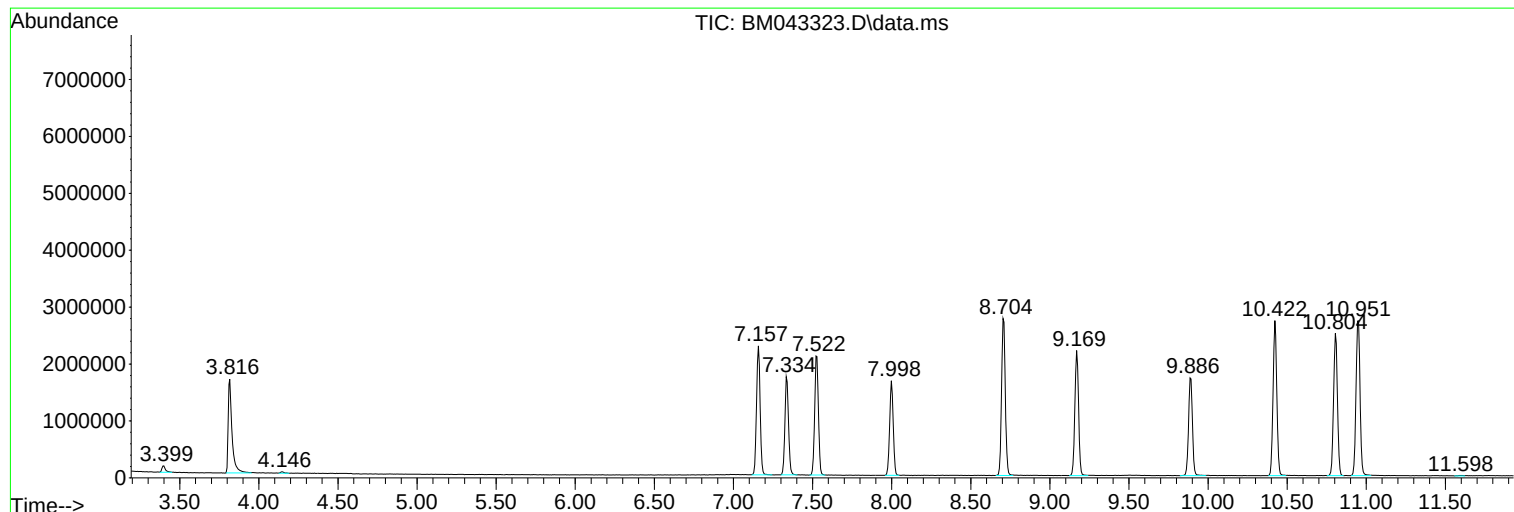

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043323.D
Acq On : 14 Dec 2023 04:48
Operator : MA/JU
Sample : PB157724BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043323.D
Acq On : 14 Dec 2023 04:48
Operator : MA/JU
Sample : PB157724BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------