

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043324.D
 Acq On : 14 Dec 2023 05:24
 Operator : MA/JU
 Sample : PB157680BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	32	35	47	rVB	148203	227266	1.81%	0.153%
2	3.810	103	106	126	rBV	2056212	3491915	27.81%	2.355%
3	4.146	160	163	172	rVB2	28566	44795	0.36%	0.030%
4	6.981	641	645	654	rBV2	5474	13005	0.10%	0.009%
5	7.157	668	675	687	rVB	2913941	4528168	36.06%	3.053%
6	7.334	699	705	716	rVB	2167093	3447509	27.46%	2.325%
7	7.522	729	737	748	rBV	2644190	4370372	34.81%	2.947%
8	7.998	810	818	831	rBV	1967354	3137563	24.99%	2.116%
9	8.710	929	939	953	rBV	3429652	5694176	45.35%	3.840%
10	9.169	1008	1017	1027	rBV	2732211	4569778	36.39%	3.081%
11	9.886	1130	1139	1153	rBV	2226902	3745037	29.83%	2.525%
12	10.422	1221	1230	1243	rBV	3451205	5708631	45.46%	3.849%
13	10.804	1288	1295	1302	rBV	2970914	5085898	40.51%	3.430%
14	10.851	1302	1303	1311	rVB	35943	47479	0.38%	0.032%
15	10.951	1311	1320	1330	rBV	3465930	6159711	49.06%	4.154%
16	12.386	1558	1564	1571	rVB2	59987	103438	0.82%	0.070%
17	12.457	1571	1576	1582	rBV	36200	60160	0.48%	0.041%
18	12.674	1607	1613	1619	rBV2	18540	33800	0.27%	0.023%
19	13.463	1743	1747	1751	rVB3	15539	21350	0.17%	0.014%
20	13.527	1751	1758	1763	rVV	60039	98872	0.79%	0.067%
21	13.598	1766	1770	1777	rVB7	10658	19034	0.15%	0.013%
22	14.045	1835	1846	1853	rBV	5968824	8094384	64.47%	5.458%
23	14.321	1885	1893	1905	rBV	6882620	10102693	80.46%	6.812%
24	14.627	1937	1945	1951	rBV	4355835	6644113	52.91%	4.480%
25	14.686	1951	1955	1965	rVB	93670	136581	1.09%	0.092%
26	14.821	1970	1978	1995	rBV	3028771	4430381	35.28%	2.987%
27	15.021	2007	2012	2021	rVB	64960	110564	0.88%	0.075%
28	15.286	2053	2057	2061	rBV6	13881	21129	0.17%	0.014%
29	15.615	2102	2113	2119	rBV	8520126	11856791	94.43%	7.995%
30	15.668	2119	2122	2127	rVV	85106	116819	0.93%	0.079%
31	15.733	2127	2133	2146	rVV	1525038	2149084	17.12%	1.449%
32	15.851	2146	2153	2160	rVB2	41853	84284	0.67%	0.057%
33	16.180	2205	2209	2214	rBV8	10912	20304	0.16%	0.014%
34	16.398	2242	2246	2249	rVB5	9490	13294	0.11%	0.009%
35	17.045	2350	2356	2359	rBV8	11383	18135	0.14%	0.012%
36	17.180	2377	2379	2386	rVB2	14845	20613	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043324.D
 Acq On : 14 Dec 2023 05:24
 Operator : MA/JU
 Sample : PB157680BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK680

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	17.362	2403	2410	2415	rBV	5053272	7242652	57.68%	4.884%
38	17.404	2415	2417	2421	rVV	225478	288602	2.30%	0.195%
39	17.462	2421	2427	2439	rVB2	8526972	12323445	98.15%	8.310%
40	17.615	2447	2453	2464	rBV5	31363	67590	0.54%	0.046%
41	17.745	2471	2475	2476	rBV2	11721	14301	0.11%	0.010%
42	18.251	2557	2561	2564	rBV6	11969	22953	0.18%	0.015%
43	18.286	2564	2567	2572	rVB4	11638	19660	0.16%	0.013%
44	18.439	2588	2593	2596	rBV3	20627	32097	0.26%	0.022%
45	18.592	2615	2619	2627	rVB3	10492	19958	0.16%	0.013%
46	18.739	2641	2644	2649	rBV6	15345	23805	0.19%	0.016%
47	19.151	2709	2714	2720	rBV10	10517	23536	0.19%	0.016%
48	19.315	2737	2742	2748	rVB2	89813	127908	1.02%	0.086%
49	19.380	2748	2753	2756	rBV	92927	136576	1.09%	0.092%
50	19.409	2756	2758	2764	rVB	93089	120334	0.96%	0.081%
51	19.686	2803	2805	2809	rBV3	25064	29185	0.23%	0.020%
52	19.750	2809	2816	2829	rVV	9274470	12556217	100.00%	8.467%
53	21.533	3113	3119	3130	rBV	4654384	5728282	45.62%	3.863%
54	23.250	3407	3411	3418	rVB	165990	273653	2.18%	0.185%
55	23.797	3496	3504	3513	rVV2	4676326	8966270	71.41%	6.046%
56	23.891	3516	3520	3523	rVV	224019	374580	2.98%	0.253%
57	23.950	3523	3530	3543	rVB	2505092	5044753	40.18%	3.402%
58	24.638	3642	3647	3655	rVB	205062	434060	3.46%	0.293%




Sum of corrected areas: 148297543

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043324.D
Acq On : 14 Dec 2023 05:24
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

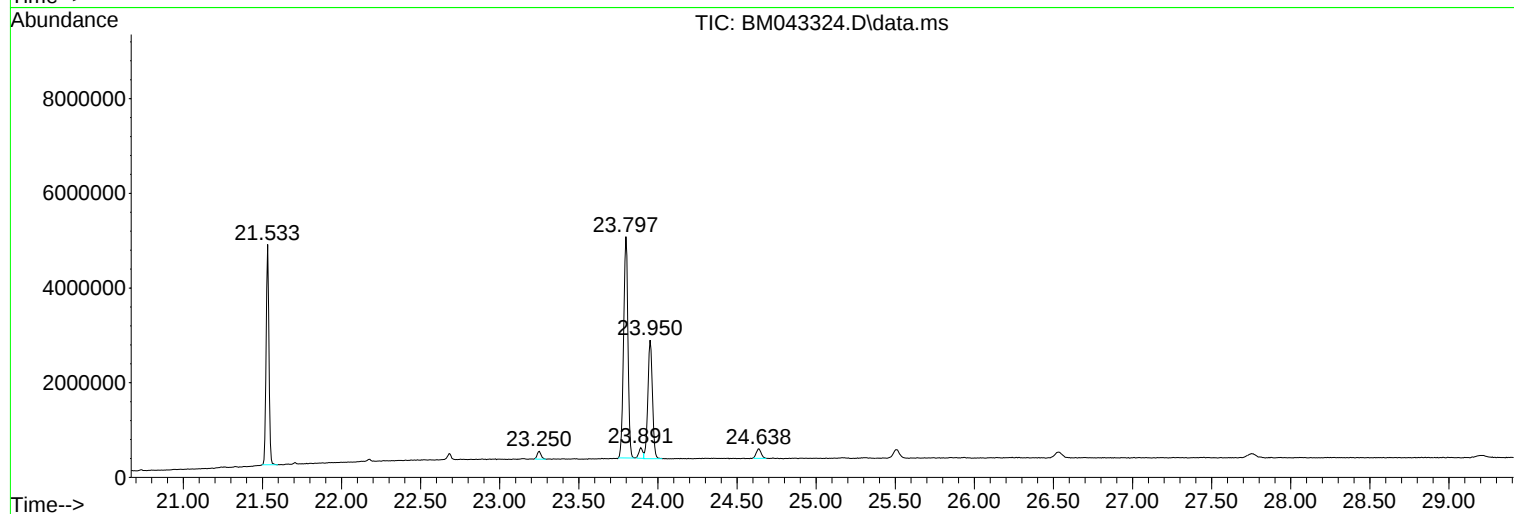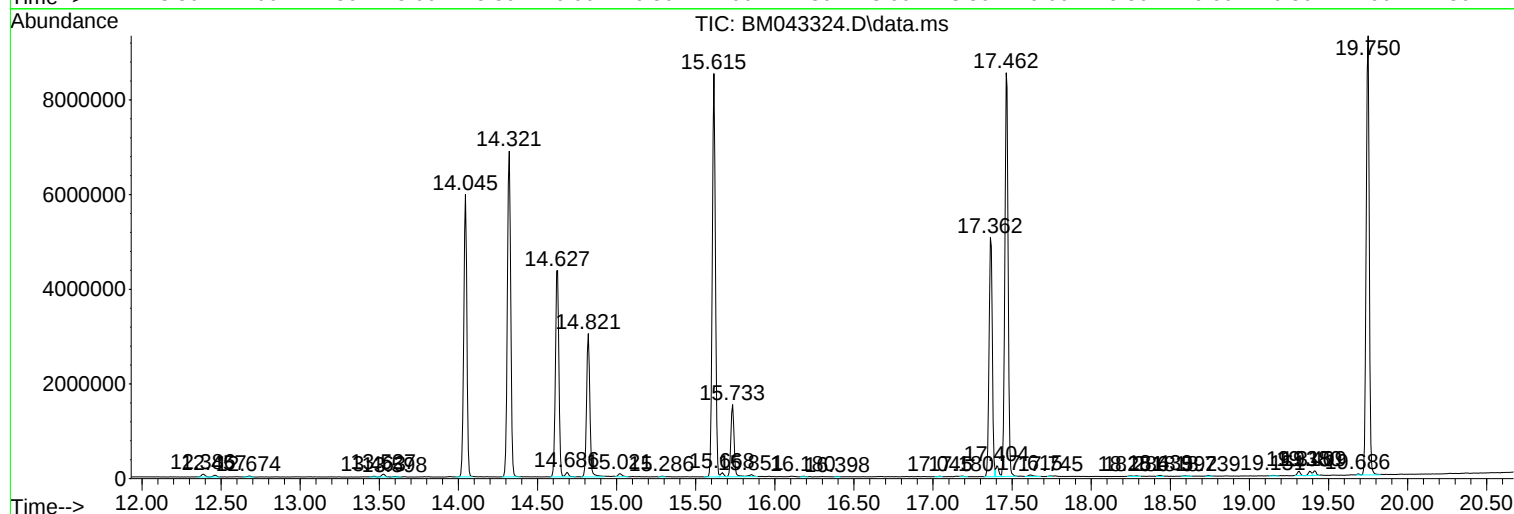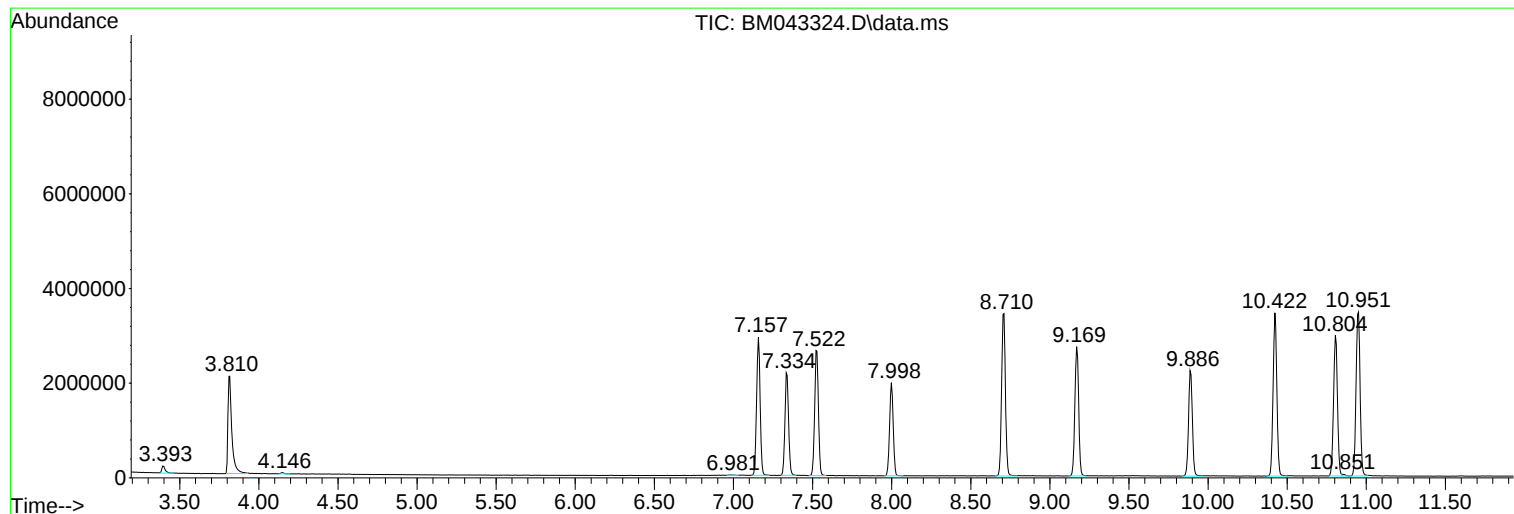

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043324.D
Acq On : 14 Dec 2023 05:24
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043324.D
Acq On : 14 Dec 2023 05:24
Operator : MA/JU
Sample : PB157680BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK680

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc