

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043325.D
 Acq On : 14 Dec 2023 05:59
 Operator : MA/JU
 Sample : 05686-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCH84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	45	rVB	111645	171430	1.27%	0.125%
2	3.816	103	107	126	rBV	882118	1479718	10.98%	1.077%
3	4.052	142	147	151	rVB	42190	68043	0.50%	0.050%
4	4.146	159	163	169	rBV	29911	45206	0.34%	0.033%
5	4.528	225	228	235	rVB6	21135	33324	0.25%	0.024%
6	6.969	640	643	646	rBV5	10619	15980	0.12%	0.012%
7	7.157	668	675	684	rVB	563056	890983	6.61%	0.648%
8	7.334	698	705	720	rVB	2379283	3754850	27.86%	2.732%
9	7.522	729	737	748	rBV	2106574	3463667	25.70%	2.520%
10	7.604	748	751	760	rVB8	14379	28521	0.21%	0.021%
11	7.998	810	818	826	rBV	1924295	3016012	22.38%	2.195%
12	8.704	930	938	948	rBV	1693575	2758755	20.47%	2.007%
13	9.169	1009	1017	1031	rBV	3023539	4947455	36.71%	3.600%
14	9.334	1040	1045	1053	rVB	5989	14173	0.11%	0.010%
15	9.887	1130	1139	1149	rBV	2263364	3826959	28.40%	2.785%
16	10.422	1222	1230	1242	rBV	3274971	5447149	40.42%	3.963%
17	10.804	1287	1295	1309	rVB	2898177	4884532	36.25%	3.554%
18	10.945	1311	1319	1335	rBV	3412218	5995336	44.49%	4.362%
19	11.463	1400	1407	1413	rVB	7389	16965	0.13%	0.012%
20	11.598	1425	1430	1437	rBV8	13287	22594	0.17%	0.016%
21	11.733	1446	1453	1465	rBV2	203563	464203	3.44%	0.338%
22	12.386	1558	1564	1573	rBV2	61382	106877	0.79%	0.078%
23	12.598	1592	1600	1605	rBV9	6544	14017	0.10%	0.010%
24	13.527	1753	1758	1765	rBV	75785	124301	0.92%	0.090%
25	13.604	1765	1771	1776	rVB4	16815	32643	0.24%	0.024%
26	14.045	1838	1846	1855	rBV	6241025	8693414	64.51%	6.326%
27	14.322	1885	1893	1909	rBV	7210434	10840824	80.45%	7.888%
28	14.622	1937	1944	1953	rBV	4283489	6301603	46.76%	4.585%
29	14.816	1970	1977	1990	rBV	447555	740244	5.49%	0.539%
30	15.039	2009	2015	2023	rVB	25331	50887	0.38%	0.037%
31	15.286	2053	2057	2062	rVB6	11261	15734	0.12%	0.011%
32	15.616	2105	2113	2121	rBV	9264299	12901169	95.73%	9.387%
33	15.733	2126	2133	2145	rVV	1597627	2217844	16.46%	1.614%
34	15.851	2148	2153	2164	rVB2	42591	84682	0.63%	0.062%
35	16.398	2241	2246	2253	rBV10	9573	17756	0.13%	0.013%
36	17.157	2367	2375	2382	rBV3	12095	31736	0.24%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
 Data File : BM043325.D
 Acq On : 14 Dec 2023 05:59
 Operator : MA/JU
 Sample : 05686-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCH84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Title : SVOA CALIBRATION

37	17.363	2403	2410	2420	rBV	4704023	6801315	50.47%	4.949%
38	17.463	2420	2427	2439	rBV	9087415	13441158	99.74%	9.780%
39	17.557	2439	2443	2447	rVB3	33797	47480	0.35%	0.035%
40	17.615	2447	2453	2457	rBV4	32311	54409	0.40%	0.040%
41	17.739	2472	2474	2480	rVB3	9477	15469	0.11%	0.011%
42	18.257	2558	2562	2567	rBV3	45570	60933	0.45%	0.044%
43	18.745	2641	2645	2649	rVB7	13884	18346	0.14%	0.013%
44	19.315	2737	2742	2749	rVB2	92588	127919	0.95%	0.093%
45	19.380	2749	2753	2757	rBV	95347	135727	1.01%	0.099%
46	19.451	2762	2765	2770	rVB6	16427	26064	0.19%	0.019%
47	19.533	2776	2779	2783	rBV5	30203	37936	0.28%	0.028%
48	19.692	2802	2806	2809	rBV2	42510	53200	0.39%	0.039%
49	19.751	2809	2816	2823	rBV	10203175	13476060	100.00%	9.806%
50	20.733	2980	2983	2986	rBV3	36692	39113	0.29%	0.028%
51	21.533	3114	3119	3127	rVB	4219795	5319938	39.48%	3.871%
52	23.797	3496	3504	3513	rBV2	4783453	9536155	70.76%	6.939%
53	23.950	3523	3530	3542	rVB	2294842	4722600	35.04%	3.436%




Sum of corrected areas: 137433408

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043325.D
Acq On : 14 Dec 2023 05:59
Operator : MA/JU
Sample : 05686-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCH84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

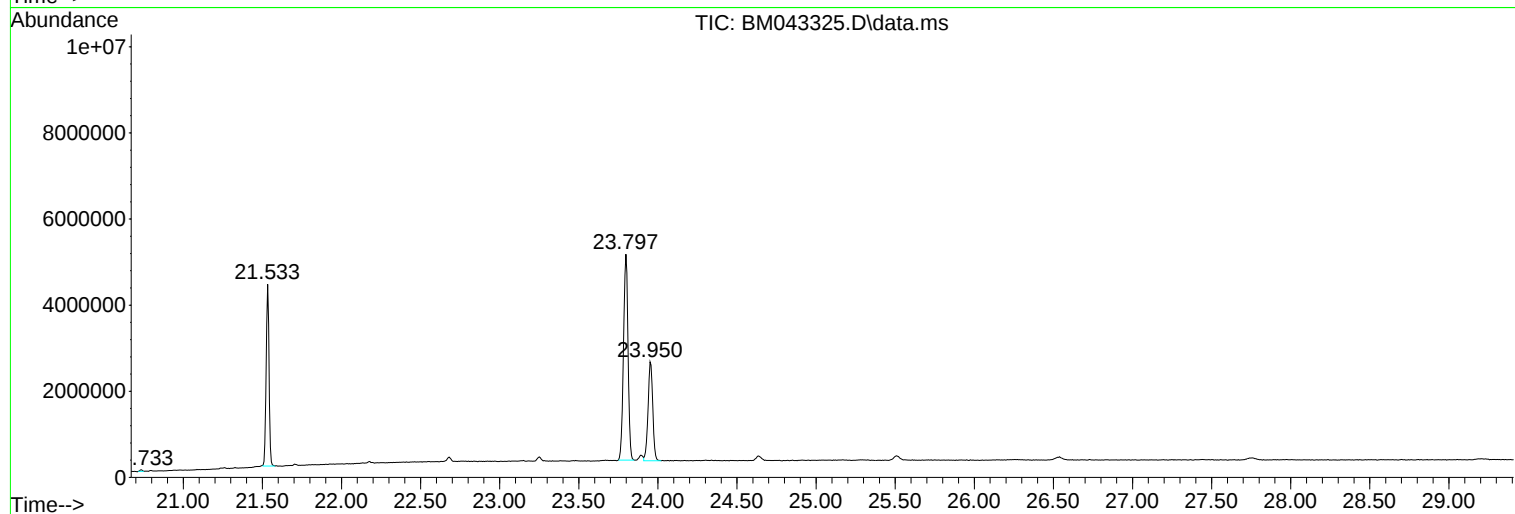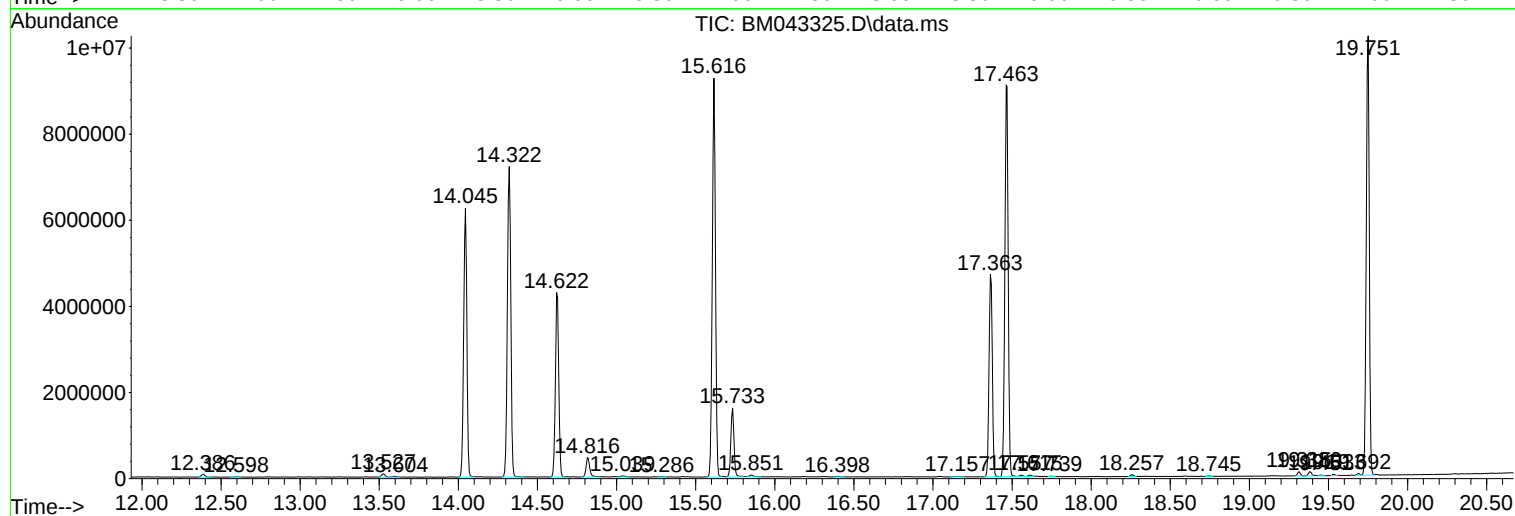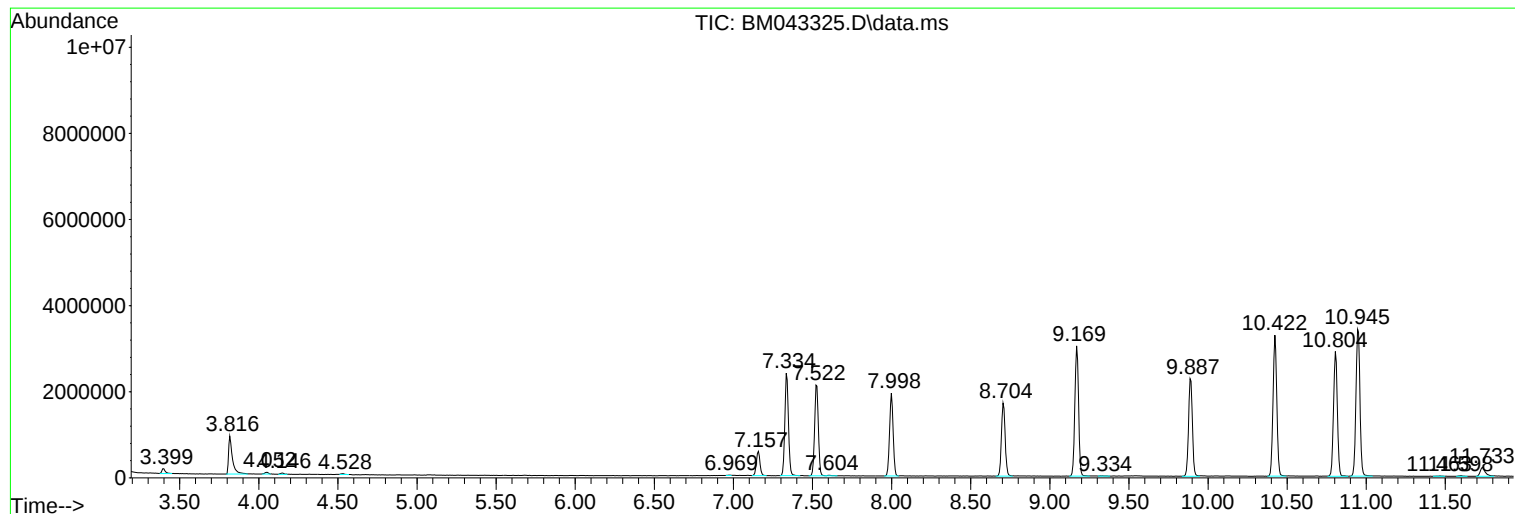

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043325.D
Acq On : 14 Dec 2023 05:59
Operator : MA/JU
Sample : 05686-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCH84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121323\
Data File : BM043325.D
Acq On : 14 Dec 2023 05:59
Operator : MA/JU
Sample : 05686-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCH84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc