

Data File : BM018186.D
Acq On : 15 Dec 2018 02:47
Operator : JU/SJ
Sample : J6297-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9E45

Quant Time: Dec 15 03:56:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 15 03:53:40 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	186551	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	812347	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.16	164	433902	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.92	188	944814	20.00	ng/ul	0.00
77) Chrysene-d12	21.14	240	731907	20.00	ng/ul	0.00
85) Perylene-d12	23.29	264	667673	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	14021	3.59	ng/uL	0.00
5) Phenol-d5	6.70	99	322387	17.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.86	67	189668	19.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	265483	18.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	244394	16.81	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	125671	18.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.37	143	148443	18.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	249480	18.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	235088	19.48	ng/ul	0.00
43) Dimethylphthalate-d6	13.59	166	749594	19.53	ng/ul	0.00
46) Acenaphthylene-d8	13.85	160	936372	20.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.41	143	87092	12.57	ng/ul	0.00
57) Fluorene-d10	15.16	176	650906	20.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.32	200	60177	8.36	ng/ul	0.00
70) Anthracene-d10	17.02	188	956336	20.03	ng/ul	0.00
78) Pyrene-d10	19.33	212	937490	26.71	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.16	264	731943	19.79	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	6.73	94	64792	3.675	ng/ul	98
44) Dimethylphthalate	13.63	163	207421	5.676	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM018186.D
Acq On : 15 Dec 2018 02:47
Operator : JU/SJ
Sample : J6297-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9E45

Quant Time: Dec 15 03:56:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 15 03:53:40 2018
Response via : Initial Calibration

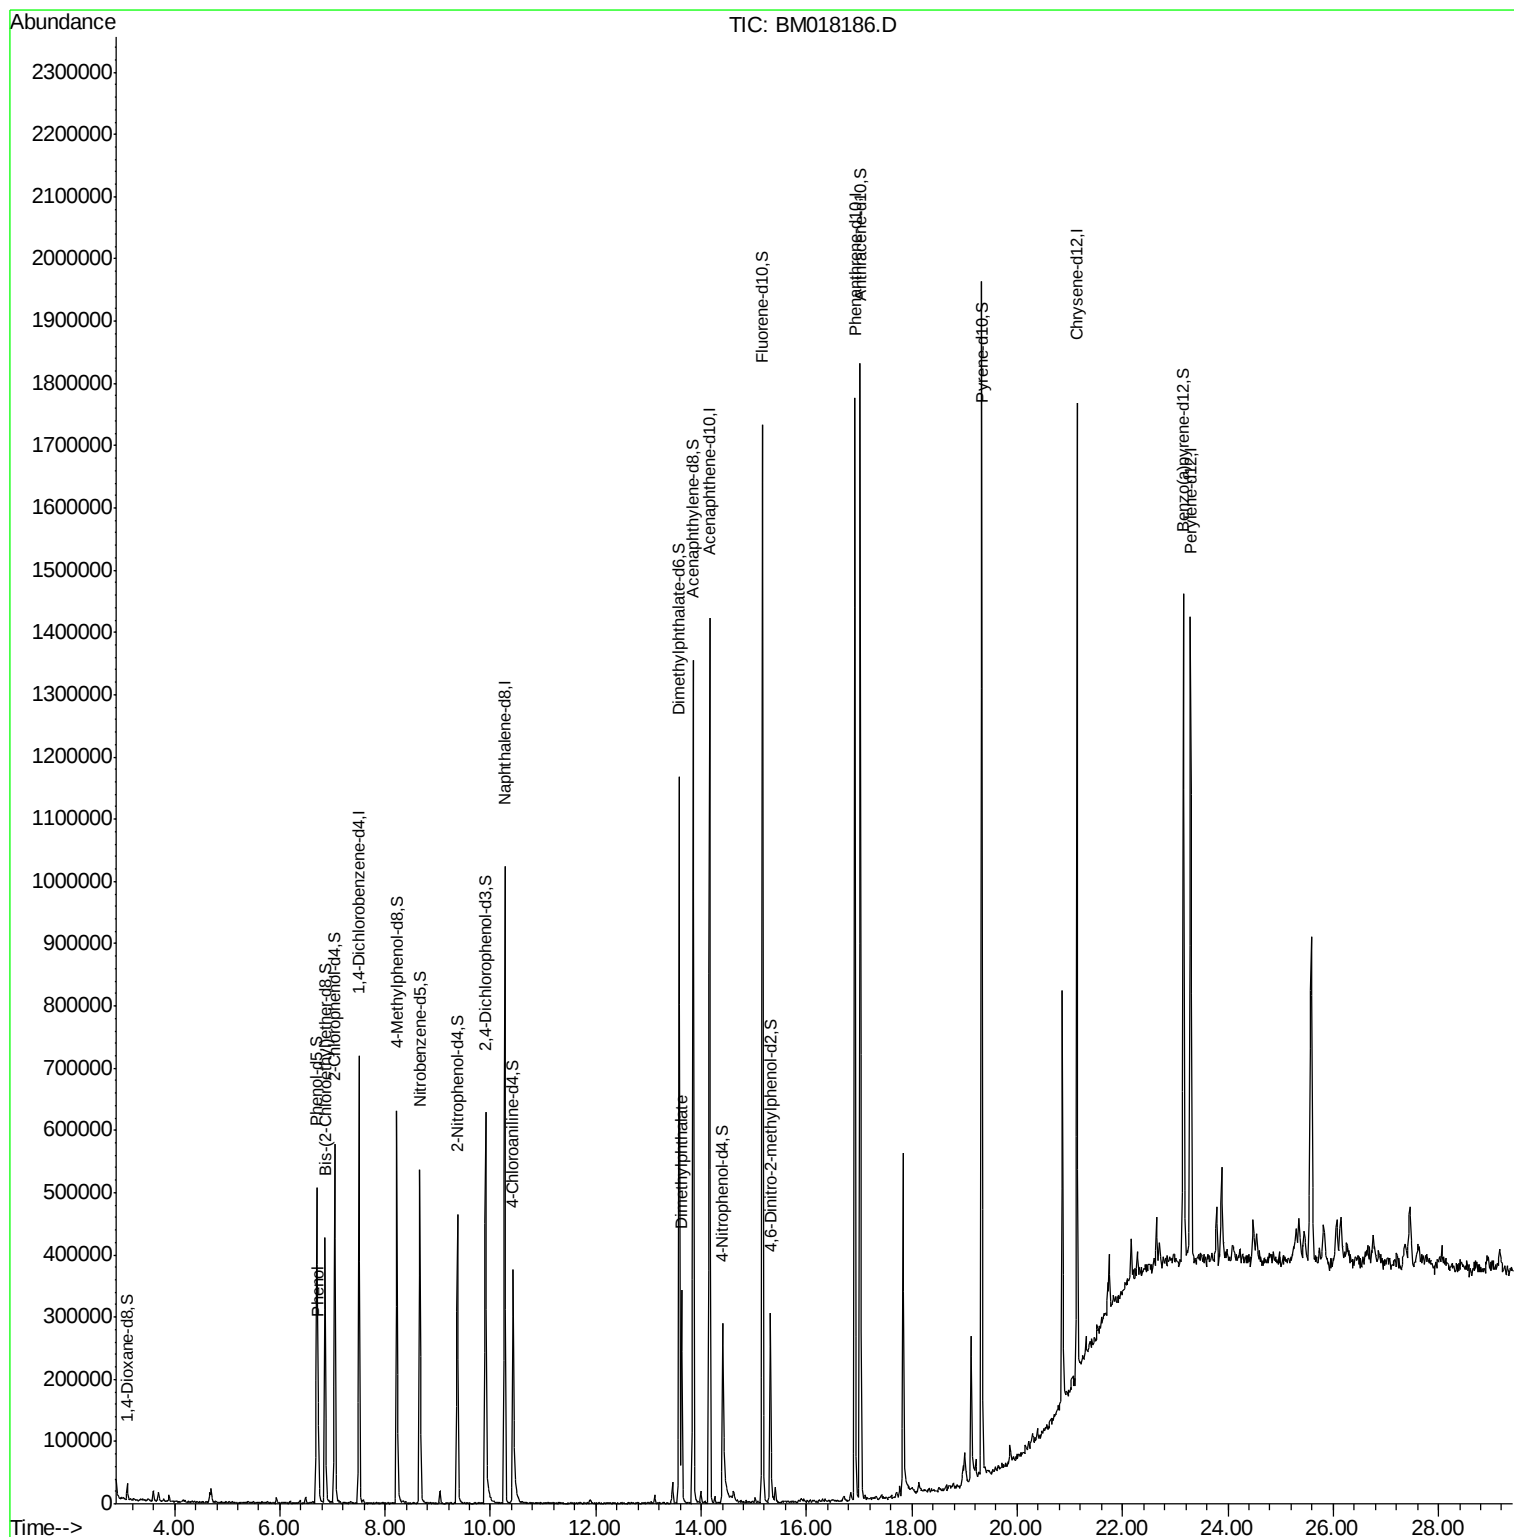

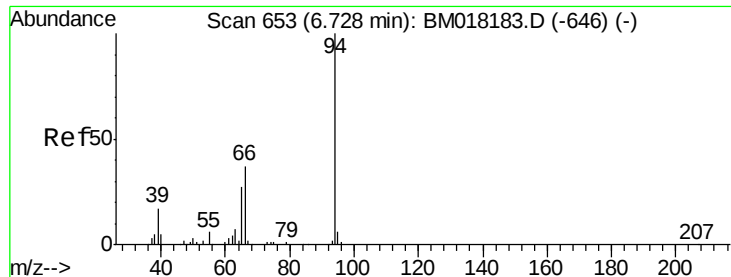

#6

Phenol

Concen: 3.675 ng/ul

RT: 6.73 min Scan# 653

Delta R.T. 0.00 min

Lab File: BM018186.D

Acq: 15 Dec 2018 02:47

Instrument :

BNA_M

ClientSampleId :

F9E45


Tgt Ion: 94 Resp: 64792

Ion Ratio Lower Upper

94 100

65 27.2 22.0 33.0




66 40.2 30.3 45.5

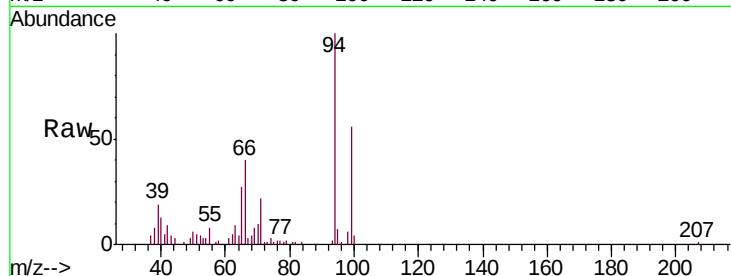

Abundance Ion 94.00 (93.70 to 94.70): BM018186.D (-646) (-)

Ion 65.00 (64.70 to 65.70): BM018186.D (-646) (-)

Ion 66.00 (65.70 to 66.70): BM018186.D (-646) (-)

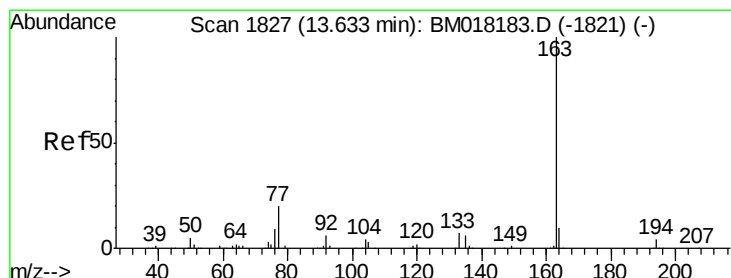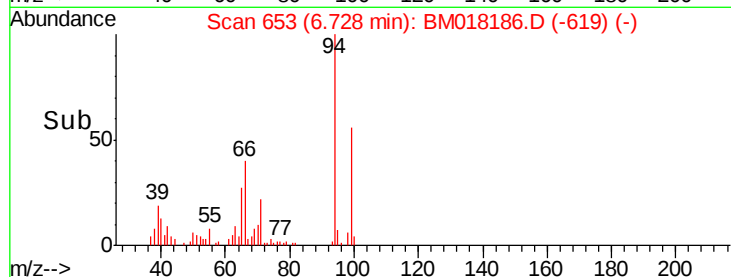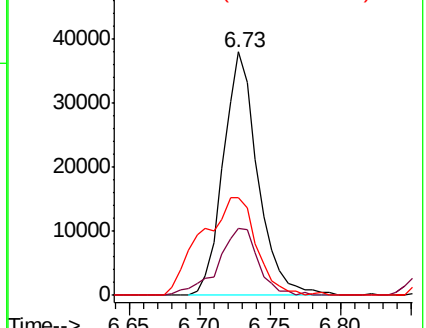

#44

Dimethylphthalate

Concen: 5.676 ng/ul

RT: 13.63 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BM018186.D

Acq: 15 Dec 2018 02:47


Tgt Ion: 163 Resp: 207421

Ion Ratio Lower Upper

163 100

194 4.4 3.7 5.5

164 10.6 8.2 12.4

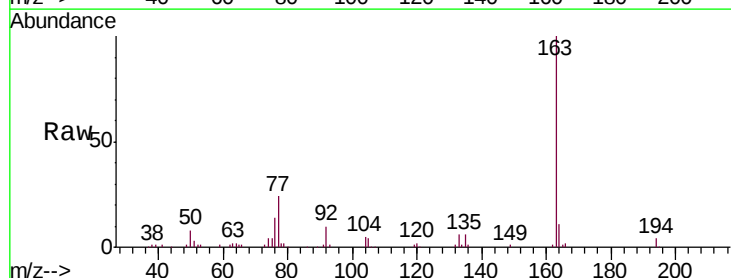

Abundance Ion 163.00 (162.70 to 163.70): BM018186.D (-1793) (-)

Ion 194.00 (193.70 to 194.70): BM018186.D (-1793) (-)

Ion 164.00 (163.70 to 164.70): BM018186.D (-1793) (-)

