

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
 Data File : BM037991.D
 Acq On : 14 Dec 2022 11:12
 Operator : CG/JU
 Sample : PB149616BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK616

Quant Time: Dec 14 23:25:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.068	152	4500	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	13205	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	7407	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	15046	0.400	ng/ul	0.00
17) Chrysene-d12	21.588	240	10791	0.400	ng/ul	0.00
23) Perylene-d12	24.044	264	10308	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	28418	4.478	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	4931	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	9927	0.270	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	1881	0.054	ng/ul#	14
20) Pyrene	19.803	202	1805	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.886	252	3214	0.069	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
Data File : BM037991.D
Acq On : 14 Dec 2022 11:12
Operator : CG/JU
Sample : PB149616BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK616

Quant Time: Dec 14 23:25:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 01:30:33 2022
Response via : Initial Calibration




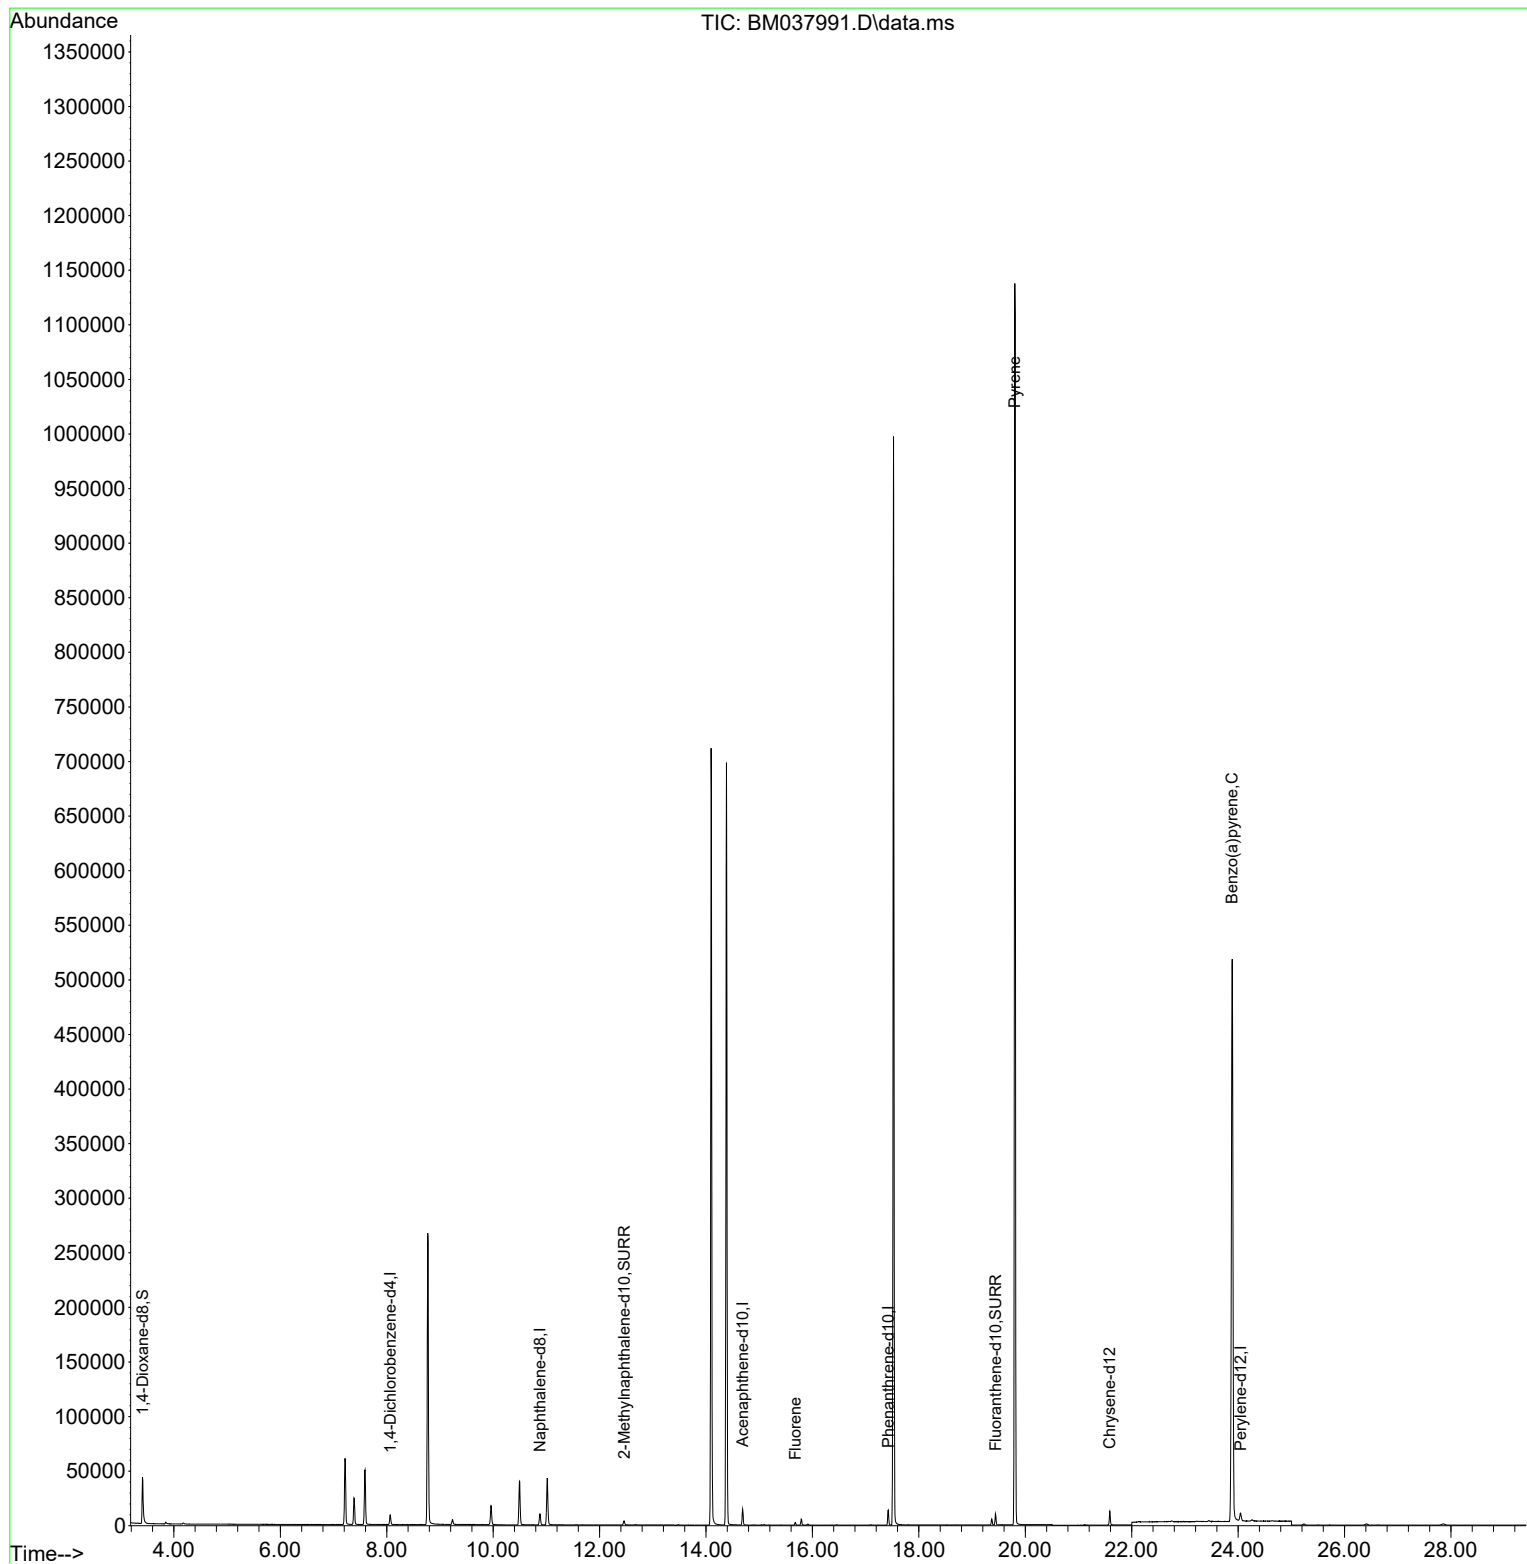


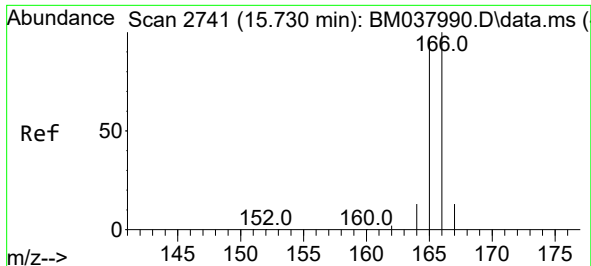

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.679 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM037991.D
Acq: 14 Dec 2022 11:12




Instrument :
BNA_M
ClientSampleId :
SBLK616


Tgt Ion:166 Resp: 1881
Ion Ratio Lower Upper
166 100
165 9.5 79.8 119.6#
167 36.2 11.7 17.5#

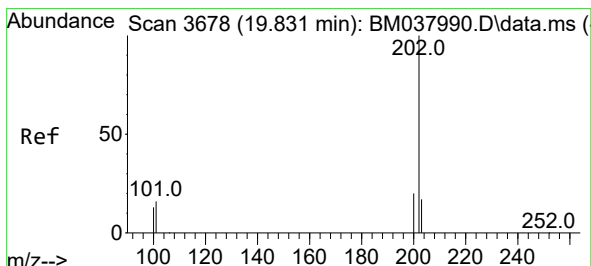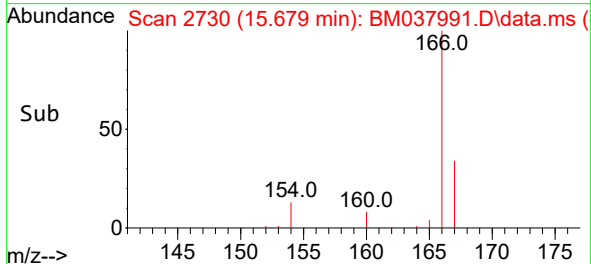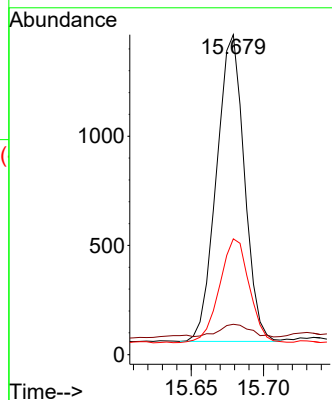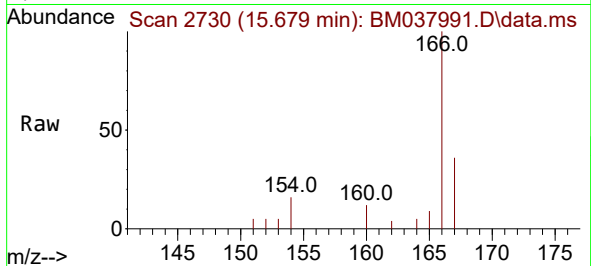

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.803 min Scan# 3672
Delta R.T. -0.033 min
Lab File: BM037991.D
Acq: 14 Dec 2022 11:12


Tgt Ion:202 Resp: 1805
Ion Ratio Lower Upper
202 100
101 159.8 12.6 19.0#
100 1174.2 10.6 15.8#

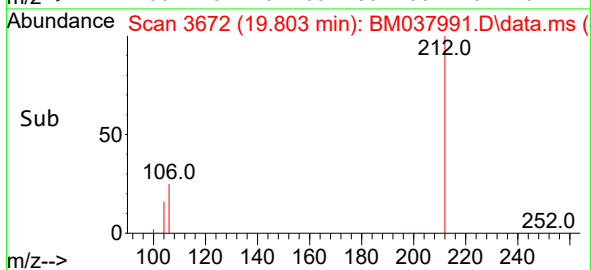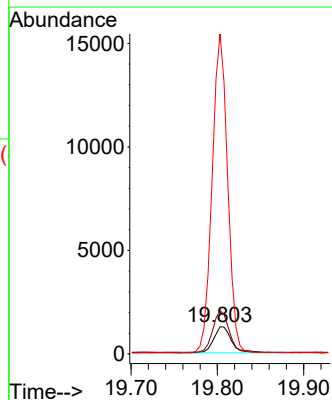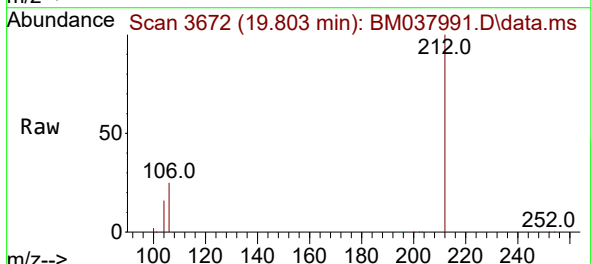

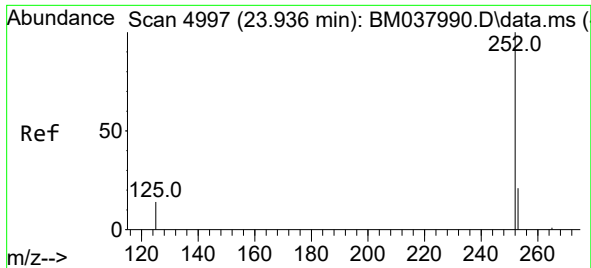

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.886 min Scan# 4997
Delta R.T. -0.053 min
Lab File: BM037991.D
Acq: 14 Dec 2022 11:12

Instrument :
BNA_M
ClientSampleId :
SBLK616

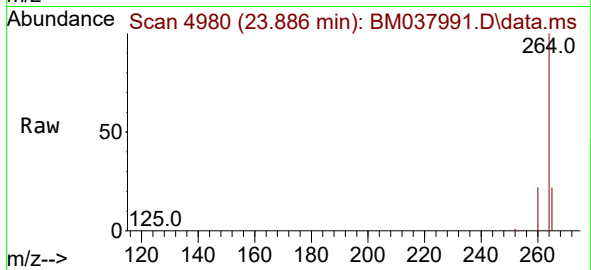

Tgt Ion:252 Resp: 3214
Ion Ratio Lower Upper
252 100
253 46.7 21.7 32.5#
125 66.6 20.4 30.6#

