

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
 Data File : BM038000.D
 Acq On : 14 Dec 2022 16:43
 Operator : CG/JU
 Sample : PB149556BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK556

Quant Time: Dec 14 23:27:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.068	152	4888	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	14721	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	8402	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	18128	0.400	ng/ul	0.00
17) Chrysene-d12	21.588	240	12554	0.400	ng/ul	0.00
23) Perylene-d12	24.047	264	13026	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	26652	3.866	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.462	152	5135	0.246	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	11127	0.260	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	1958	0.050	ng/ul#	16
20) Pyrene	19.808	202	2021	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.889	252	3818	0.065	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
Data File : BM038000.D
Acq On : 14 Dec 2022 16:43
Operator : CG/JU
Sample : PB149556BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK556

Quant Time: Dec 14 23:27:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 01:30:33 2022
Response via : Initial Calibration




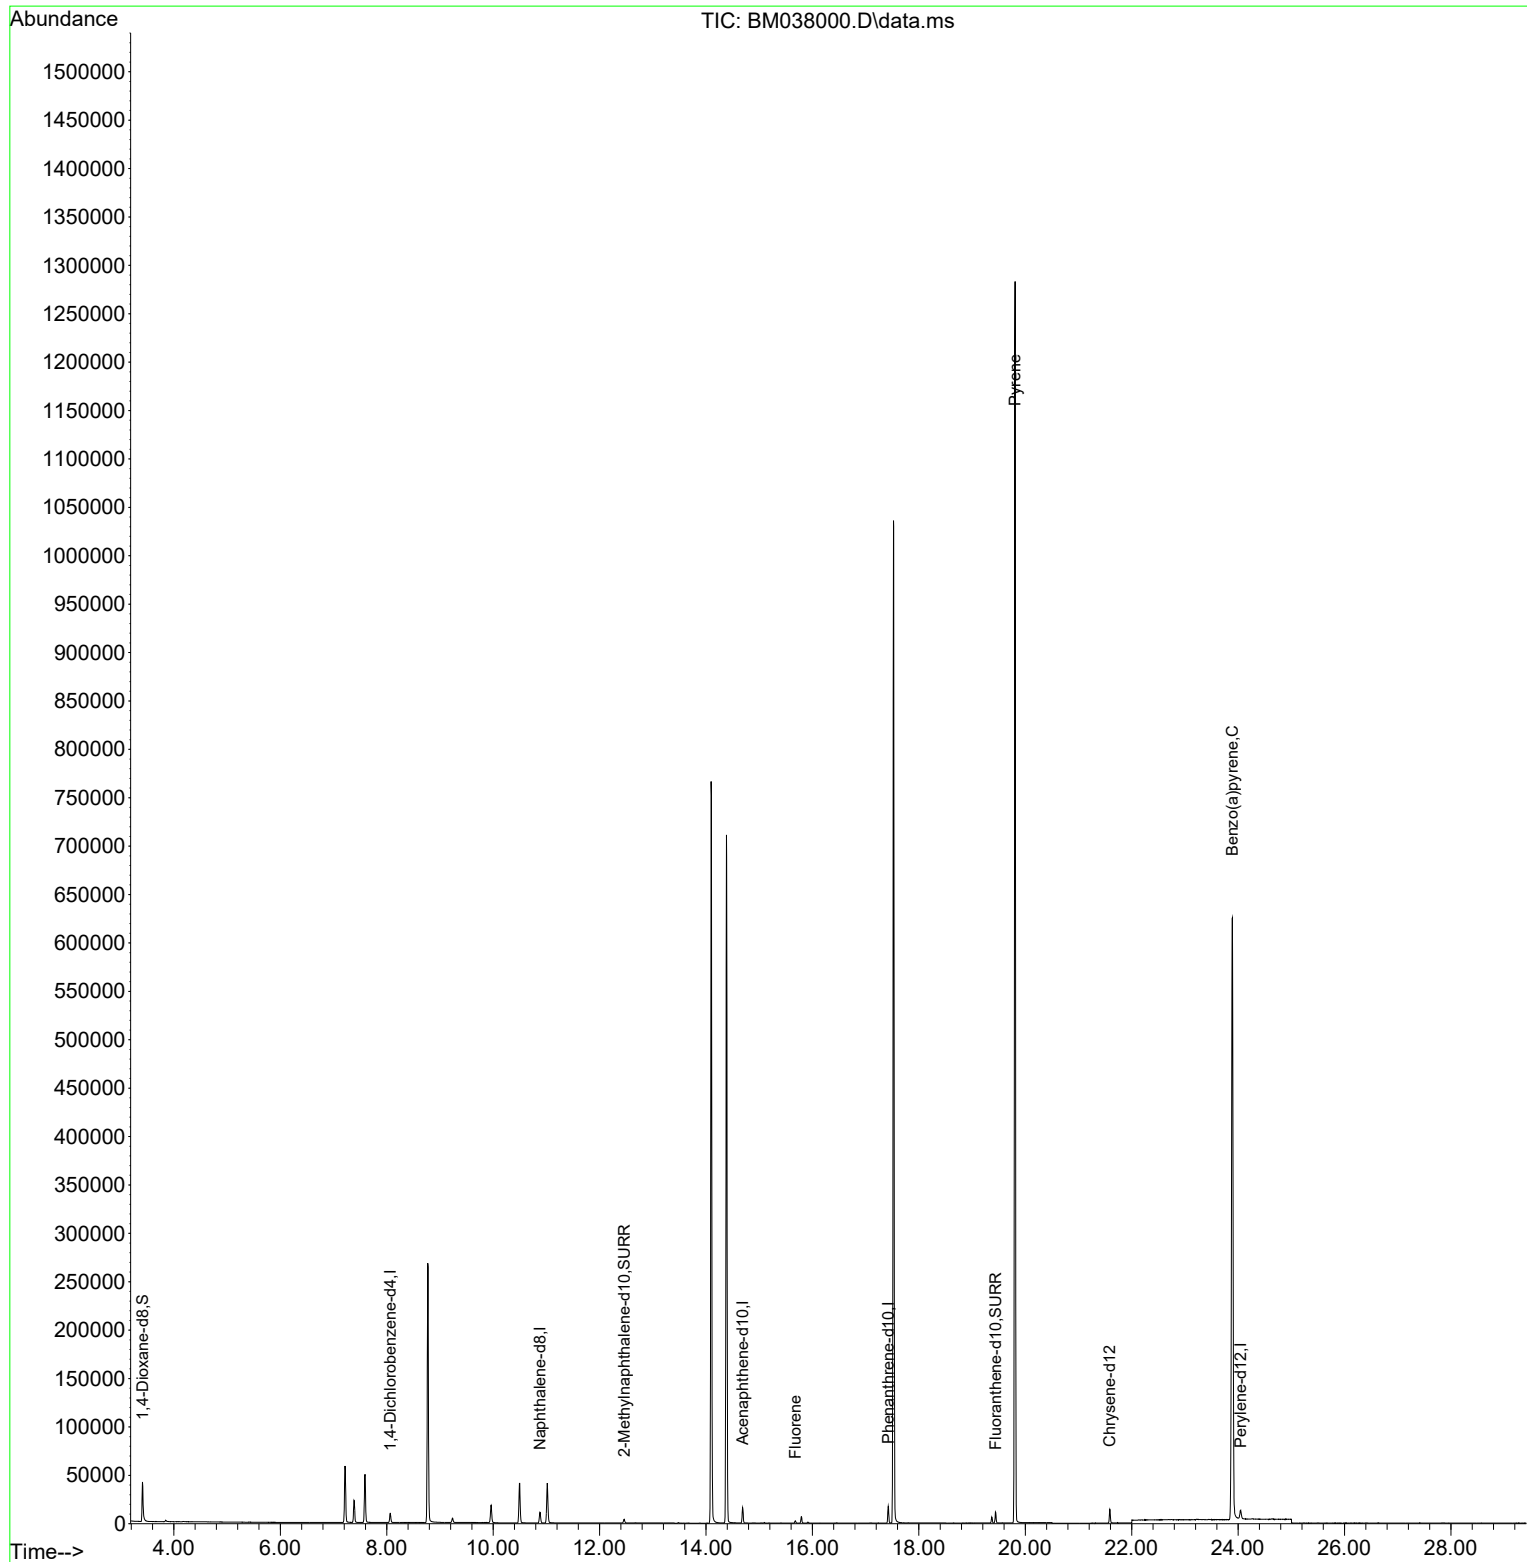


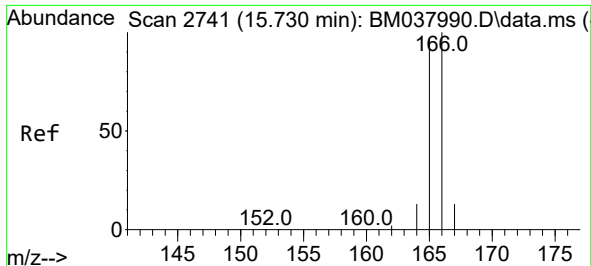

#12
Fluorene
Concen: 0.050 ng/ul
RT: 15.679 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM038000.D
Acq: 14 Dec 2022 16:43




Instrument :
BNA_M
ClientSampleId :
SBLK556


Tgt Ion:166 Resp: 1958
Ion Ratio Lower Upper
166 100
165 10.6 79.8 119.6#
167 35.0 11.7 17.5#

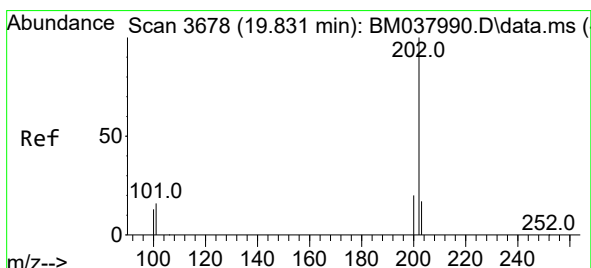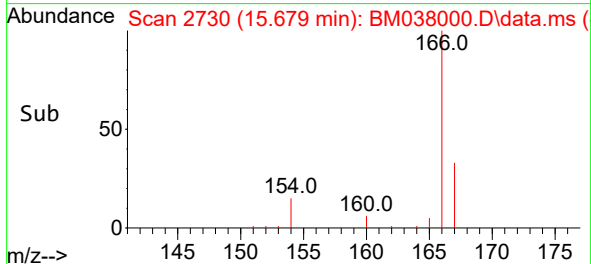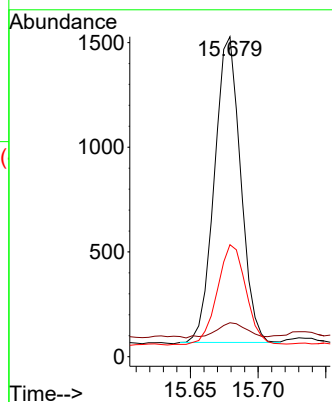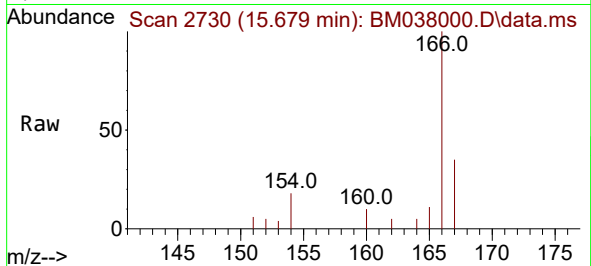

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.808 min Scan# 3673
Delta R.T. -0.028 min
Lab File: BM038000.D
Acq: 14 Dec 2022 16:43


Tgt Ion:202 Resp: 2021
Ion Ratio Lower Upper
202 100
101 142.6 12.6 19.0#
100 998.1 10.6 15.8#

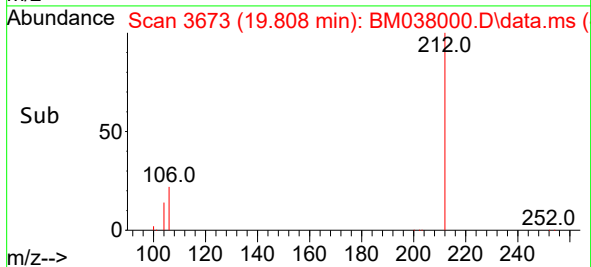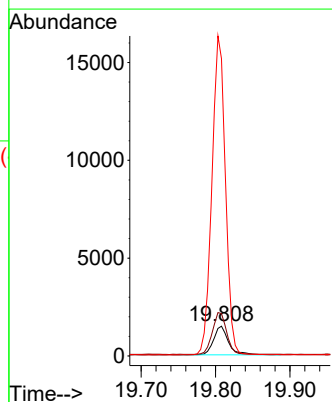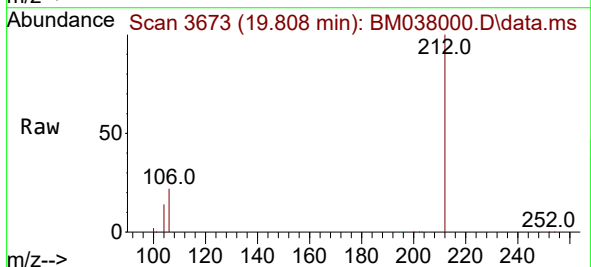

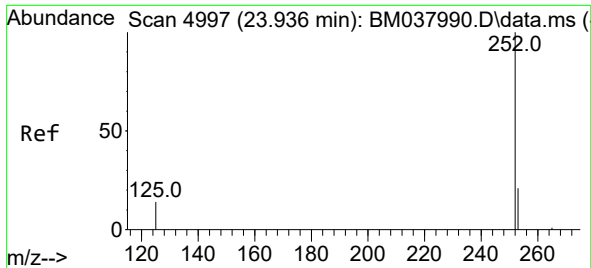

#26
Benzo(a)pyrene
Concen: 0.065 ng/ul
RT: 23.889 min Scan# 4981
Delta R.T. -0.050 min
Lab File: BM038000.D
Acq: 14 Dec 2022 16:43

Instrument :
BNA_M
ClientSampleId :
SBLK556

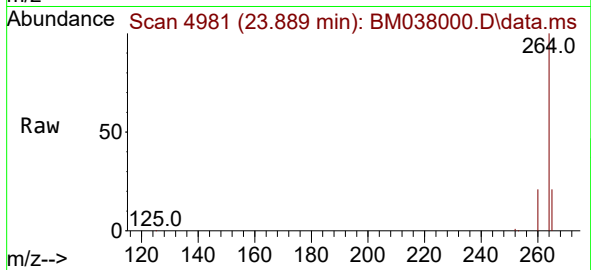

Tgt Ion:252 Resp: 3818
Ion Ratio Lower Upper
252 100
253 47.0 21.7 32.5#
125 63.7 20.4 30.6#

