

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
 Data File : BM037995.D
 Acq On : 14 Dec 2022 13:39
 Operator : CG/JU
 Sample : N6018-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBYJ9

Quant Time: Dec 14 23:26:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	4419	0.400	ng/u1	0.00
4) Naphthalene-d8	10.884	136	13033	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.689	164	7351	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.426	188	15486	0.400	ng/u1	0.00
17) Chrysene-d12	21.589	240	10467	0.400	ng/u1	0.00
23) Perylene-d12	24.047	264	10462	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	21979	3.527	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.462	152	5629	0.305	ng/u1	0.00
18) Fluoranthene-d10	19.441	212	13656	0.382	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	17.080	266	192	0.029	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
Data File : BM037995.D
Acq On : 14 Dec 2022 13:39
Operator : CG/JU
Sample : N6018-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBYJ9


Quant Time: Dec 14 23:26:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 01:30:33 2022
Response via : Initial Calibration

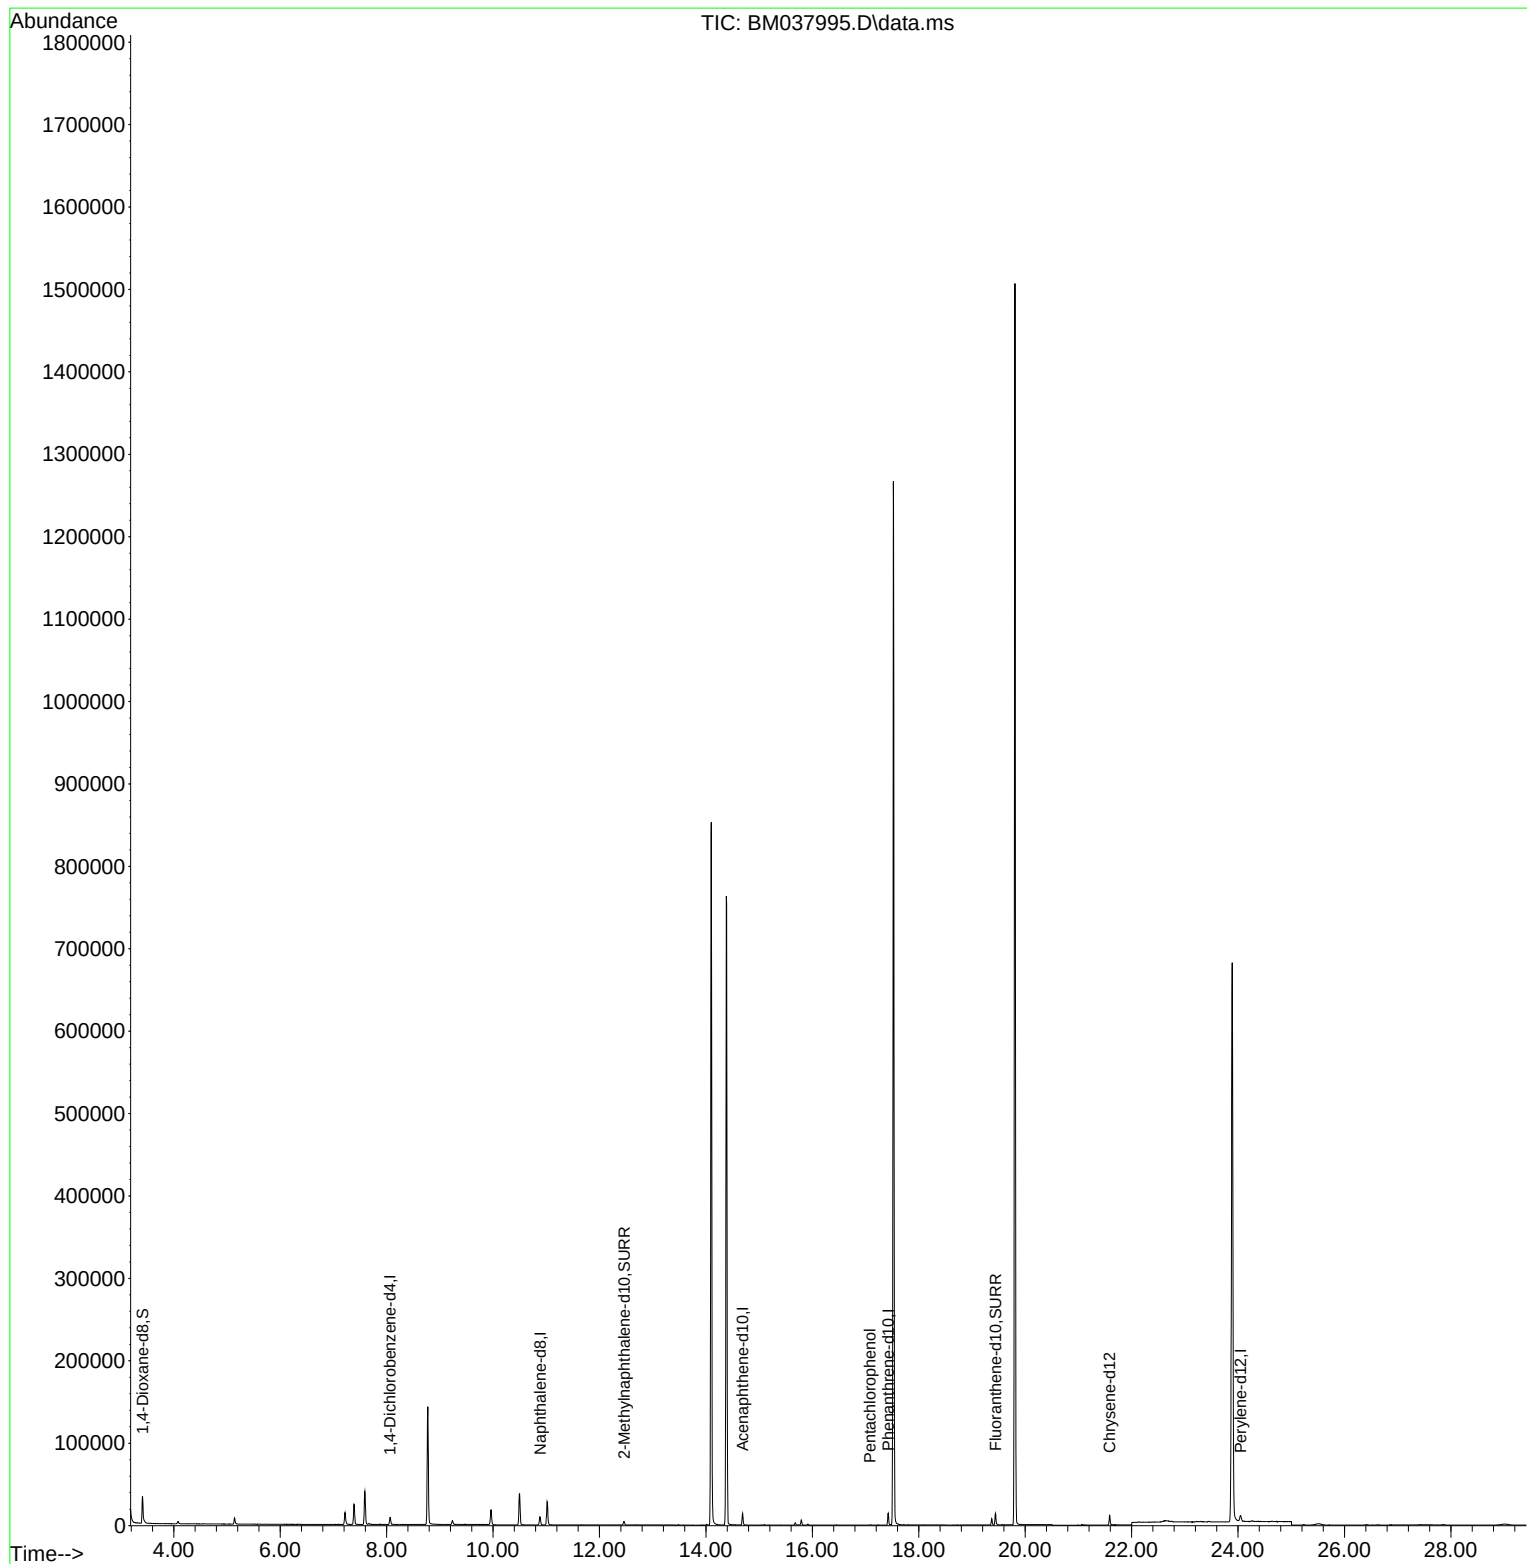

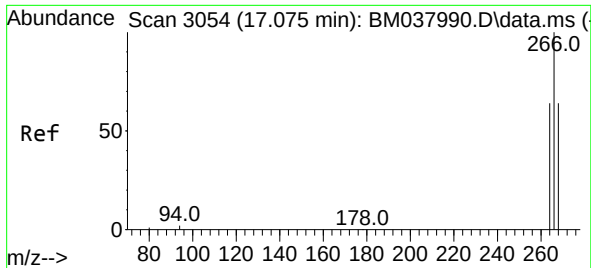

#14
 Pentachlorophenol
 Concen: 0.029 ng/ul
 RT: 17.080 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BM037995.D
 Acq: 14 Dec 2022 13:39

Instrument :
 BNA_M
 ClientSampleId :
 DBYJ9

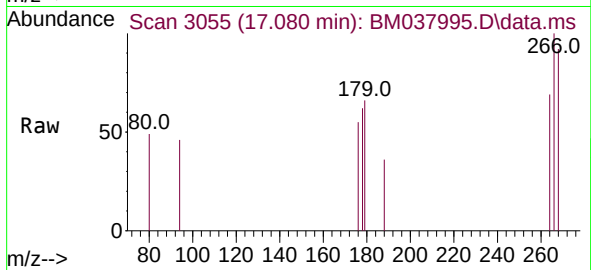

Tgt Ion: 266 Resp: 192

Ion	Ratio	Lower	Upper
266	100		
264	60.9	50.9	76.3
268	67.7	50.4	75.6

