

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
 Data File : BM038013.D
 Acq On : 15 Dec 2022 00:42
 Operator : CG/JU
 Sample : N5983-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD8

Quant Time: Dec 15 01:32:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	6037	0.400	ng/u1	0.00
4) Naphthalene-d8	10.878	136	18631	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.689	164	10436	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.422	188	21838	0.400	ng/u1	0.00
17) Chrysene-d12	21.586	240	14659	0.400	ng/u1	0.00
23) Perylene-d12	24.041	264	13744	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	27470	3.227	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	6497	0.246	ng/u1	0.00
18) Fluoranthene-d10	19.441	212	13571	0.271	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	17.075	266	620	0.067	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
Data File : BM038013.D
Acq On : 15 Dec 2022 00:42
Operator : CG/JU
Sample : N5983-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD8

Quant Time: Dec 15 01:32:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 01:30:33 2022
Response via : Initial Calibration

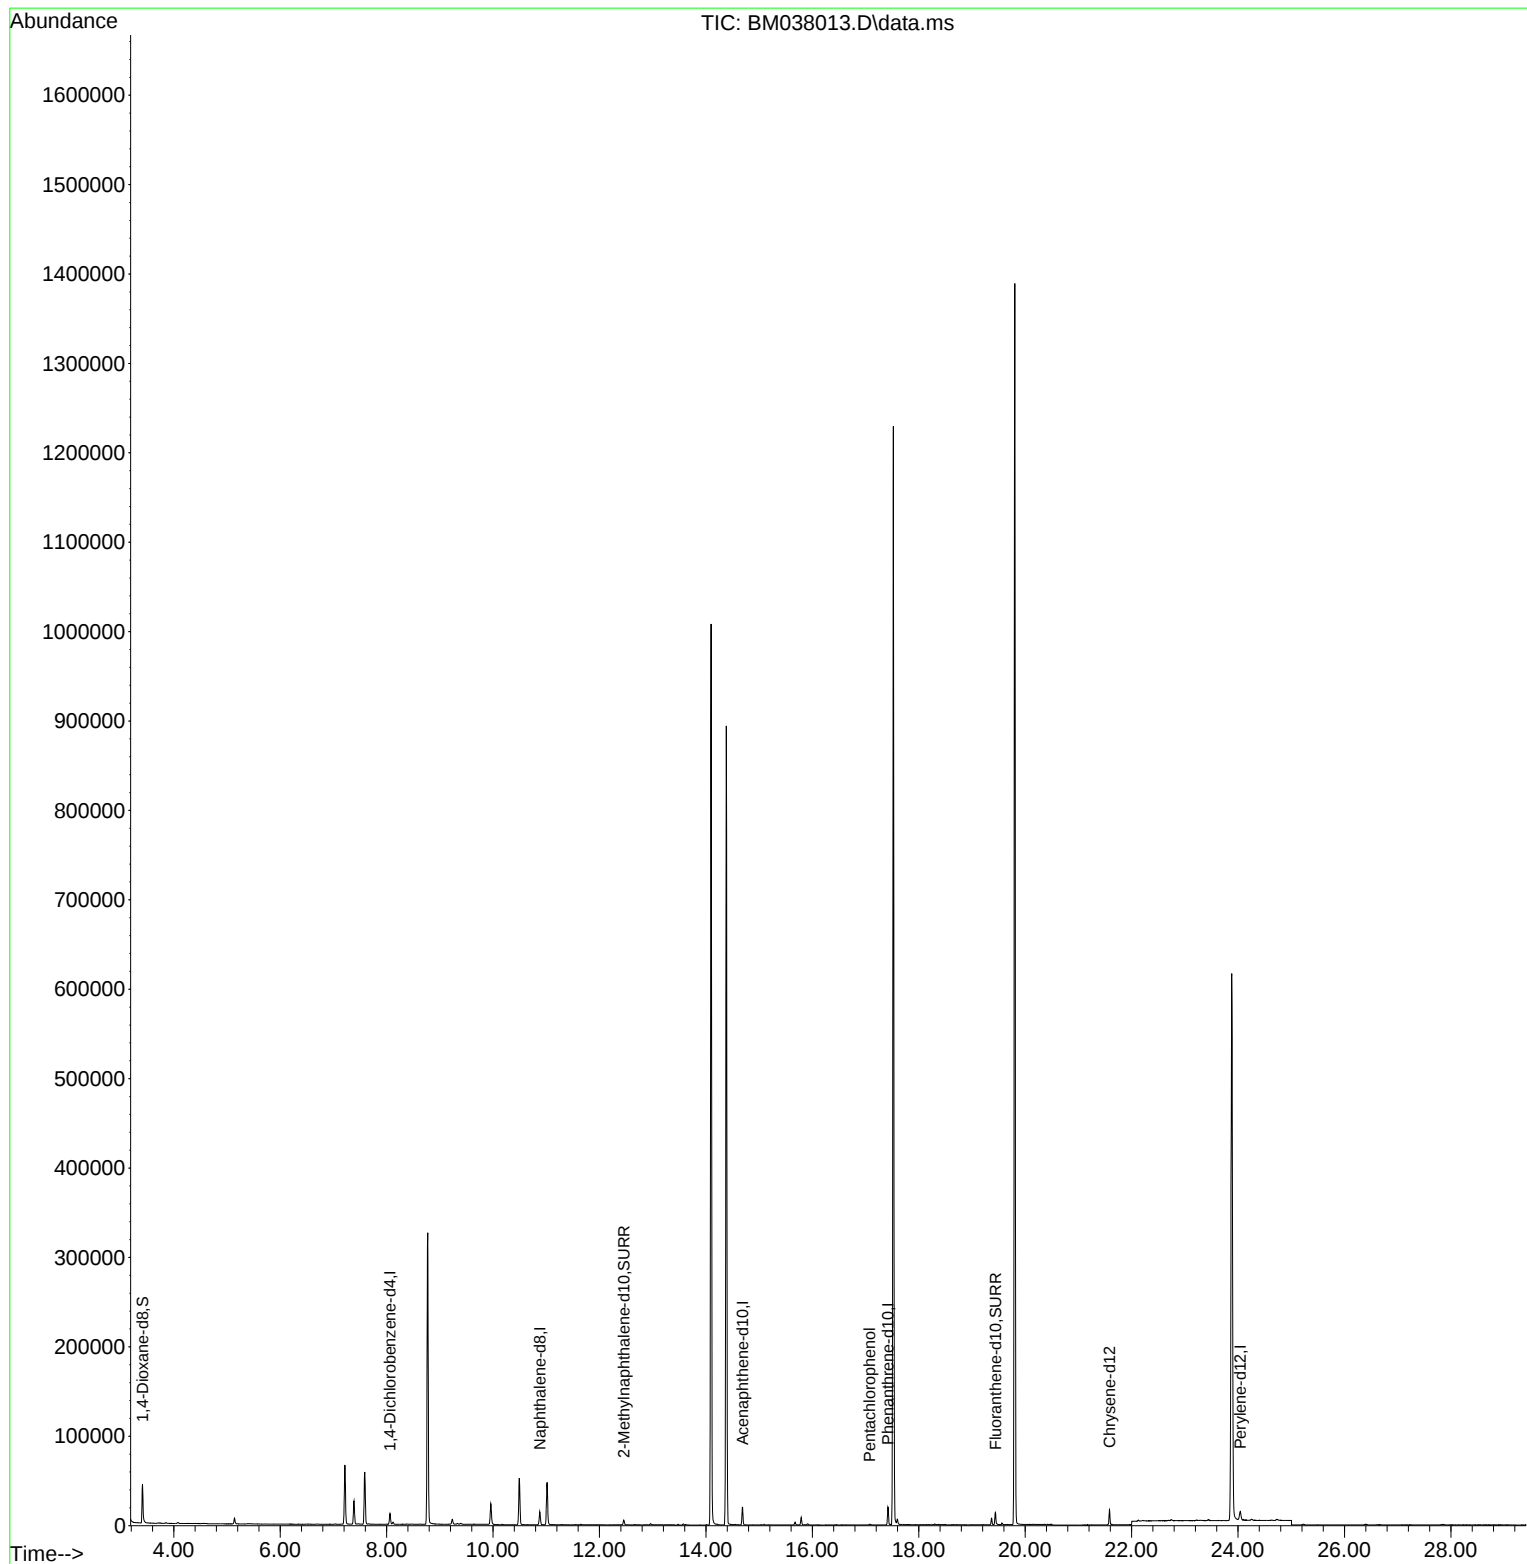

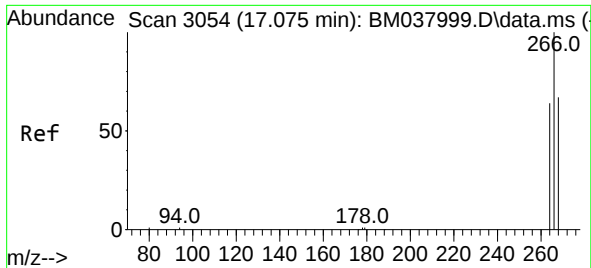

#14

Pentachlorophenol

Concen: 0.067 ng/ul

RT: 17.075 min Scan# 30

Delta R.T. -0.004 min

Lab File: BM038013.D


Acq: 15 Dec 2022 00:42

Instrument :

BNA_M

ClientSampleId :

COLD8

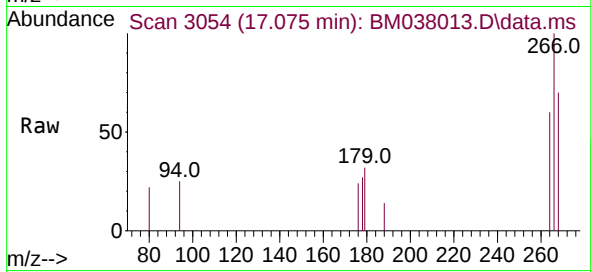

Tgt Ion:266 Resp: 620

Ion Ratio Lower Upper

266 100

264 65.6 50.9 76.3

268 58.5 50.4 75.6

