

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
 Data File : BM038014.D
 Acq On : 15 Dec 2022 01:18
 Operator : CG/JU
 Sample : N5983-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLB9

Quant Time: Dec 15 02:18:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 14 01:30:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	4992	0.400	ng/u1	0.00
4) Naphthalene-d8	10.878	136	15262	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.685	164	8771	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.422	188	19282	0.400	ng/u1	0.00
17) Chrysene-d12	21.583	240	13605	0.400	ng/u1	0.00
23) Perylene-d12	24.038	264	13646	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	27807	3.950	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	6738	0.312	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	14556	0.314	ng/u1	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	17.071	266	85156	10.388	ng/u1	99
24) Benzo(b)fluoranthene	23.287	252	2181	0.029	ng/u1#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121422\
Data File : BM038014.D
Acq On : 15 Dec 2022 01:18
Operator : CG/JU
Sample : N5983-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLB9

Quant Time: Dec 15 02:18:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 14 01:30:33 2022
Response via : Initial Calibration




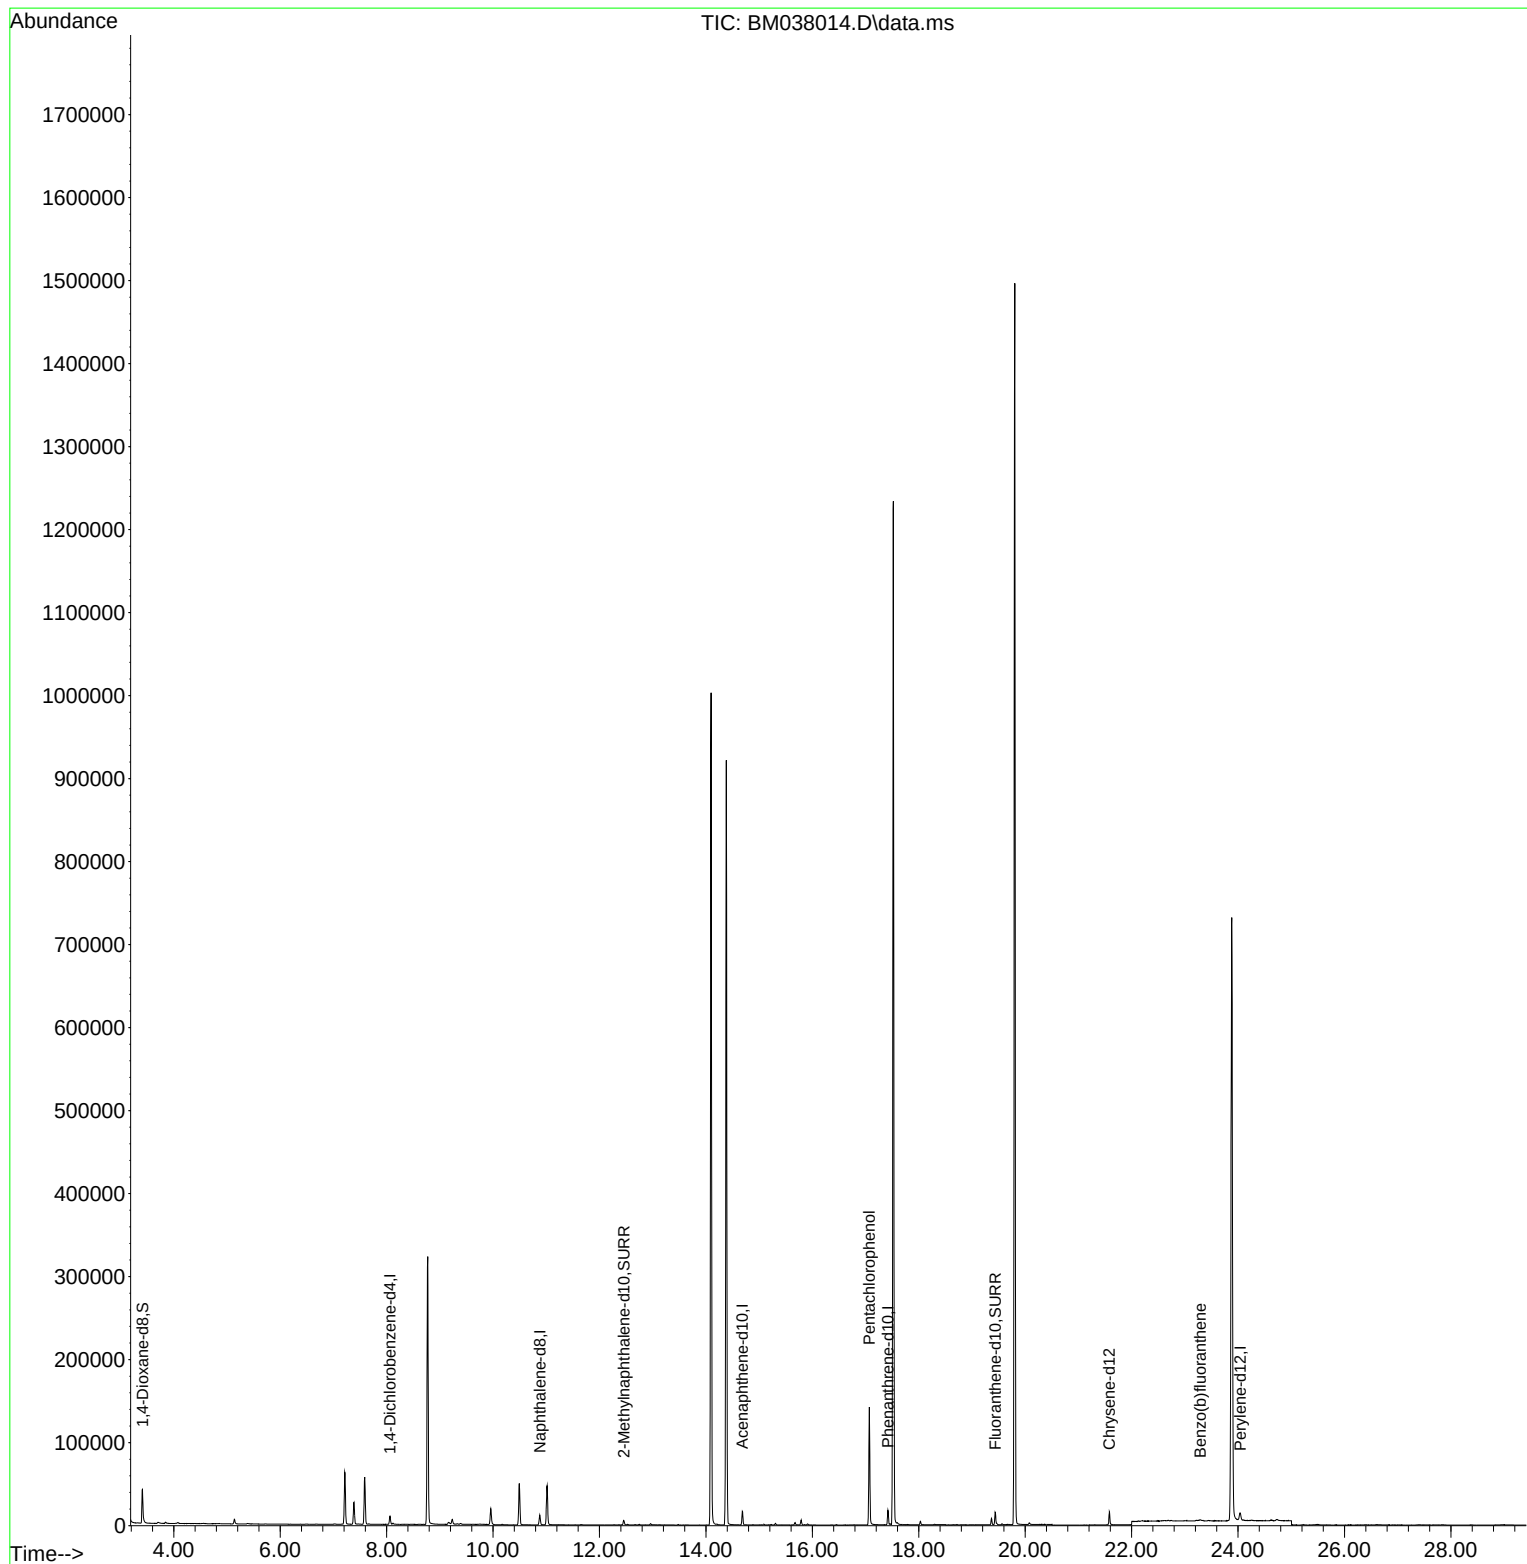


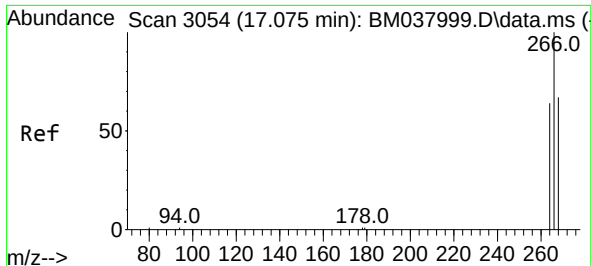

#14
 Pentachlorophenol
 Concen: 10.388 ng/ul
 RT: 17.071 min Scan# 3054
 Delta R.T. -0.009 min
 Lab File: BM038014.D
 Acq: 15 Dec 2022 01:18

Instrument :
 BNA_M
 ClientSampleId :
 COLB9

Tgt Ion:266 Resp: 85156
 Ion Ratio Lower Upper
 266 100
 264 62.5 50.9 76.3
 268 63.9 50.4 75.6

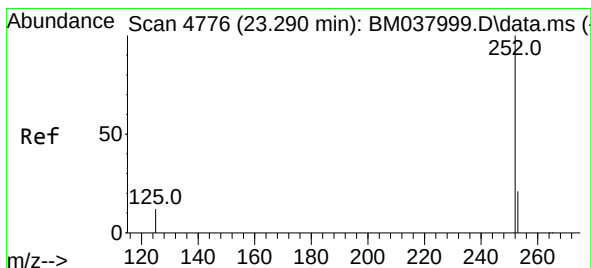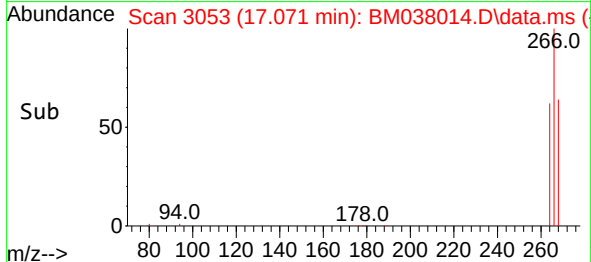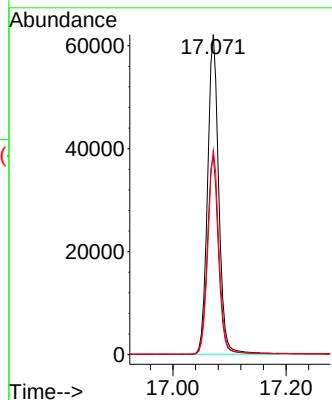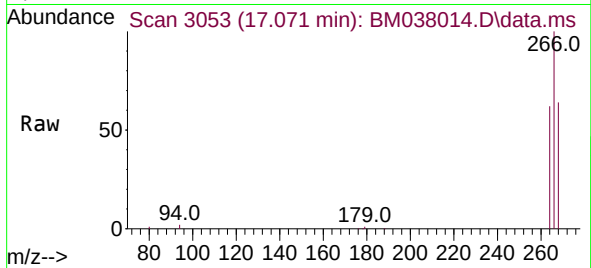

#24
 Benzo(b)fluoranthene
 Concen: 0.029 ng/ul
 RT: 23.287 min Scan# 4775
 Delta R.T. -0.009 min
 Lab File: BM038014.D
 Acq: 15 Dec 2022 01:18

Tgt Ion:252 Resp: 2181
 Ion Ratio Lower Upper
 252 100
 253 55.7 0.0 49.6#
 125 75.8 0.0 39.6#

