


Instrument :
BNA_M
ClientSampleId :

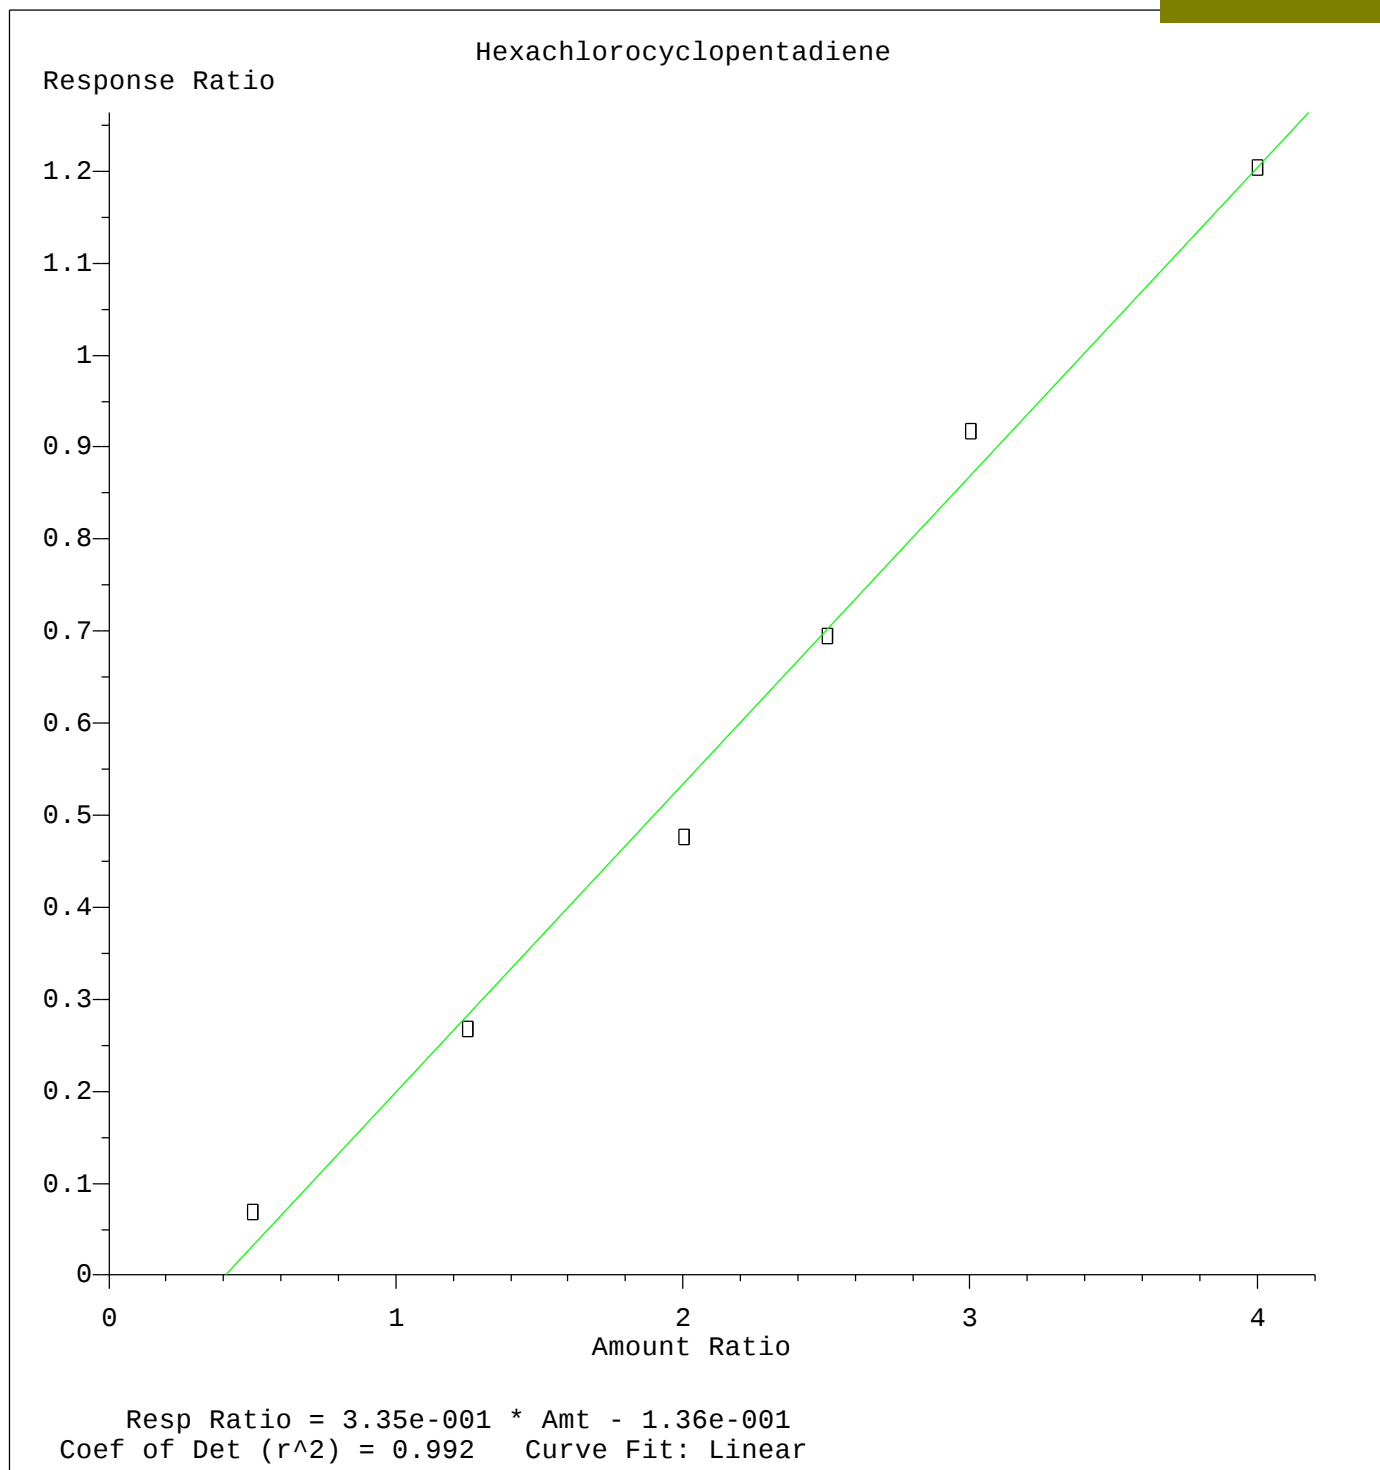

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Calibration Table Last Updated: Sat Dec 15 21:39:37 2018