

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018255.D
 Acq On : 17 Dec 2018 18:52
 Operator : JU/SJ
 Sample : J6340-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-03A

Quant Time: Dec 18 00:52:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	151128	20.00	ng	-0.01
21) Naphthalene-d8	10.26	136	561506	20.00	ng	-0.01
39) Acenaphthene-d10	14.15	164	269153	20.00	ng	-0.01
64) Phenanthrene-d10	16.92	188	470465	20.00	ng	0.00
76) Chrysene-d12	21.13	240	477218	20.00	ng	-0.01
87) Perylene-d12	23.30	264	548404	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	1074126	118.73	ng	0.00
7) Phenol-d6	6.70	99	1420808	112.99	ng	0.00
23) Nitrobenzene-d5	8.65	82	921180	84.15	ng	-0.01
42) 2,4,6-Tribromophenol	15.66	330	340545	86.20	ng	0.00
45) 2-Fluorobiphenyl	12.76	172	1687428	81.20	ng	-0.01
79) Terphenyl-d14	19.57	244	1464684	69.41	ng	0.00
Target Compounds						
10) Phenol	6.72	94	77871	5.847	ng	94
50) Dimethylphthalate	13.62	163	125598	5.613	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
Data File : BM018255.D
Acq On : 17 Dec 2018 18:52
Operator : JU/SJ
Sample : J6340-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-03A

Quant Time: Dec 18 00:52:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

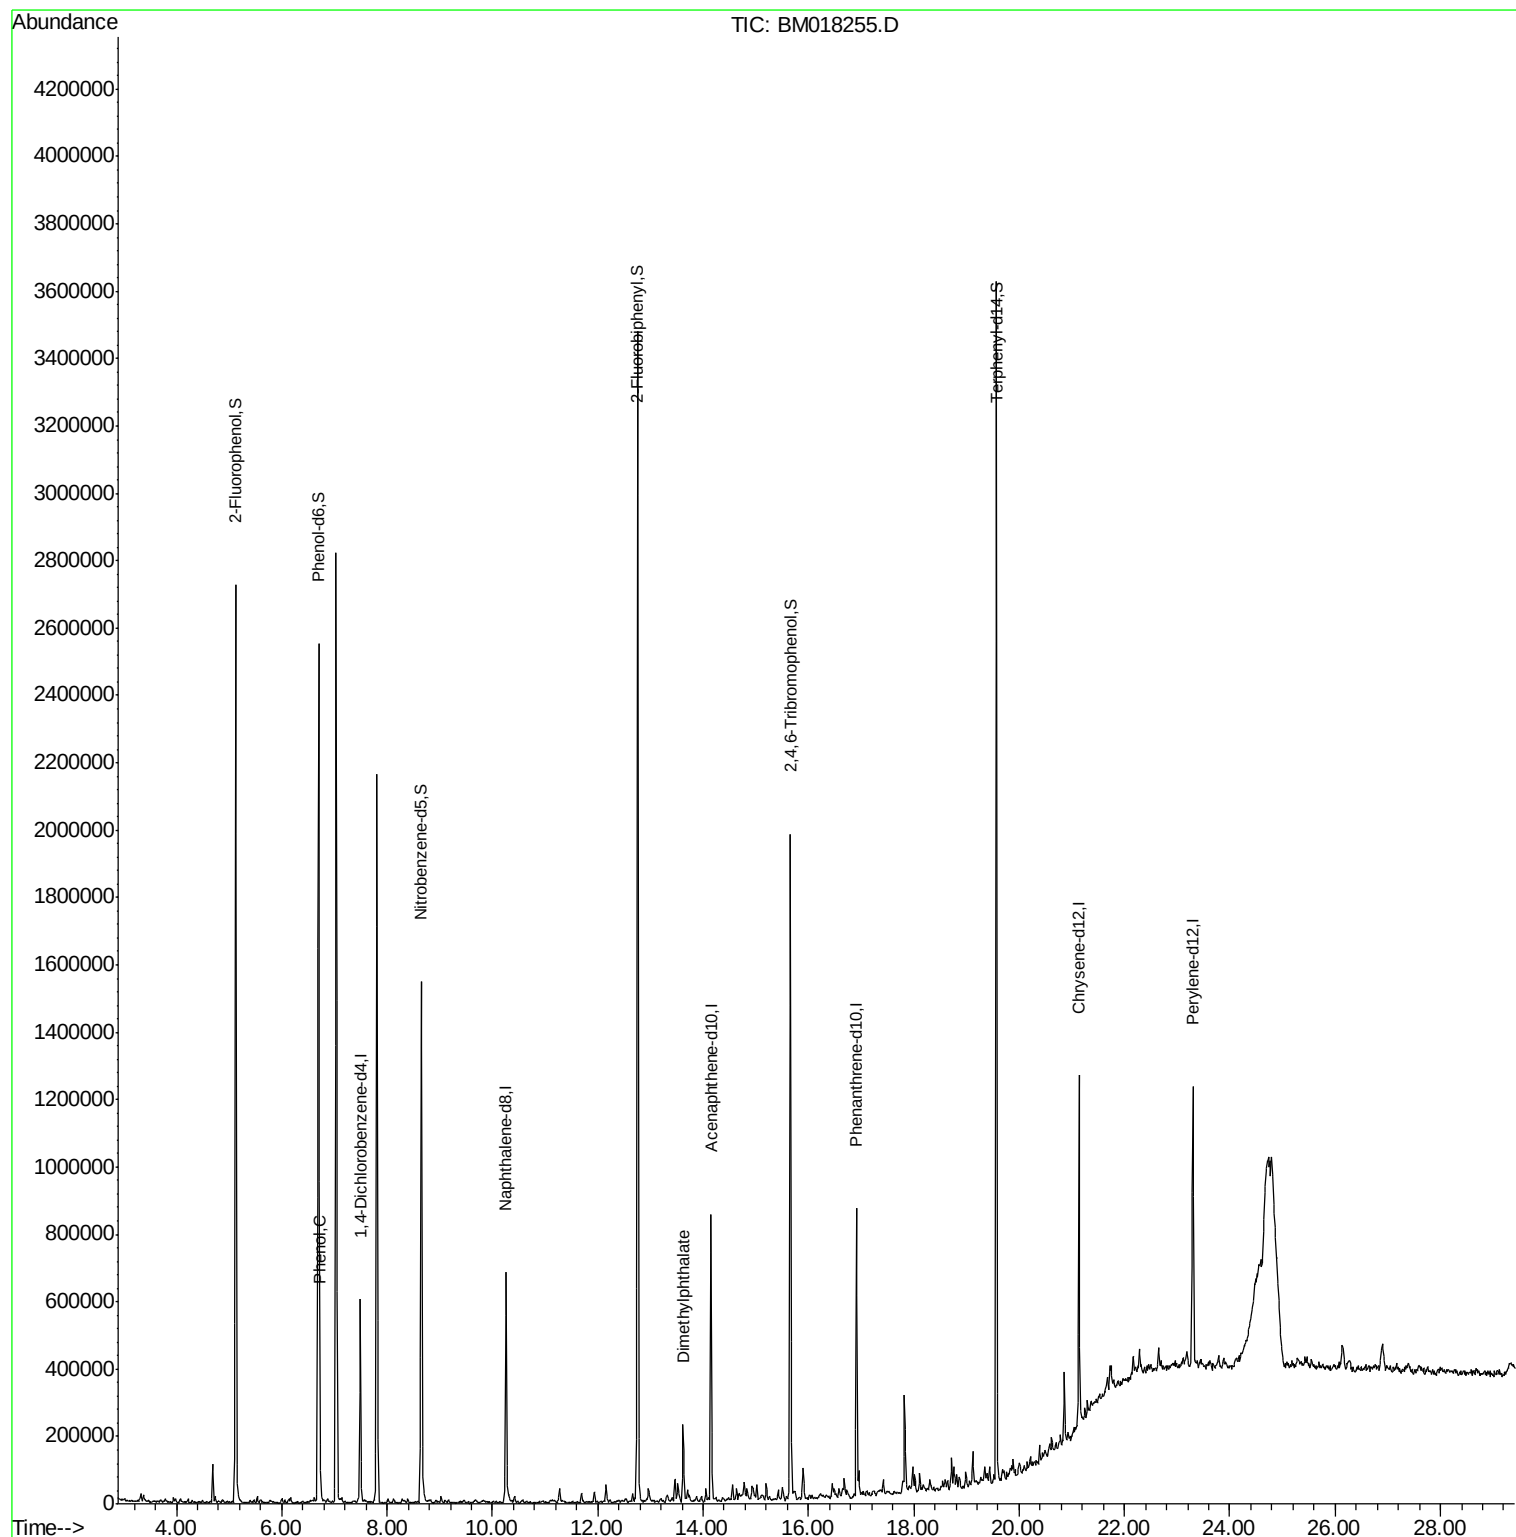

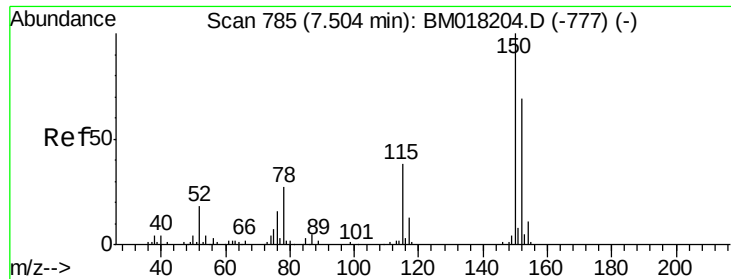


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 783
Delta R.T. -0.01 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52

Instrument :
BNA_M
ClientSampleId :
SB-03A

Tgt Ion:152 Resp: 151128
Ion Ratio Lower Upper
152 100
150 148.2 116.1 174.1
115 60.0 44.6 67.0

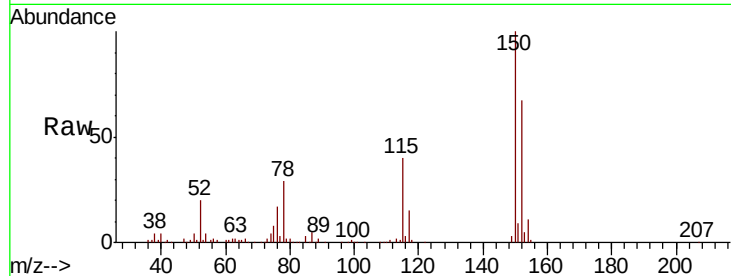


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

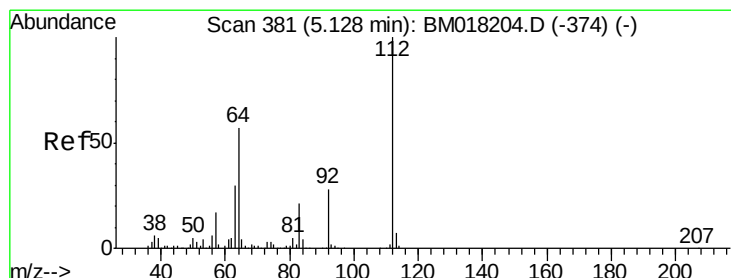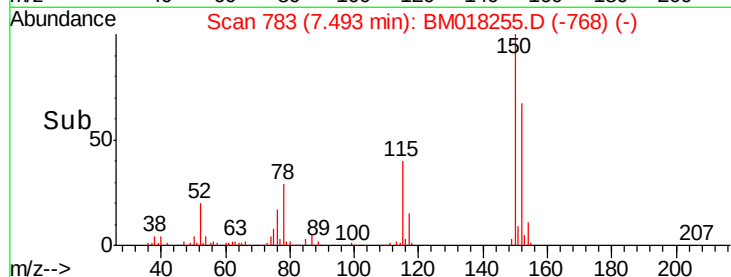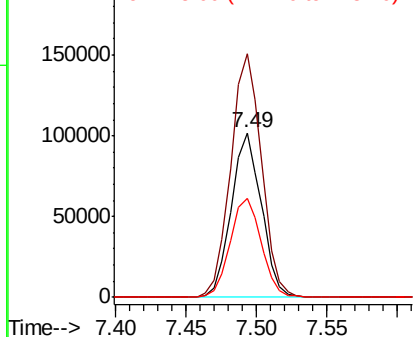



#5


2-Fluorophenol
Concen: 118.728 ng
RT: 5.13 min Scan# 381
Delta R.T. 0.00 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52

Tgt Ion:112 Resp: 1074126
Ion Ratio Lower Upper
112 100
64 56.5 45.4 68.2
63 31.1 24.0 36.0

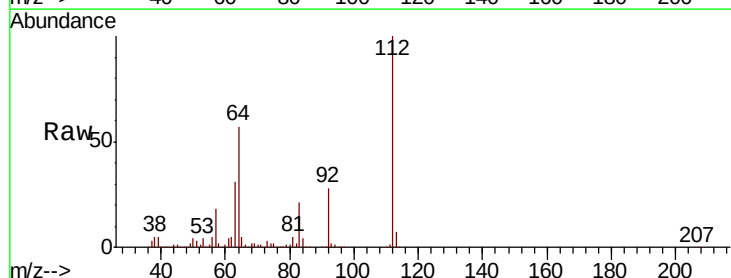

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

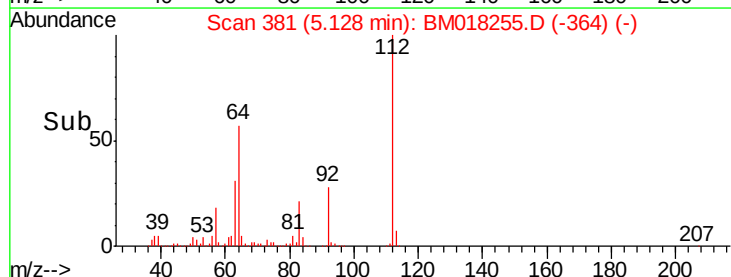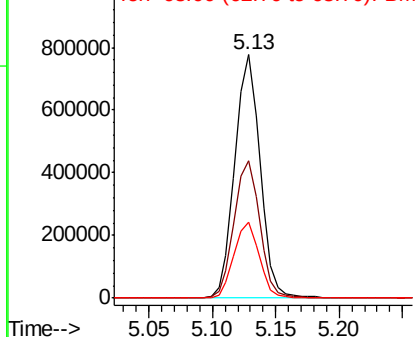

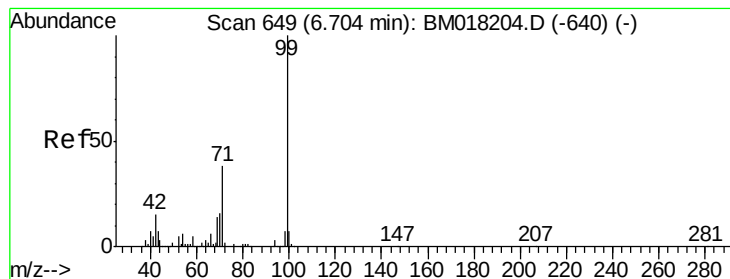

#7

Phenol-d6

Concen: 112.991 ng

RT: 6.70 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52

Instrument :

BNA_M

ClientSampleId :

SB-03A





Tgt Ion: 99 Resp: 1420808

Ion Ratio Lower Upper

99 100

42 15.9 12.3 18.5

71 38.9 30.2 45.2

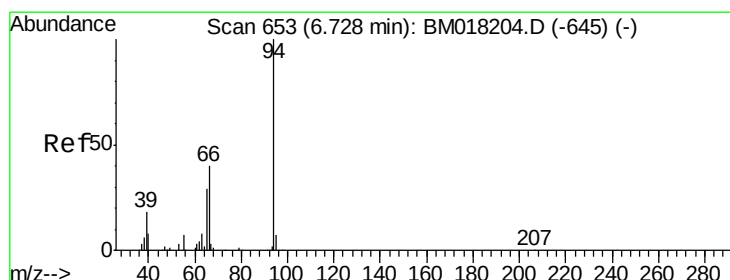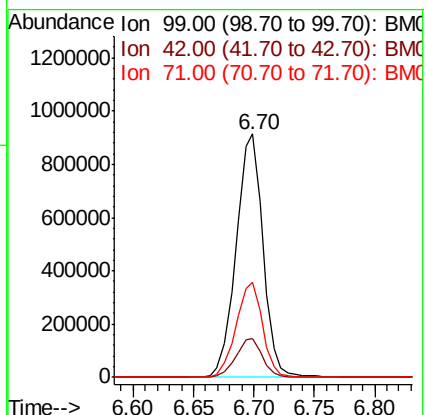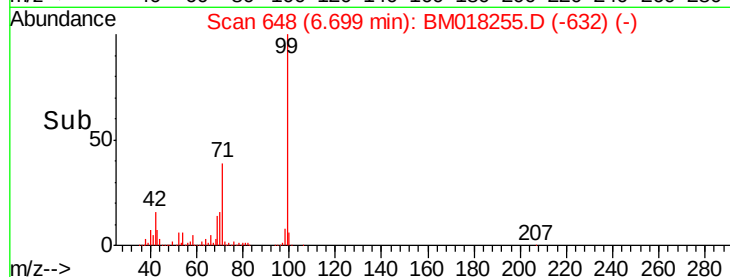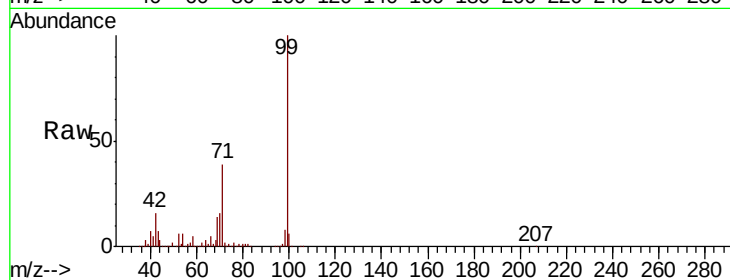

#10

Phenol

Concen: 5.847 ng

RT: 6.72 min Scan# 652

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52




Tgt Ion: 94 Resp: 77871


Ion Ratio Lower Upper

94 100

65 31.1 9.5 49.5

66 46.8 21.3 61.3

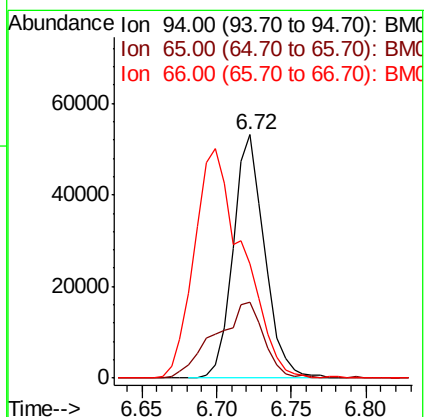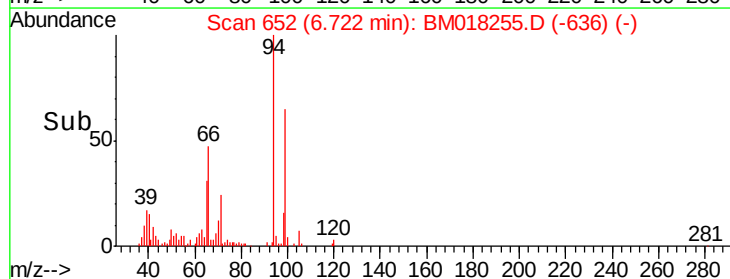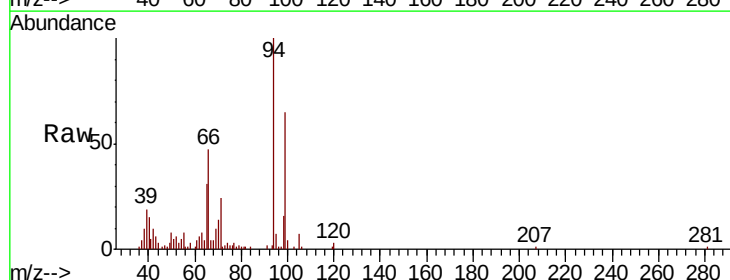


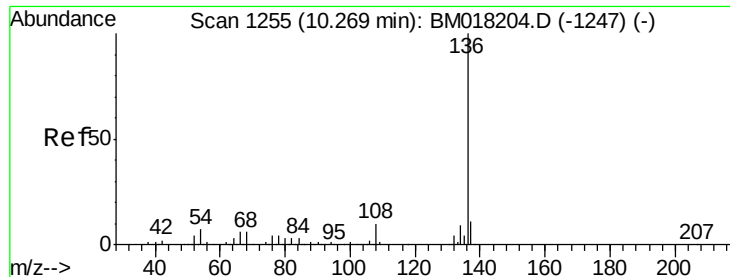




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.26 min Scan# 1253
Delta R.T. -0.01 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52

Instrument :
BNA_M
ClientSampleId :
SB-03A

Tgt Ion:	136	Resp:	561506
Ion	Ratio	Lower	Upper
136	100		
137	10.6	9.2	13.8
54	6.5	5.2	7.8
68	6.1	5.0	7.6

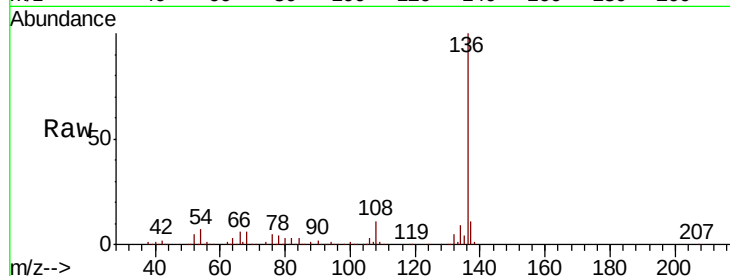


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

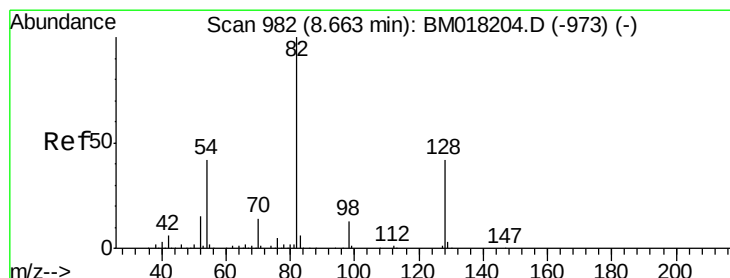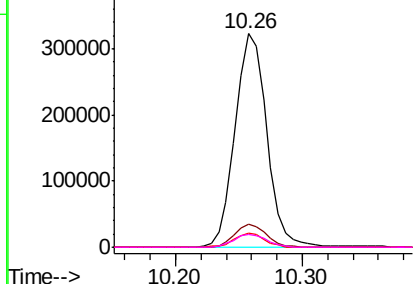
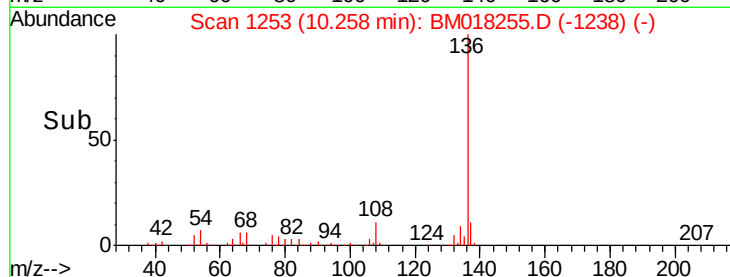



#23
Nitrobenzene-d5
Concen: 84.150 ng
RT: 8.65 min Scan# 980
Delta R.T. -0.01 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52

Tgt Ion:	82	Resp:	921180
Ion	Ratio	Lower	Upper
82	100		
128	39.6	33.4	50.2
54	41.7	33.4	50.2

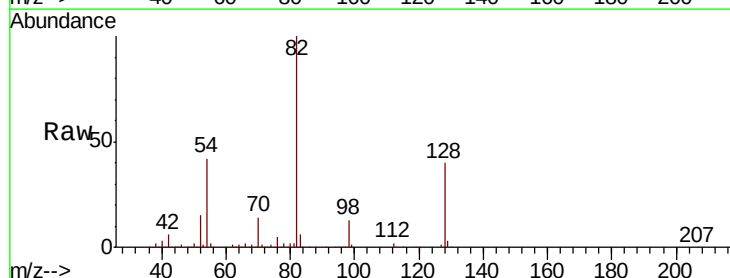

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

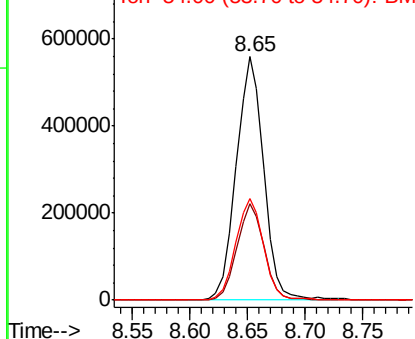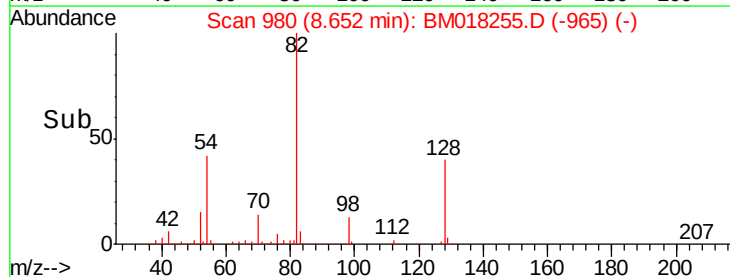

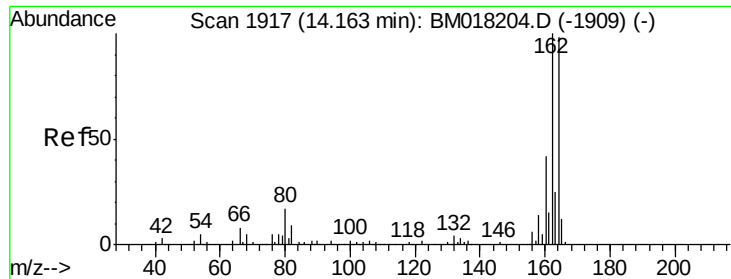

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.15 min Scan# 1915

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52

Instrument :

BNA_M

ClientSampleId :

SB-03A


Tgt Ion:164 Resp: 269153

Ion Ratio Lower Upper

164 100

162 102.8 81.8 122.6




160 45.3 34.6 51.8

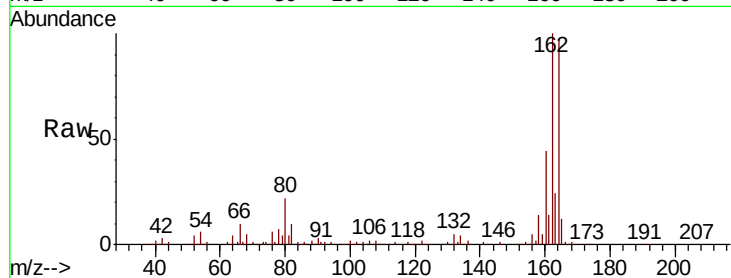

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

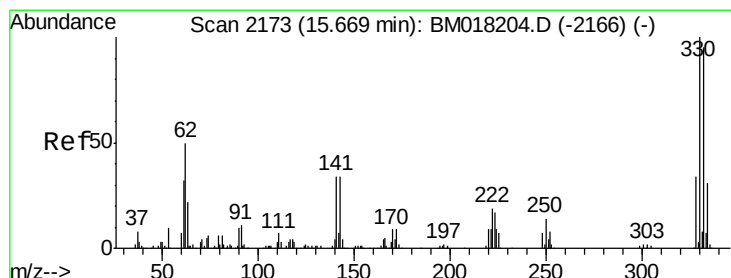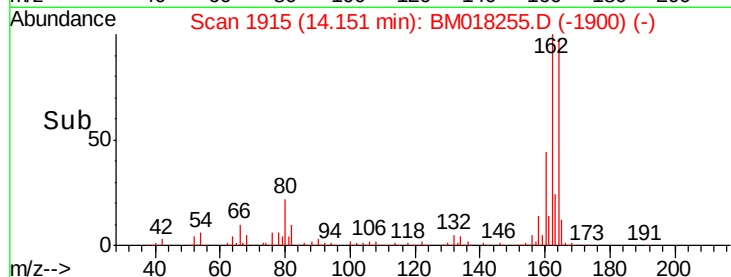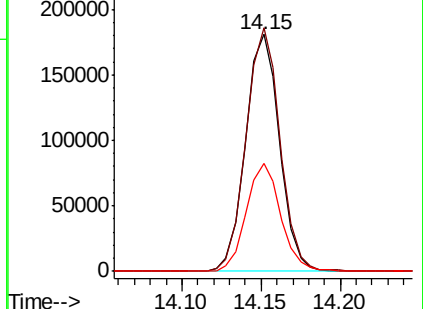

#42

2,4,6-Tribromophenol

Concen: 86.205 ng

RT: 15.66 min Scan# 2172

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52


Tgt Ion:330 Resp: 340545

Ion Ratio Lower Upper

330 100

332 98.2 78.6 118.0



141 36.5 27.1 40.7

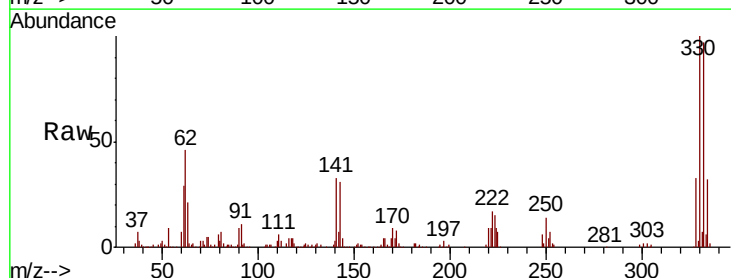


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



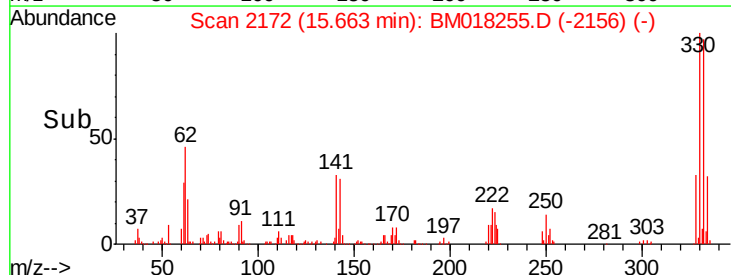
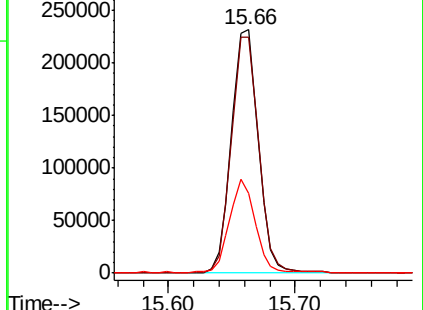


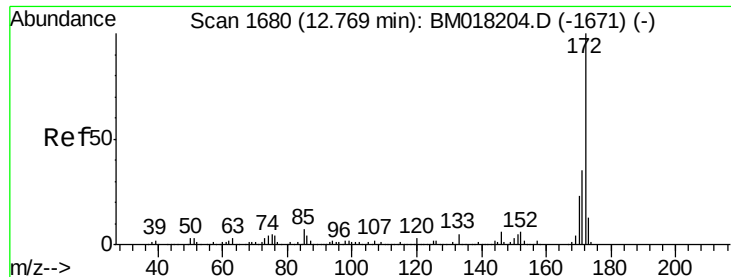

#45
2-Fluorobiphenyl
Concen: 81.204 ng
RT: 12.76 min Scan# 1678
Delta R.T. -0.01 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52




Instrument :
BNA_M
ClientSampleId :
SB-03A


Tgt Ion:172 Resp: 1687428
Ion Ratio Lower Upper
172 100
171 35.0 28.3 42.5
170 22.2 18.1 27.1

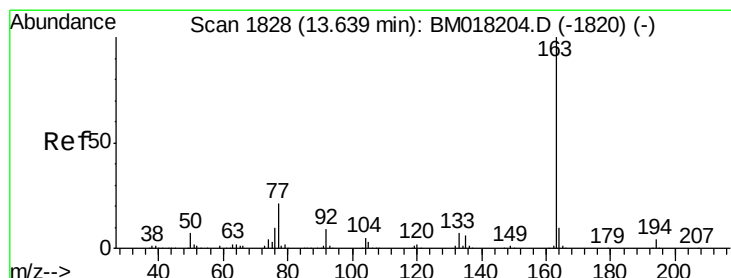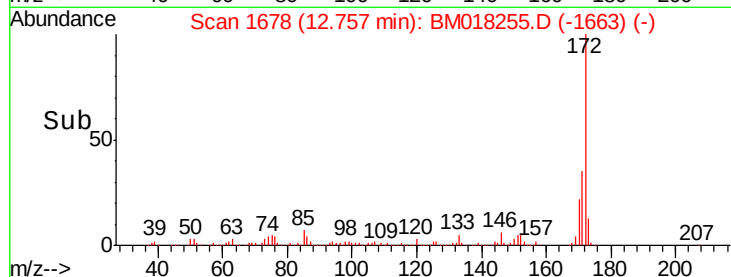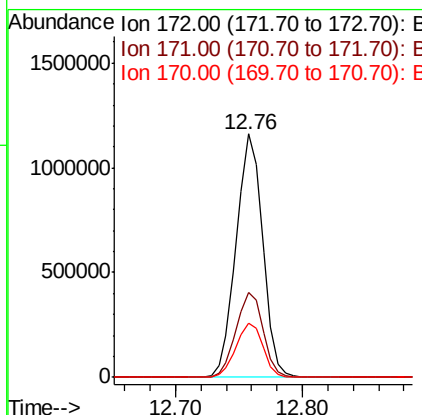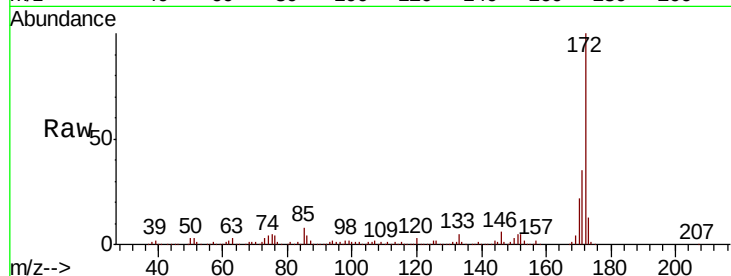

#50
Dimethylphthalate
Concen: 5.613 ng
RT: 13.62 min Scan# 1825
Delta R.T. -0.02 min
Lab File: BM018255.D
Acq: 17 Dec 2018 18:52

Tgt Ion:163 Resp: 125598
Ion Ratio Lower Upper
163 100
194 4.3 3.1 4.7
164 9.8 7.9 11.9

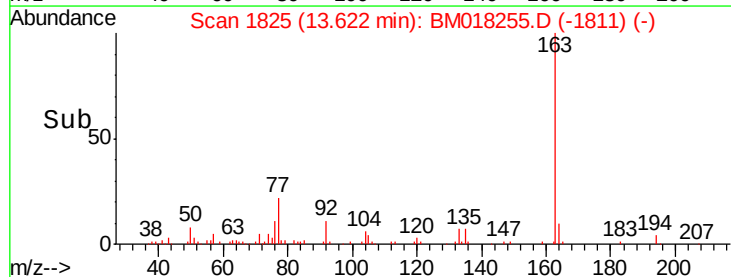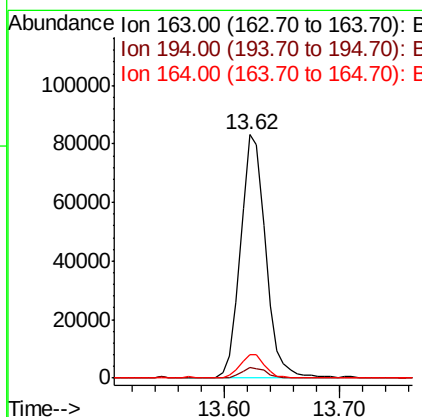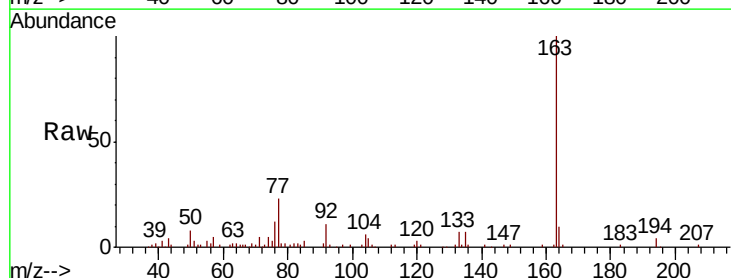

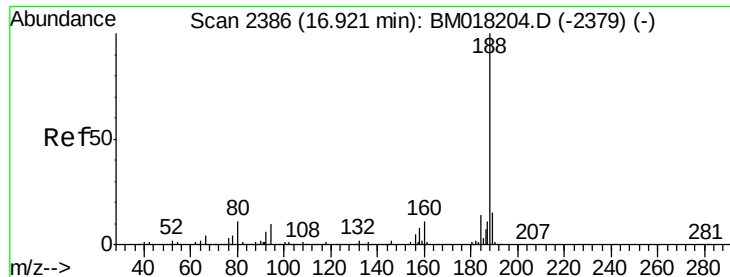

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.92 min Scan# 2385

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52

Instrument :

BNA_M

ClientSampleId :

SB-03A


Tgt Ion:188 Resp: 470465

Ion Ratio Lower Upper

188 100

94 9.3 8.0 12.0




80 11.6 9.0 13.6

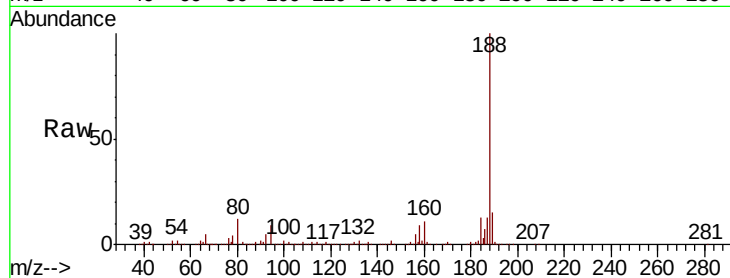

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

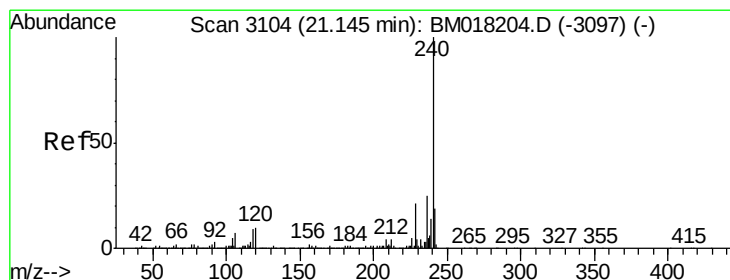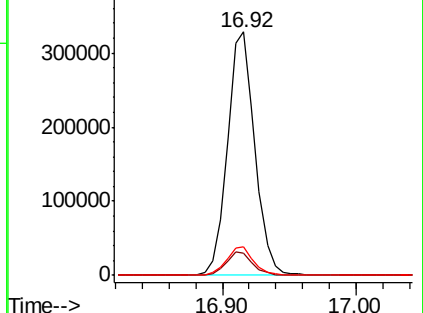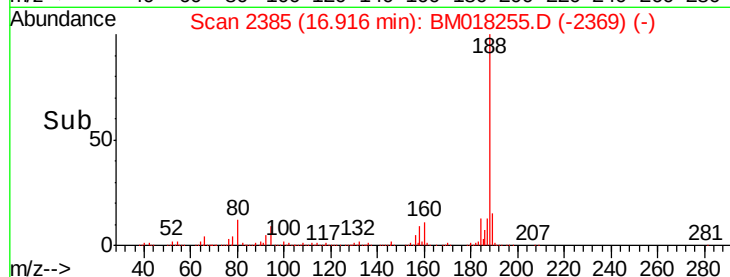

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.13 min Scan# 3102

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52


Tgt Ion:240 Resp: 477218

Ion Ratio Lower Upper

240 100

120 10.5 8.2 12.2



236 24.4 20.3 30.5

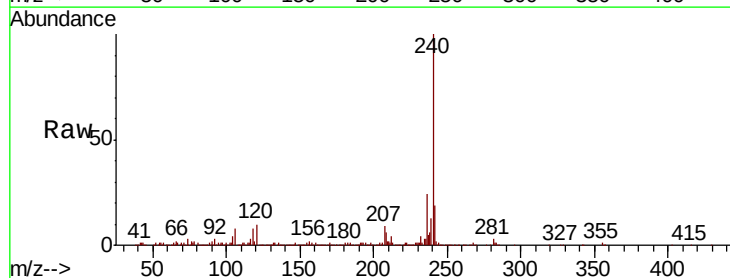


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

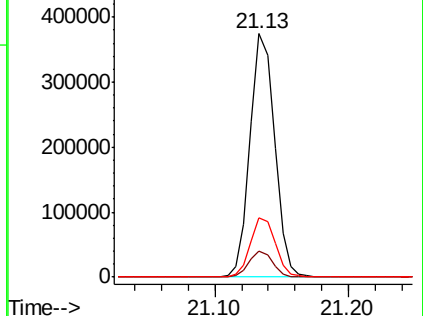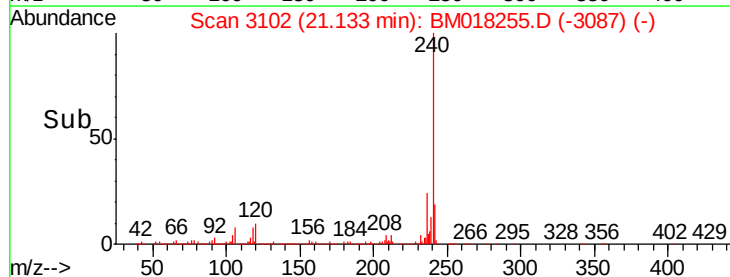

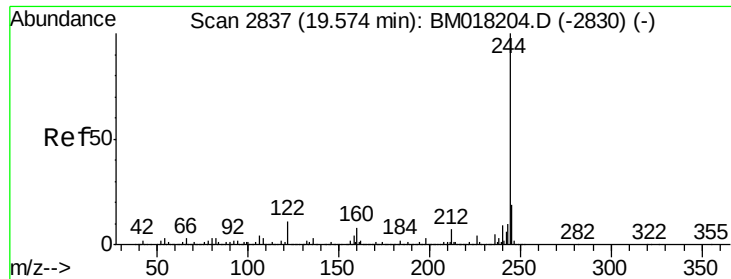

#79

Terphenyl-d14

Concen: 69.415 ng

RT: 19.57 min Scan# 2836

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52

Instrument :

BNA_M

ClientSampleId :

SB-03A


Tgt Ion:244 Resp: 1464684

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8




122 10.8 9.0 13.6

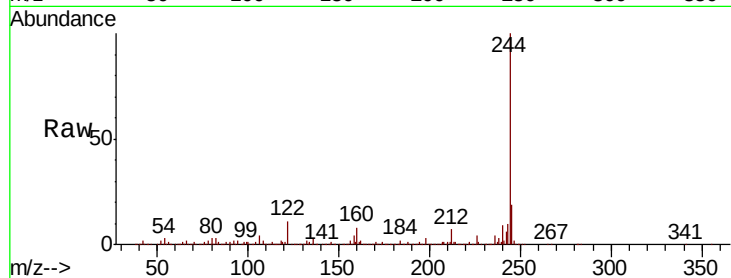

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

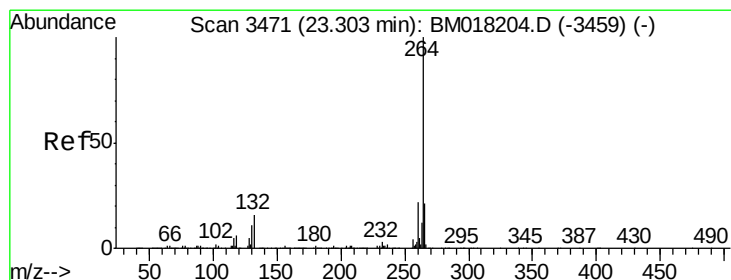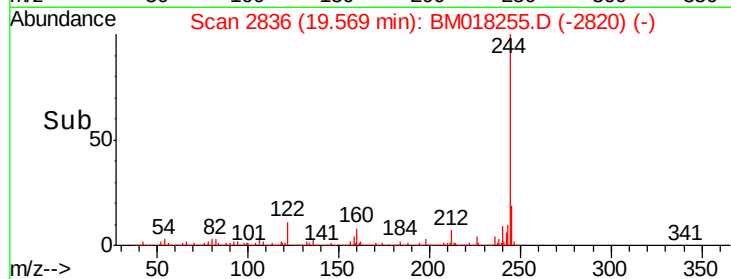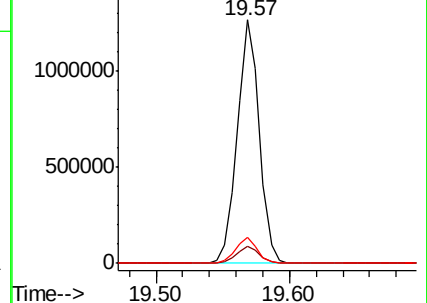

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.30 min Scan# 3470

Delta R.T. -0.01 min

Lab File: BM018255.D

Acq: 17 Dec 2018 18:52


Tgt Ion:264 Resp: 548404

Ion Ratio Lower Upper

264 100

260 23.6 17.5 26.3

265 22.9 17.3 25.9

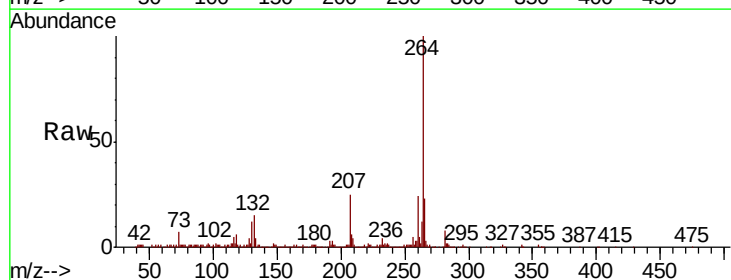

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

