

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018259.D
 Acq On : 17 Dec 2018 22:30
 Operator : JU/SJ
 Sample : PB115777BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB115777BL

Quant Time: Dec 18 00:53:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	121248	20.00	ng	-0.01
21) Naphthalene-d8	10.26	136	422819	20.00	ng	-0.01
39) Acenaphthene-d10	14.15	164	205271	20.00	ng	-0.01
64) Phenanthrene-d10	16.92	188	362054	20.00	ng	0.00
76) Chrysene-d12	21.14	240	373865	20.00	ng	0.00
87) Perylene-d12	23.30	264	432173	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	539172	74.28	ng	0.00
7) Phenol-d6	6.69	99	675787	66.99	ng	-0.01
23) Nitrobenzene-d5	8.65	82	640211	77.67	ng	-0.01
42) 2,4,6-Tribromophenol	15.66	330	169441	56.24	ng	0.00
45) 2-Fluorobiphenyl	12.76	172	1225628	77.34	ng	-0.01
79) Terphenyl-d14	19.57	244	1138590	68.88	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
Data File : BM018259.D
Acq On : 17 Dec 2018 22:30
Operator : JU/SJ
Sample : PB115777BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB115777BL

Quant Time: Dec 18 00:53:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

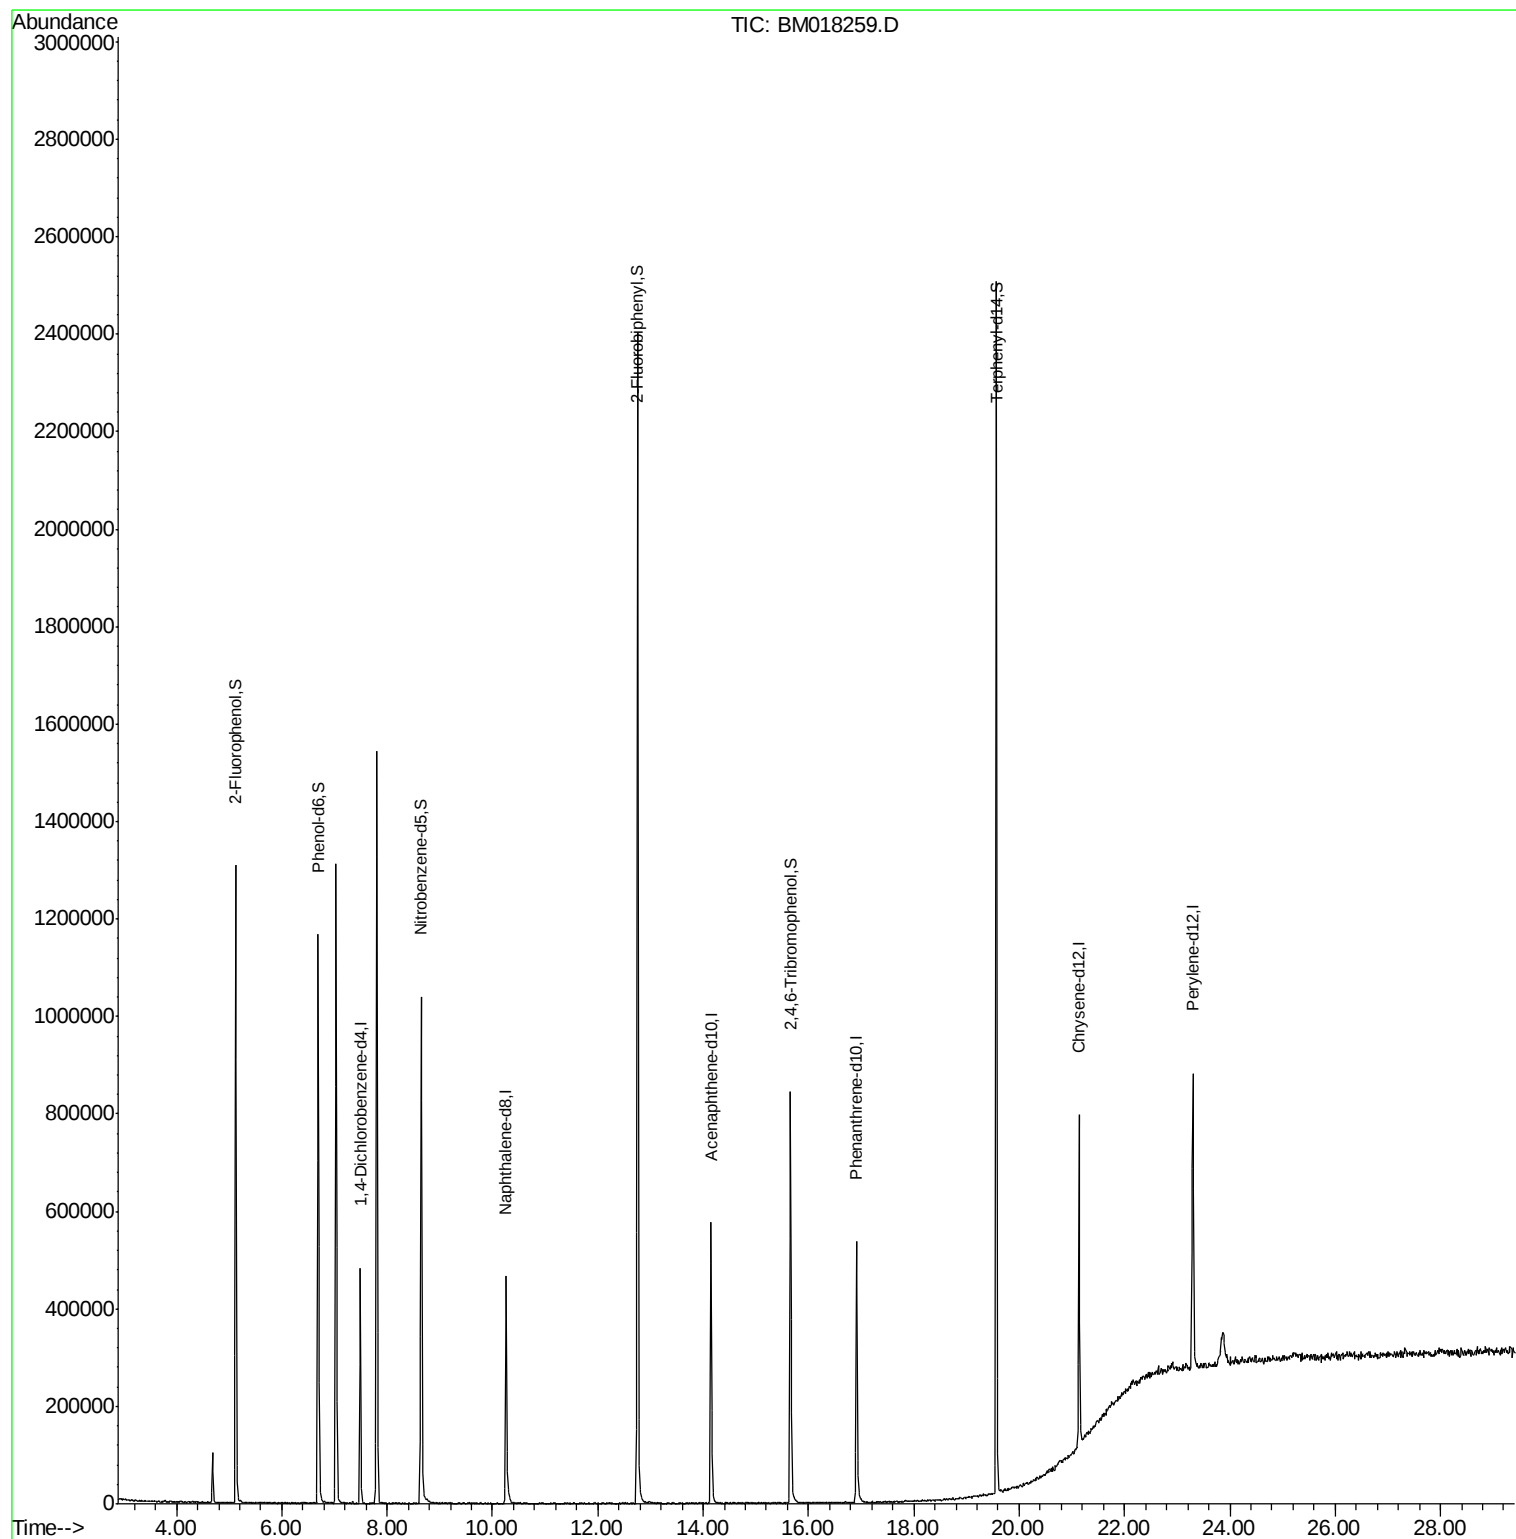

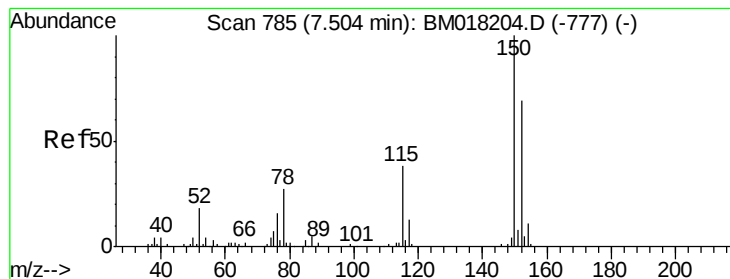


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 783
Delta R.T. -0.01 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30

Instrument :
BNA_M
ClientSampleId :
PB115777BL

Tgt Ion:152 Resp: 121248
Ion Ratio Lower Upper
152 100
150 161.6 116.1 174.1
115 65.8 44.6 67.0

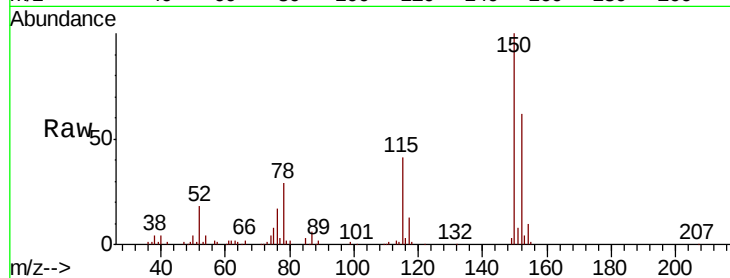


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

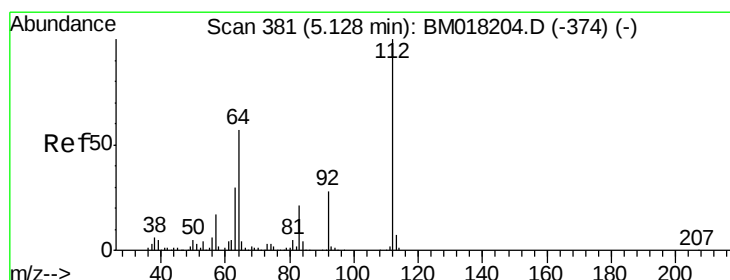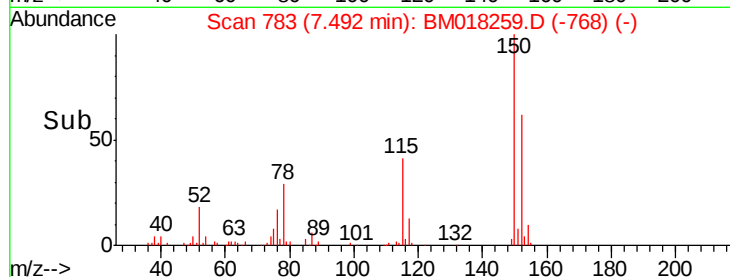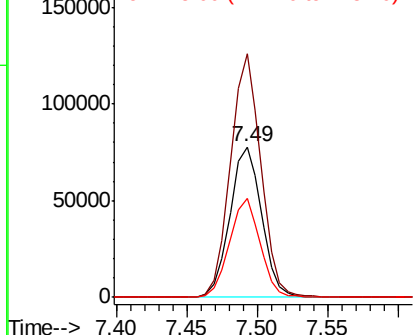



#5


2-Fluorophenol
Concen: 74.284 ng
RT: 5.13 min Scan# 381
Delta R.T. -0.00 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30

Tgt Ion:112 Resp: 539172
Ion Ratio Lower Upper
112 100
64 56.8 45.4 68.2
63 31.2 24.0 36.0

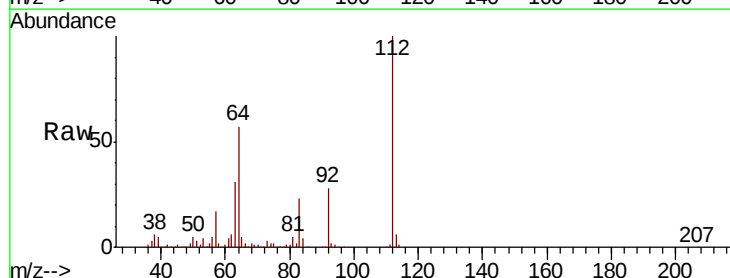

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

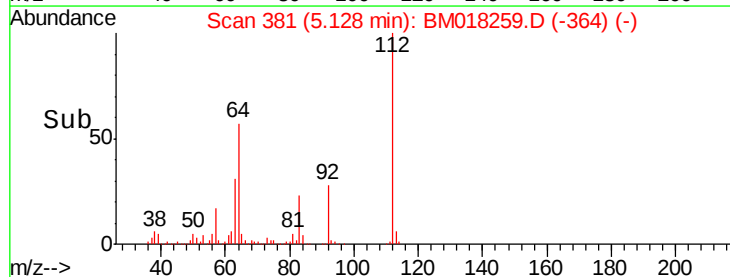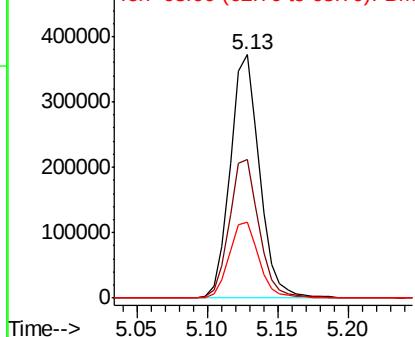

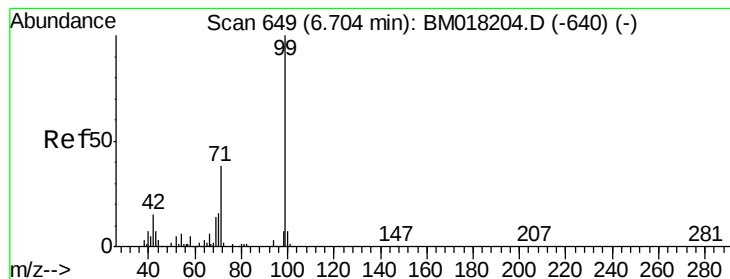

#7

Phenol-d6

Concen: 66.987 ng

RT: 6.69 min Scan# 647

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30

Instrument :

BNA_M

ClientSampleId :

PB115777BL


Tgt Ion: 99 Resp: 675787

Ion Ratio Lower Upper

99 100

42 15.8 12.3 18.5

71 38.9 30.2 45.2



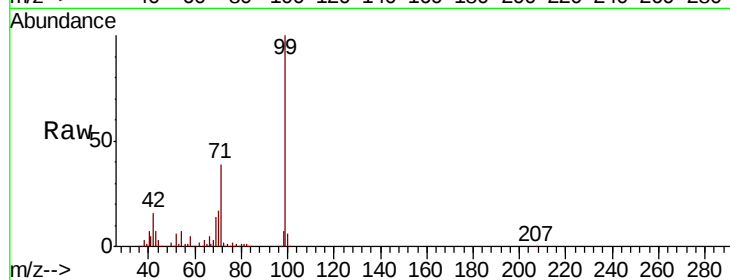


Abundance

Ion 99.00 (98.70 to 99.70): BM018204.D (-640) (-)

Ion 42.00 (41.70 to 42.70): BM018204.D (-640) (-)

Ion 71.00 (70.70 to 71.70): BM018204.D (-640) (-)

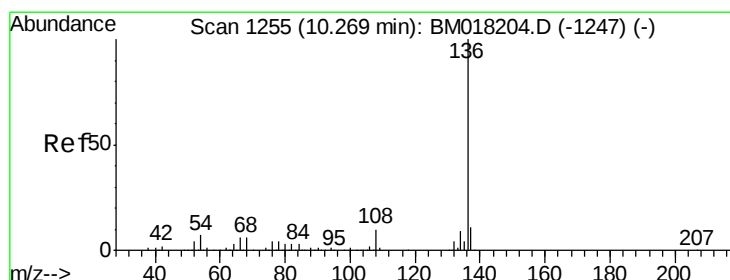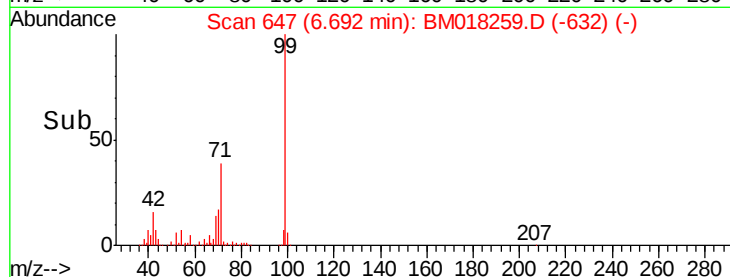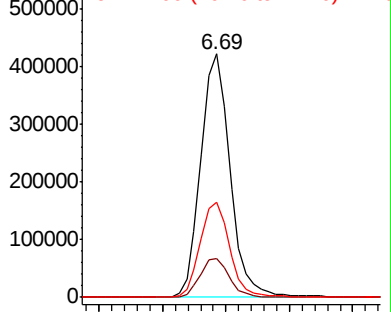

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.26 min Scan# 1253

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30

Tgt Ion: 136 Resp: 422819


Ion Ratio Lower Upper

136 100

137 10.9 9.2 13.8

54 6.0 5.2 7.8

68 5.2 5.0 7.6

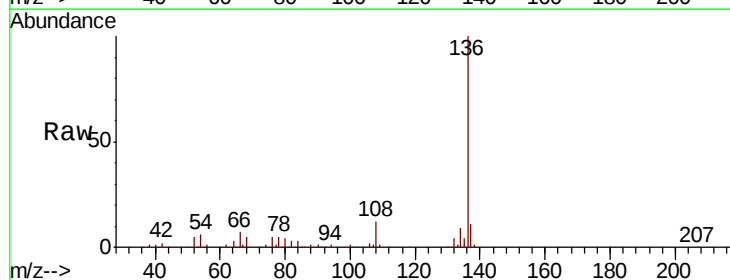



Abundance


Ion 136.00 (135.70 to 136.70): BM018204.D (-1247) (-)

Ion 137.00 (136.70 to 137.70): BM018204.D (-1247) (-)

Ion 54.00 (53.70 to 54.70): BM018204.D (-1247) (-)

Ion 68.00 (67.70 to 68.70): BM018204.D (-1247) (-)



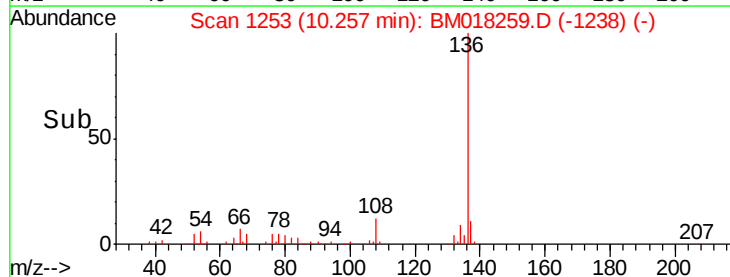
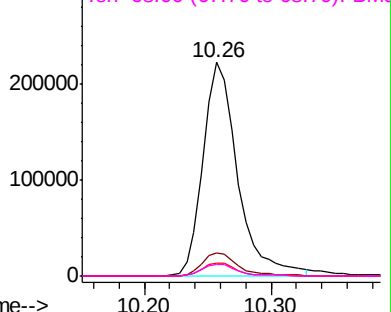


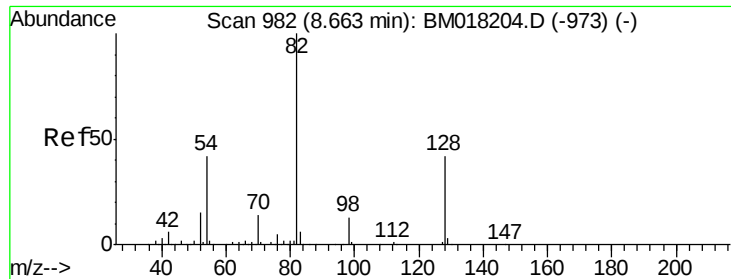

#23
Nitrobenzene-d5
Concen: 77.666 ng
RT: 8.65 min Scan# 980
Delta R.T. -0.01 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30




Instrument :
BNA_M
ClientSampleId :
PB115777BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	40.4	33.4	50.2
54	41.7	33.4	50.2

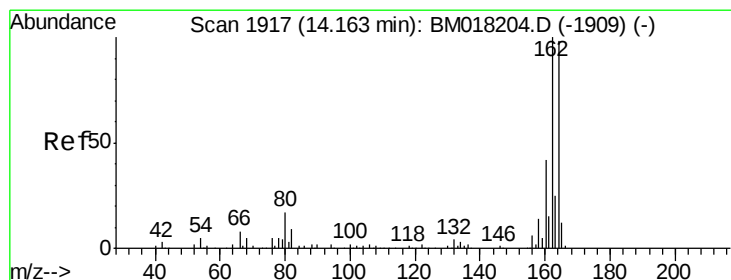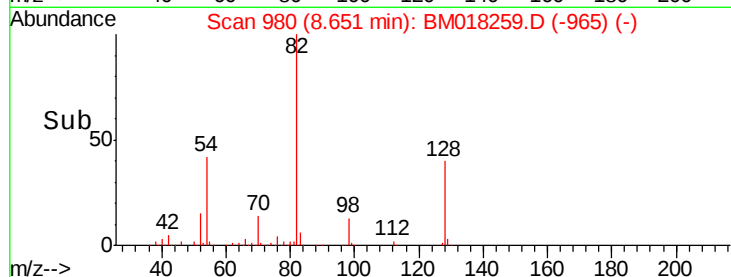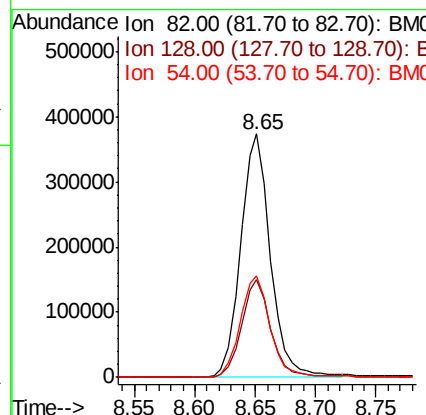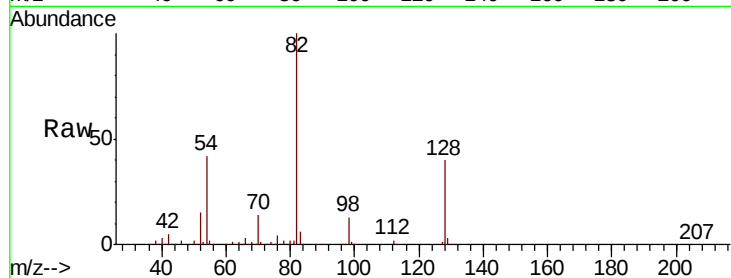

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.15 min Scan# 1915
Delta R.T. -0.01 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.2	81.8	122.6
160	45.2	34.6	51.8

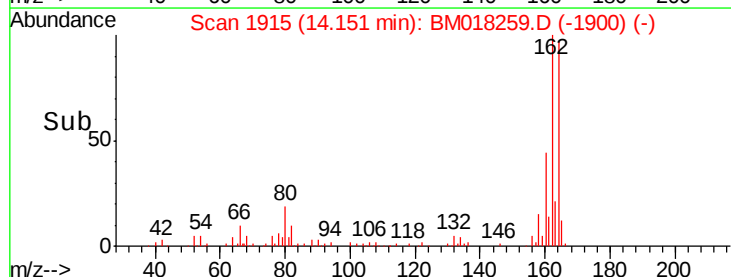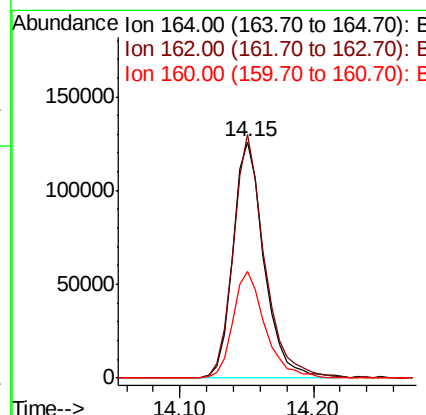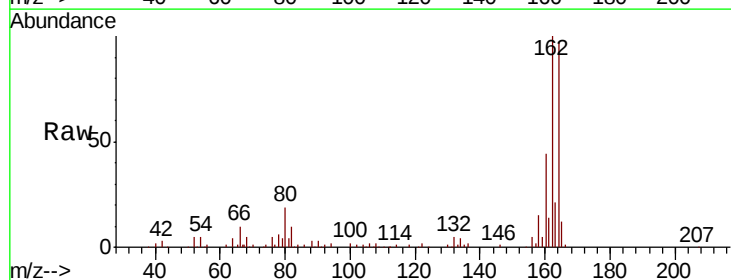

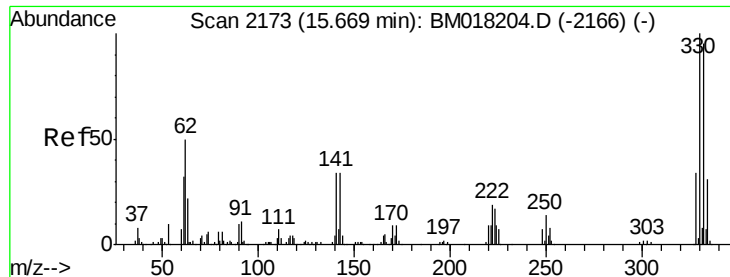

#42

2,4,6-Tribromophenol

Concen: 56.240 ng

RT: 15.66 min Scan# 2172

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30

Instrument :

BNA_M

ClientSampled :

PB115777BL


Tgt Ion:330 Resp: 169441

Ion Ratio Lower Upper

330 100

332 96.6 78.6 118.0




141 36.6 27.1 40.7

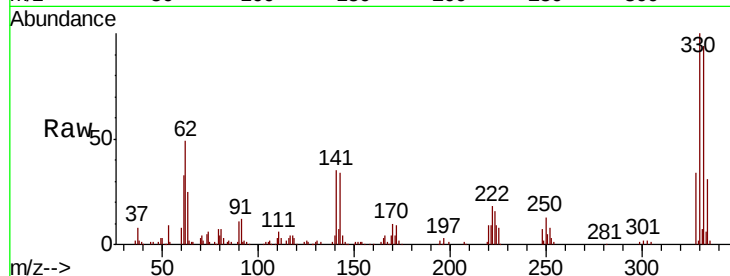

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

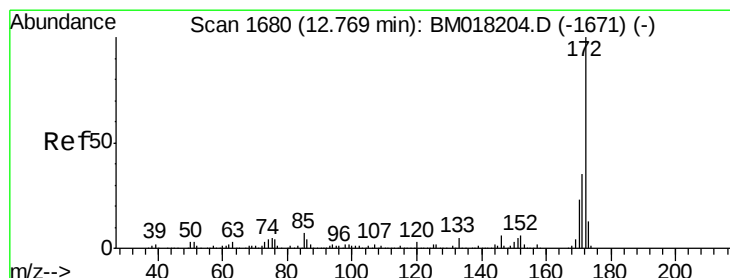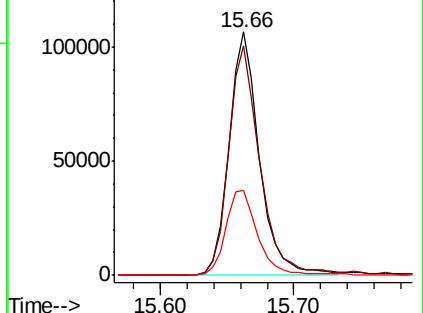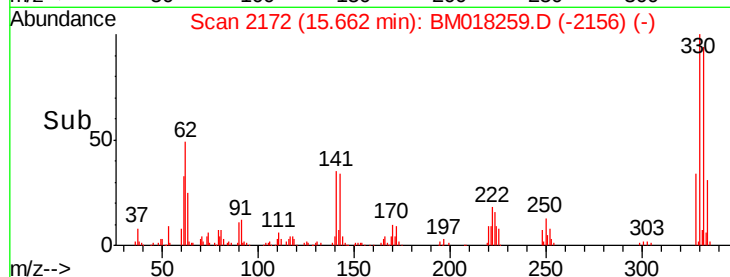

#45

2-Fluorobiphenyl

Concen: 77.336 ng

RT: 12.76 min Scan# 1678

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30


Tgt Ion:172 Resp: 1225628

Ion Ratio Lower Upper

172 100

171 34.7 28.3 42.5



170 22.7 18.1 27.1

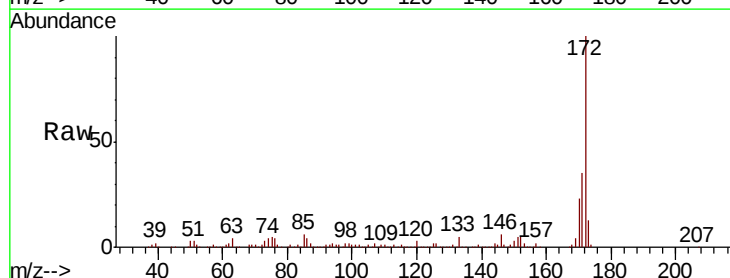


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

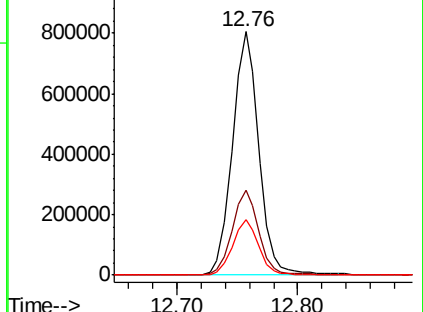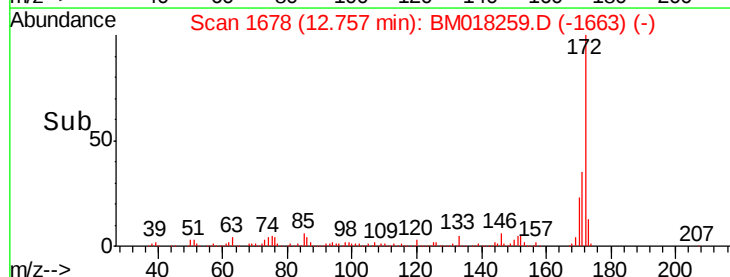


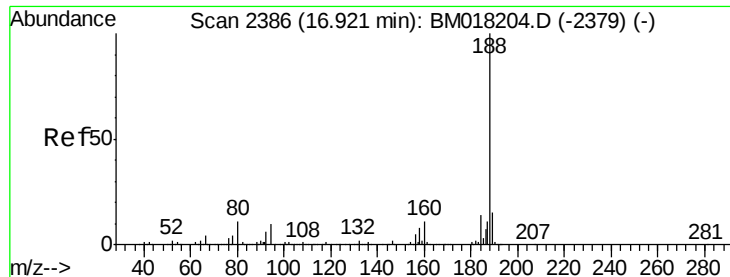




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.92 min Scan# 2385
Delta R.T. -0.01 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30

Instrument :
BNA_M
ClientSampleId :
PB115777BL

Tgt Ion:188 Resp: 362054
Ion Ratio Lower Upper
188 100
94 8.5 8.0 12.0
80 10.7 9.0 13.6

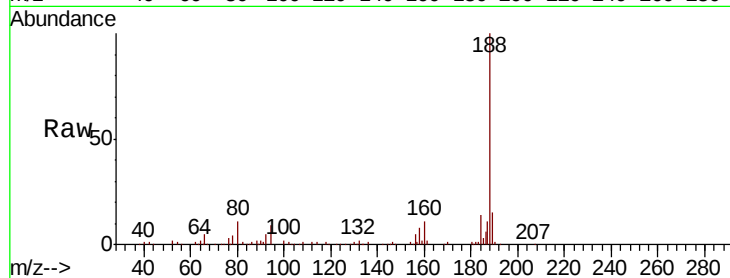


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

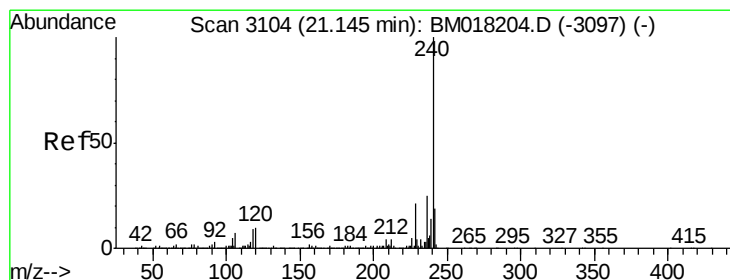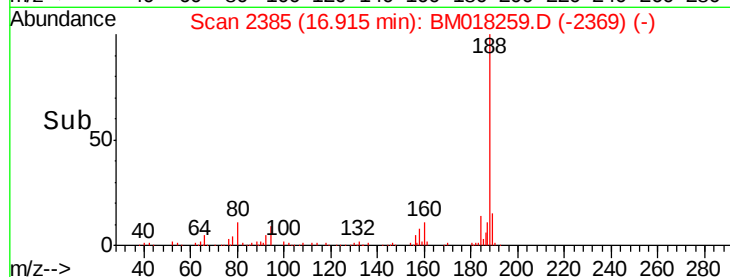
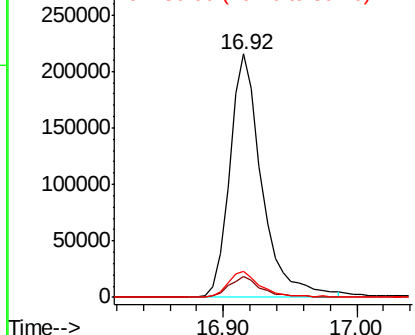



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.14 min Scan# 3103
Delta R.T. -0.01 min
Lab File: BM018259.D
Acq: 17 Dec 2018 22:30

Tgt Ion:240 Resp: 373865
Ion Ratio Lower Upper
240 100
120 8.5 8.2 12.2
236 25.2 20.3 30.5

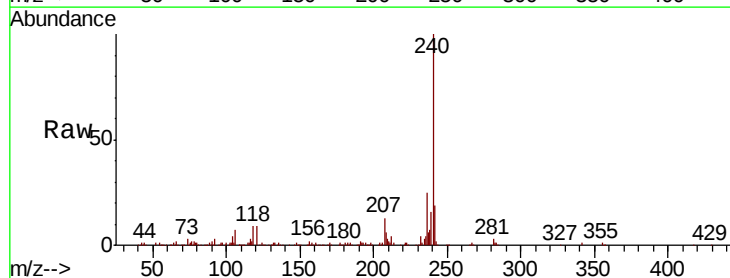

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

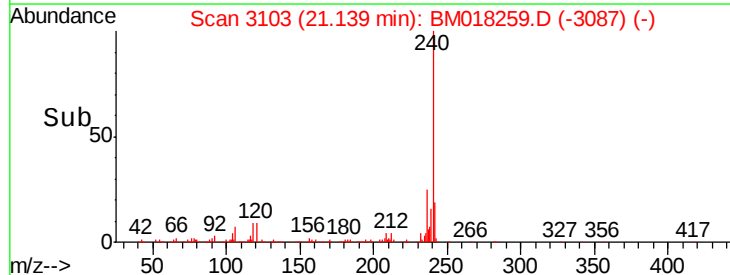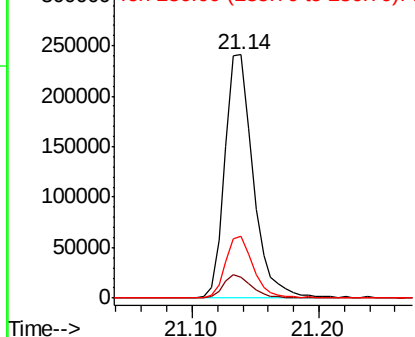

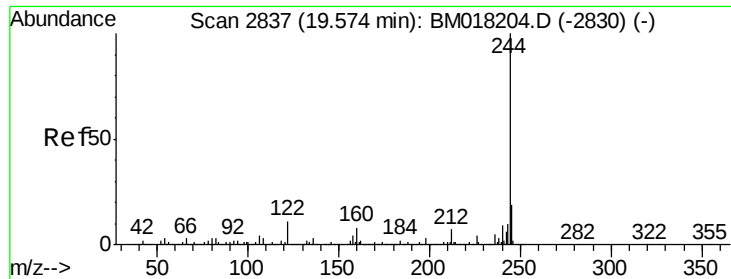

#79

Terphenyl-d14

Concen: 68.878 ng

RT: 19.57 min Scan# 2836

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30

Instrument :

BNA_M

ClientSampleId :

PB115777BL


Tgt Ion:244 Resp: 1138590

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8




122 10.3 9.0 13.6

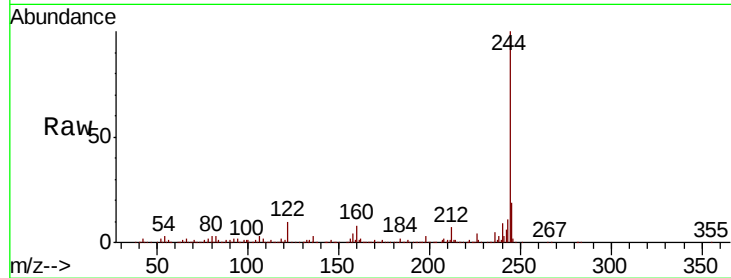

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

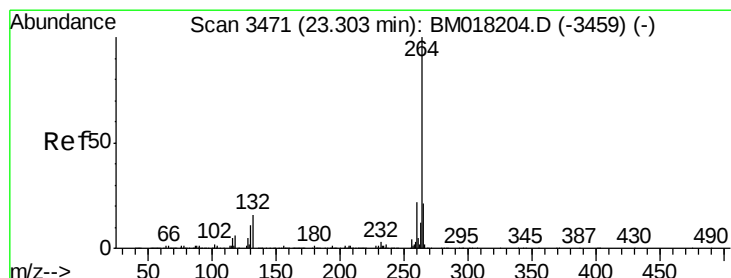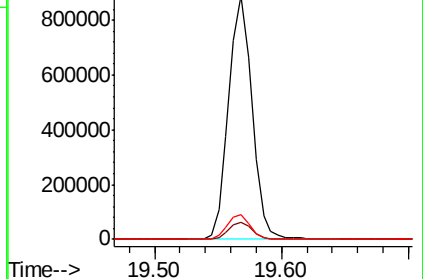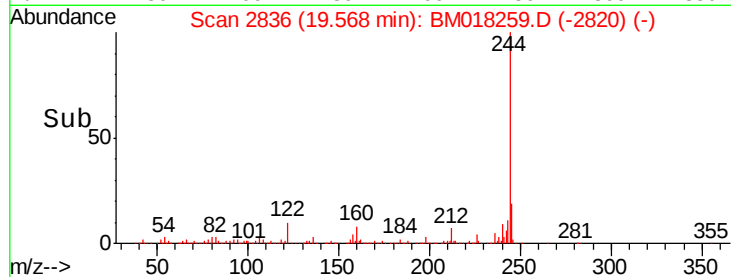

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.30 min Scan# 3470

Delta R.T. -0.01 min

Lab File: BM018259.D

Acq: 17 Dec 2018 22:30


Tgt Ion:264 Resp: 432173

Ion Ratio Lower Upper

264 100

260 21.8 17.5 26.3

265 22.2 17.3 25.9

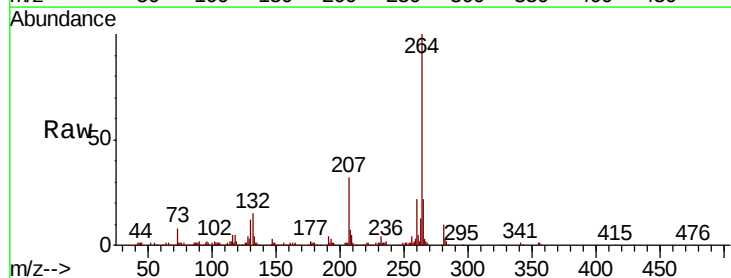

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

