

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018267.D
 Acq On : 18 Dec 2018 03:20
 Operator : JU/SJ
 Sample : J6385-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 121218-JETT-F-U-B

Quant Time: Dec 18 05:04:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	121180	20.00	ng	-0.02
21) Naphthalene-d8	10.26	136	432035	20.00	ng	-0.01
39) Acenaphthene-d10	14.15	164	194299	20.00	ng	-0.01
64) Phenanthrene-d10	16.91	188	380733	20.00	ng	-0.01
76) Chrysene-d12	21.13	240	387051	20.00	ng	-0.01
87) Perylene-d12	23.29	264	288971	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	346314	47.74	ng	0.00
7) Phenol-d6	6.69	99	252753	25.07	ng	-0.02
23) Nitrobenzene-d5	8.65	82	1072983	127.39	ng	-0.01
42) 2,4,6-Tribromophenol	15.66	330	287939	100.97	ng	-0.01
45) 2-Fluorobiphenyl	12.76	172	2036870	135.78	ng	-0.01
79) Terphenyl-d14	19.57	244	2002794	117.03	ng	0.00
Target Compounds						
10) Phenol	6.72	94	27108	2.539	ng	Qvalue 95
15) Benzyl Alcohol	7.80	79	17160	2.089	ng	# 41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
Data File : BM018267.D
Acq On : 18 Dec 2018 03:20
Operator : JU/SJ
Sample : J6385-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
121218-JETT-F-U-B

Quant Time: Dec 18 05:04:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

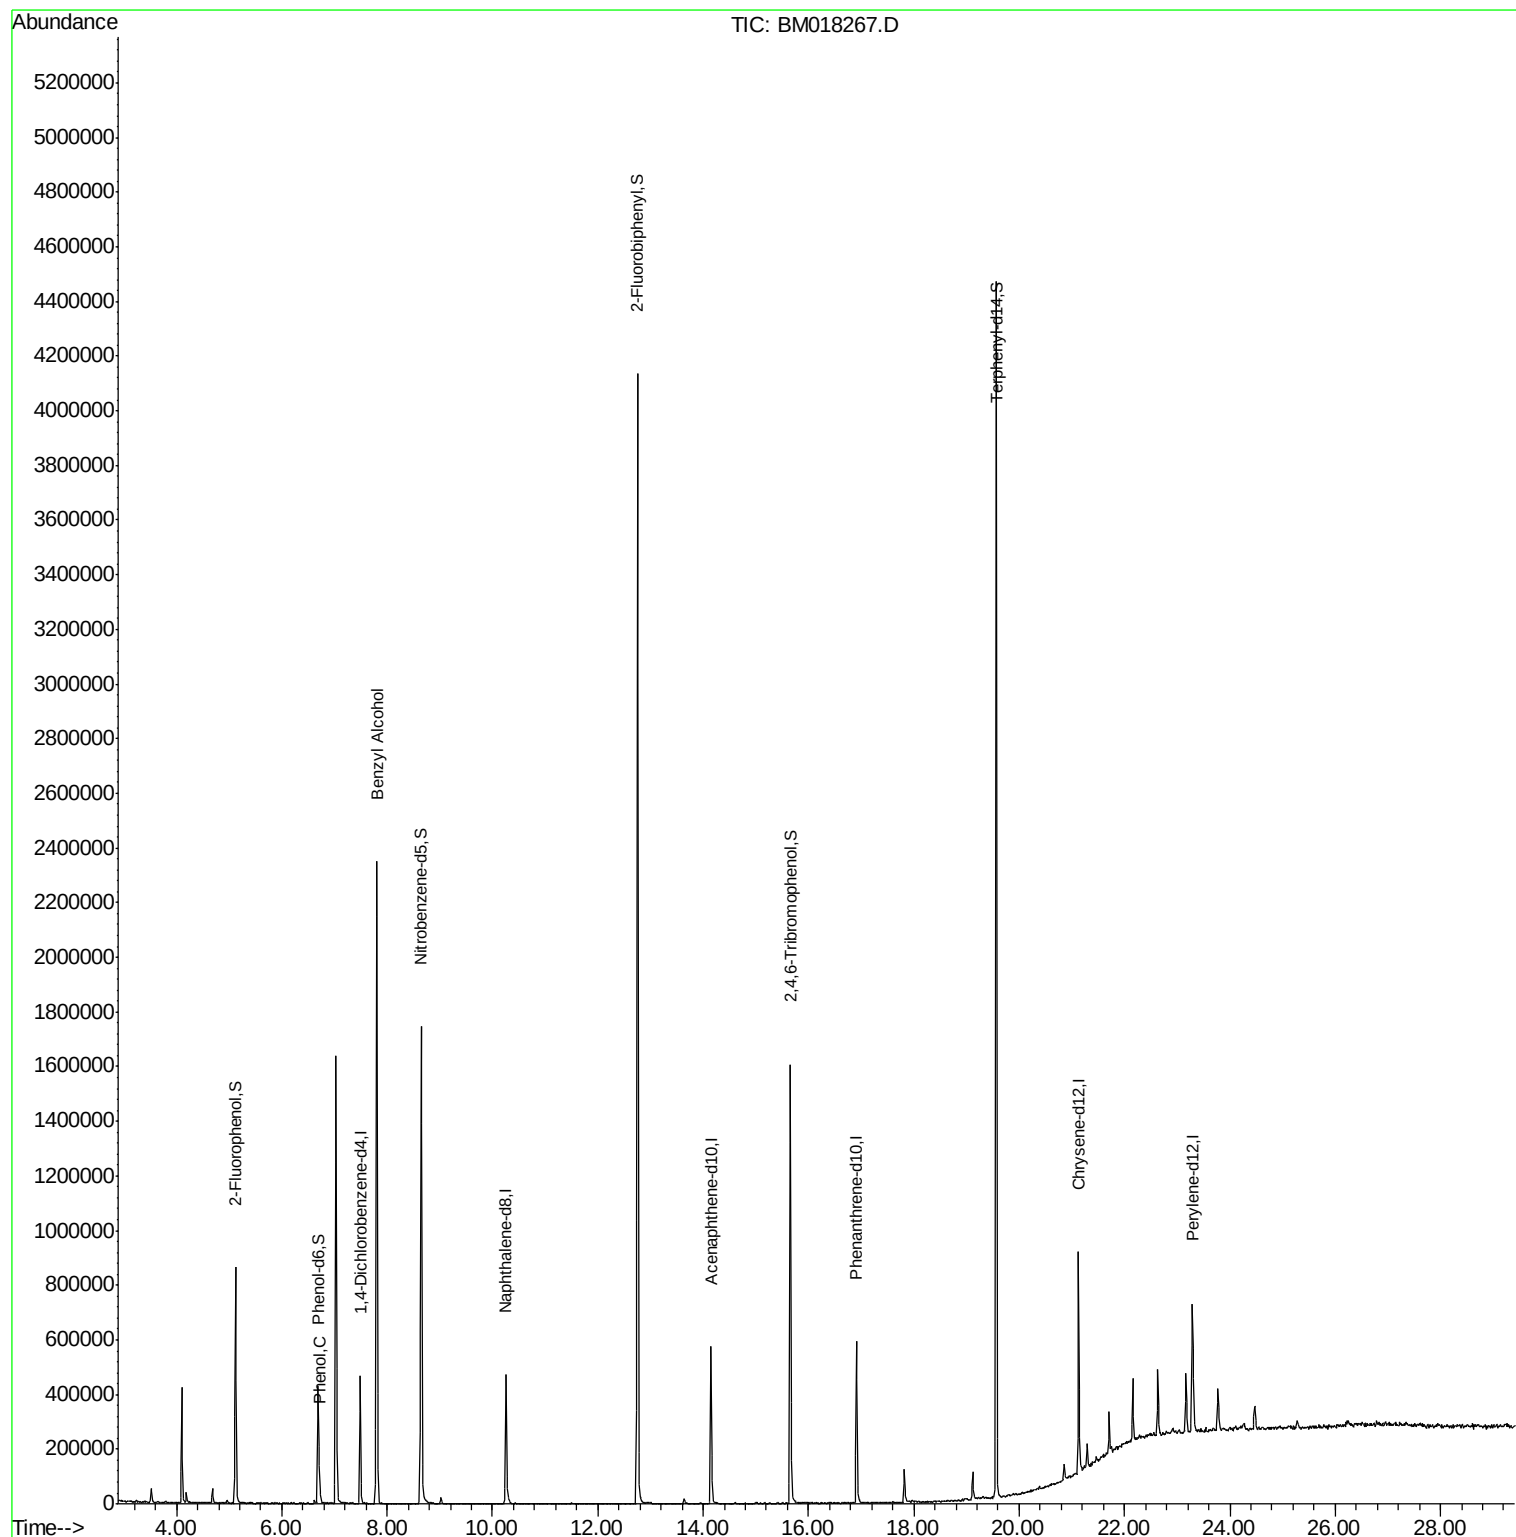

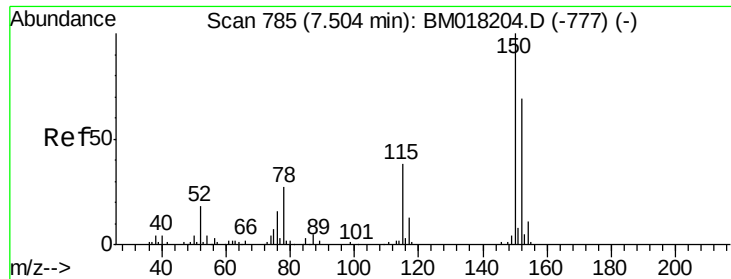


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 782
Delta R.T. -0.02 min
Lab File: BM018267.D
Acq: 18 Dec 2018 03:20

Instrument :
BNA_M
ClientSampleId :
121218-JETT-F-U-B

Tgt Ion:152 Resp: 121180
Ion Ratio Lower Upper
152 100
150 151.5 116.1 174.1
115 62.3 44.6 67.0

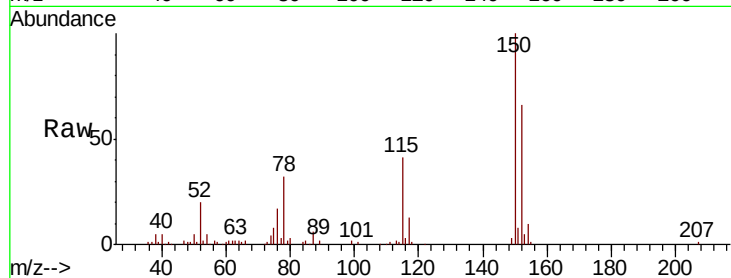


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

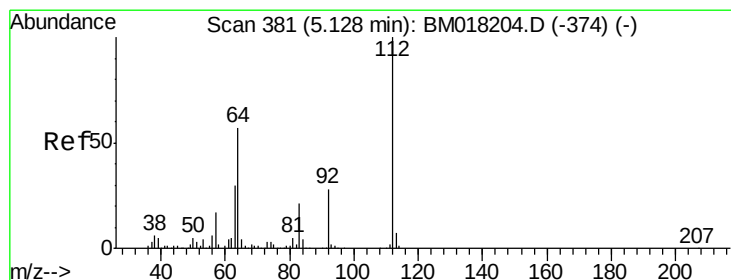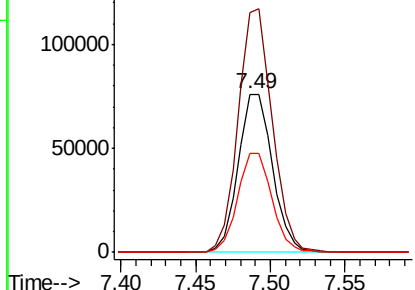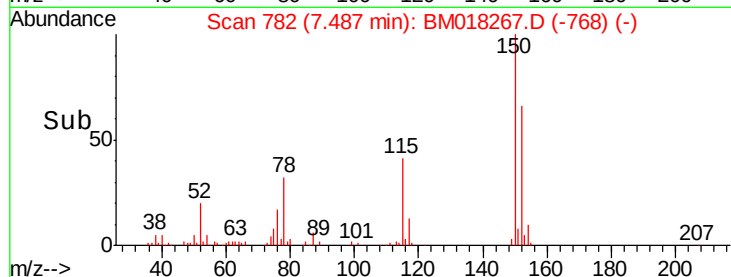



#5


2-Fluorophenol
Concen: 47.740 ng
RT: 5.12 min Scan# 380
Delta R.T. -0.01 min
Lab File: BM018267.D
Acq: 18 Dec 2018 03:20

Tgt Ion:112 Resp: 346314
Ion Ratio Lower Upper
112 100
64 60.3 45.4 68.2
63 31.3 24.0 36.0

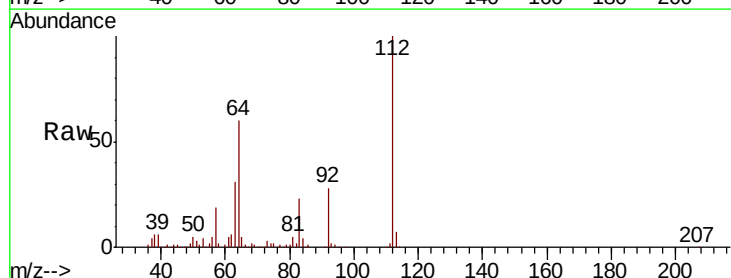

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

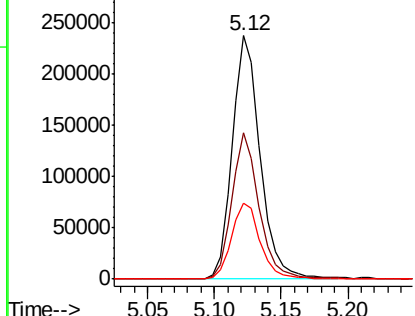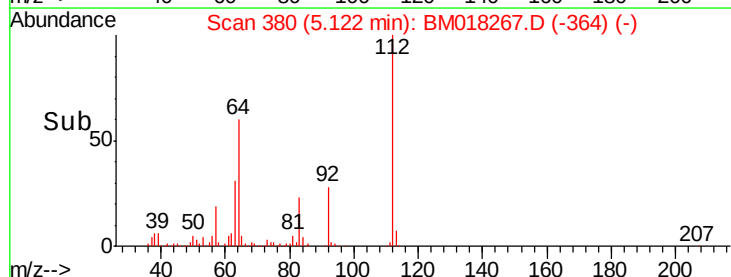

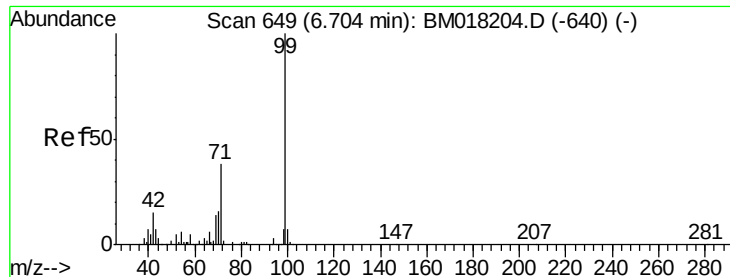

#7

Phenol-d6

Concen: 25.068 ng

RT: 6.69 min Scan# 646

Delta R.T. -0.02 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Instrument :

BNA_M

ClientSampleId :

121218-JETT-F-U-B


Tgt Ion: 99 Resp: 252753

Ion Ratio Lower Upper

99 100

42 16.4 12.3 18.5




71 39.1 30.2 45.2

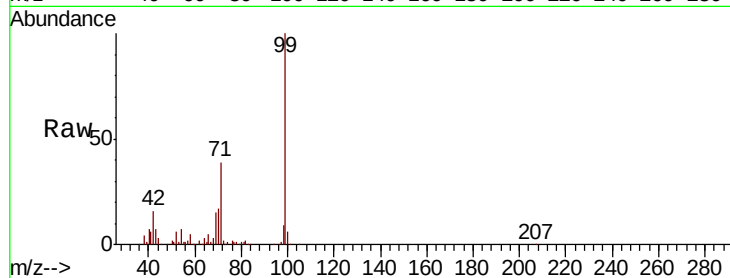

Abundance Ion 99.00 (98.70 to 99.70): BM018267.D (-632) (-)

Ion 42.00 (41.70 to 42.70): BM018267.D (-632) (-)

Ion 71.00 (70.70 to 71.70): BM018267.D (-632) (-)

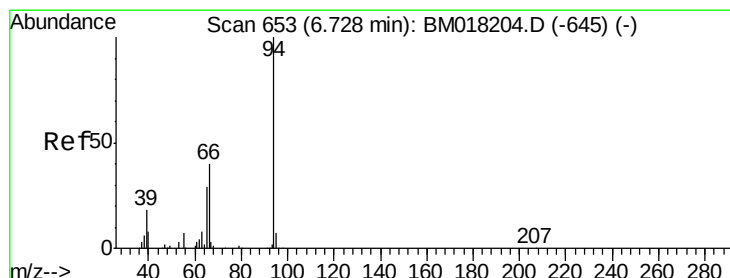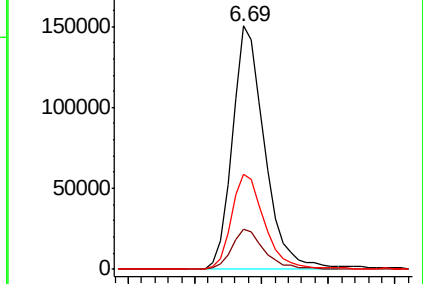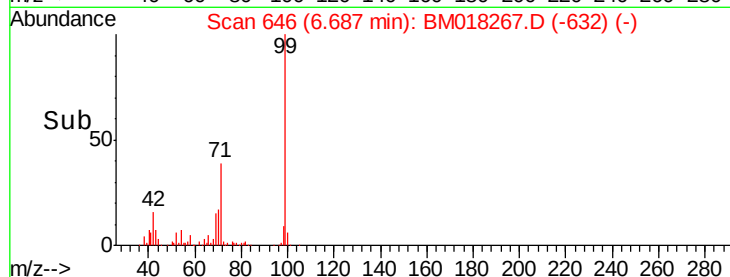

#10

Phenol

Concen: 2.539 ng

RT: 6.72 min Scan# 651

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20


Tgt Ion: 94 Resp: 27108

Ion Ratio Lower Upper

94 100

65 29.5 9.5 49.5



66 46.2 21.3 61.3

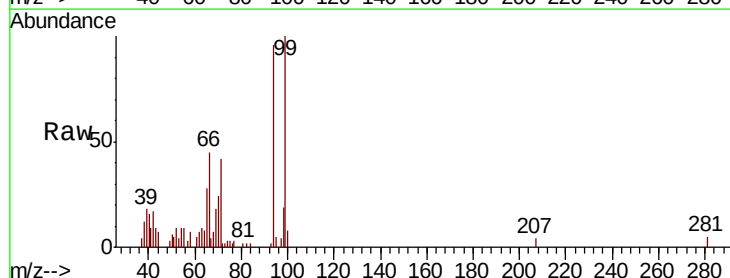


Abundance Ion 94.00 (93.70 to 94.70): BM018267.D (-636) (-)

Ion 65.00 (64.70 to 65.70): BM018267.D (-636) (-)

Ion 66.00 (65.70 to 66.70): BM018267.D (-636) (-)

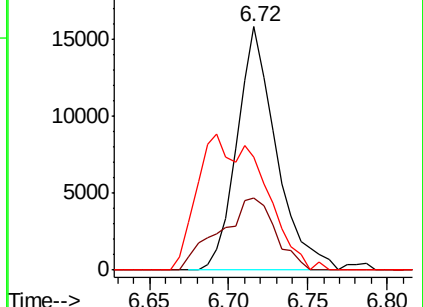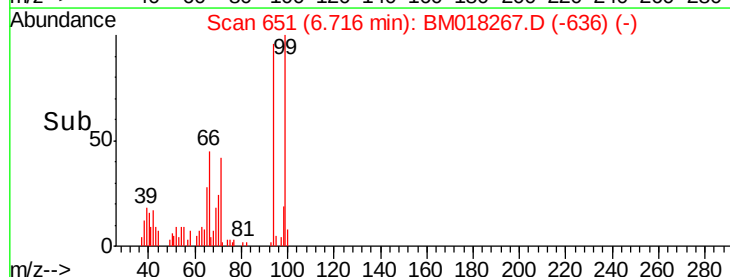

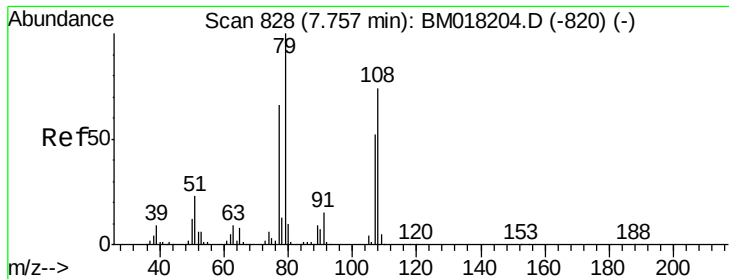

#15

Benzyl Alcohol

Concen: 2.089 ng

RT: 7.80 min Scan# 836

Delta R.T. 0.05 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Instrument :

BNA_M

ClientSampleId :

121218-JETT-F-U-B


Tgt Ion: 79 Resp: 17160

Ion Ratio Lower Upper




79 100

108 41.0 59.3 88.9#

77 130.6 53.0 79.4#

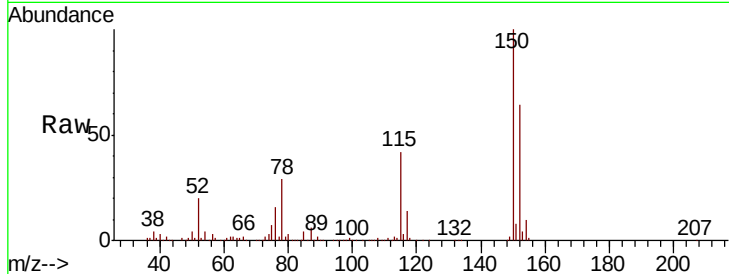

Abundance Ion 79.00 (78.70 to 79.70): BM018204.D (-820) (-)

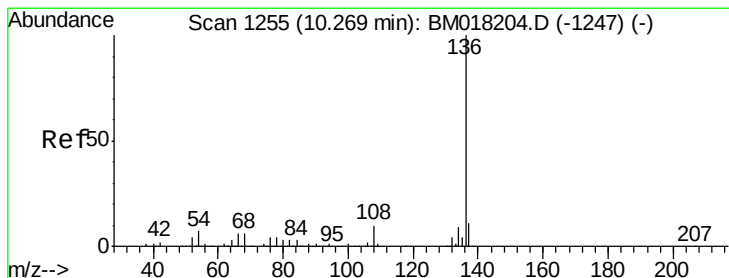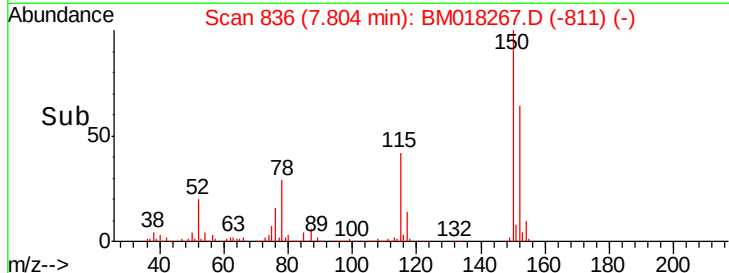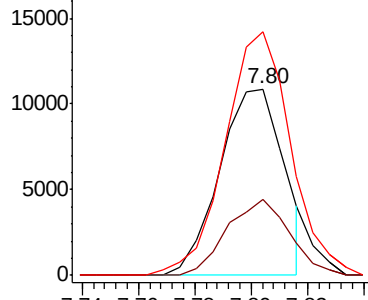

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.26 min Scan# 1253

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Tgt Ion: 136 Resp: 432035


Ion Ratio Lower Upper

136 100



137 11.9 9.2 13.8


54 6.3 5.2 7.8

68 6.3 5.0 7.6

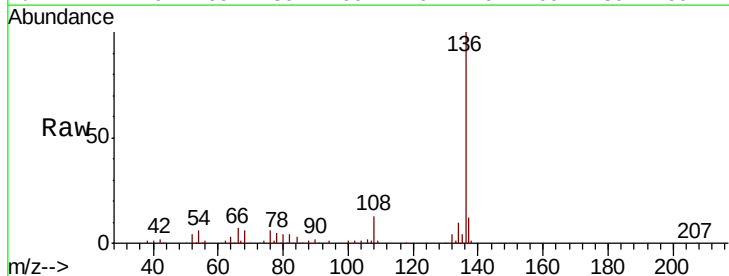

Abundance Ion 136.00 (135.70 to 136.70): BM018204.D (-1247) (-)

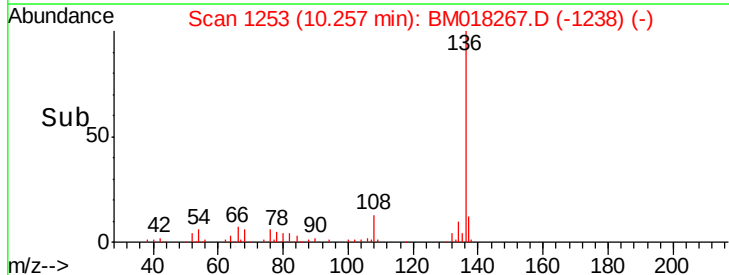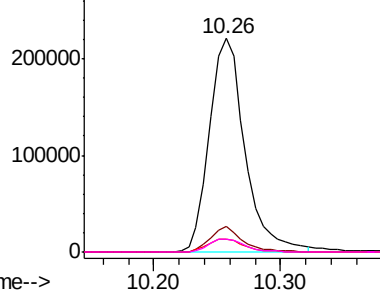

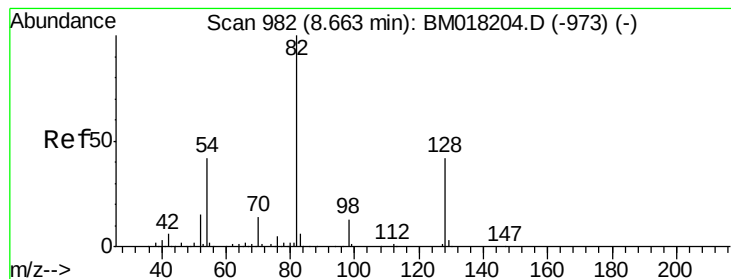

#23

Nitrobenzene-d5

Concen: 127.390 ng

RT: 8.65 min Scan# 980

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Instrument :

BNA_M

ClientSampleId :

121218-JETT-F-U-B





Tgt Ion: 82 Resp: 1072983

Ion Ratio Lower Upper

82 100

128 37.7 33.4 50.2

54 41.5 33.4 50.2

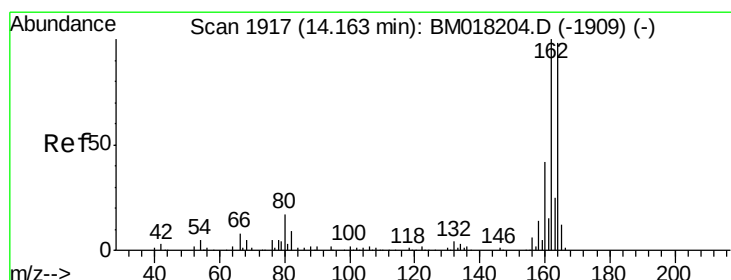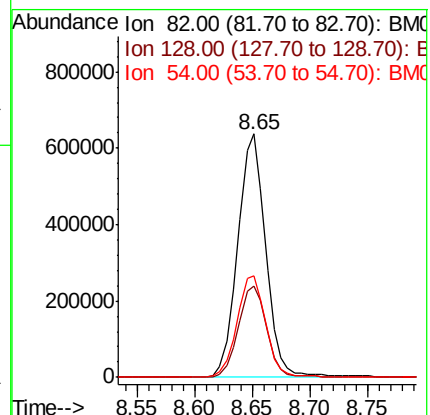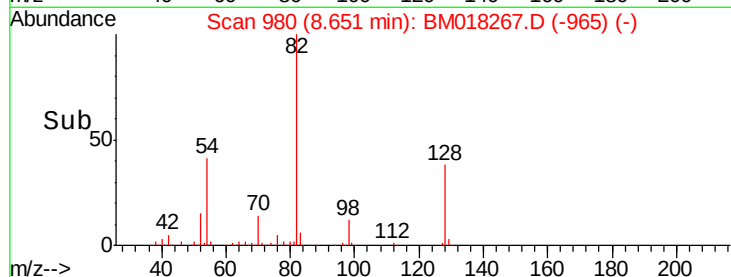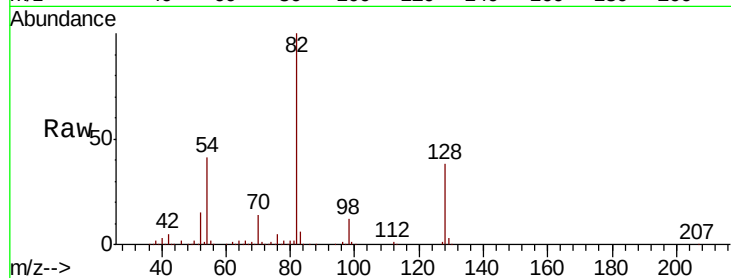

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.15 min Scan# 1915

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20




Tgt Ion: 164 Resp: 194299


Ion Ratio Lower Upper

164 100

162 105.3 81.8 122.6

160 47.9 34.6 51.8

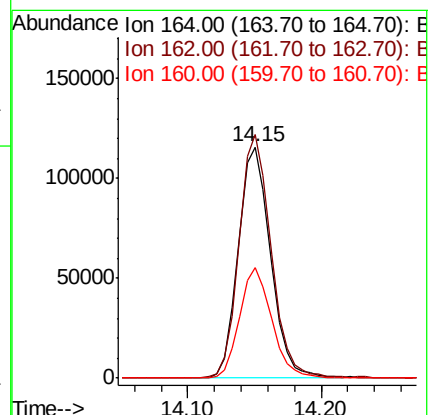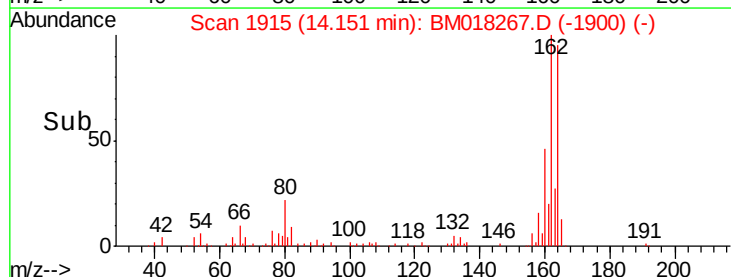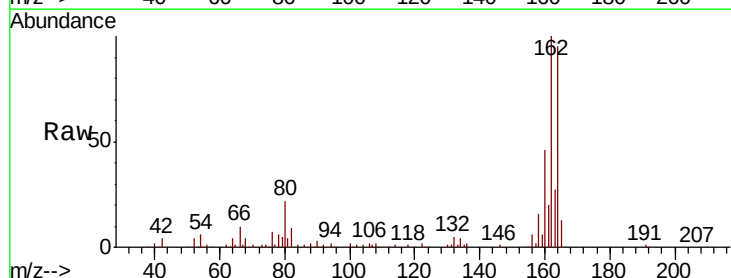


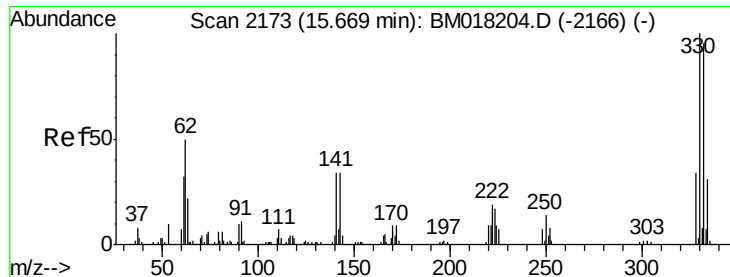

#42
 2,4,6-Tribromophenol
 Concen: 100.968 ng
 RT: 15.66 min Scan# 2171
 Delta R.T. -0.01 min
 Lab File: BM018267.D
 Acq: 18 Dec 2018 03:20

Instrument :
 BNA_M
 ClientSampleId :
 121218-JETT-F-U-B

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	78.6	118.0
141	38.5	27.1	40.7



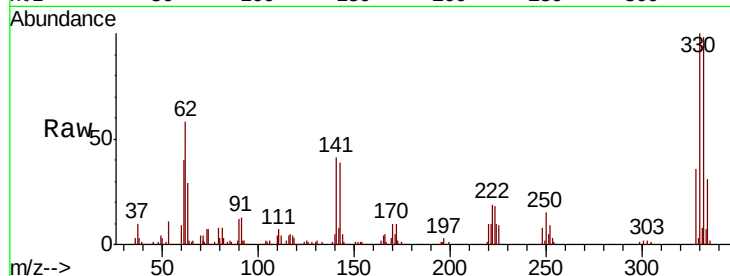


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

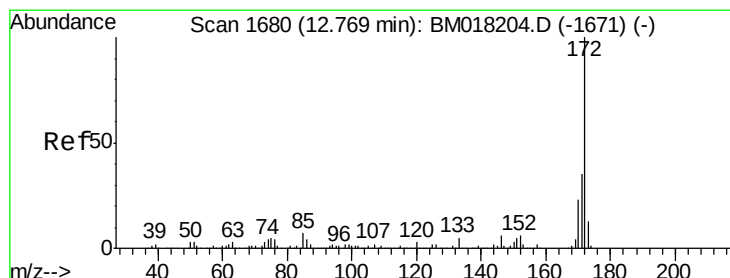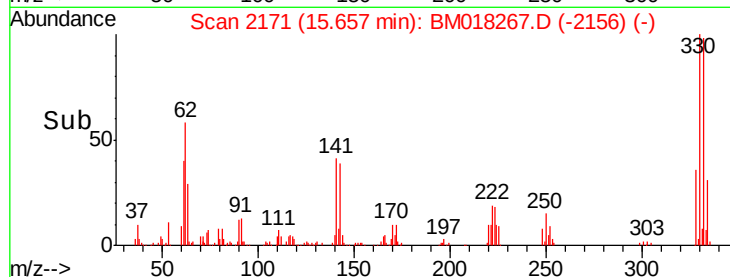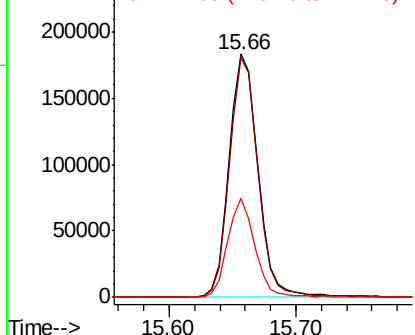

#45
 2-Fluorobiphenyl
 Concen: 135.782 ng
 RT: 12.76 min Scan# 1678
 Delta R.T. -0.01 min
 Lab File: BM018267.D
 Acq: 18 Dec 2018 03:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.4	28.3	42.5
170	22.4	18.1	27.1


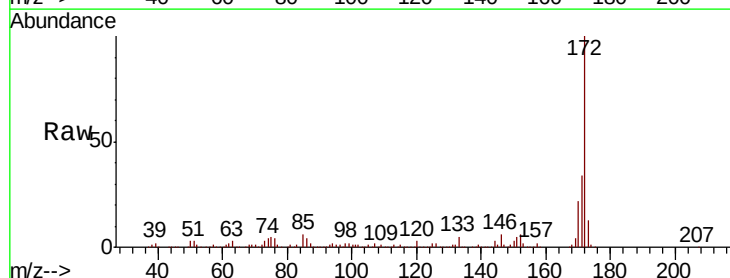



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



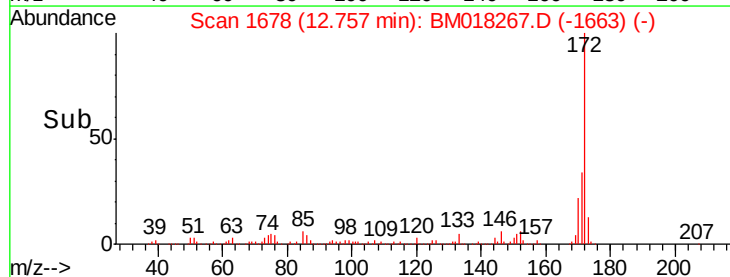
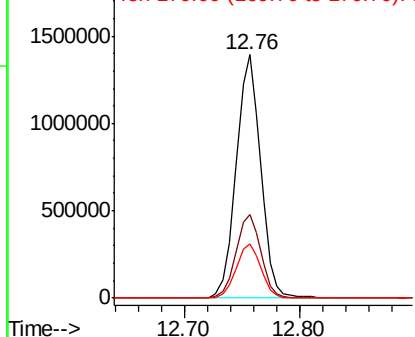


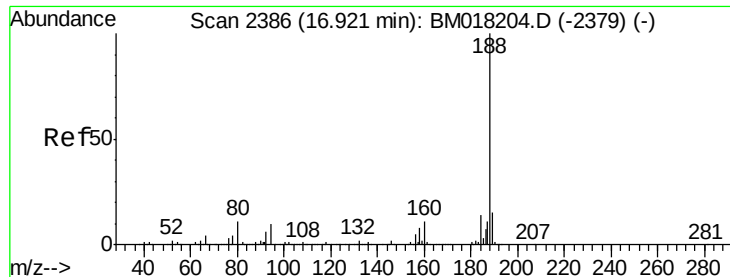

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.91 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BM018267.D
Acq: 18 Dec 2018 03:20




Instrument :
BNA_M
ClientSampleId :
121218-JETT-F-U-B


Tgt Ion:188 Resp: 380733
Ion Ratio Lower Upper
188 100
94 8.7 8.0 12.0
80 10.1 9.0 13.6

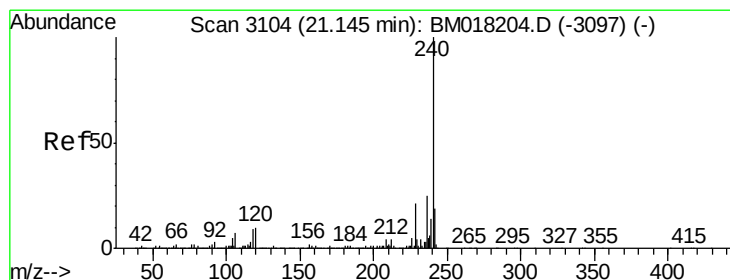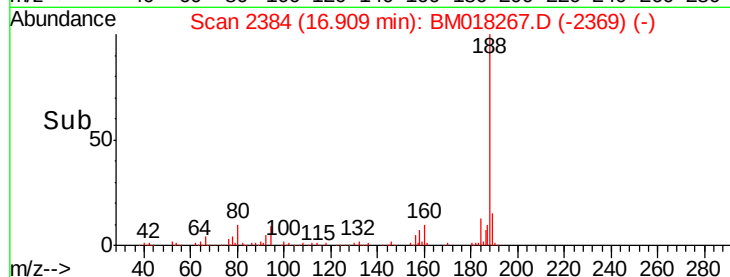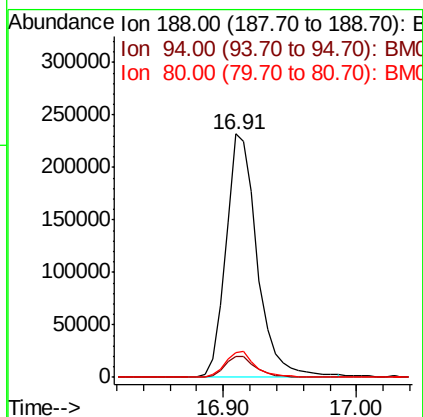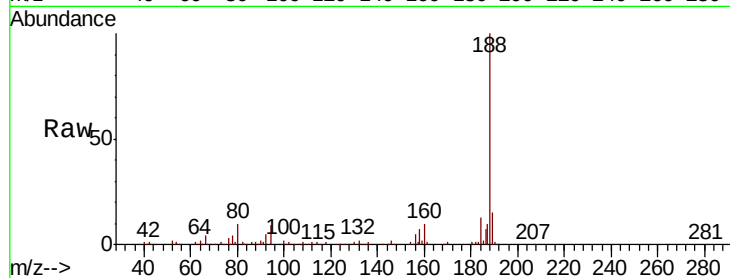

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.13 min Scan# 3102
Delta R.T. -0.01 min
Lab File: BM018267.D
Acq: 18 Dec 2018 03:20

Tgt Ion:240 Resp: 387051
Ion Ratio Lower Upper
240 100
120 8.7 8.2 12.2
236 25.2 20.3 30.5

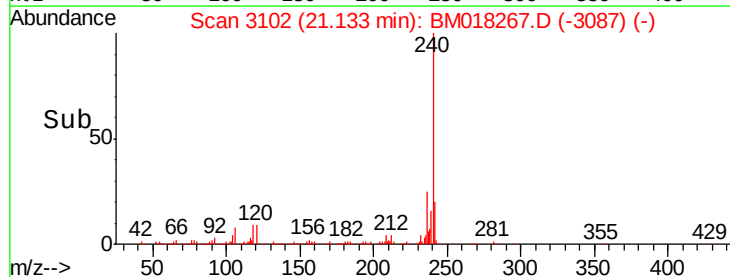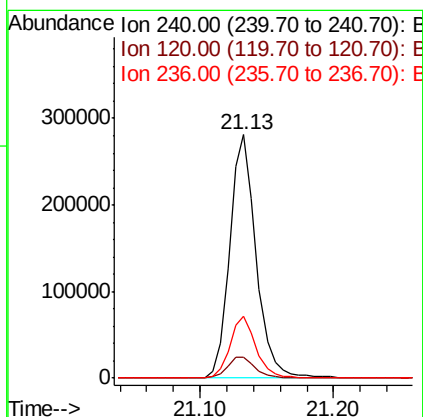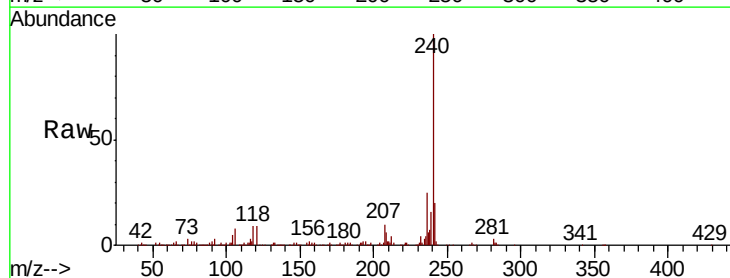

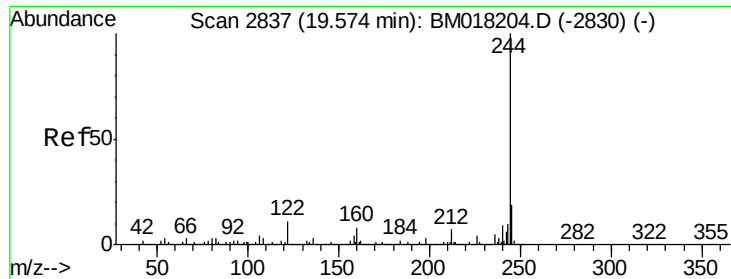

#79

Terphenyl-d14

Concen: 117.029 ng

RT: 19.57 min Scan# 2836

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Instrument :

BNA_M

ClientSampleId :

121218-JETT-F-U-B





Tgt Ion:244 Resp: 2002794

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8

122 9.7 9.0 13.6

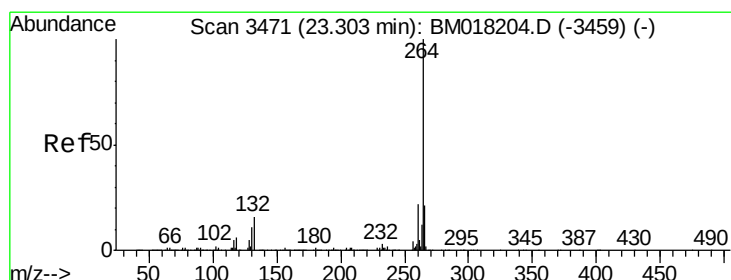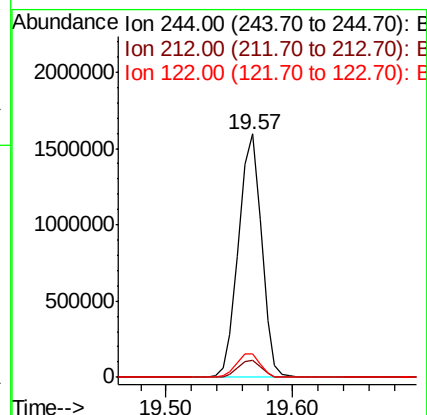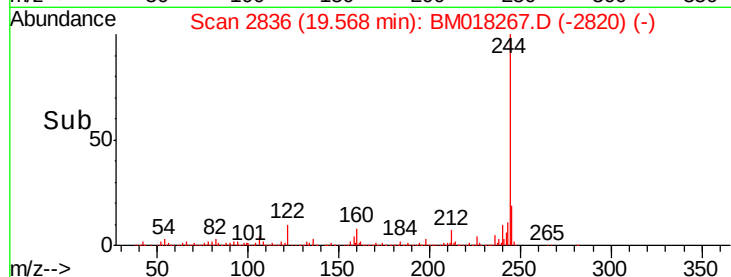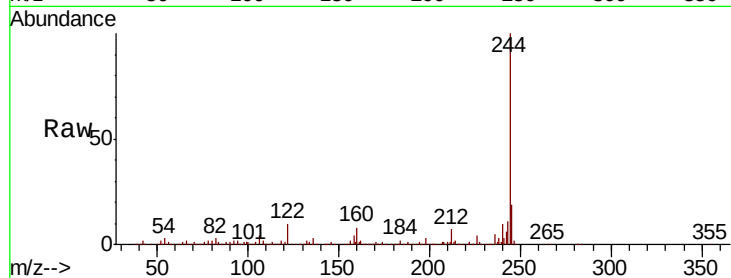

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.29 min Scan# 3469

Delta R.T. -0.01 min

Lab File: BM018267.D

Acq: 18 Dec 2018 03:20

Tgt Ion:264 Resp: 288971

Ion Ratio Lower Upper

264 100

260 24.1 17.5 26.3

265 21.6 17.3 25.9

