

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018246.D
 Acq On : 17 Dec 2018 13:23
 Operator : JU/SJ
 Sample : J6388-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P001-SS010-0006-01

Quant Time: Dec 18 00:49:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	128940	20.00	ng	-0.01
21) Naphthalene-d8	10.26	136	496632	20.00	ng	0.00
39) Acenaphthene-d10	14.15	164	237163	20.00	ng	-0.01
64) Phenanthrene-d10	16.92	188	437159	20.00	ng	0.00
76) Chrysene-d12	21.14	240	421281	20.00	ng	0.00
87) Perylene-d12	23.30	264	488013	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.13	112	798828	103.49	ng	0.00
7) Phenol-d6	6.69	99	1057646	98.58	ng	-0.01
23) Nitrobenzene-d5	8.65	82	599694	61.94	ng	-0.01
42) 2,4,6-Tribromophenol	15.66	330	243360	69.91	ng	0.00
45) 2-Fluorobiphenyl	12.76	172	920995	50.30	ng	-0.01
79) Terphenyl-d14	19.57	244	743057	39.89	ng	0.00
Target Compounds						
10) Phenol	6.72	94	74302	6.540	ng	98
50) Dimethylphthalate	13.63	163	172034	8.725	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
Data File : BM018246.D
Acq On : 17 Dec 2018 13:23
Operator : JU/SJ
Sample : J6388-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-SS010-0006-01

Quant Time: Dec 18 00:49:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

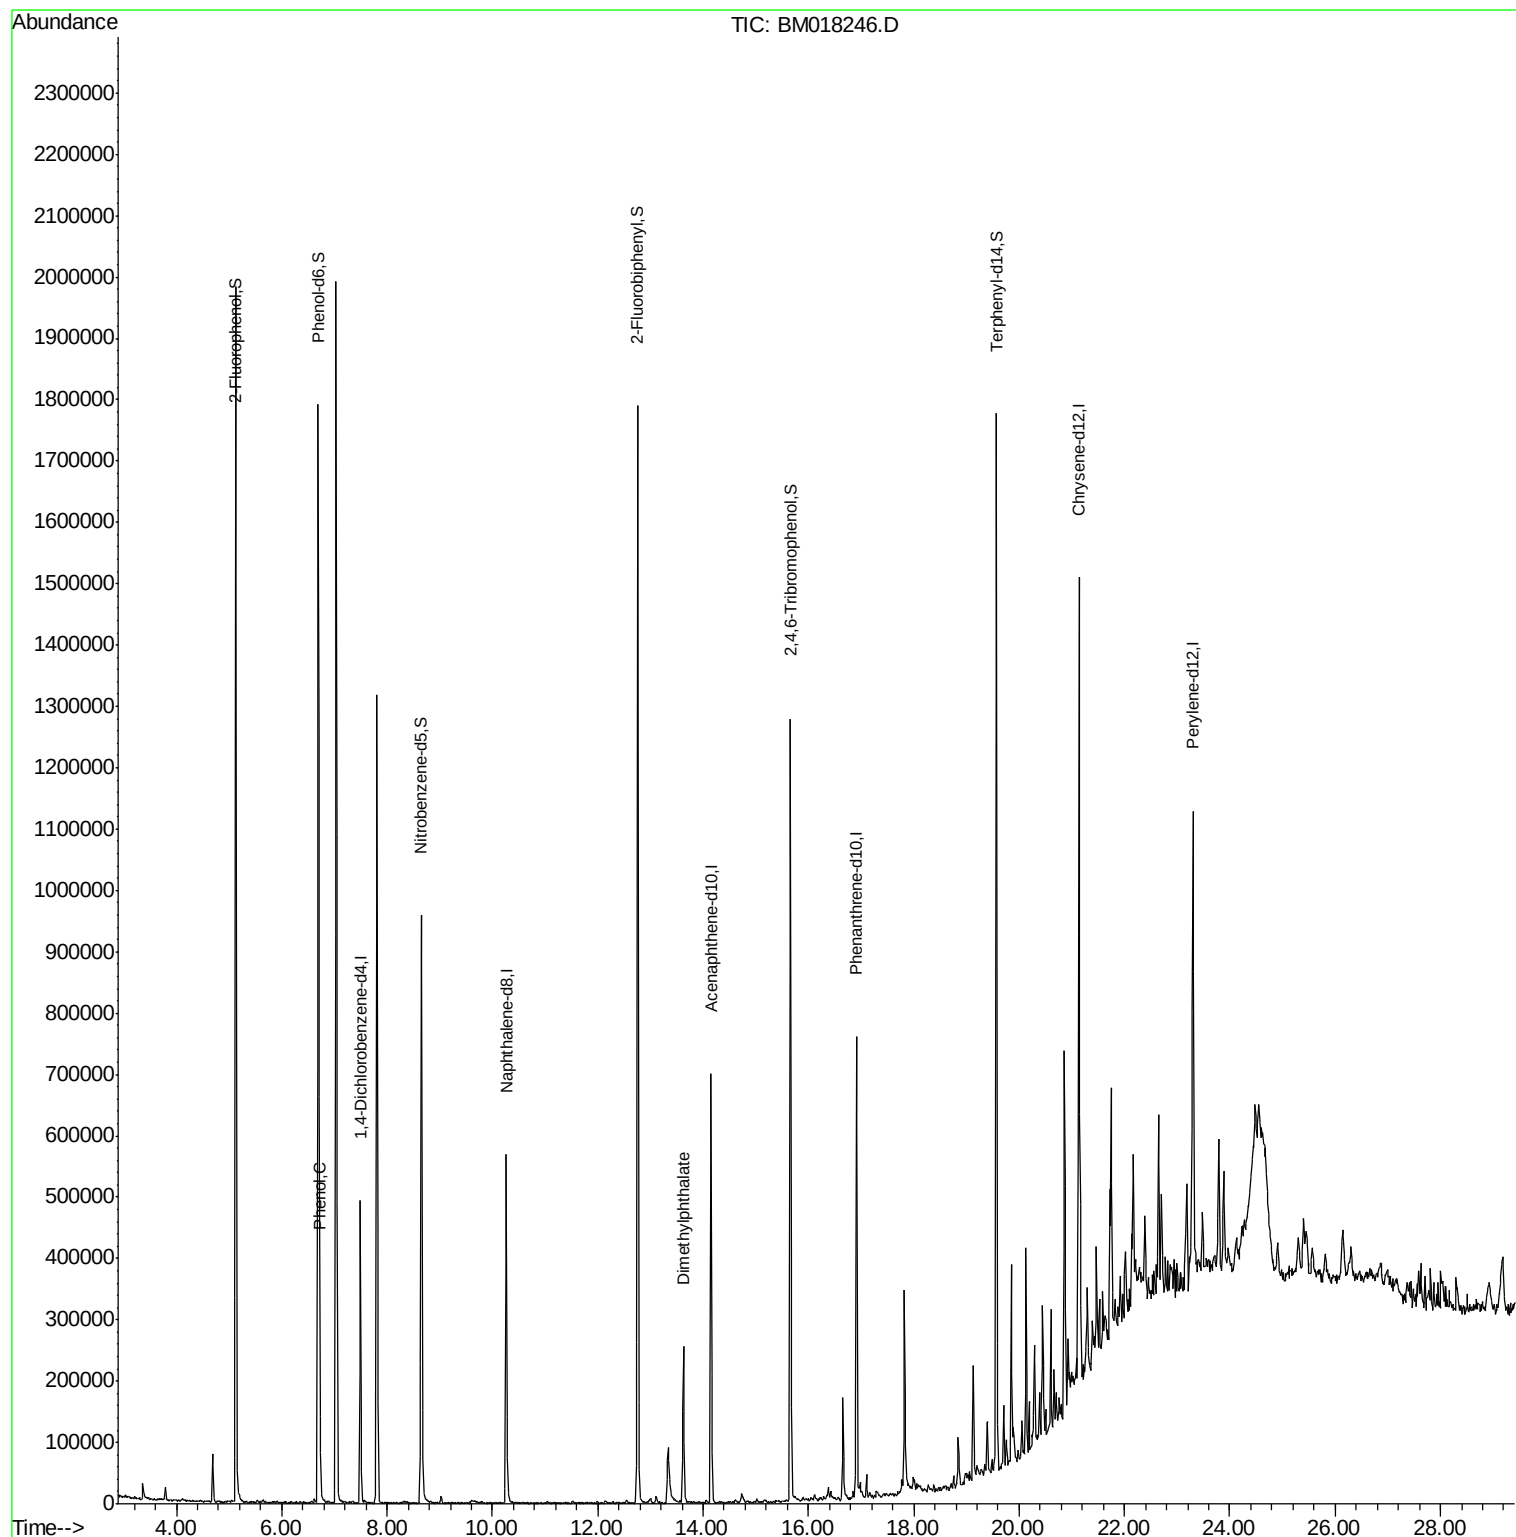

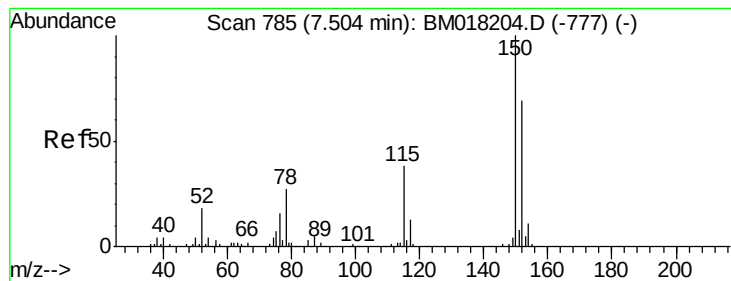


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 783
Delta R.T. -0.01 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23

Instrument :
BNA_M
ClientSampleId :
P001-SS010-0006-01

Tgt Ion:152 Resp: 128940
Ion Ratio Lower Upper
152 100
150 152.1 116.1 174.1
115 59.0 44.6 67.0

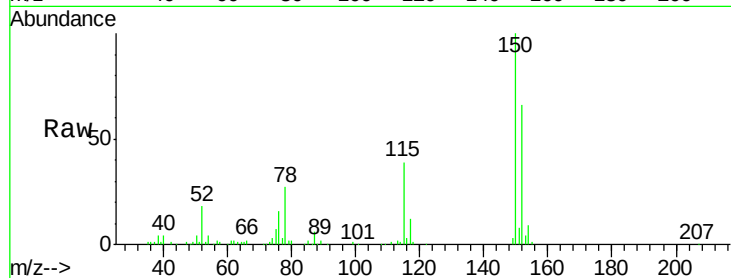


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

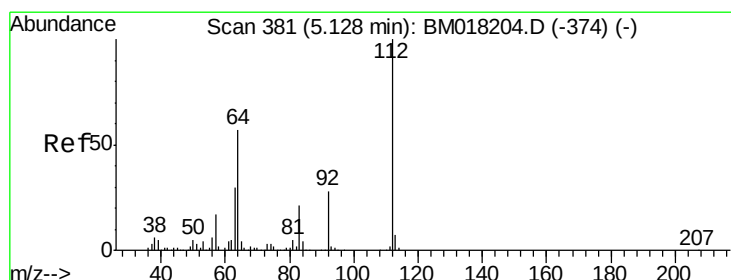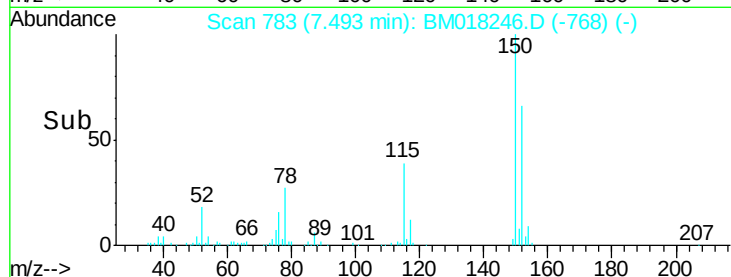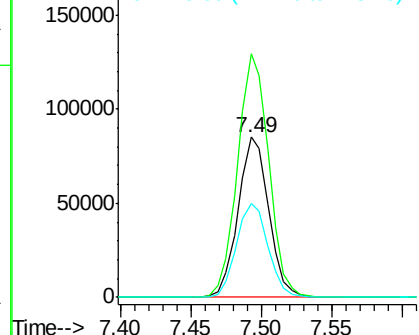



#5




2-Fluorophenol
Concen: 103.492 ng
RT: 5.13 min Scan# 381
Delta R.T. -0.00 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23

Tgt Ion:112 Resp: 798828
Ion Ratio Lower Upper
112 100
64 56.3 45.4 68.2
63 30.0 24.0 36.0

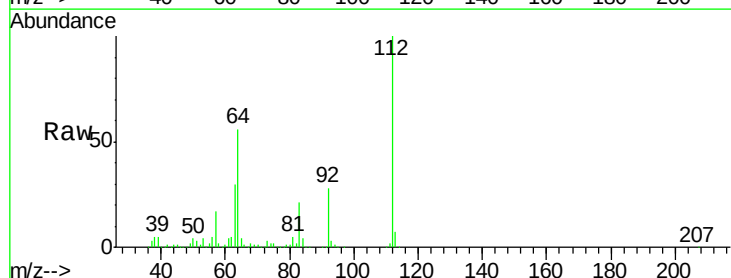

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

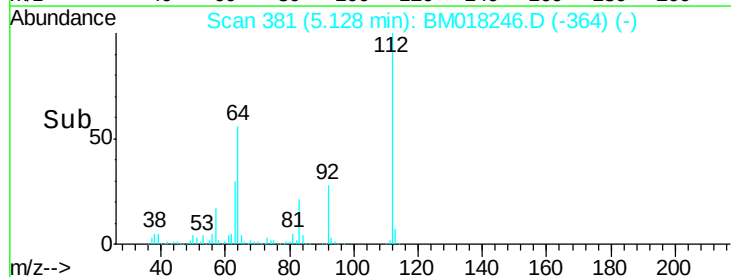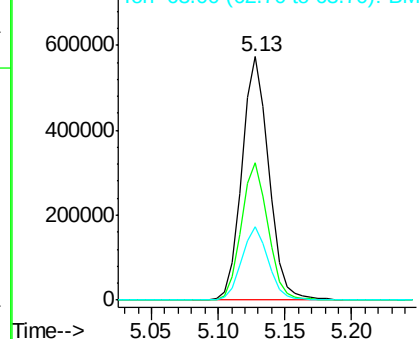

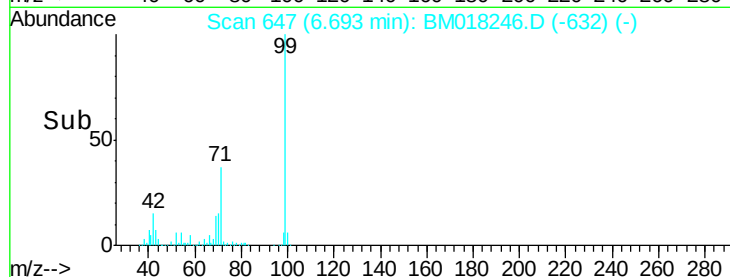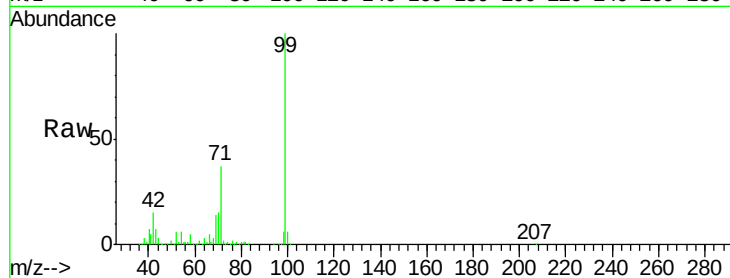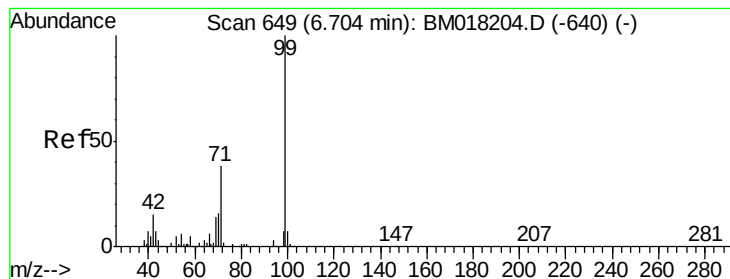

#7

Phenol-d6

Concen: 98.584 ng

RT: 6.69 min Scan# 647

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23

Instrument :

BNA_M

ClientSampleId :

P001-SS010-0006-01





Tgt Ion: 99 Resp: 1057646

Ion Ratio Lower Upper

99 100

42 14.8 12.3 18.5

71 37.4 30.2 45.2

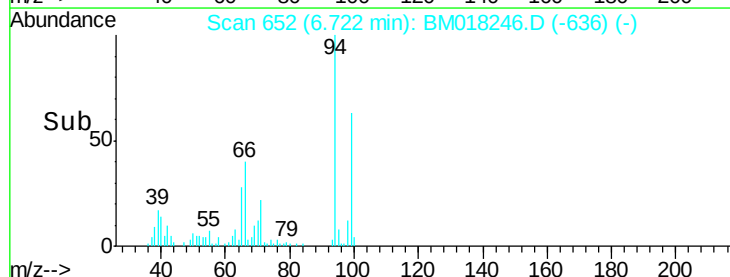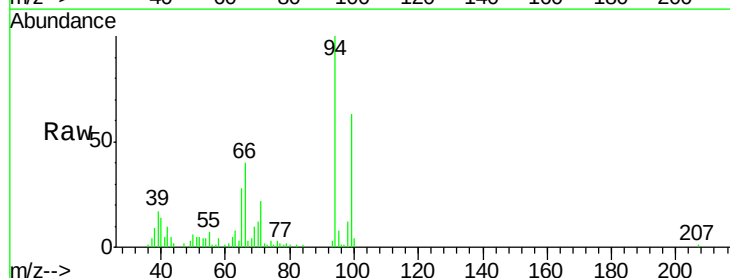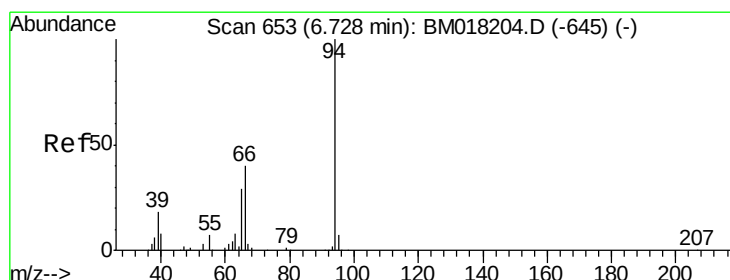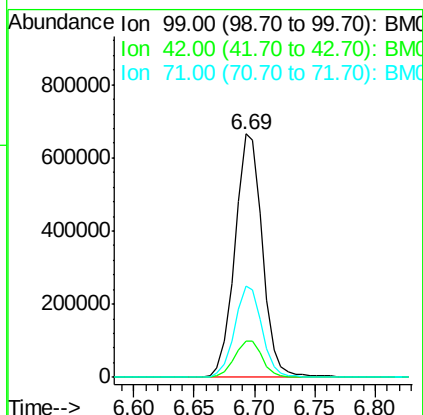

#10

Phenol

Concen: 6.540 ng

RT: 6.72 min Scan# 652

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23


Tgt Ion: 94 Resp: 74302


Ion Ratio Lower Upper

94 100

65 27.5 9.5 49.5

66 40.5 21.3 61.3

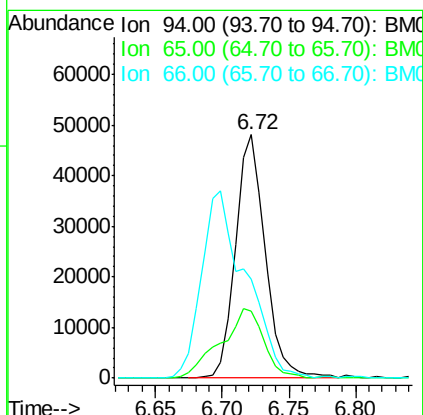


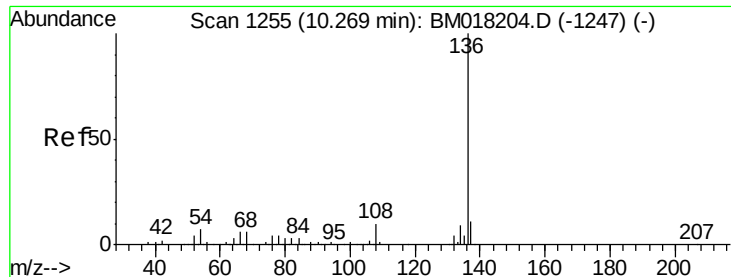




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.26 min Scan# 1254
Delta R.T. -0.01 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23

Instrument :
BNA_M
ClientSampleId :
P001-SS010-0006-01

Tgt Ion:	136	Resp:	496632
Ion	Ratio	Lower	Upper
136	100		
137	10.5	9.2	13.8
54	6.5	5.2	7.8
68	6.5	5.0	7.6

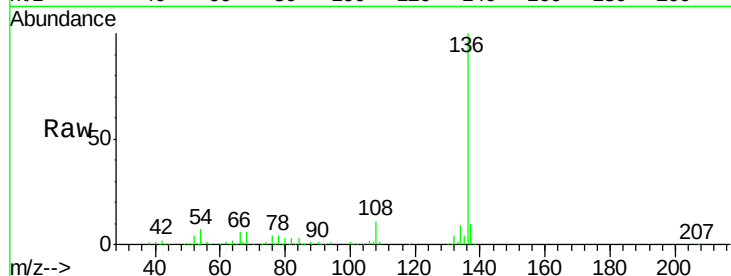


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

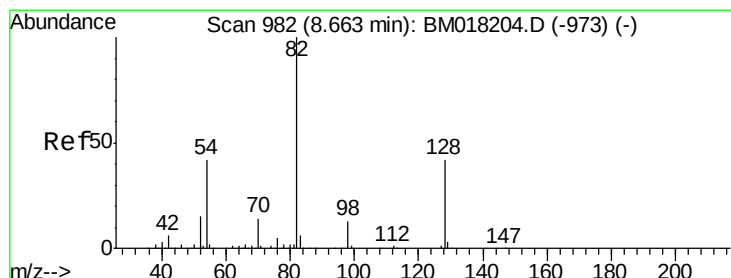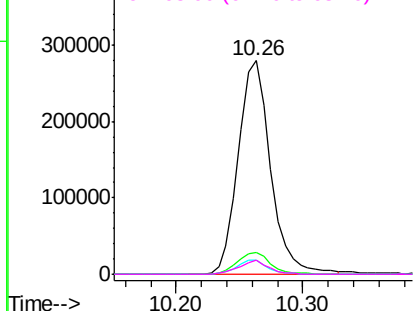
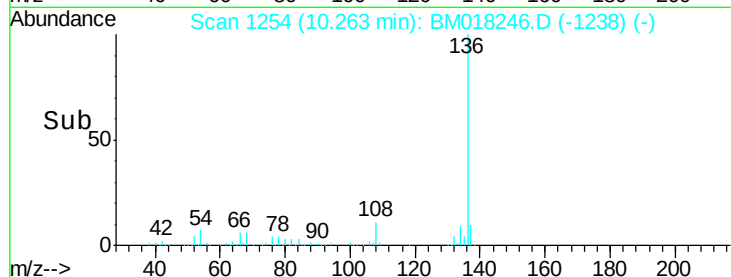



#23
Nitrobenzene-d5
Concen: 61.938 ng
RT: 8.65 min Scan# 980
Delta R.T. -0.01 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23

Tgt Ion:	82	Resp:	599694
Ion	Ratio	Lower	Upper
82	100		
128	42.4	33.4	50.2
54	40.3	33.4	50.2

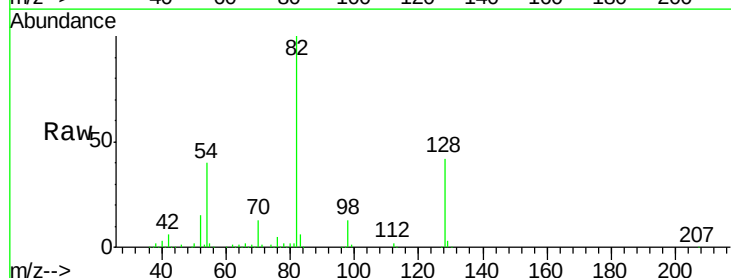

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

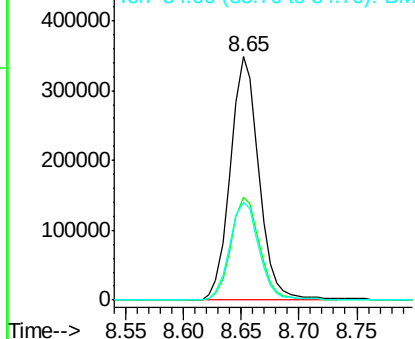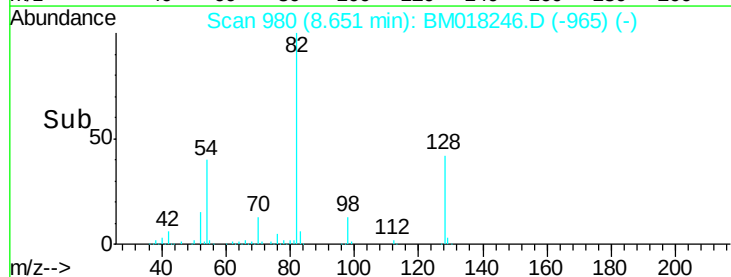

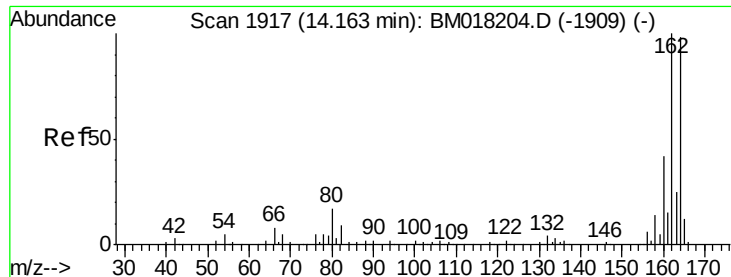

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.15 min Scan# 1915

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23

Instrument :

BNA_M

ClientSampleId :

P001-SS010-0006-01


Tgt Ion:164 Resp: 237163

Ion Ratio Lower Upper

164 100

162 99.6 81.8 122.6




160 46.0 34.6 51.8

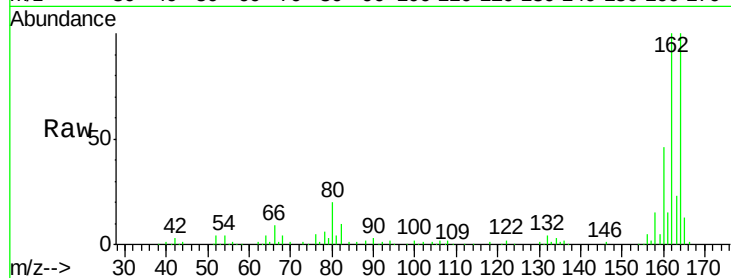

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

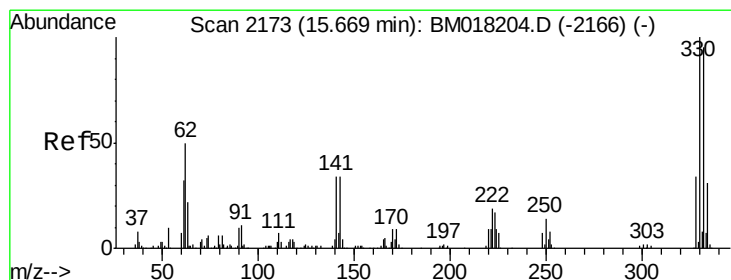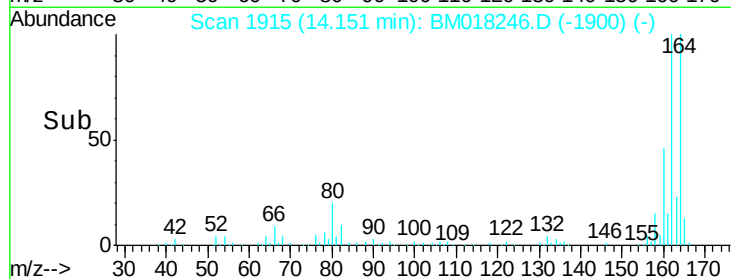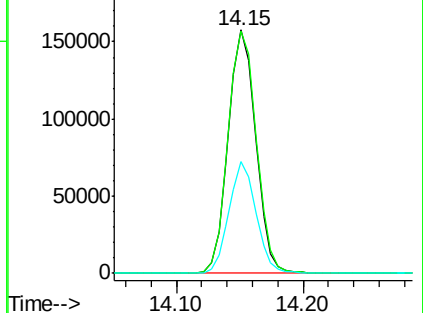

#42

2,4,6-Tribromophenol

Concen: 69.913 ng

RT: 15.66 min Scan# 2172

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23


Tgt Ion:330 Resp: 243360

Ion Ratio Lower Upper

330 100

332 94.2 78.6 118.0



141 35.7 27.1 40.7

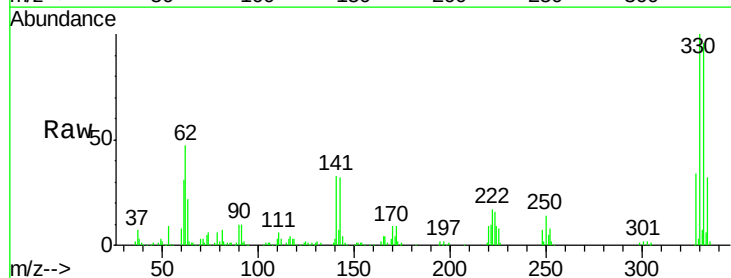


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



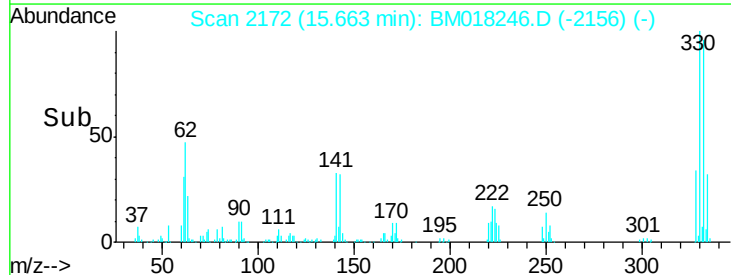
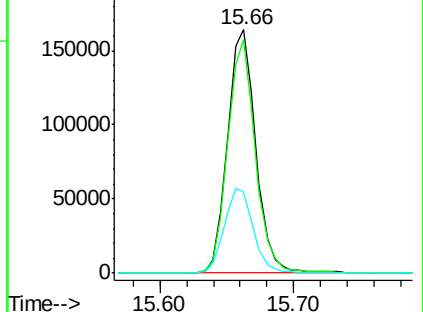


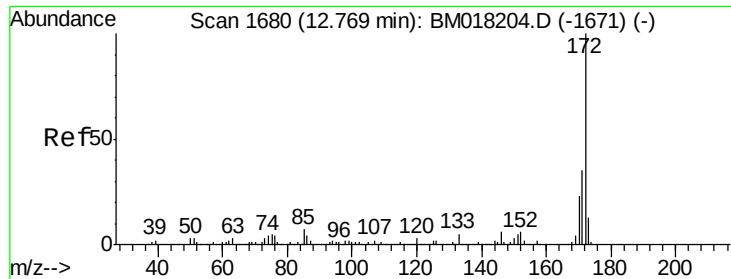

#45
2-Fluorobiphenyl
Concen: 50.299 ng
RT: 12.76 min Scan# 1678
Delta R.T. -0.01 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23




Instrument :
BNA_M
ClientSampleId :
P001-SS010-0006-01


Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.3	42.5
170	22.0	18.1	27.1

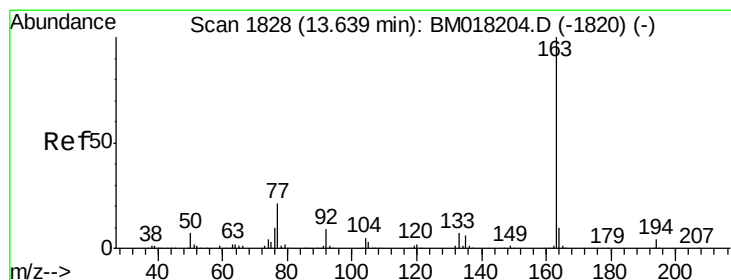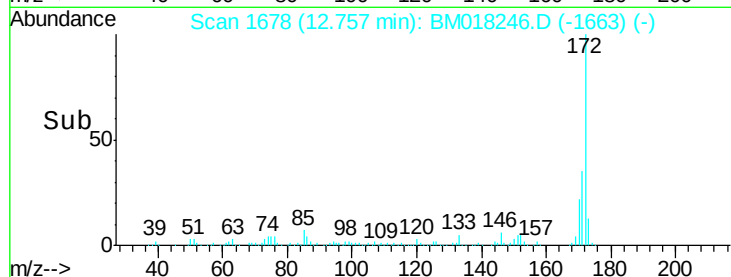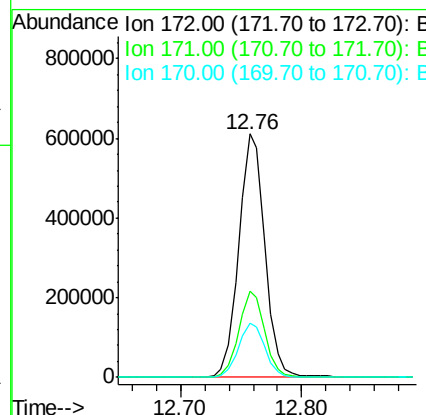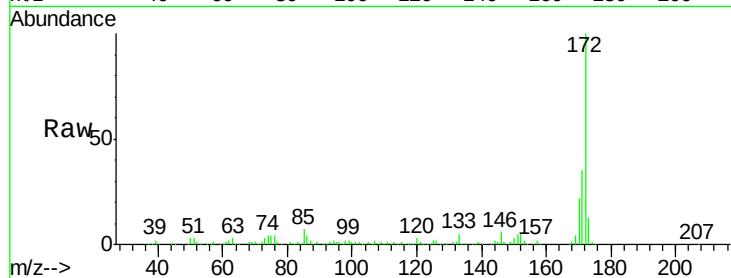

#50
Dimethylphthalate
Concen: 8.725 ng
RT: 13.63 min Scan# 1826
Delta R.T. -0.01 min
Lab File: BM018246.D
Acq: 17 Dec 2018 13:23

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.1	4.7
164	10.1	7.9	11.9

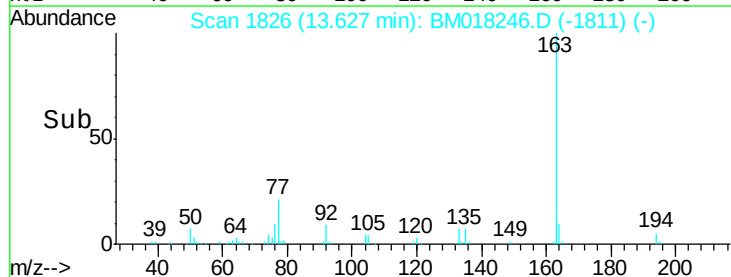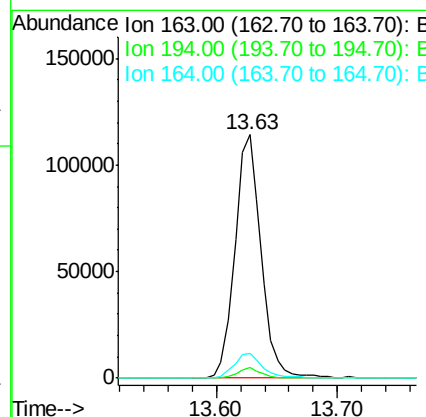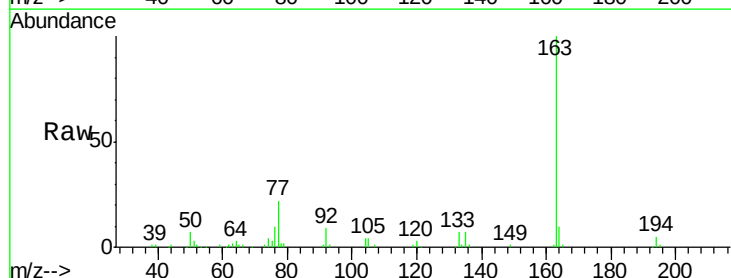

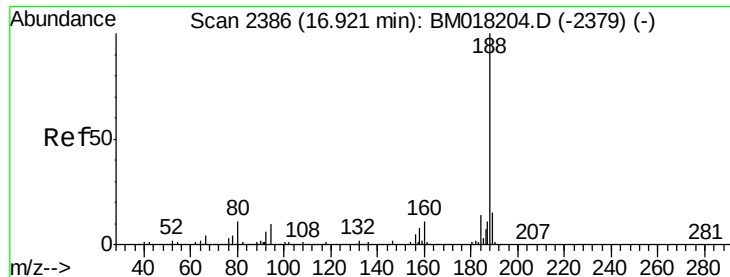

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.92 min Scan# 2385

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23

Instrument :

BNA_M

ClientSampleId :

P001-SS010-0006-01


Tgt Ion:188 Resp: 437159

Ion Ratio Lower Upper

188 100

94 9.4 8.0 12.0




80 11.3 9.0 13.6

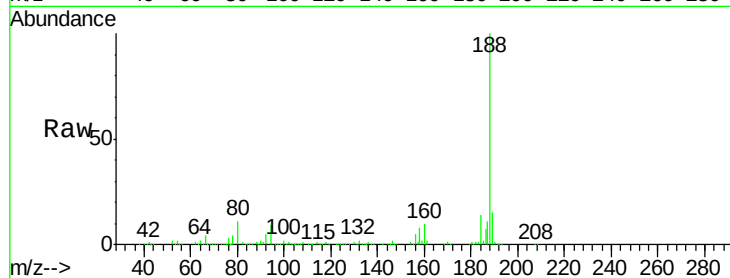

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

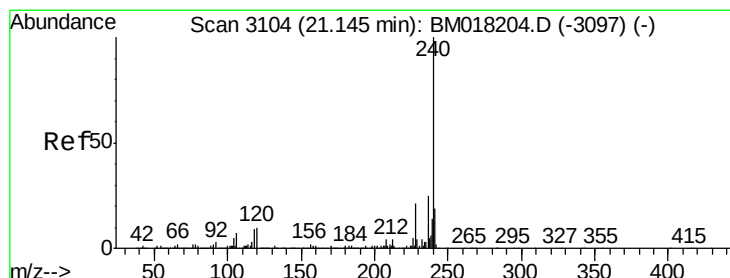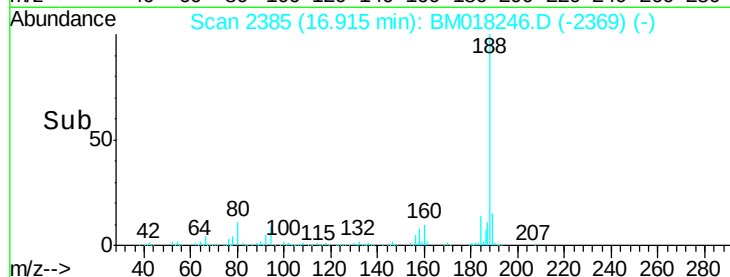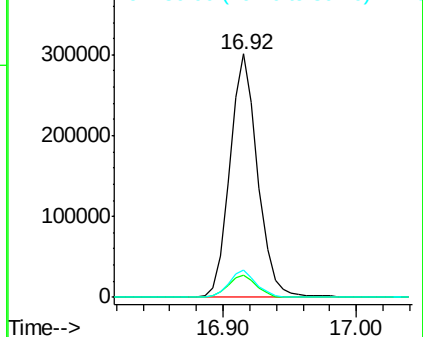

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.14 min Scan# 3103

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23


Tgt Ion:240 Resp: 421281

Ion Ratio Lower Upper

240 100

120 36.5 8.2 12.2#



236 24.8 20.3 30.5

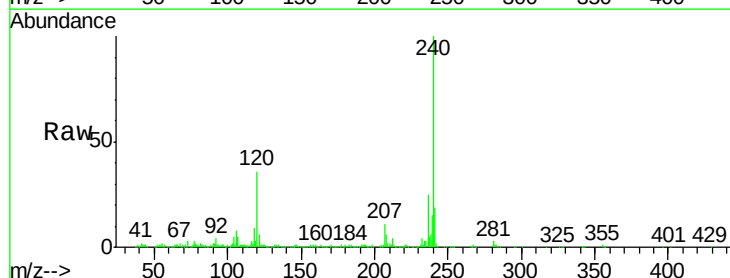


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

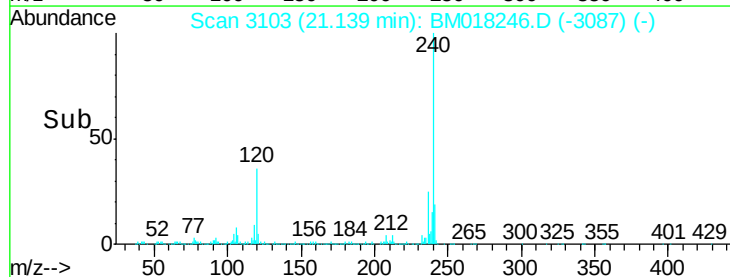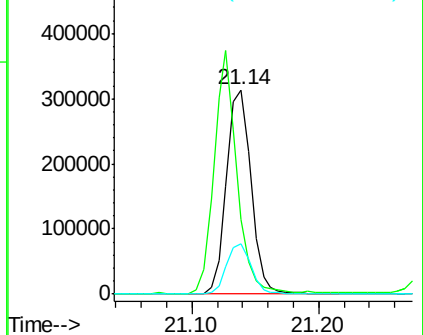

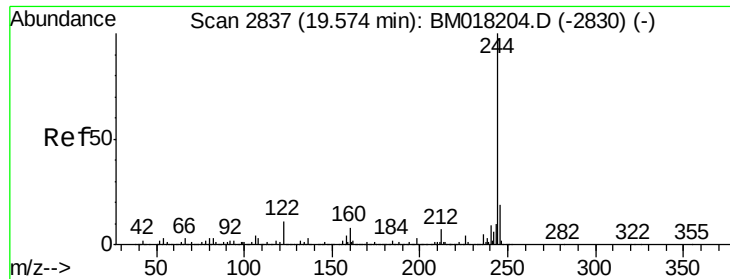

#79

Terphenyl-d14

Concen: 39.891 ng

RT: 19.57 min Scan# 2836

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23

Instrument :

BNA_M

ClientSampleId :

P001-SS010-0006-01


Tgt Ion:244 Resp: 743057

Ion Ratio Lower Upper

244 100

212 6.8 5.8 8.8




122 9.9 9.0 13.6

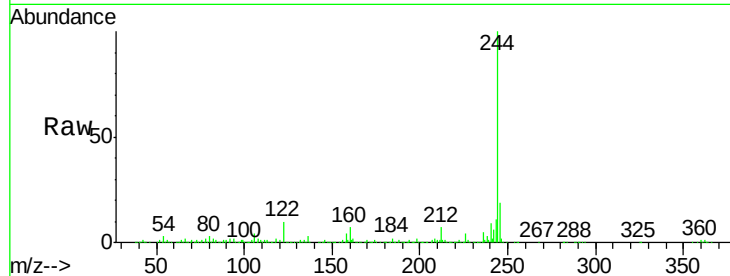

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

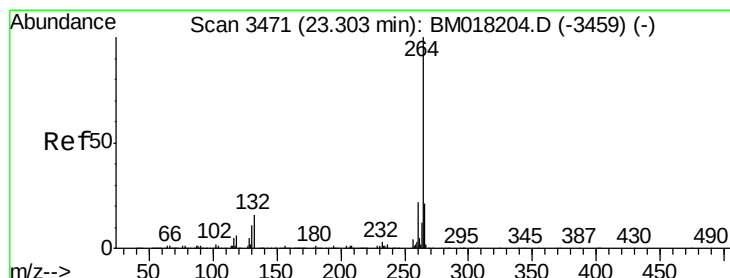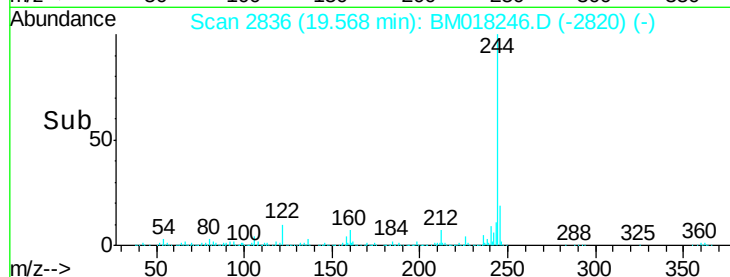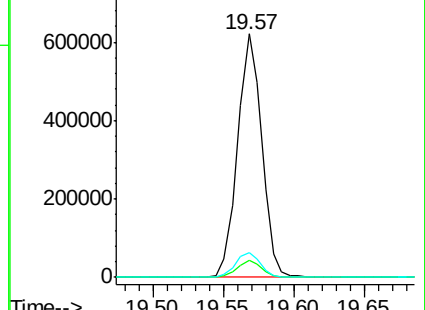

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.30 min Scan# 3470

Delta R.T. -0.01 min

Lab File: BM018246.D

Acq: 17 Dec 2018 13:23


Tgt Ion:264 Resp: 488013

Ion Ratio Lower Upper

264 100

260 24.2 17.5 26.3

265 21.6 17.3 25.9

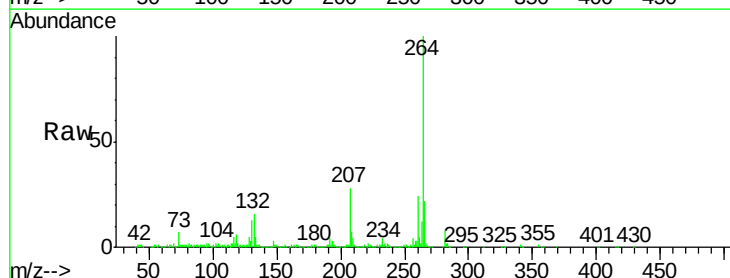

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

