


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018239.D
 Acq On : 17 Dec 2018 08:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

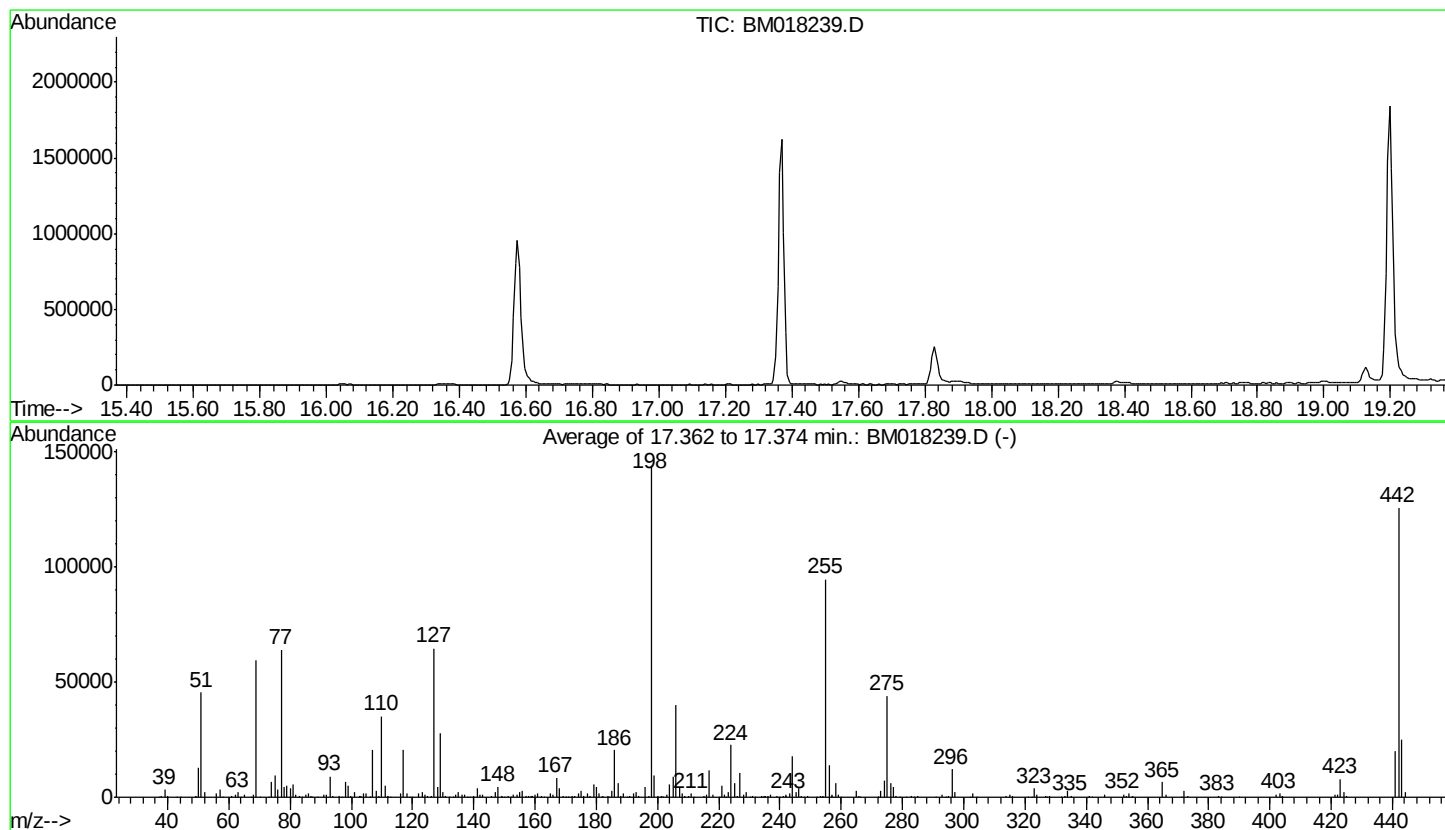

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	45418	PASS
68	69	0.00	2	1.9	1117	PASS
69	198	0.00	100	41.2	59306	PASS
70	69	0.00	2	0.5	273	PASS
127	198	10	80	44.9	64709	PASS
197	198	0.00	2	0.6	800	PASS
198	198	100	100	100.0	144077	PASS
199	198	5	9	6.5	9343	PASS
275	198	10	60	30.6	44024	PASS
365	198	1	100	4.6	6672	PASS
441	198	0.01	100	13.8	19822	PASS
442	198	50	100	87.4	125957	PASS
443	442	15	24	19.9	25056	PASS