


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121718\
 Data File : BM018257.D
 Acq On : 17 Dec 2018 20:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

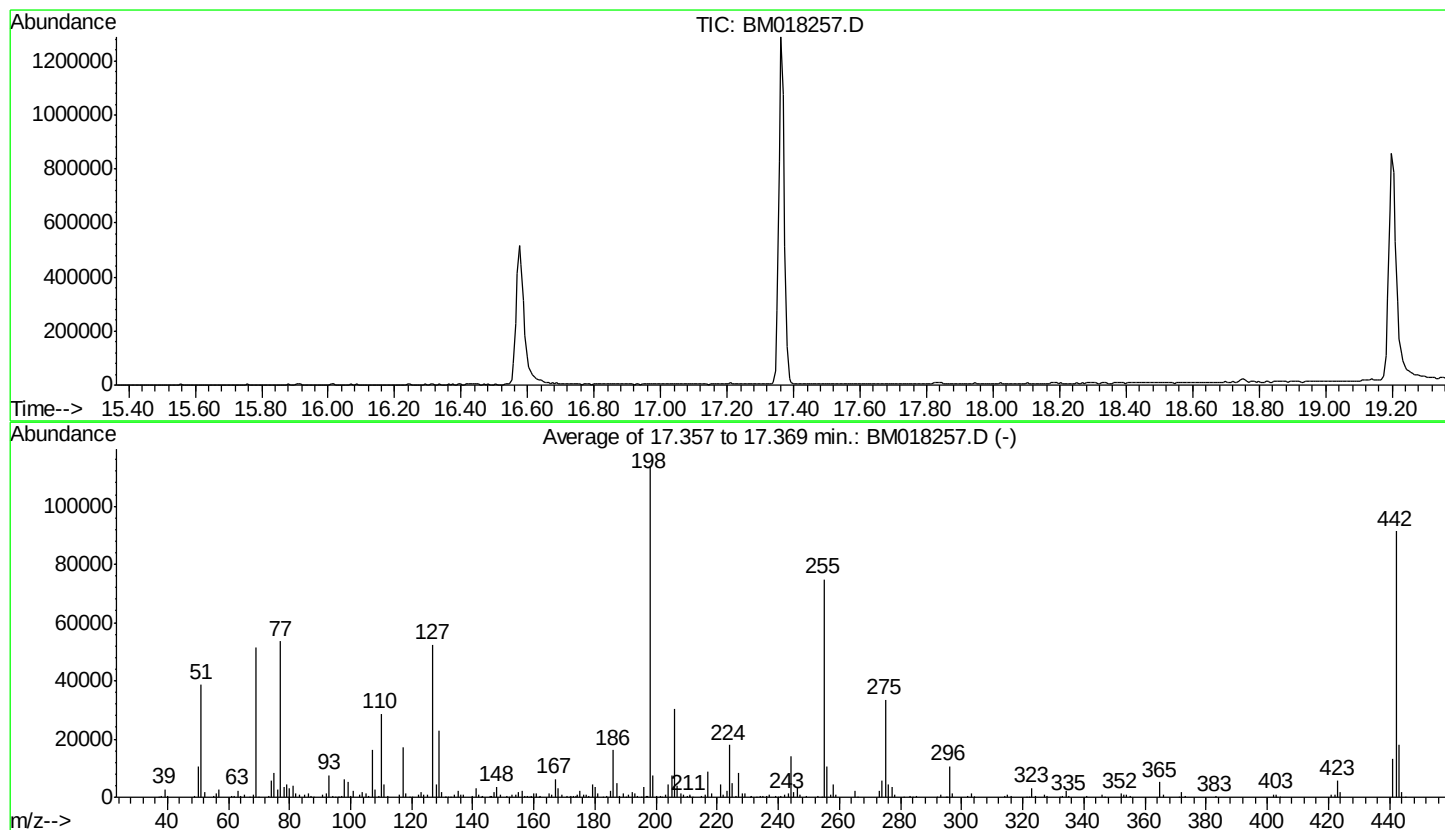

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	38536	PASS
68	69	0.00	2	1.5	772	PASS
69	198	0.00	100	45.1	51328	PASS
70	69	0.00	2	0.3	158	PASS
127	198	10	80	46.1	52498	PASS
197	198	0.00	2	0.5	521	PASS
198	198	100	100	100.0	113904	PASS
199	198	5	9	6.5	7431	PASS
275	198	10	60	29.5	33626	PASS
365	198	1	100	4.5	5141	PASS
441	198	0.01	100	11.7	13361	PASS
442	198	50	100	80.2	91389	PASS
443	442	15	24	19.8	18094	PASS