
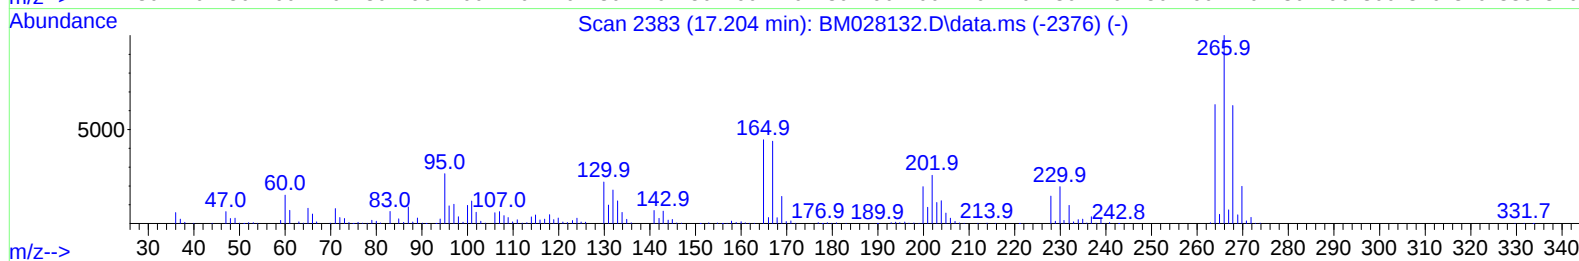
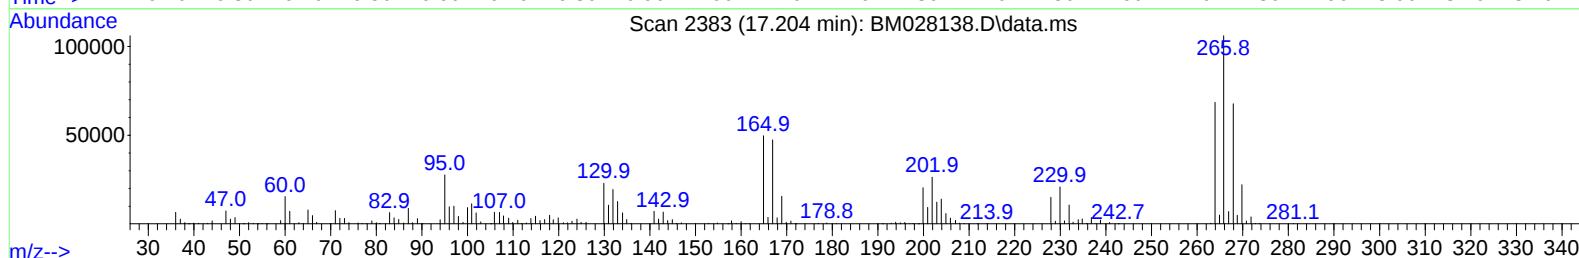


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
Data File : BM028138.D
Acq On : 17 Dec 2020 12:00
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 03:39:24 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 16 01:58:38 2020
Response via : Initial Calibration

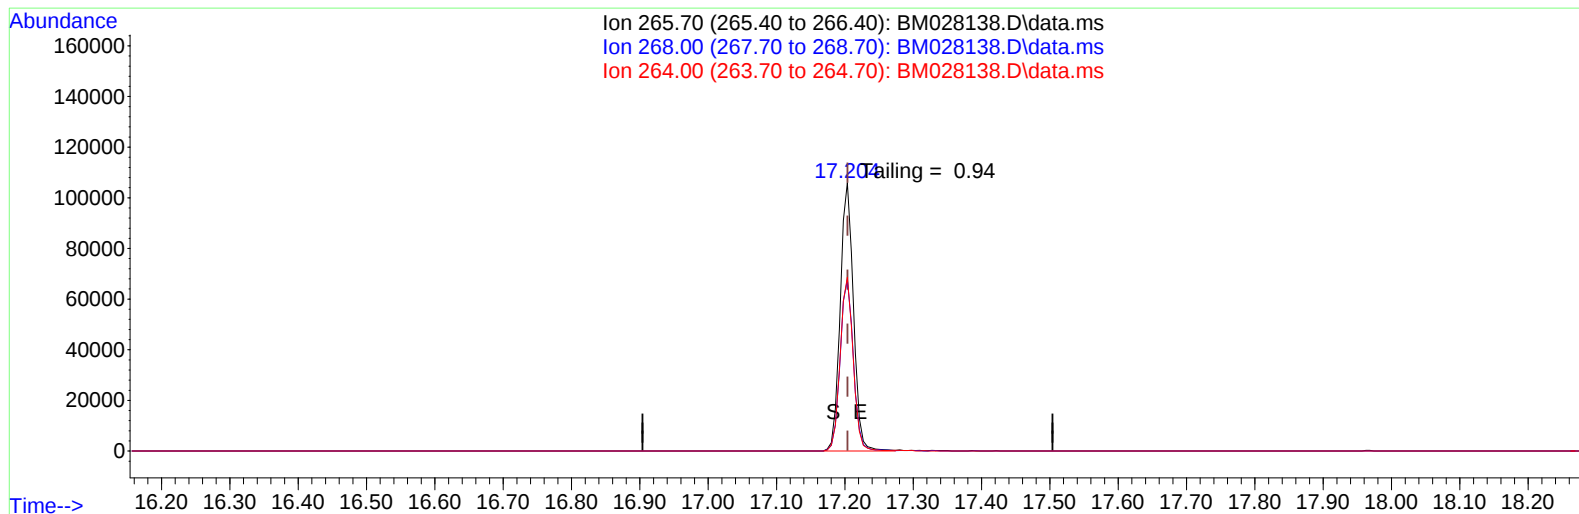

TIC: BM028138.D\data.ms

(70) Pentachlorophenol (C)




17.204min (-0.000) 0.00 ng m

response 143216

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.90
264.00	63.30	64.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
 Data File : BM028138.D
 Acq On : 17 Dec 2020 12:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 03:39:24 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 16 01:58:38 2020
 Response via : Initial Calibration

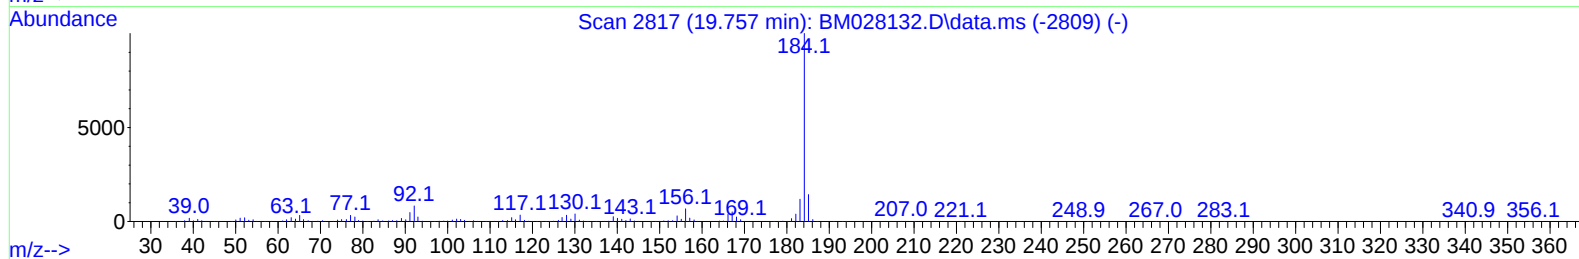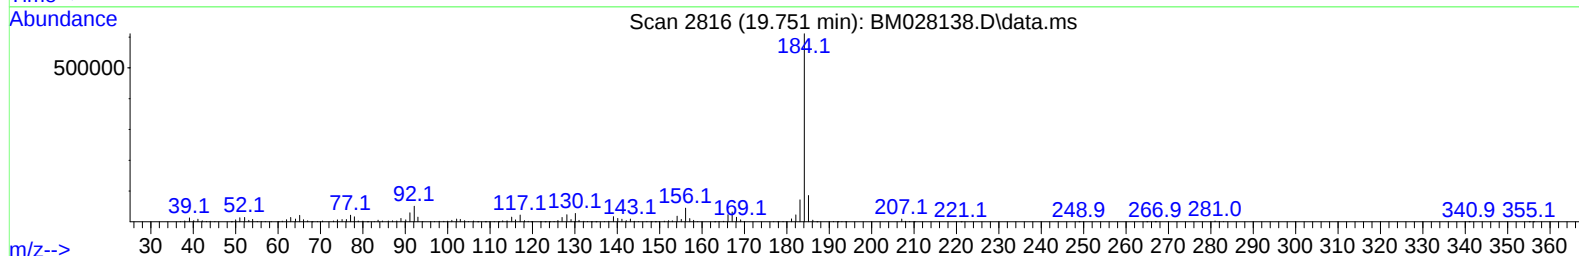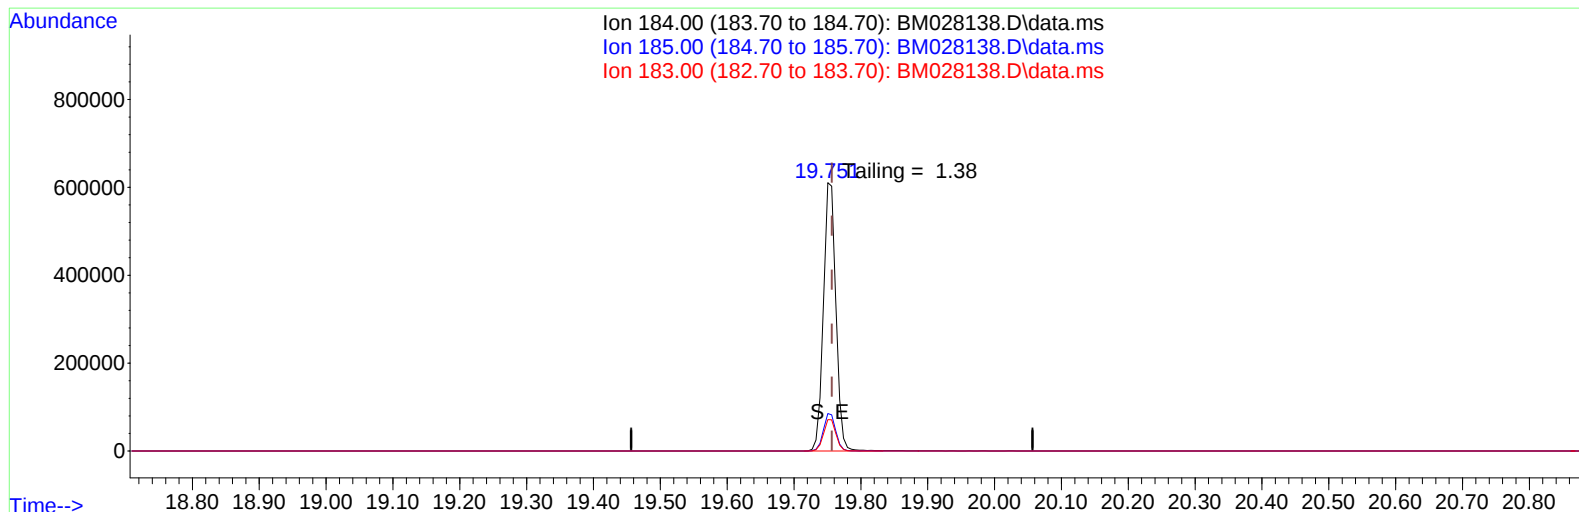

TIC: BM028138.D\data.ms

(77) Benzidine**19.751min (-0.006) 532108.49 ng****response 792040**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.99
183.00	12.10	11.68
0.00	0.00	0.00