

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
 Data File : BM028155.D
 Acq On : 17 Dec 2020 23:34
 Operator : JU/CG
 Sample : L5036-09 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.704	421	428	435	rBV	171433	263693	11.40%	1.701%
2	7.345	700	707	718	rVB	188364	307367	13.29%	1.983%
3	8.210	844	854	861	rBV	591037	939474	40.61%	6.060%
4	9.386	1046	1054	1060	rBV	108098	185134	8.00%	1.194%
5	11.039	1326	1335	1343	rBV	873371	1398886	60.47%	9.023%
6	13.463	1738	1747	1754	rVB	299080	427776	18.49%	2.759%
7	14.274	1878	1885	1892	rBV	24679	40338	1.74%	0.260%
8	14.563	1925	1934	1941	rBV	42463	76668	3.31%	0.495%
9	14.839	1974	1981	1988	rVB	1294814	1901102	82.18%	12.263%
10	15.809	2141	2146	2152	rBV2	18981	32176	1.39%	0.208%
11	16.304	2225	2230	2237	rBV	229191	329966	14.26%	2.128%
12	17.286	2392	2397	2402	rBV8	15434	34064	1.47%	0.220%
13	17.556	2437	2443	2448	rBV	1643914	2278252	98.48%	14.695%
14	17.598	2448	2450	2457	rVB	106904	119652	5.17%	0.772%
15	17.686	2462	2465	2470	rVB	45523	59944	2.59%	0.387%
16	18.415	2584	2589	2594	rBV2	56280	104686	4.53%	0.675%
17	18.468	2594	2598	2603	rVB	53658	79348	3.43%	0.512%
18	18.550	2608	2612	2616	rBV	30618	39293	1.70%	0.253%
19	18.609	2618	2622	2626	rBV2	56640	105713	4.57%	0.682%
20	18.909	2670	2673	2677	rVB	32576	40691	1.76%	0.262%
21	19.456	2763	2766	2770	rBV2	40030	62081	2.68%	0.400%
22	19.580	2782	2787	2794	rBV	619350	811472	35.08%	5.234%
23	19.903	2838	2842	2844	rBV2	93081	135342	5.85%	0.873%
24	19.939	2844	2848	2856	rVB	554118	730068	31.56%	4.709%
25	20.127	2875	2880	2884	rVB	508399	629123	27.19%	4.058%
26	20.421	2927	2930	2936	rVB2	136348	171550	7.42%	1.107%
27	21.668	3136	3142	3146	rBV2	1493919	2313459	100.00%	14.922%
28	21.703	3146	3148	3153	rVB	292450	315228	13.63%	2.033%
29	24.038	3540	3545	3552	rVB	860304	1570794	67.90%	10.132%




Sum of corrected areas: 15503340

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
Data File : BM028155.D
Acq On : 17 Dec 2020 23:34
Operator : JU/CG
Sample : L5036-09 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
B-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

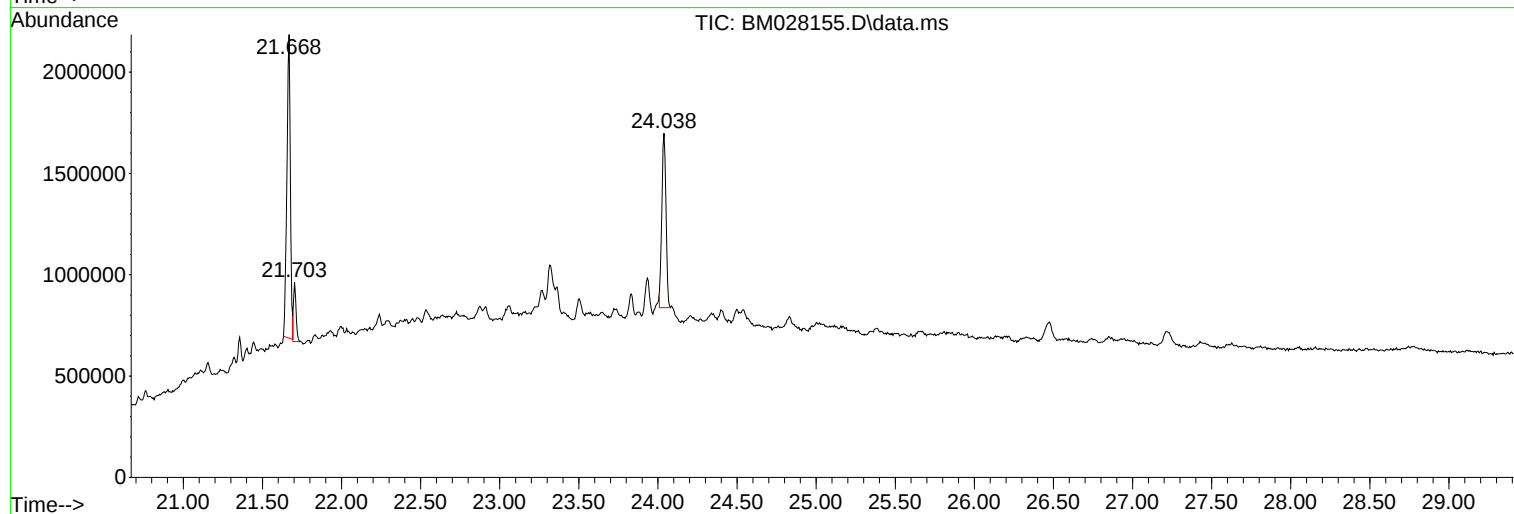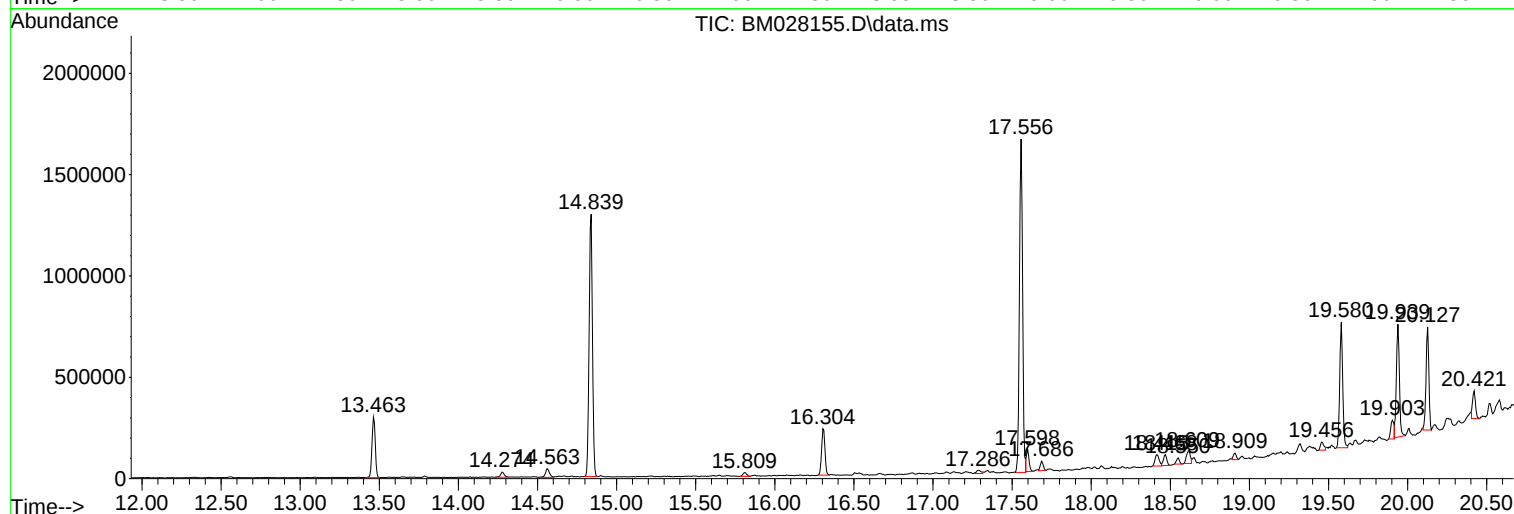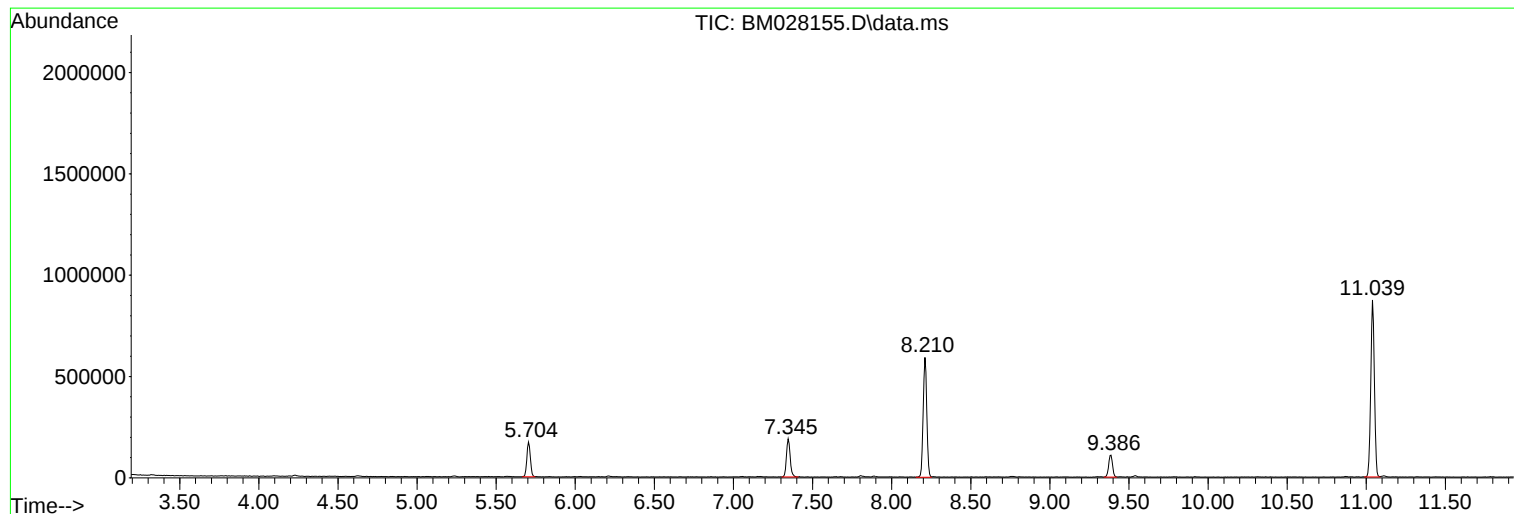

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
Data File : BM028155.D
Acq On : 17 Dec 2020 23:34
Operator : JU/CG
Sample : L5036-09 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
Data File : BM028155.D
Acq On : 17 Dec 2020 23:34
Operator : JU/CG
Sample : L5036-09 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
