
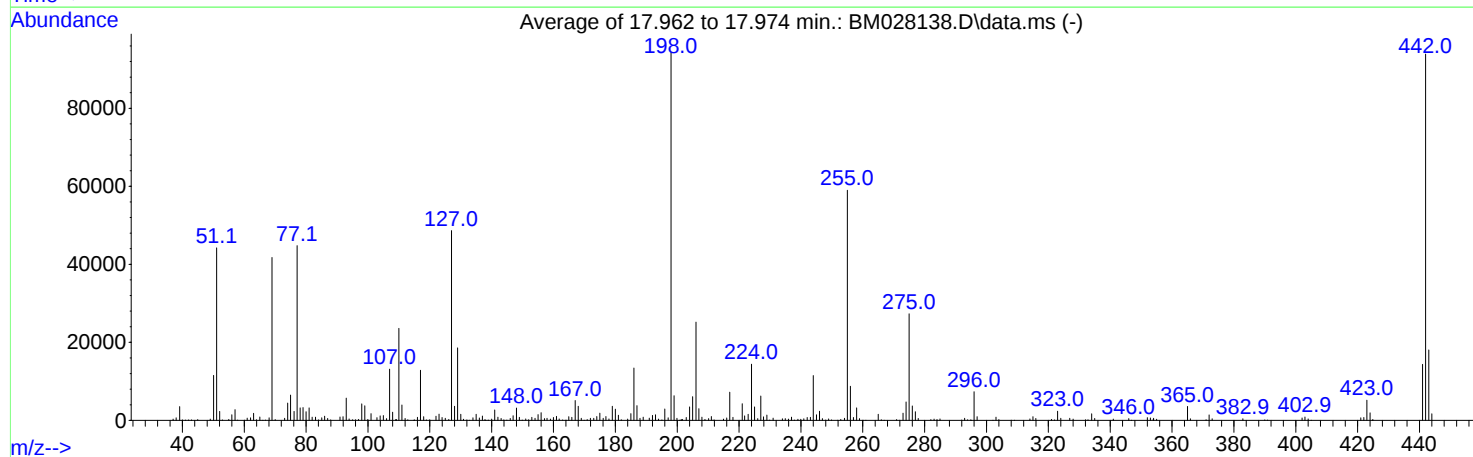


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121720\
 Data File : BM028138.D
 Acq On : 17 Dec 2020 12:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 16 01:58:38 2020

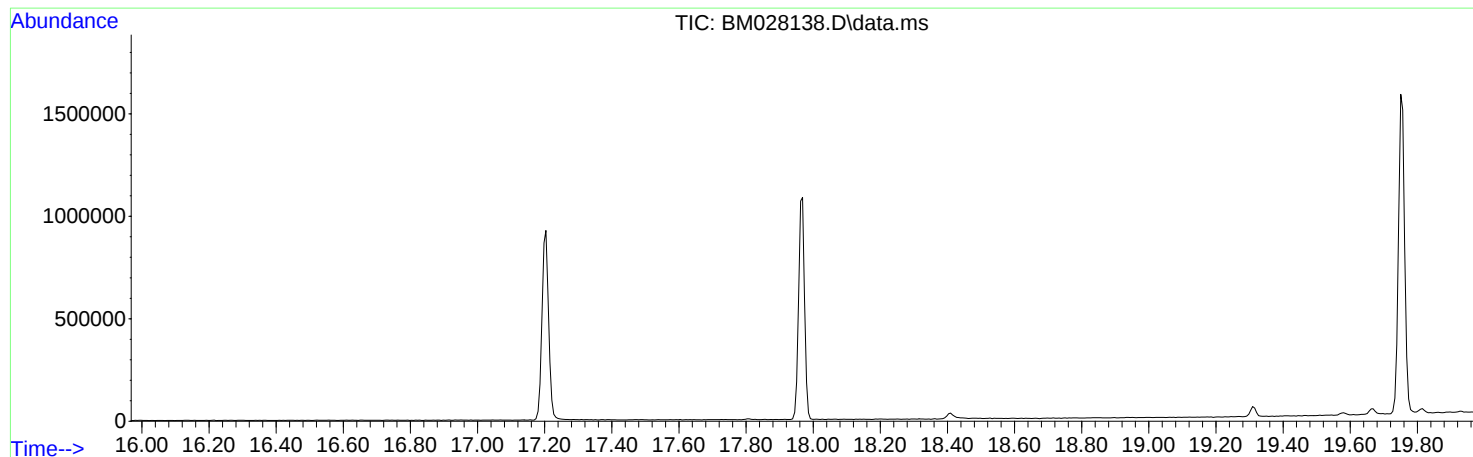

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	44227	PASS
68	69	0.00	2	1.6	675	PASS
69	198	0.00	100	44.3	41755	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	51.6	48645	PASS
197	198	0.00	2	0.7	664	PASS
198	198	100	100	100.0	94312	PASS
199	198	5	9	6.7	6327	PASS
275	198	10	60	29.0	27309	PASS
365	198	1	100	3.8	3556	PASS
441	198	0.01	100	15.2	14372	PASS
442	198	50	100	99.6	93923	PASS
443	442	15	24	19.2	18059	PASS