
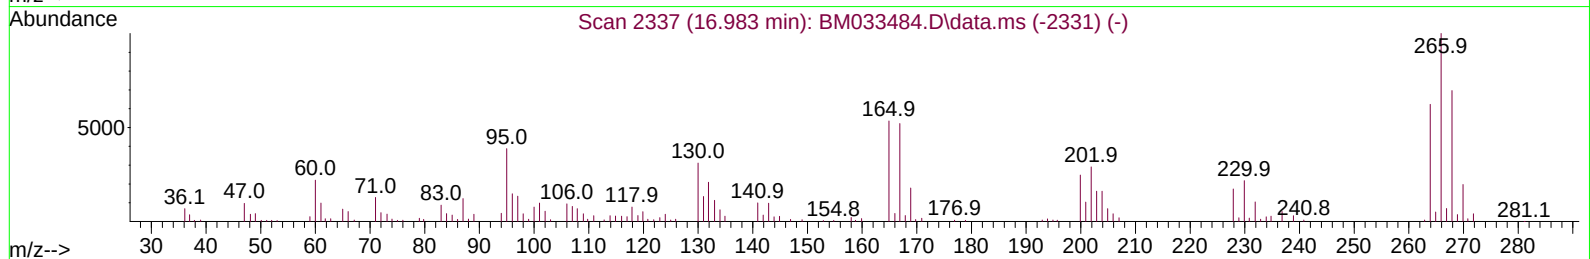
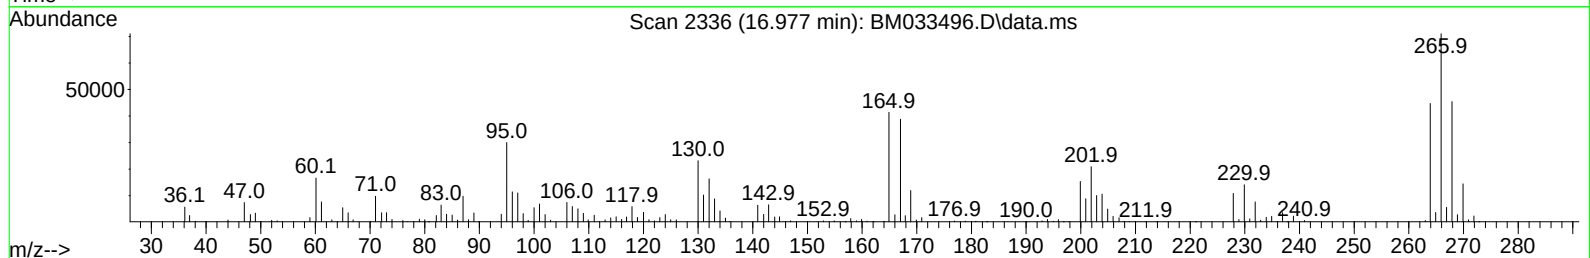


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033496.D
Acq On : 17 Dec 2021 07:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 10:49:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

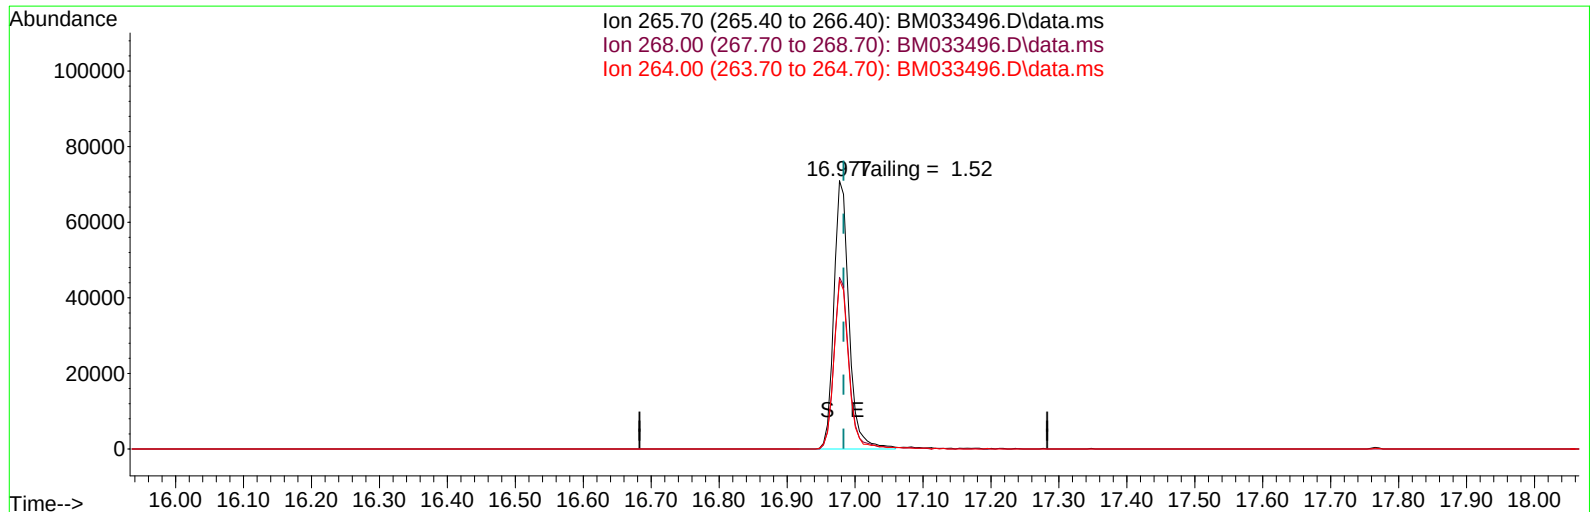

TIC: BM033496.D\data.ms

(70) Pentachlorophenol (C)




16.977min (-0.006) 0.00 ng

response 109886

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.99
264.00	61.40	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
 Data File : BM033496.D
 Acq On : 17 Dec 2021 07:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 10:49:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 17:10:15 2021
 Response via : Initial Calibration

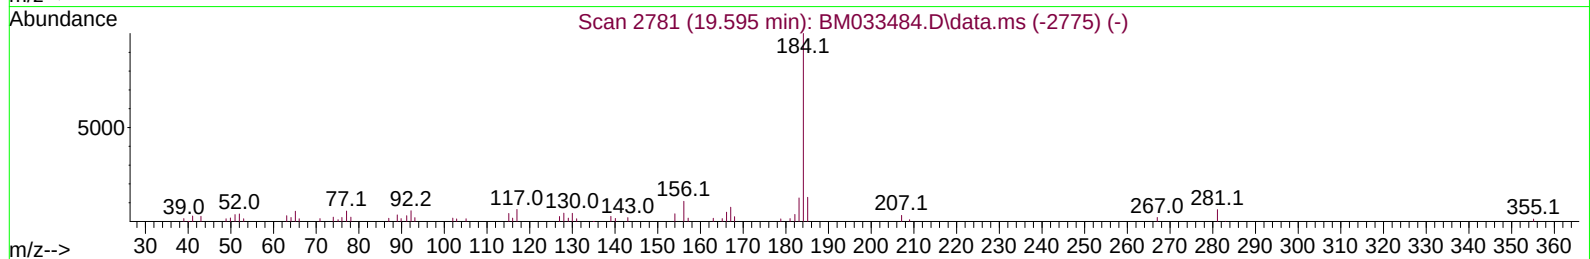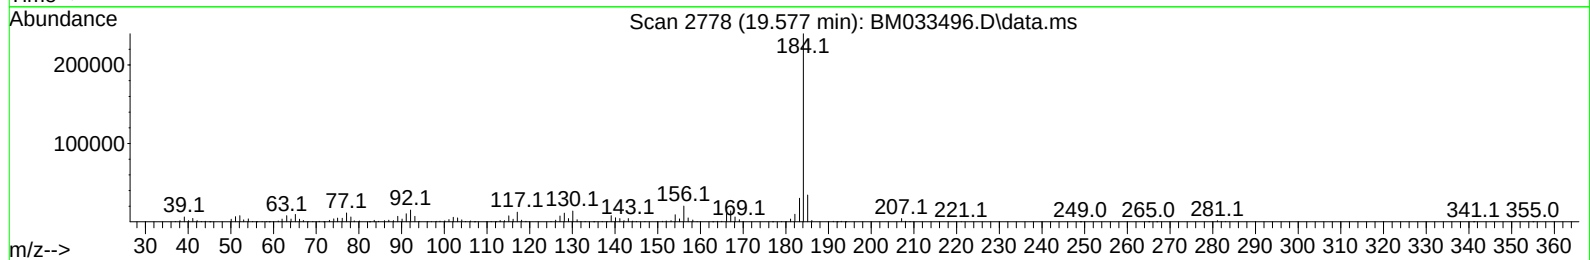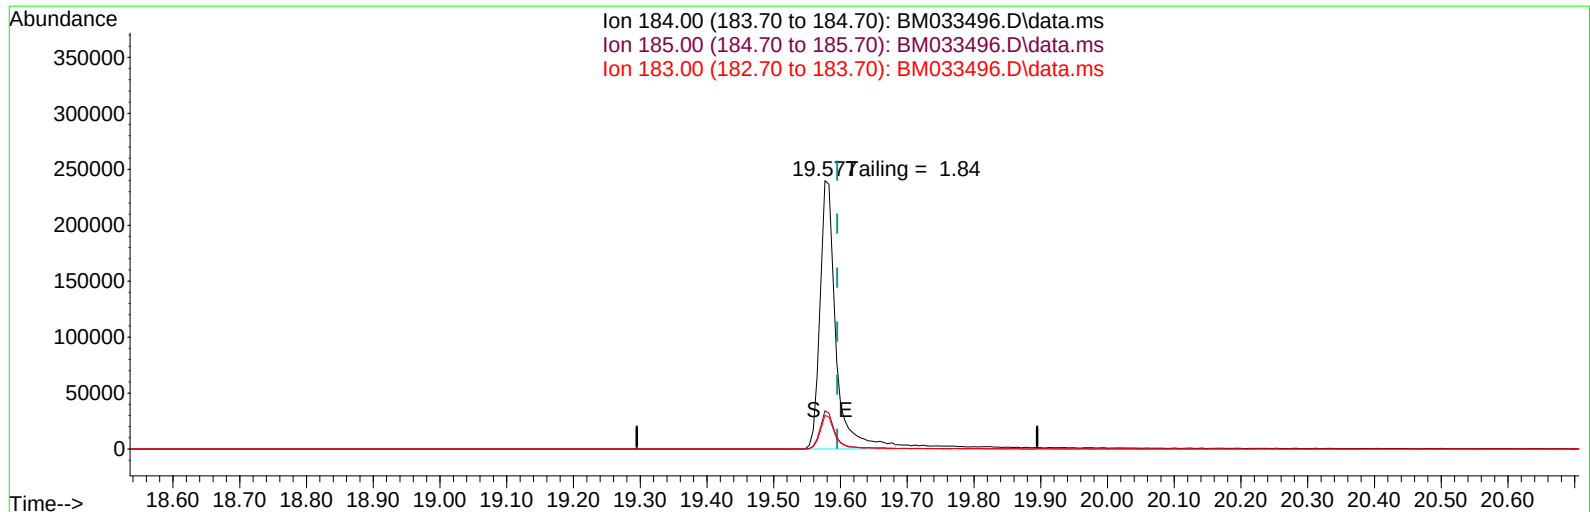

TIC: BM033496.D\data.ms

(77) Benzidine**19.577min (-0.018) 767354.59 ng****response 401846**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.28
183.00	12.10	12.55
0.00	0.00	0.00