

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
 Data File : BM033499.D
 Acq On : 17 Dec 2021 10:32
 Operator : CG/JU
 Sample : PB141339BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141339BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	379	385	402	rBV	499420	752415	46.28%	9.848%
2	7.107	651	658	673	rBV	461132	778772	47.90%	10.193%
3	7.937	793	799	815	rVB	129786	209263	12.87%	2.739%
4	9.107	991	998	1013	rBV	438645	758594	46.66%	9.929%
5	10.748	1270	1277	1291	rBV	142923	259897	15.99%	3.402%
6	13.207	1688	1695	1711	rBV	1022773	1528393	94.01%	20.005%
7	14.583	1923	1929	1940	rBV	219163	330757	20.34%	4.329%
8	16.071	2176	2182	2195	rBV	449532	688398	42.34%	9.010%
9	17.330	2390	2396	2407	rBV	218720	340670	20.95%	4.459%
10	19.948	2836	2841	2854	rBV	1246757	1625794	100.00%	21.280%
11	21.512	3102	3107	3116	rBV	146581	235701	14.50%	3.085%
12	23.930	3514	3518	3526	rVB2	63357	131329	8.08%	1.719%




Sum of corrected areas: 7639983

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033499.D
Acq On : 17 Dec 2021 10:32
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

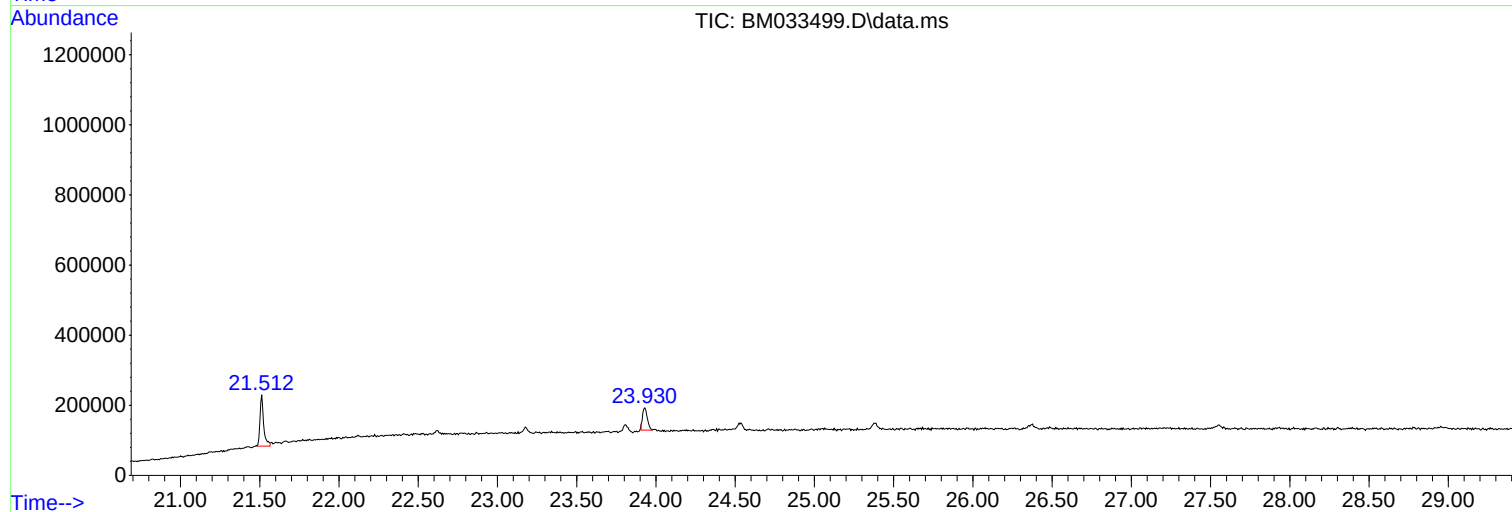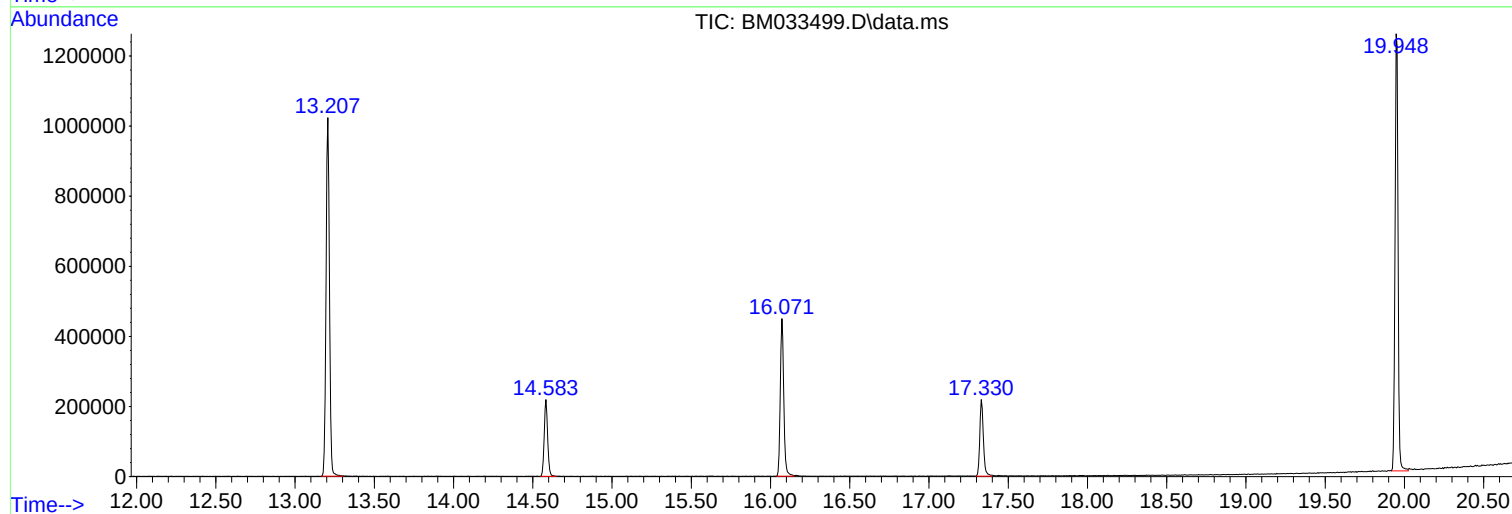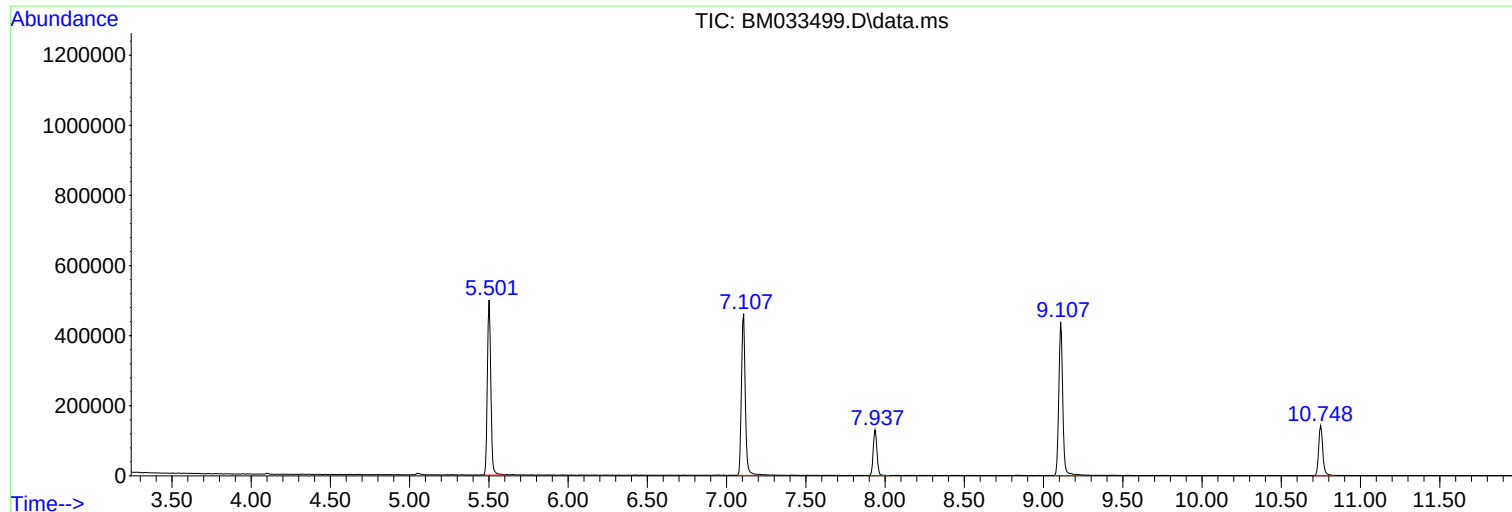

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033499.D
Acq On : 17 Dec 2021 10:32
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033499.D
Acq On : 17 Dec 2021 10:32
Operator : CG/JU
Sample : PB141339BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------