

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
 Data File : BM033508.D
 Acq On : 17 Dec 2021 16:28
 Operator : CG/JU
 Sample : M5051-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.396	24	27	36	rVB	93175	109784	3.08%	0.499%
2	4.437	199	204	215	rVB	54841	85808	2.41%	0.390%
3	4.548	217	223	229	rBV	105467	145283	4.08%	0.661%
4	5.001	294	300	303	rBV	62601	85394	2.40%	0.388%
5	5.043	303	307	317	rVB	360891	522006	14.65%	2.374%
6	5.507	379	386	392	rBV	1239358	1866893	52.38%	8.490%
7	5.554	392	394	404	rVB3	18376	41636	1.17%	0.189%
8	5.931	453	458	464	rBV	44899	67236	1.89%	0.306%
9	6.119	484	490	499	rVB	29566	45177	1.27%	0.205%
10	6.990	628	638	648	rBV3	47183	126315	3.54%	0.574%
11	7.107	648	658	664	rBV	1126389	1892474	53.10%	8.606%
12	7.578	732	738	745	rVB	68734	104936	2.94%	0.477%
13	7.654	745	751	757	rBV	79825	126375	3.55%	0.575%
14	7.936	789	799	808	rBV	206018	336919	9.45%	1.532%
15	8.042	812	817	827	rVB	59259	104055	2.92%	0.473%
16	8.307	854	862	868	rBV2	30618	51607	1.45%	0.235%
17	8.472	879	890	896	rBV6	34136	79898	2.24%	0.363%
18	9.107	991	998	1007	rBV	862147	1507776	42.31%	6.857%
19	9.425	1046	1052	1057	rVB2	25243	51396	1.44%	0.234%
20	10.001	1141	1150	1154	rBV3	42508	101948	2.86%	0.464%
21	10.107	1161	1168	1171	rBV2	76124	138487	3.89%	0.630%
22	10.154	1171	1176	1189	rVB5	50869	131056	3.68%	0.596%
23	10.448	1219	1226	1233	rBV2	63082	108724	3.05%	0.494%
24	10.625	1252	1256	1261	rVV	26333	45074	1.26%	0.205%
25	10.748	1270	1277	1281	rVV	265278	474070	13.30%	2.156%
26	10.795	1281	1285	1293	rVB	516800	850821	23.87%	3.869%
27	10.919	1299	1306	1313	rVB	24778	47330	1.33%	0.215%
28	11.554	1407	1414	1419	rBV4	39450	89064	2.50%	0.405%
29	11.977	1477	1486	1492	rBV4	24110	56439	1.58%	0.257%
30	12.142	1506	1514	1521	rVB	64542	122999	3.45%	0.559%
31	12.407	1554	1559	1569	rVB2	33933	69550	1.95%	0.316%
32	12.630	1592	1597	1604	rBV6	25183	59339	1.67%	0.270%
33	13.007	1654	1661	1664	rBV3	22408	47887	1.34%	0.218%
34	13.048	1664	1668	1674	rVB4	44999	78386	2.20%	0.356%
35	13.207	1688	1695	1702	rVB	2192789	3194869	89.65%	14.529%
36	13.560	1747	1755	1763	rBV7	18112	41992	1.18%	0.191%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
 Data File : BM033508.D
 Acq On : 17 Dec 2021 16:28
 Operator : CG/JU
 Sample : M5051-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.118	1846	1850	1855	rVV2	38588	55431	1.56%	0.252%
38	14.201	1855	1864	1872	rVB2	16568	47171	1.32%	0.215%
39	14.583	1922	1929	1938	rVB	397988	620285	17.41%	2.821%
40	15.571	2085	2097	2104	rBV	191929	438251	12.30%	1.993%
41	15.801	2128	2136	2140	rBV2	18398	37359	1.05%	0.170%
42	16.071	2175	2182	2192	rBV	1725995	2490651	69.89%	11.326%
43	16.607	2269	2273	2279	rBV	39722	51187	1.44%	0.233%
44	17.330	2388	2396	2401	rBV	491268	718114	20.15%	3.266%
45	18.412	2575	2580	2591	rBV6	23272	51195	1.44%	0.233%
46	18.753	2633	2638	2646	rBV5	28137	50682	1.42%	0.230%
47	19.947	2835	2841	2850	rBV	2735896	3563799	100.00%	16.207%
48	21.506	3101	3106	3112	rBV	347593	479017	13.44%	2.178%
49	23.918	3511	3516	3528	rVB	175975	377724	10.60%	1.718%




Sum of corrected areas: 21989869

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033508.D
Acq On : 17 Dec 2021 16:28
Operator : CG/JU
Sample : M5051-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

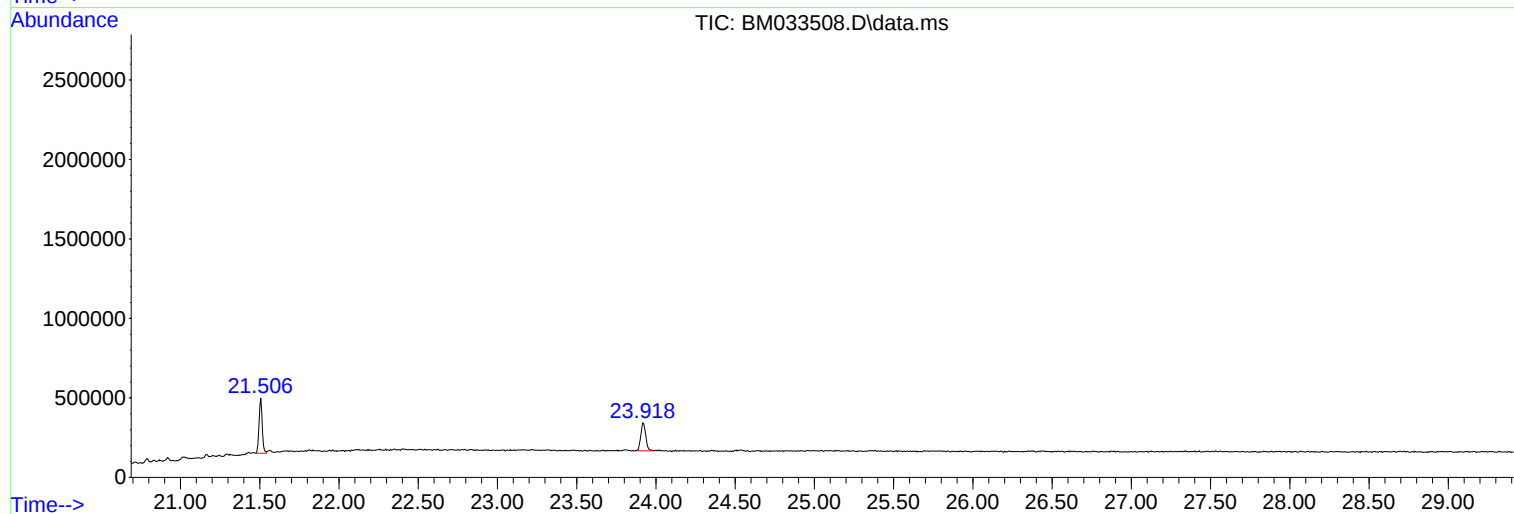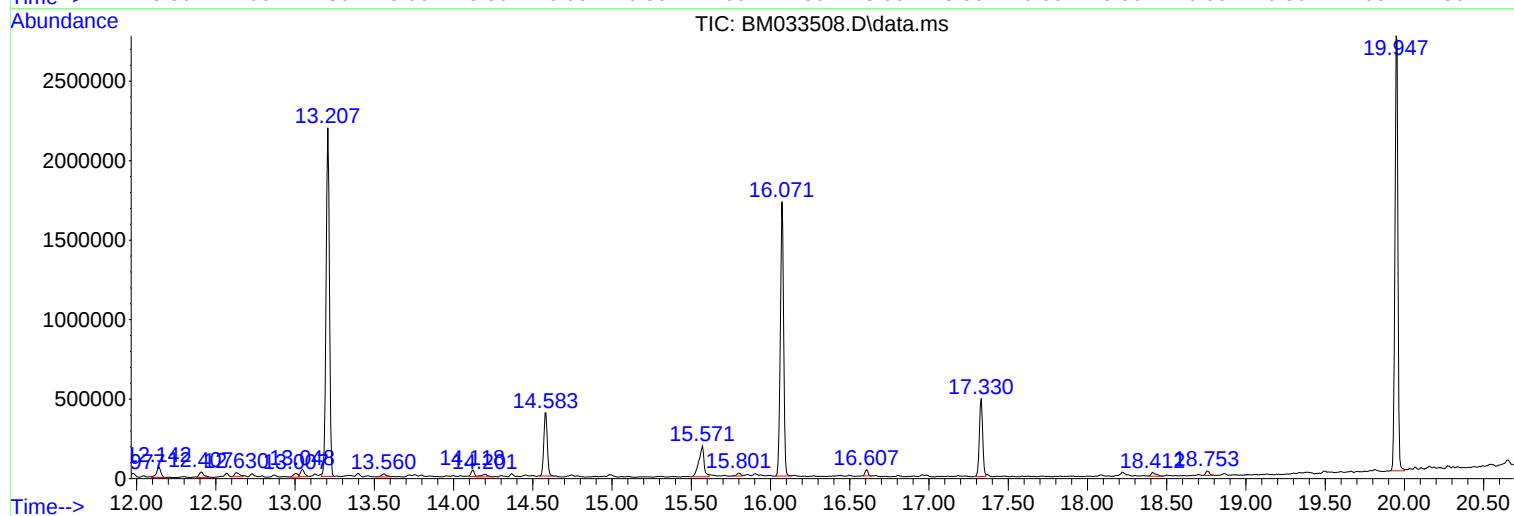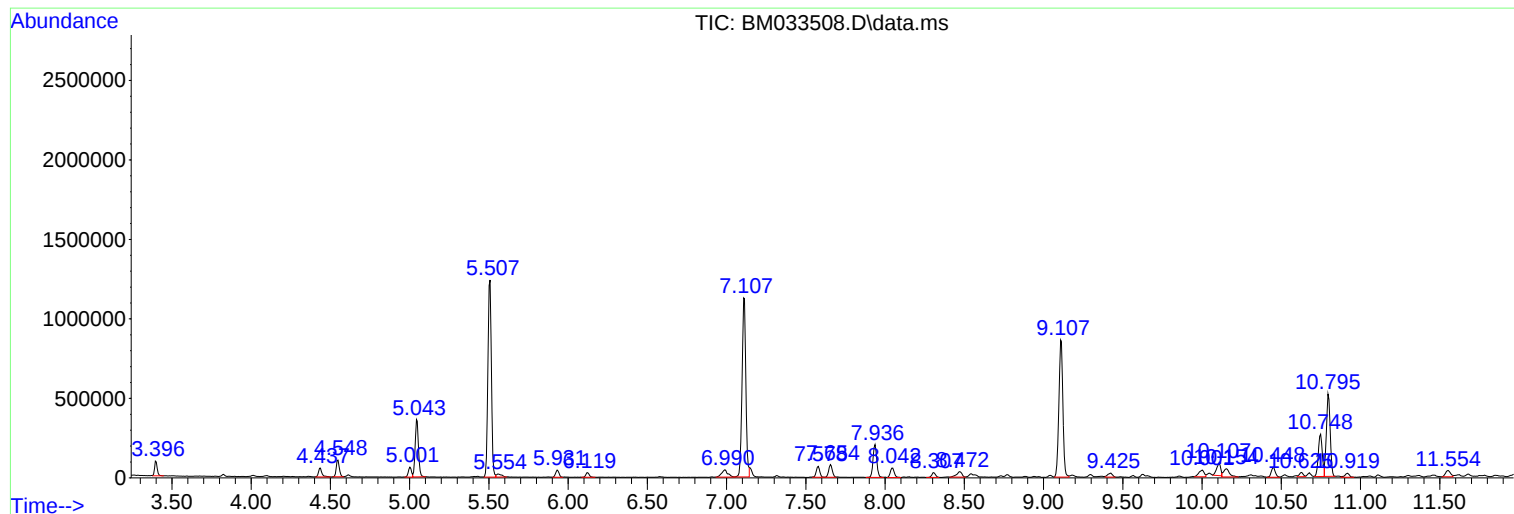

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033508.D
Acq On : 17 Dec 2021 16:28
Operator : CG/JU
Sample : M5051-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121721\
Data File : BM033508.D
Acq On : 17 Dec 2021 16:28
Operator : CG/JU
Sample : M5051-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------