

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121820\
 Data File : BM028165.D
 Acq On : 18 Dec 2020 19:16
 Operator : JU/CG
 Sample : L5068-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A54G5

Quant Time: Dec 19 00:13:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 19 00:05:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	110922	20.00	ng/ul	0.00
18) Naphthalene-d8	11.04	136	440017	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.83	164	248240	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	490166	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	477510	20.00	ng/ul	0.00
86) Perylene-d12	24.03	264	495770	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	10262	3.68	ng/uL	0.00
5) Phenol-d5	7.35	99	192486	20.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	120184	20.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.73	132	164786	20.92	ng/ul	-0.01
13) 4-Methylphenol-d8	8.91	113	155437	20.39	ng/ul	-0.01
19) Nitrobenzene-d5	9.38	128	74237	21.51	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.11	143	80039	22.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	146549	20.61	ng/ul	-0.01
29) 4-Chloroaniline-d4	11.16	131	210309	24.95	ng/ul	-0.01
44) Dimethylphthalate-d6	14.23	166	442807	23.15	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	551549	22.99	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	70099	20.16	ng/ul	0.00
58) Fluorene-d10	15.82	176	371426	21.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.92	200	54093	18.53	ng/ul	0.00
71) Anthracene-d10	17.65	188	567326	23.32	ng/ul	0.00
79) Pyrene-d10	19.91	212	621795	23.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.88	264	646819	23.69	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	7.37	94	21108	2.260	ng/ul 96
45) Dimethylphthalate	14.27	163	80517	4.120	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121820\
Data File : BM028165.D
Acq On : 18 Dec 2020 19:16
Operator : JU/CG
Sample : L5068-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A54G5

Quant Time: Dec 19 00:13:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 19 00:05:02 2020
Response via : Initial Calibration

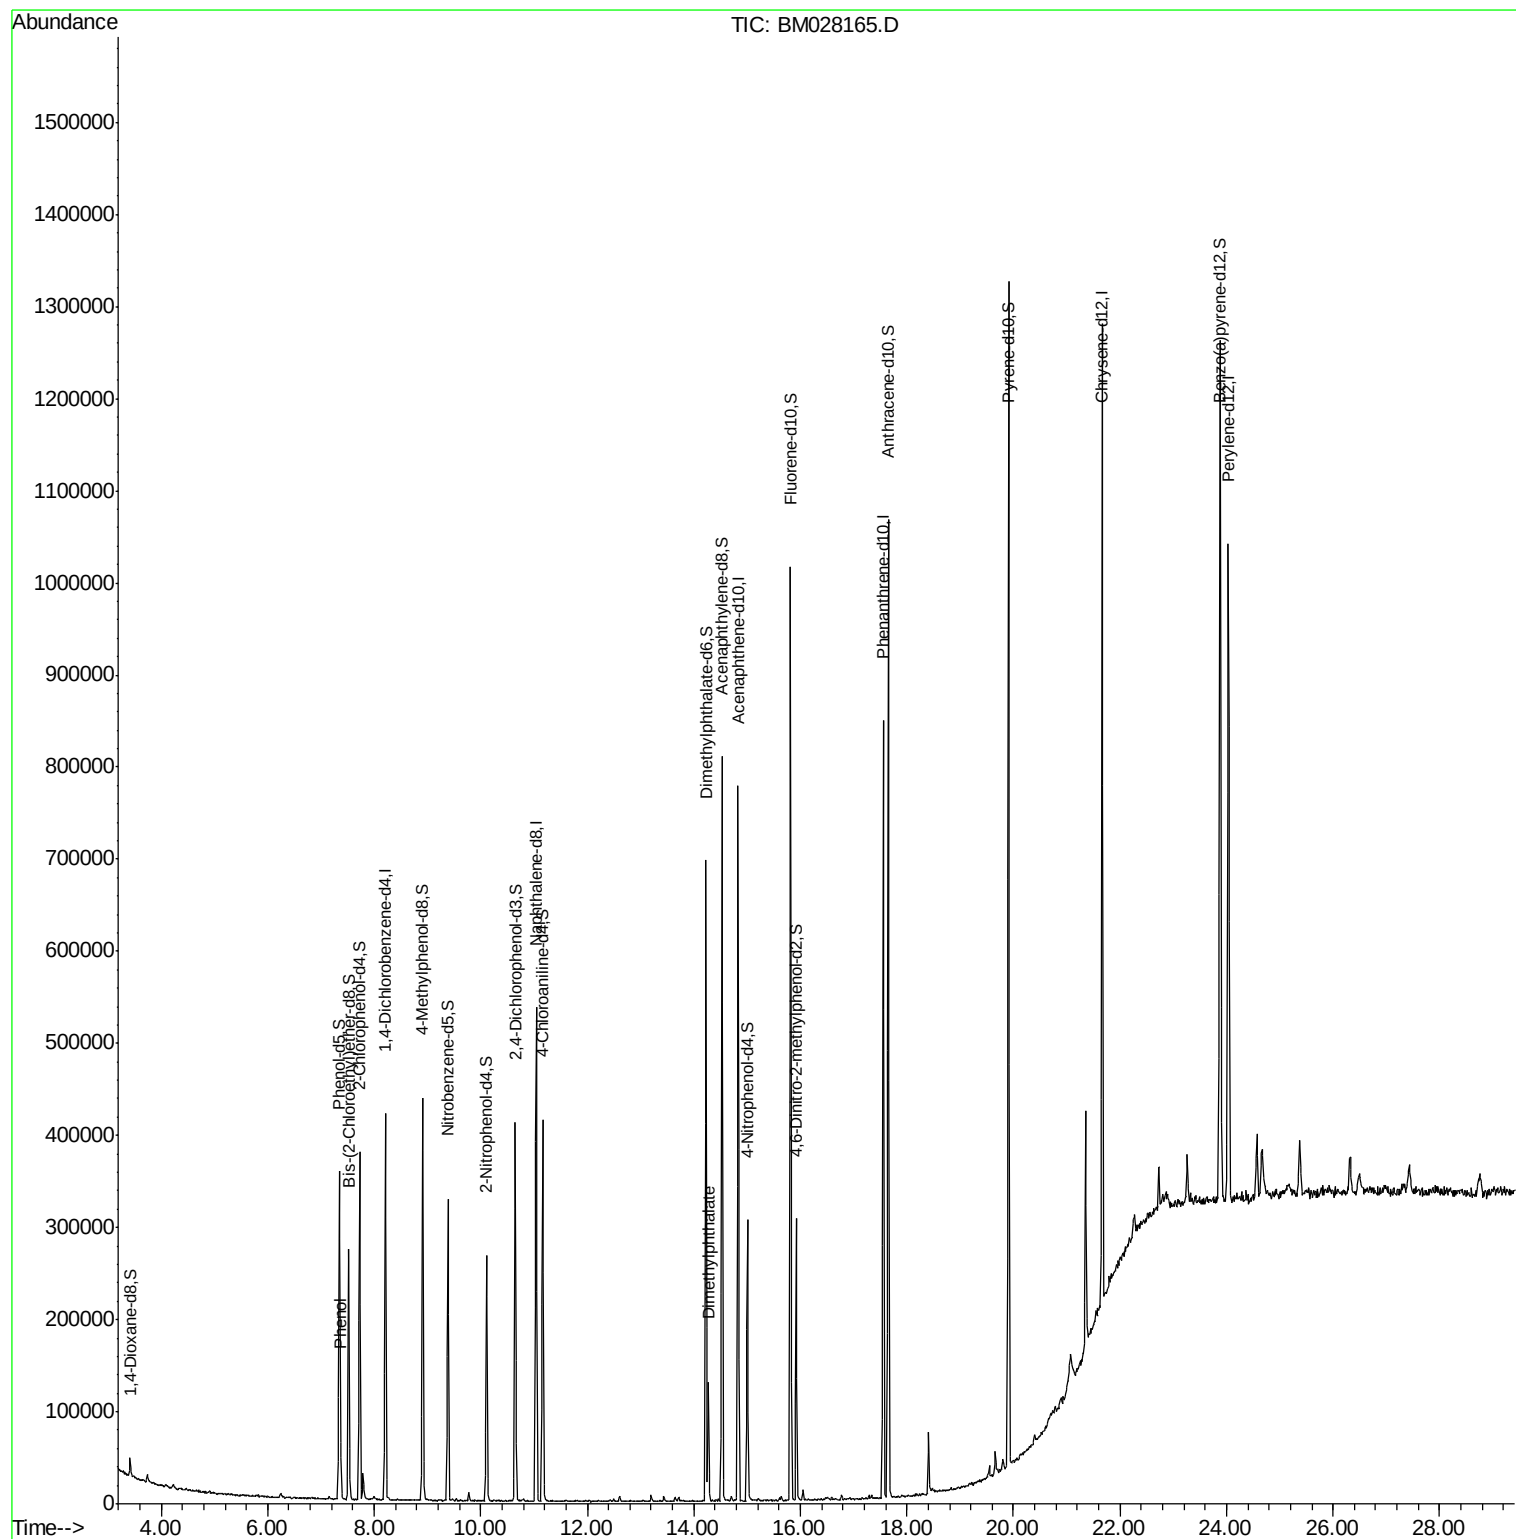

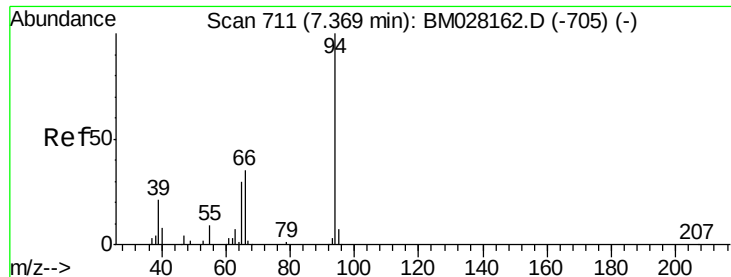





#6

Phenol

Concen: 2.260 ng/ul
 RT: 7.37 min Scan# 711
 Delta R.T. -0.01 min
 Lab File: BM028165.D
 Acq: 18 Dec 2020 19:16

Instrument :
 BNA_M
 ClientSampleId :
 A54G5

Tot Ion	Ratio	Lower	Upper
94	100		
65	30.0	25.4	38.0
66	36.4	31.5	47.3

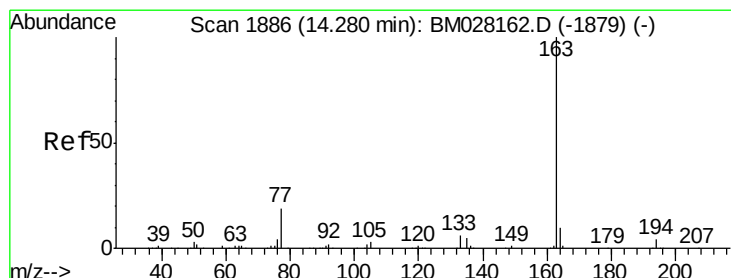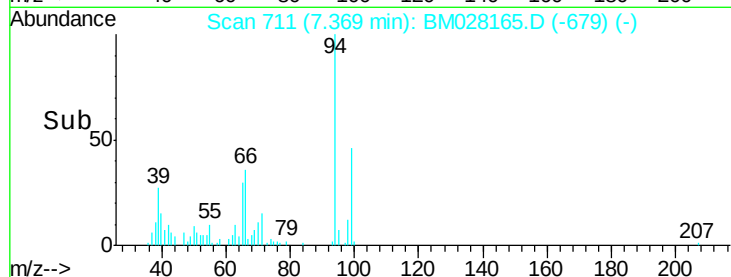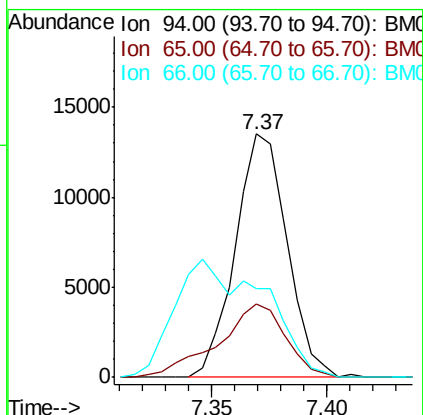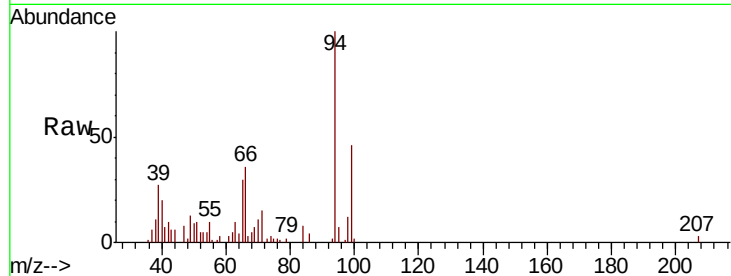

#45

Dimethylphthalate

Concen: 4.120 ng/ul
 RT: 14.27 min Scan# 1885
 Delta R.T. -0.01 min
 Lab File: BM028165.D
 Acq: 18 Dec 2020 19:16

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.3	4.9
164	10.4	8.0	12.0

