

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121820\
 Data File : BM028168.D
 Acq On : 18 Dec 2020 21:05
 Operator : JU/CG
 Sample : L5068-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A54G2

Quant Time: Dec 19 00:14:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 19 00:05:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	105281	20.00	ng/ul	0.00
18) Naphthalene-d8	11.03	136	417827	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.83	164	229943	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.55	188	459175	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	446753	20.00	ng/ul	0.00
86) Perylene-d12	24.03	264	463571	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.42	96	9297	3.51	ng/uL	0.00
5) Phenol-d5	7.35	99	172423	19.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	106669	18.98	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.73	132	147551	19.73	ng/ul	-0.01
13) 4-Methylphenol-d8	8.91	113	134794	18.63	ng/ul	-0.01
19) Nitrobenzene-d5	9.38	128	65782	20.07	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.11	143	70244	21.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	128331	19.00	ng/ul	-0.01
29) 4-Chloroaniline-d4	11.16	131	181438	22.67	ng/ul	-0.01
44) Dimethylphthalate-d6	14.23	166	364439	20.57	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	465291	20.93	ng/ul	0.00
52) 4-Nitrophenol-d4	15.00	143	55728	17.30	ng/ul	0.00
58) Fluorene-d10	15.82	176	312041	19.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.92	200	42525	15.55	ng/ul	0.00
71) Anthracene-d10	17.65	188	467800	20.53	ng/ul	0.00
79) Pyrene-d10	19.91	212	514530	20.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.88	264	536974	21.03	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.37	94	18106	2.042	ng/ul	94
45) Dimethylphthalate	14.27	163	58525	3.233	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121820\
Data File : BM028168.D
Acq On : 18 Dec 2020 21:05
Operator : JU/CG
Sample : L5068-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A54G2

Quant Time: Dec 19 00:14:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 19 00:05:02 2020
Response via : Initial Calibration

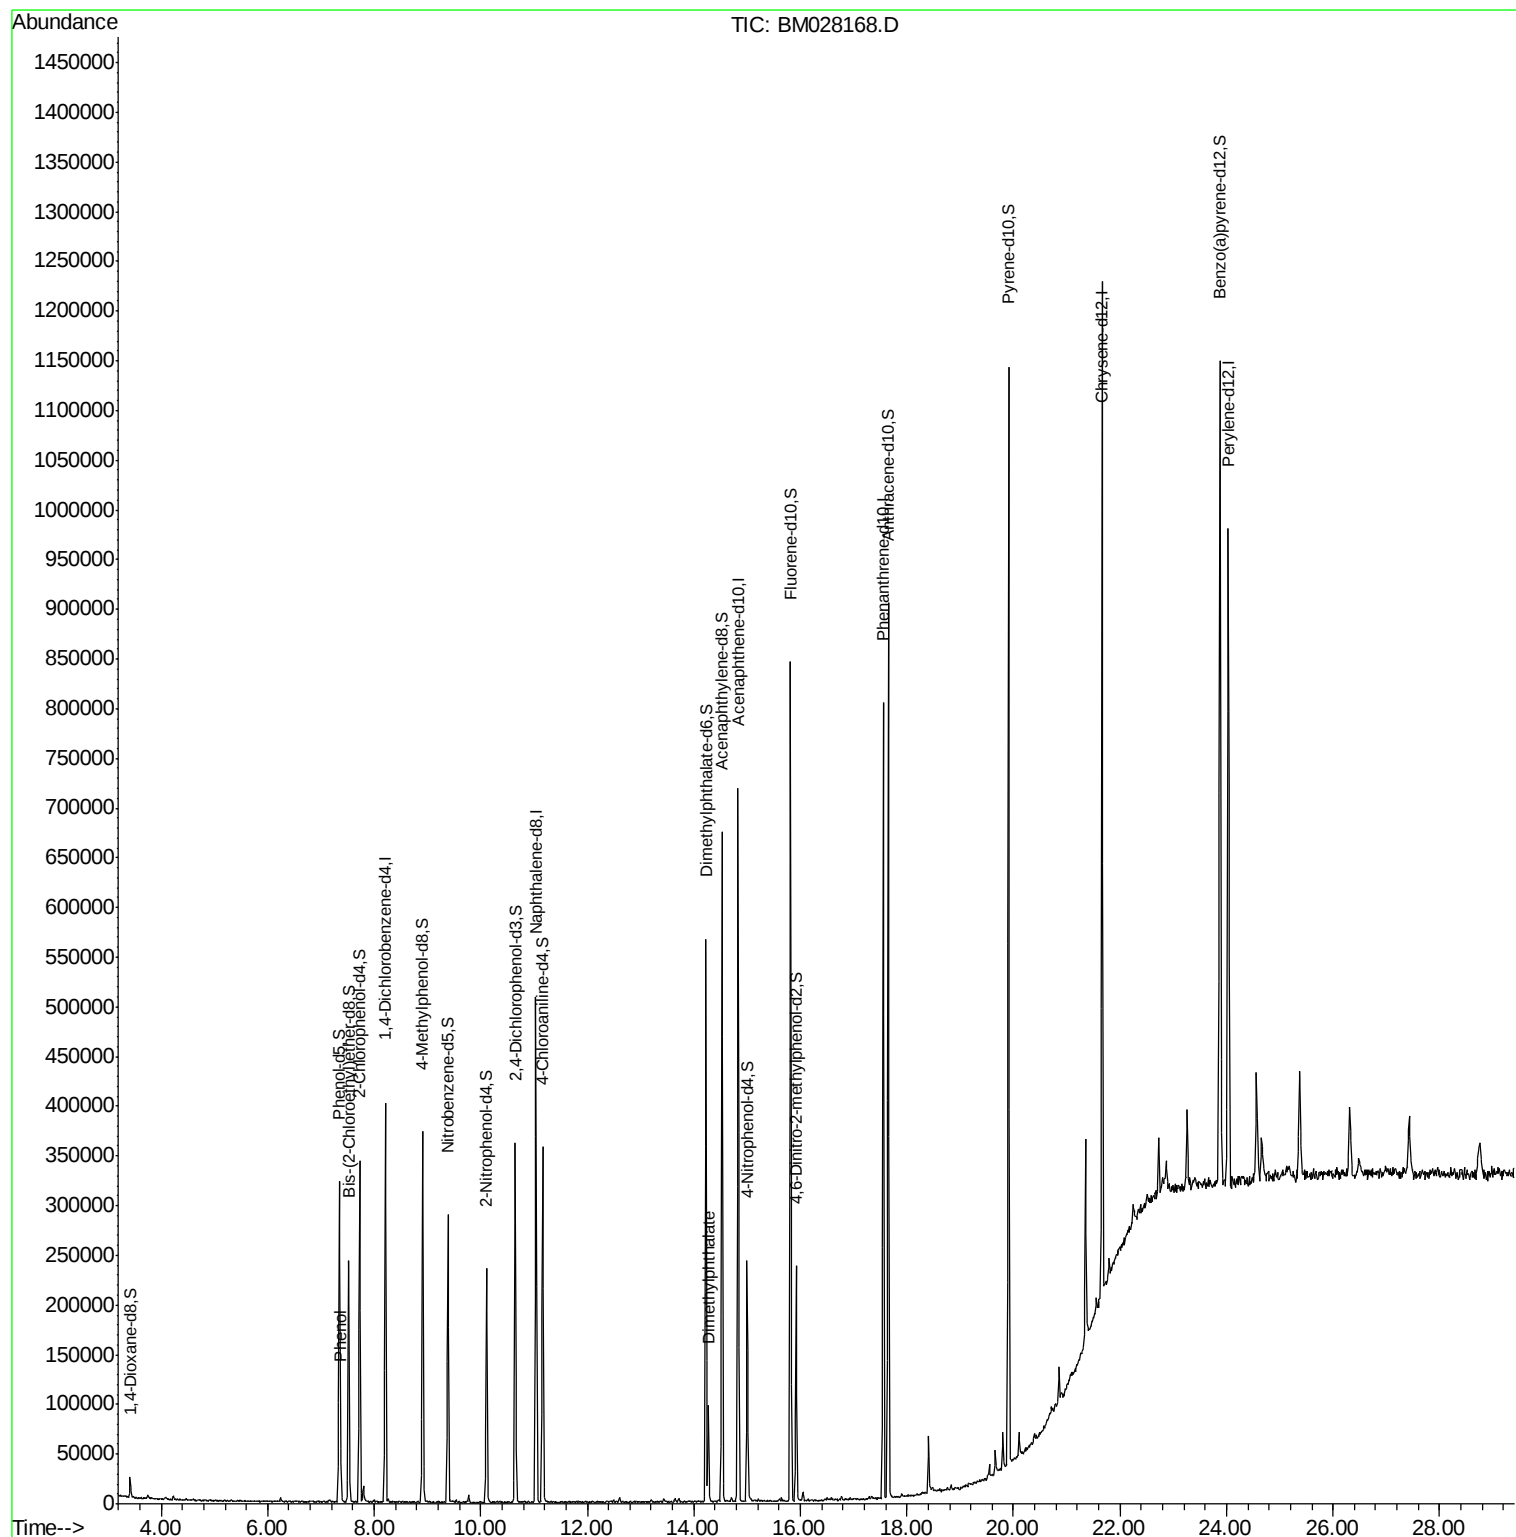

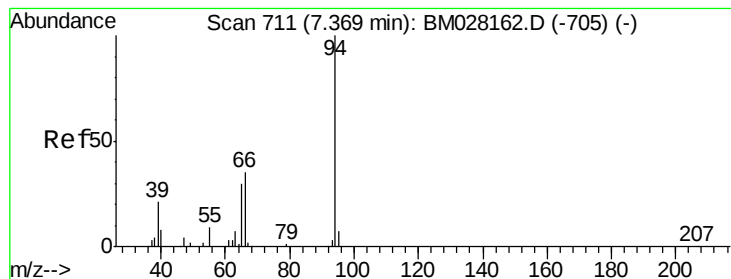

#6

Phenol

Concen: 2.042 ng/ul

RT: 7.37 min Scan# 711

Delta R.T. -0.01 min

Lab File: BM028168.D

Acq: 18 Dec 2020 21:05

Instrument :

BNA_M

ClientSampleId :

A54G2


Tot Ion: 94 Resp: 18106

Ion Ratio Lower Upper

94 100

65 37.2 25.4 38.0




66 41.3 31.5 47.3

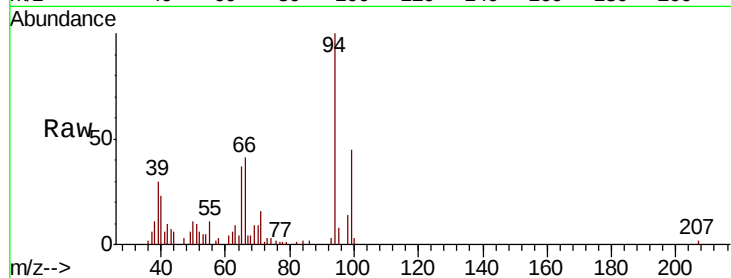

Abundance Ion 94.00 (93.70 to 94.70): BM028168.D (-679) (-)

Ion 65.00 (64.70 to 65.70): BM028168.D (-679) (-)

Ion 66.00 (65.70 to 66.70): BM028168.D (-679) (-)

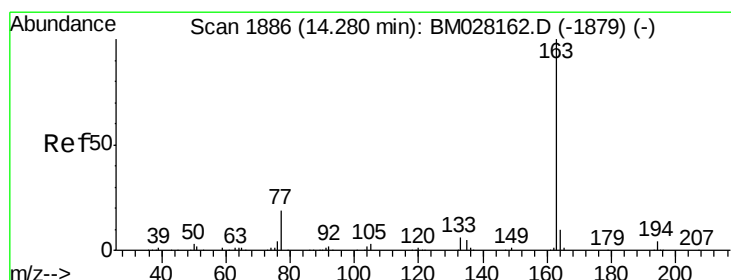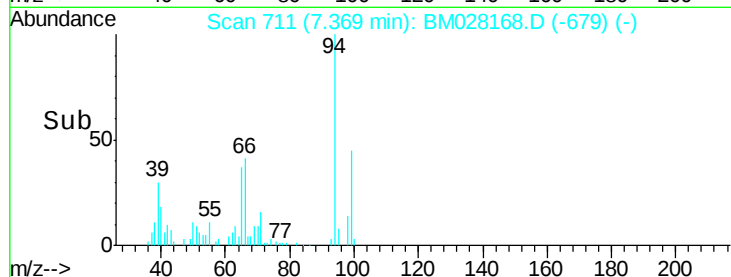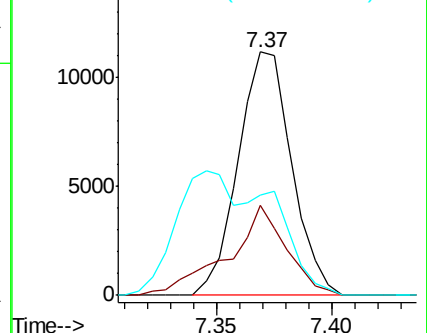

#45

Dimethylphthalate

Concen: 3.233 ng/ul

RT: 14.27 min Scan# 1885

Delta R.T. -0.01 min

Lab File: BM028168.D

Acq: 18 Dec 2020 21:05


Tgt Ion: 163 Resp: 58525

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.2 8.0 12.0

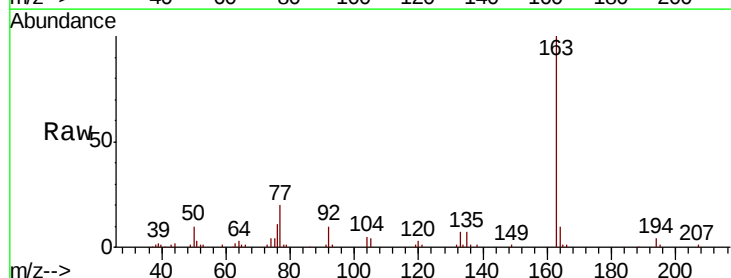

Abundance Ion 163.00 (162.70 to 163.70): BM028168.D (-1853) (-)

Ion 194.00 (193.70 to 194.70): BM028168.D (-1853) (-)

Ion 164.00 (163.70 to 164.70): BM028168.D (-1853) (-)

