
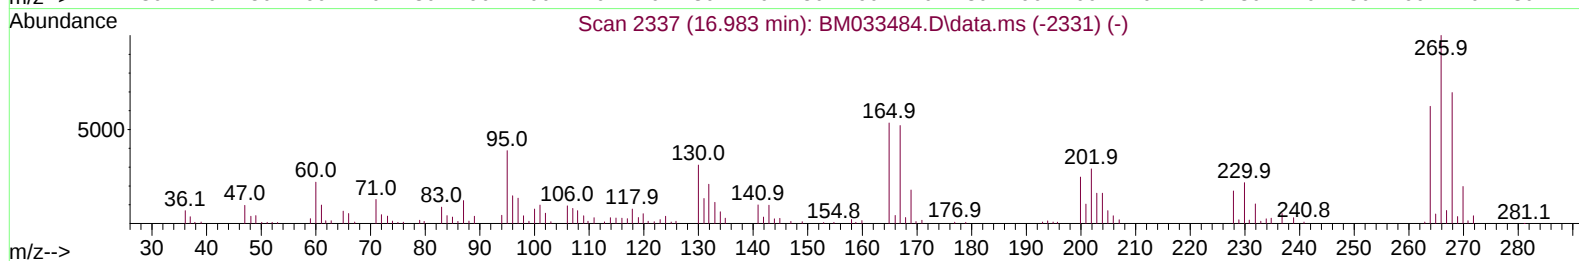
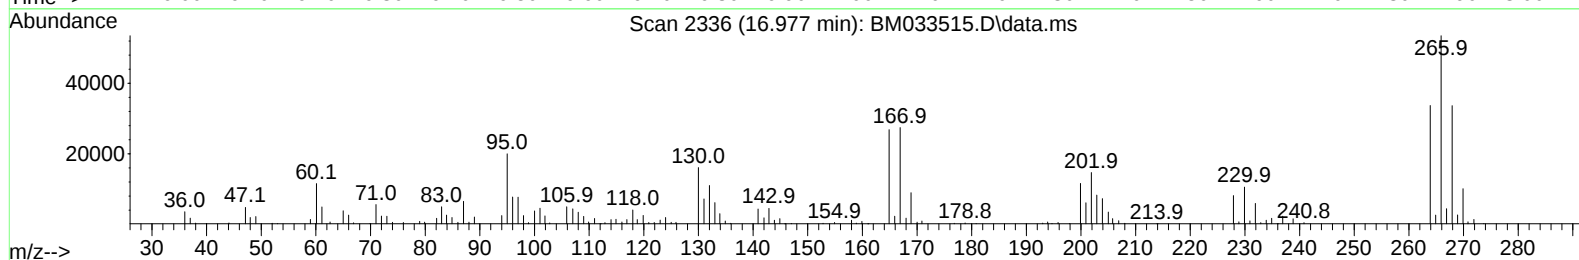


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121821\
Data File : BM033515.D
Acq On : 18 Dec 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 10:54:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

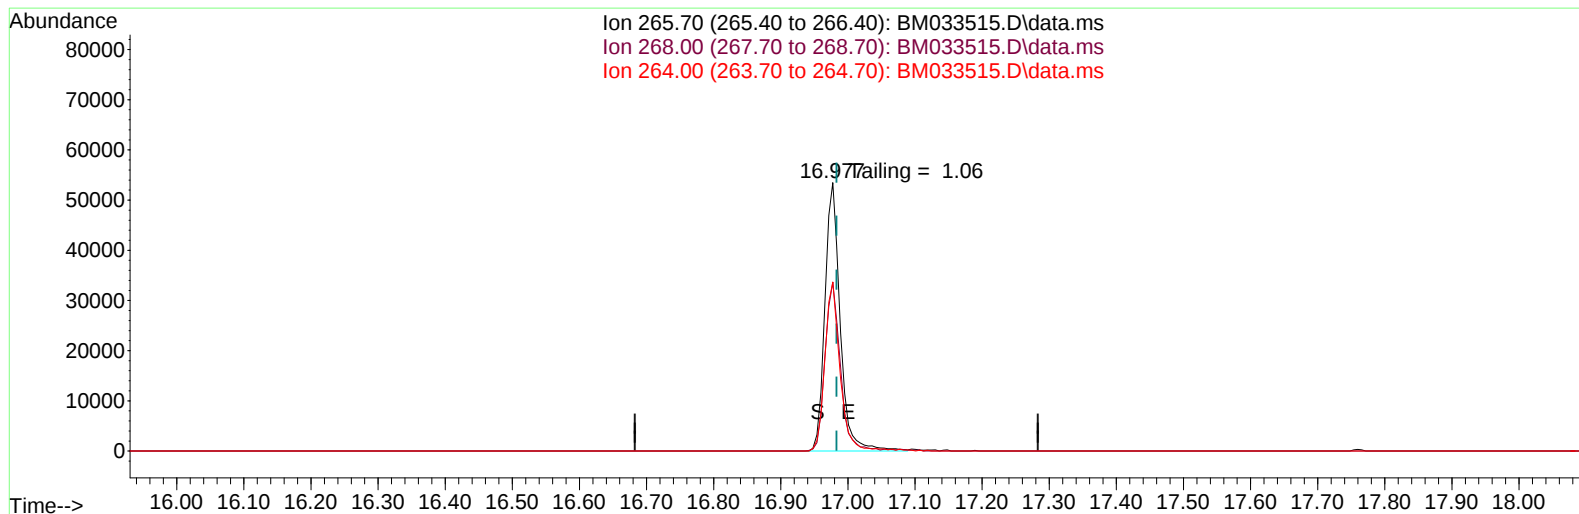

TIC: BM033515.D\data.ms

(70) Pentachlorophenol (C)


16.977min (-0.006) 0.00 ng

response 84801

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.92
264.00	61.40	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121821\
Data File : BM033515.D
Acq On : 18 Dec 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 10:54:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

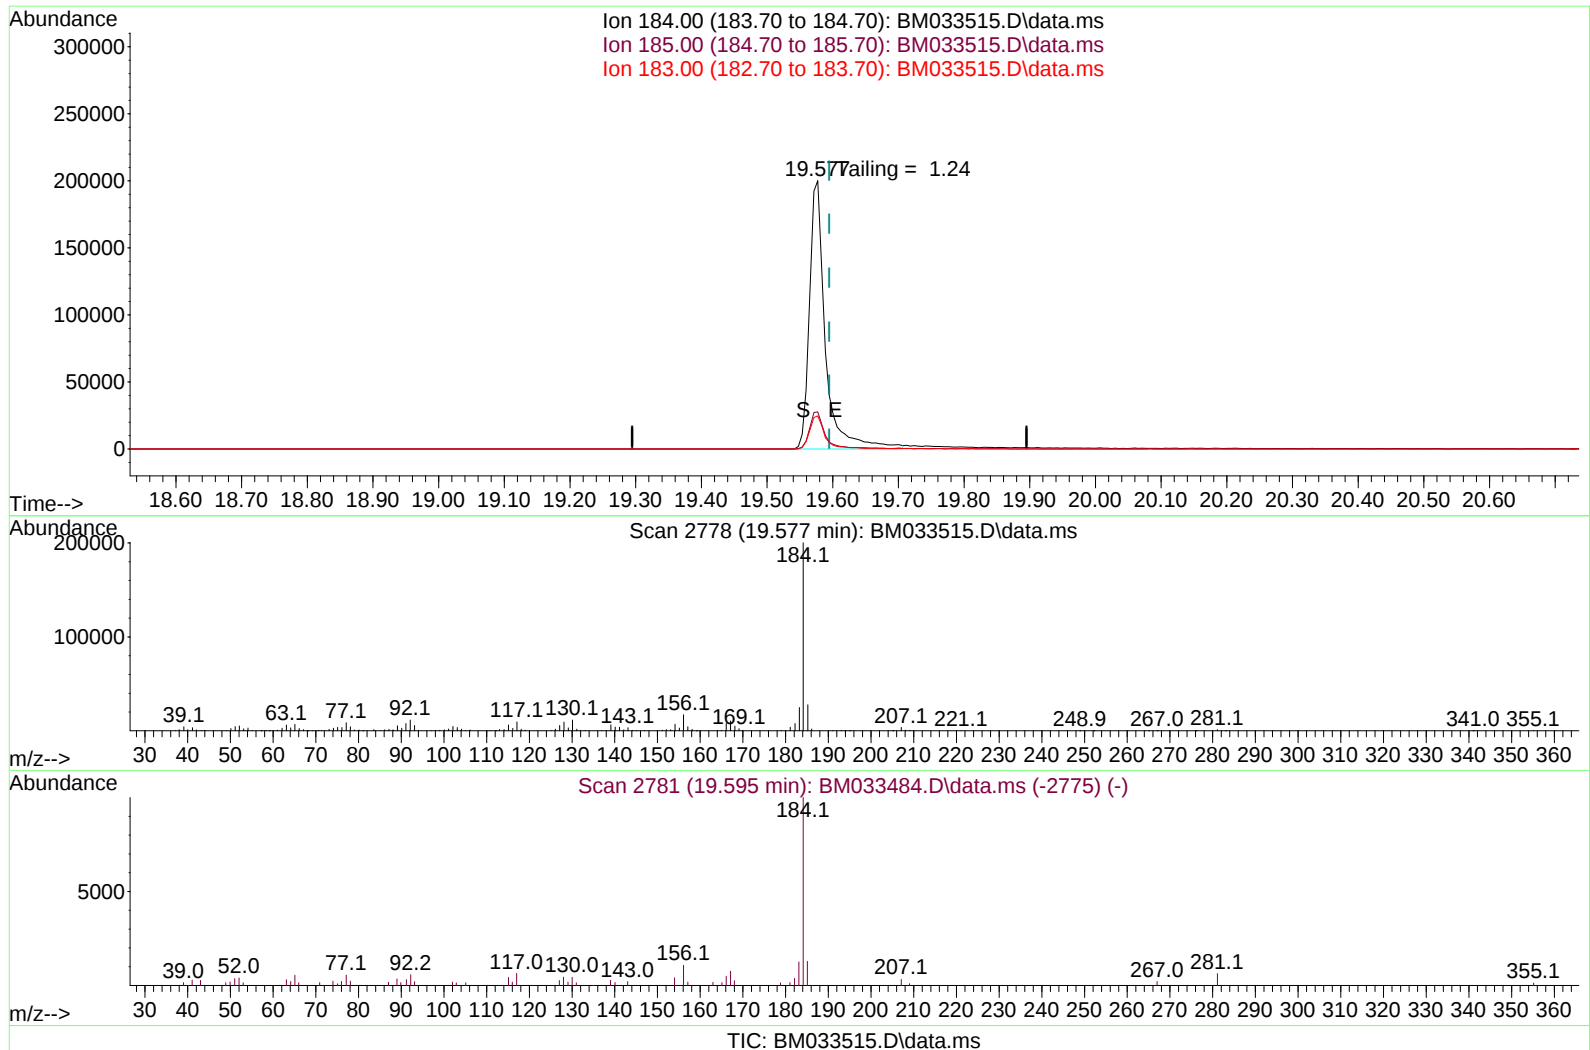**(77) Benzidine****19.577min (-0.018) 569987.96 ng****response 341131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.83
183.00	12.10	12.38
0.00	0.00	0.00