


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121821\
 Data File : BM033515.D
 Acq On : 18 Dec 2021 11:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 16 17:10:15 2021

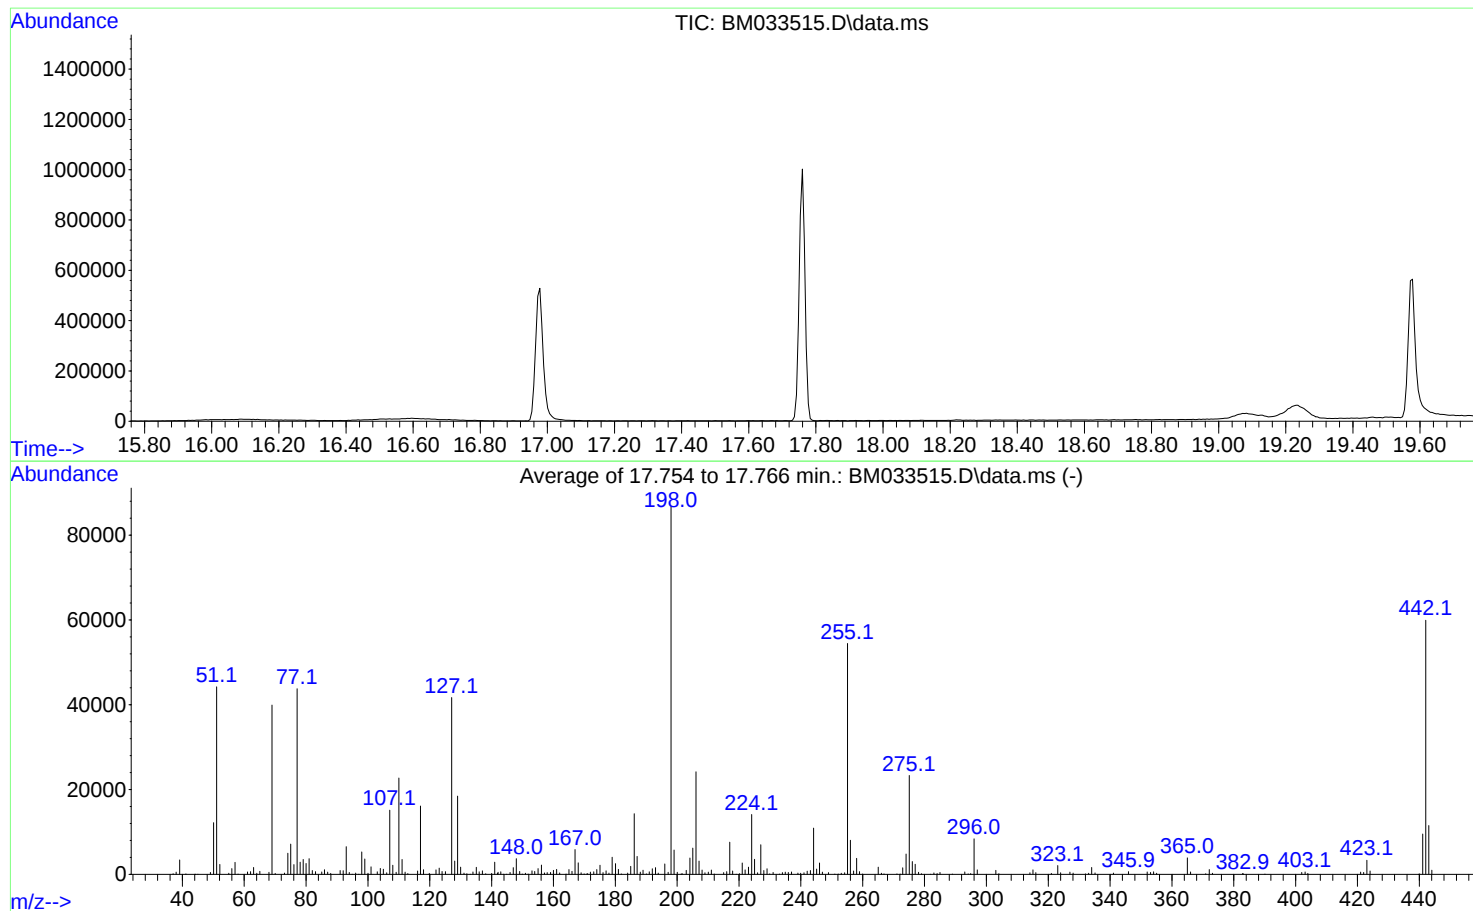




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	44232	PASS
68	69	0.00	2	1.2	479	PASS
69	198	0.00	100	46.0	39944	PASS
70	69	0.00	2	0.6	234	PASS
127	198	10	80	48.0	41685	PASS
197	198	0.00	2	0.6	492	PASS
198	198	100	100	100.0	86763	PASS
199	198	5	9	6.6	5736	PASS
275	198	10	60	26.9	23333	PASS
365	198	1	100	4.5	3898	PASS
441	198	0.01	100	11.0	9502	PASS
442	442	50	100	100.0	59949	PASS
443	442	15	24	19.2	11524	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121821\
Data File : BM033515.D
Acq On : 18 Dec 2021 11:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 20 10:54:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 17:10:15 2021
Response via : Initial Calibration

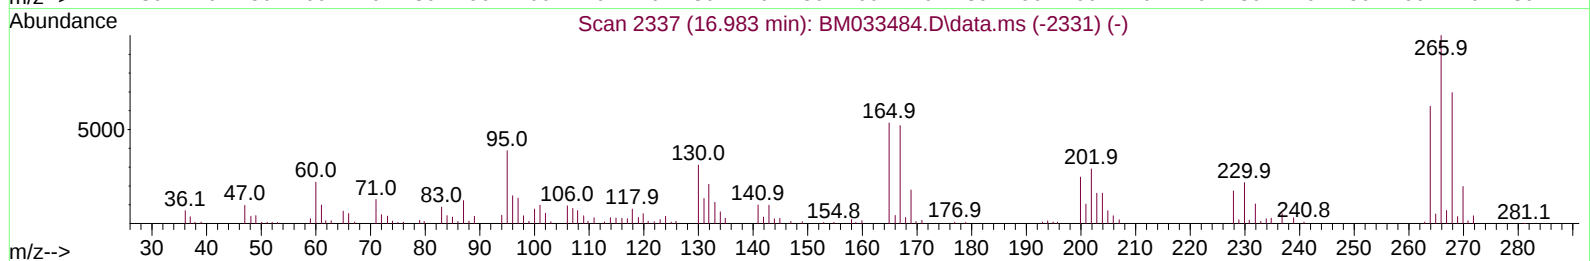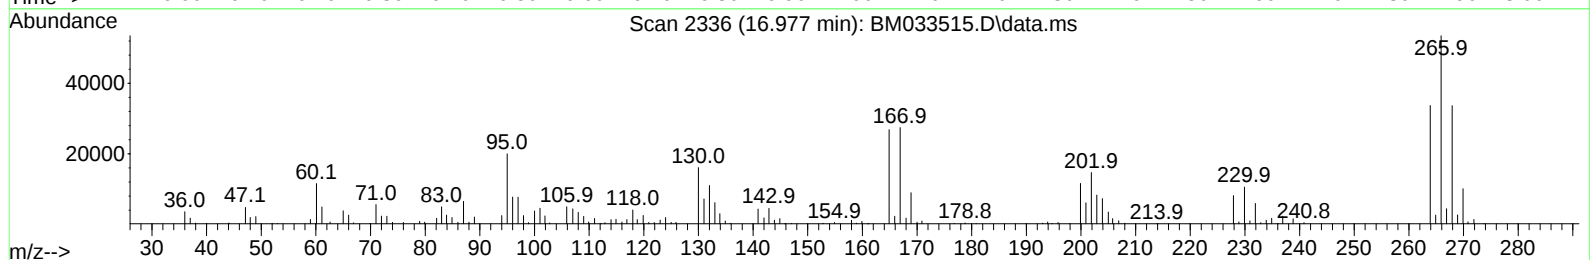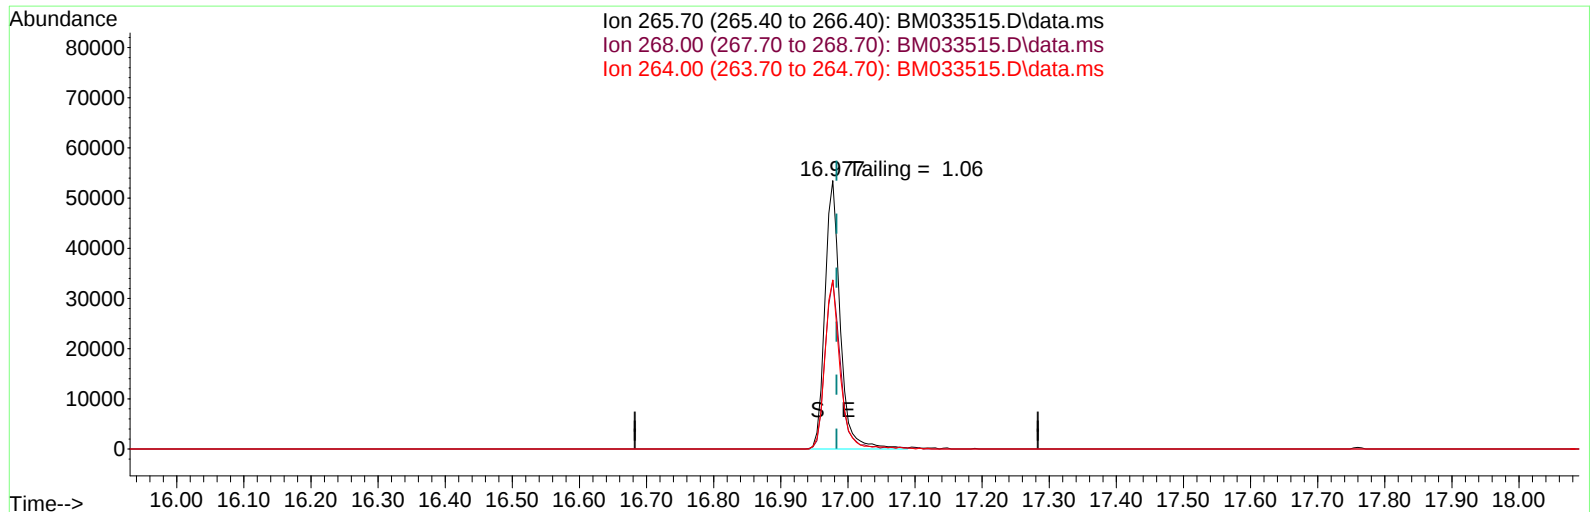

TIC: BM033515.D\data.ms

(70) Pentachlorophenol (C)

16.977min (-0.006) 0.00 ng


response 84801

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.92
264.00	61.40	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121821\
 Data File : BM033515.D
 Acq On : 18 Dec 2021 11:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 10:54:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 17:10:15 2021
 Response via : Initial Calibration

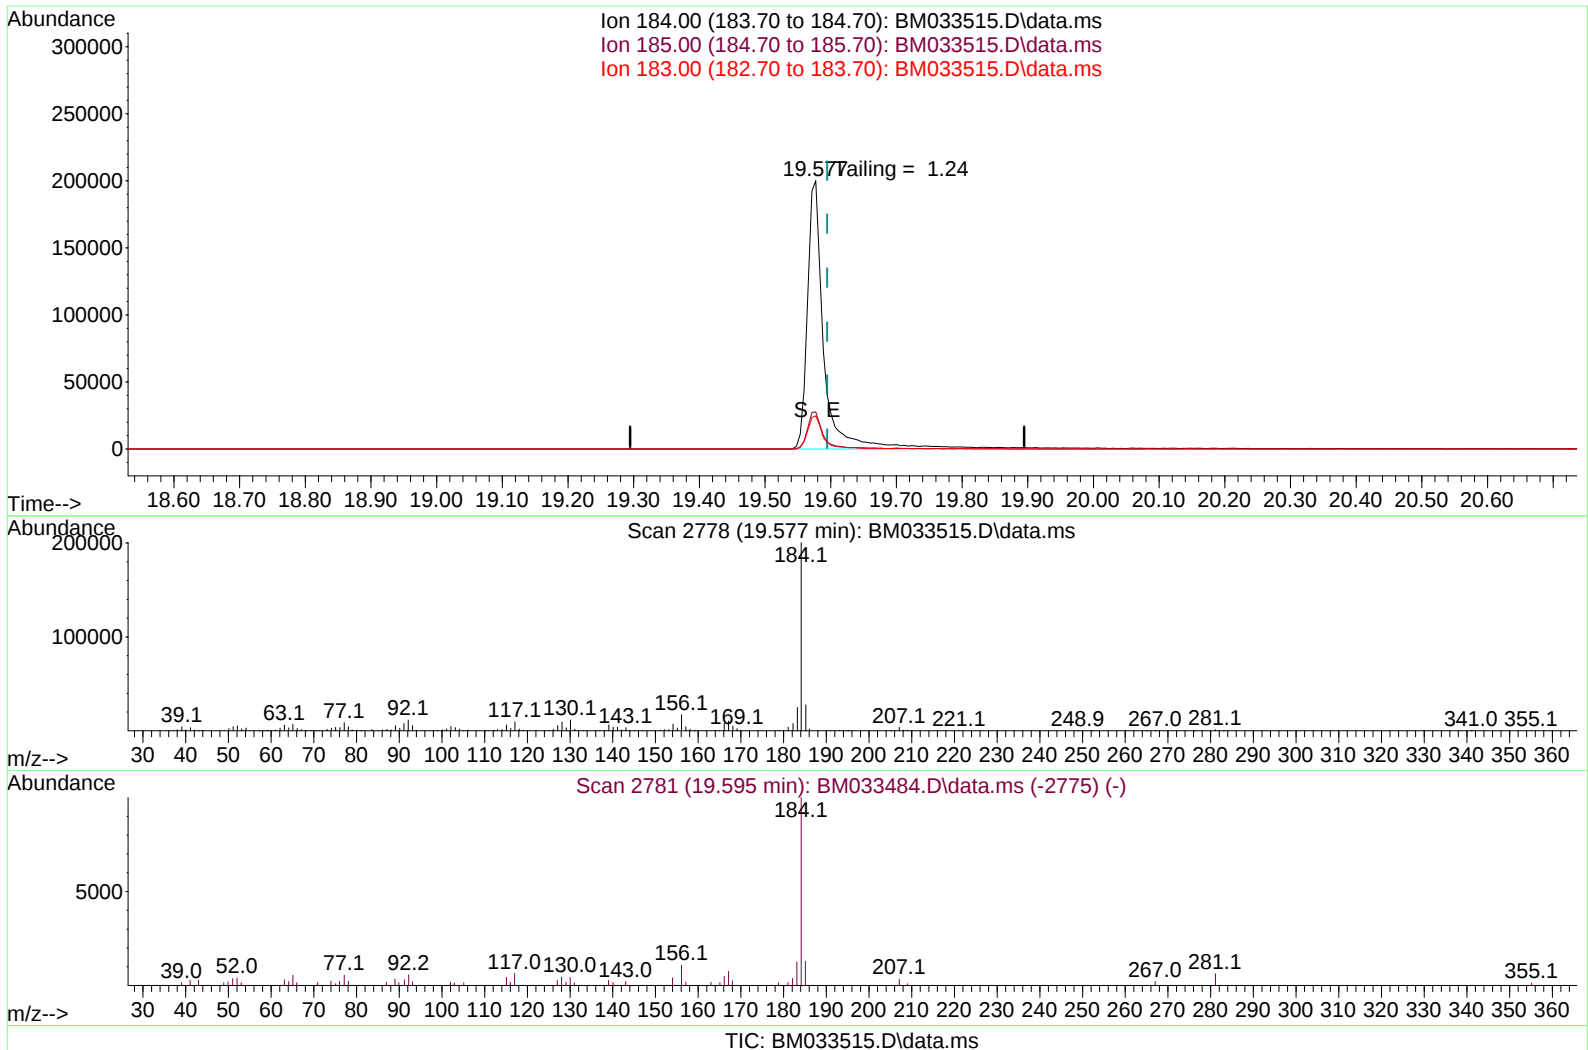

TIC: BM033515.D\data.ms

(77) Benzidine**19.577min (-0.018) 569987.96 ng****response 341131**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.83
183.00	12.10	12.38
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/18/2021	BNA_M	<u>BM033515.D</u>
Compound Name	Response	Retention Time
DDT	291381	20.795
DDD	6771	20.36
DDE	618	19.854
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7389	298770	2.47