
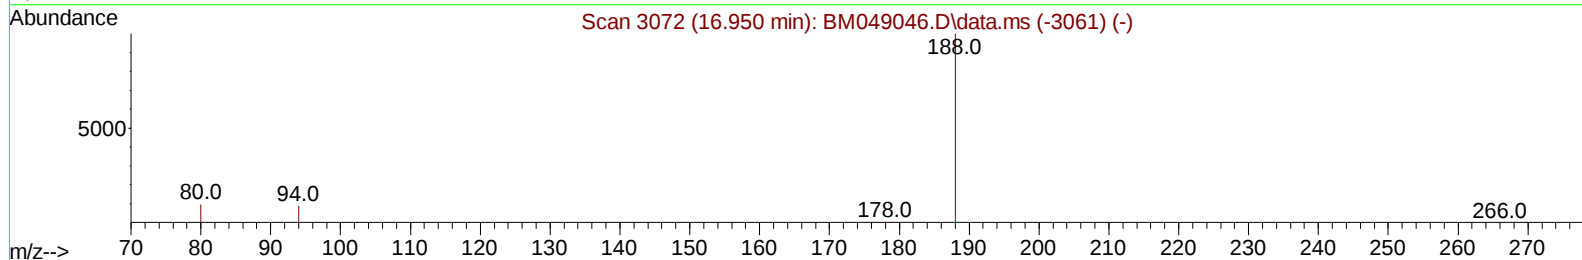
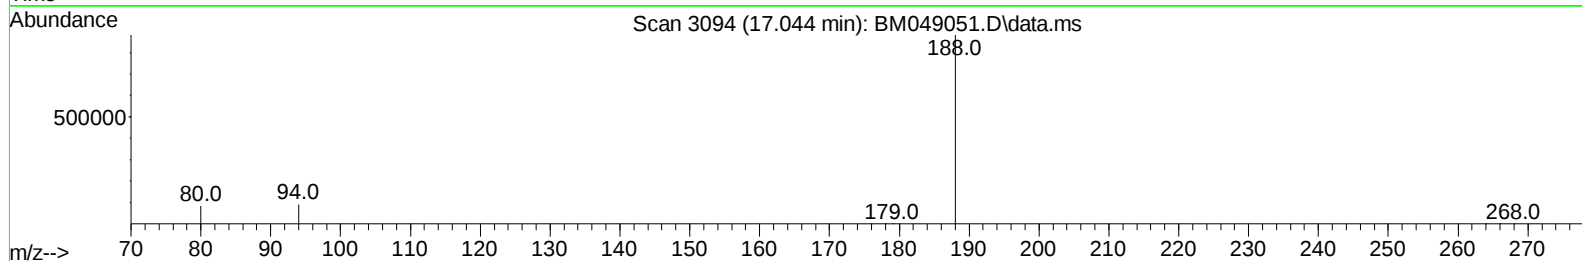


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

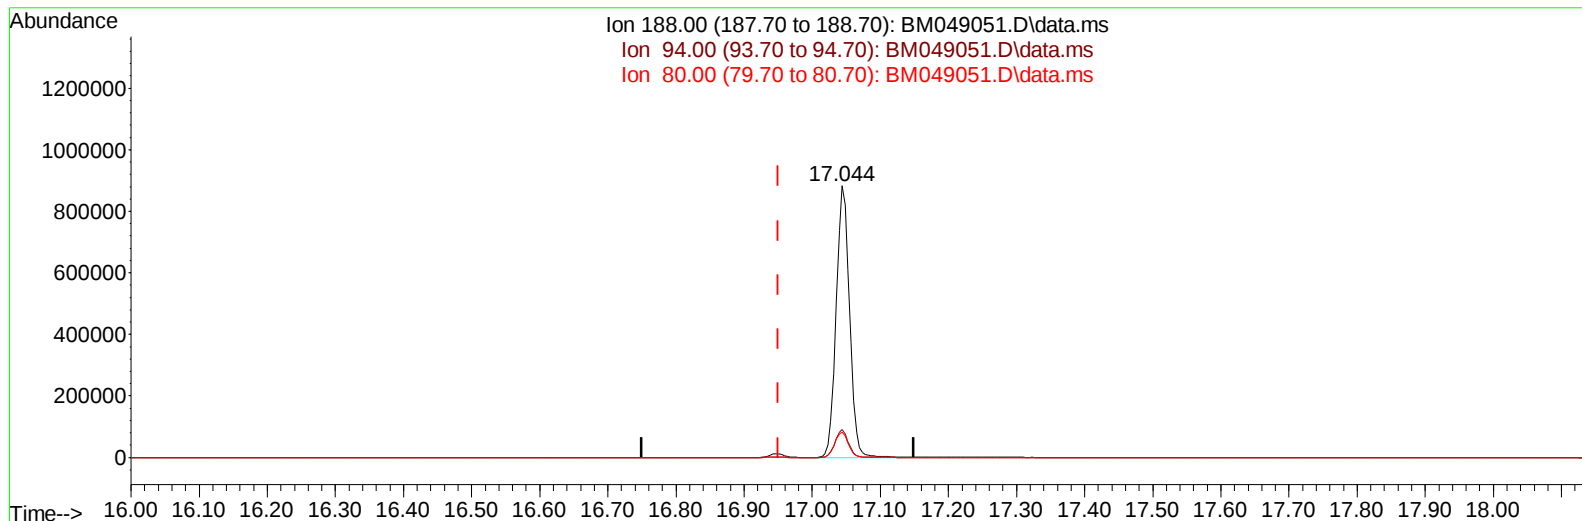

TIC: BM049051.D\data.ms

(13) Phenanthrene-d10 (I)




17.044min (+ 0.094) 0.40 ng/ul

response 1200910

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	10.26
80.00	10.70	9.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

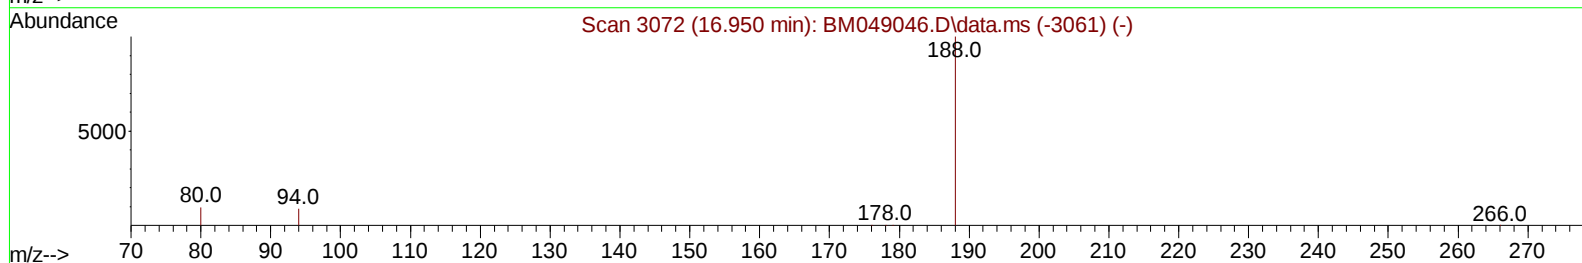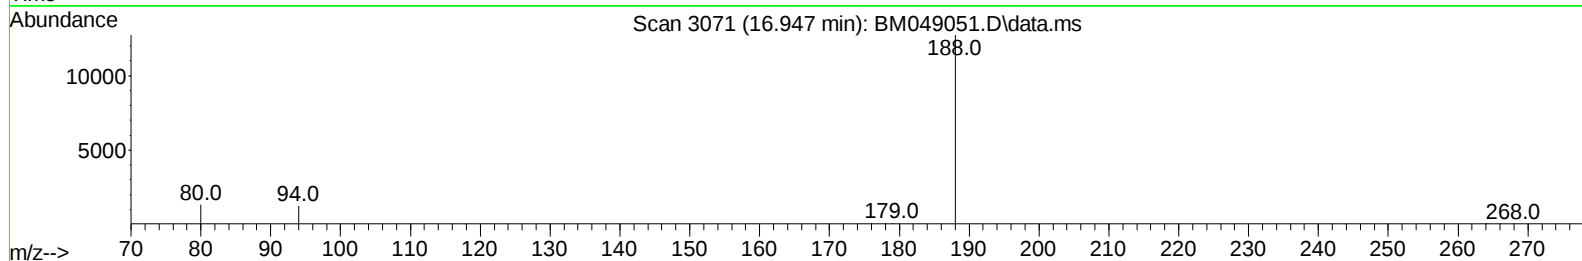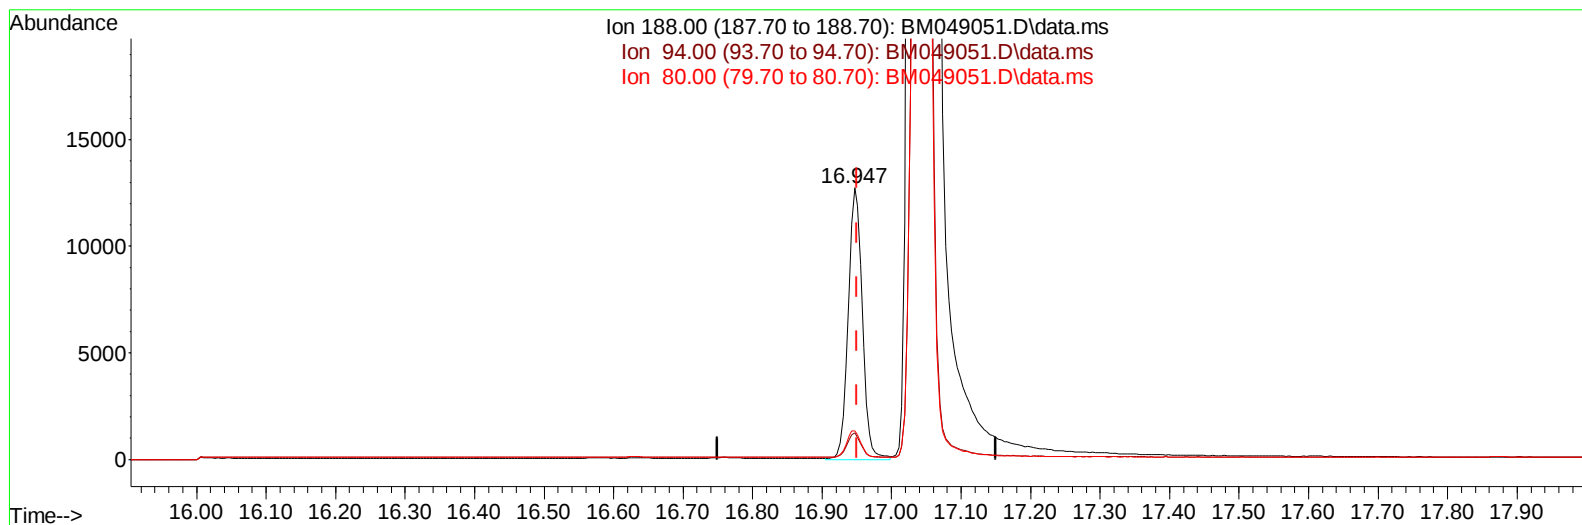

TIC: BM049051.D\data.ms

(13) Phenanthrene-d10 (I)




16.947min (-0.003) 0.40 ng/ul m

response 17983

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.85
80.00	10.70	10.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

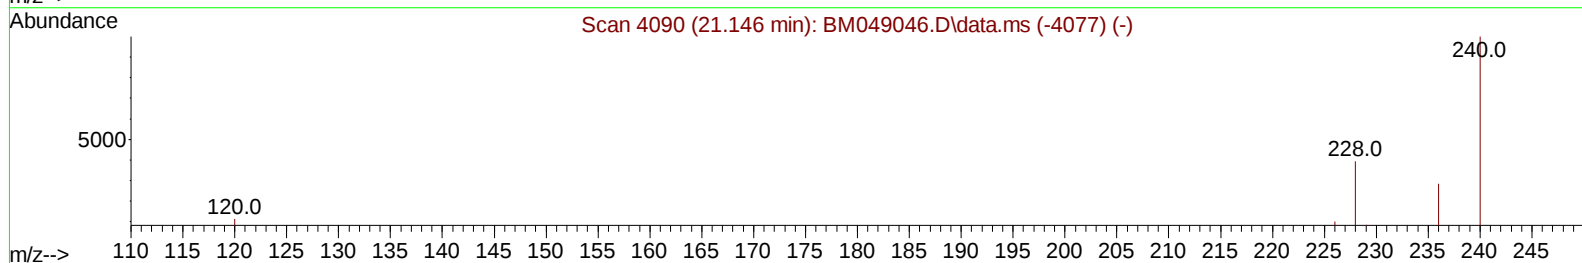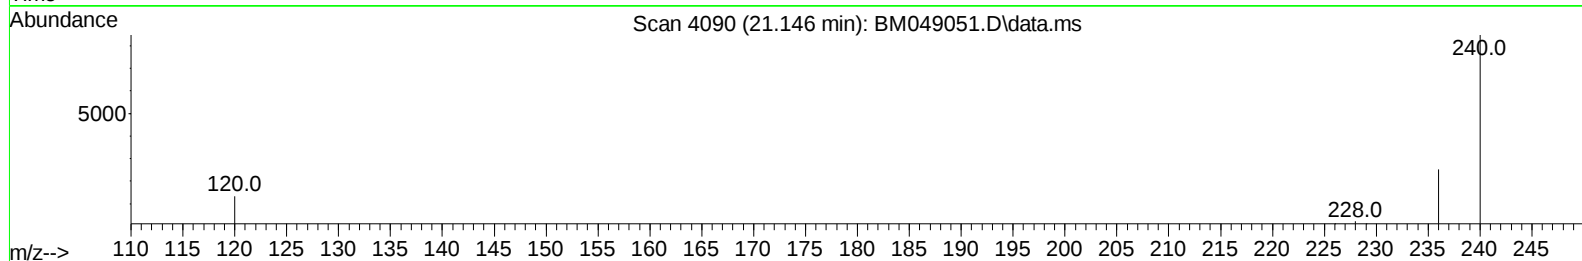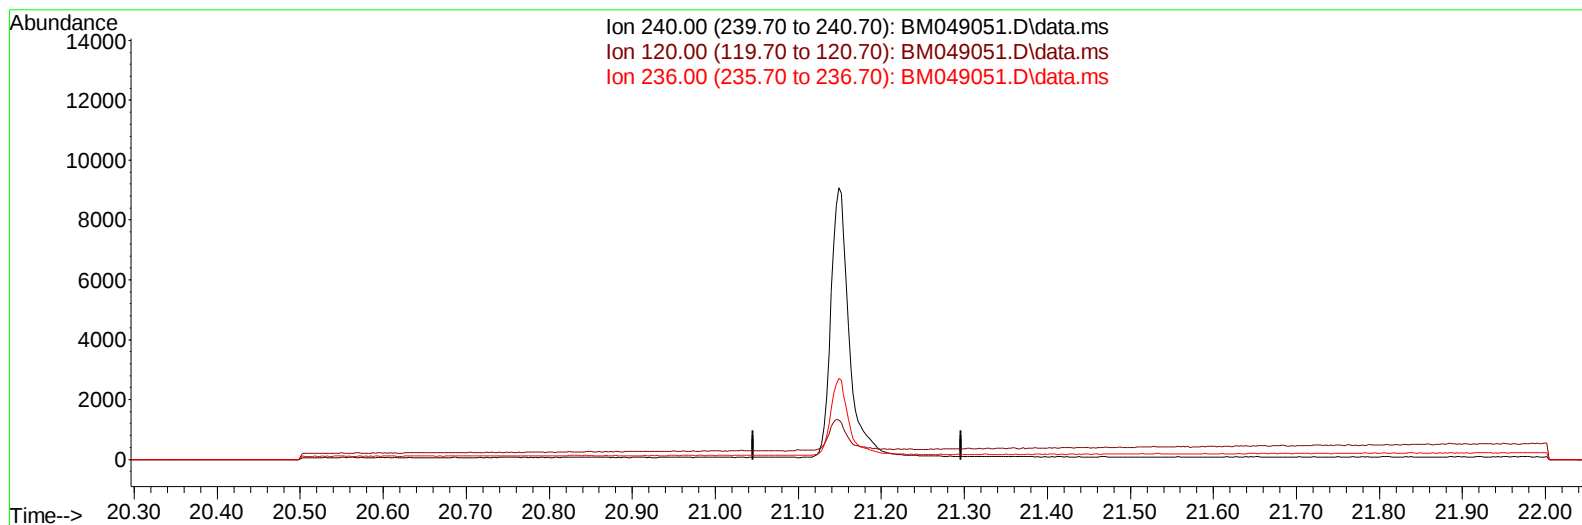

TIC: BM049051.D\data.ms

(17) Chrysene-d12




21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

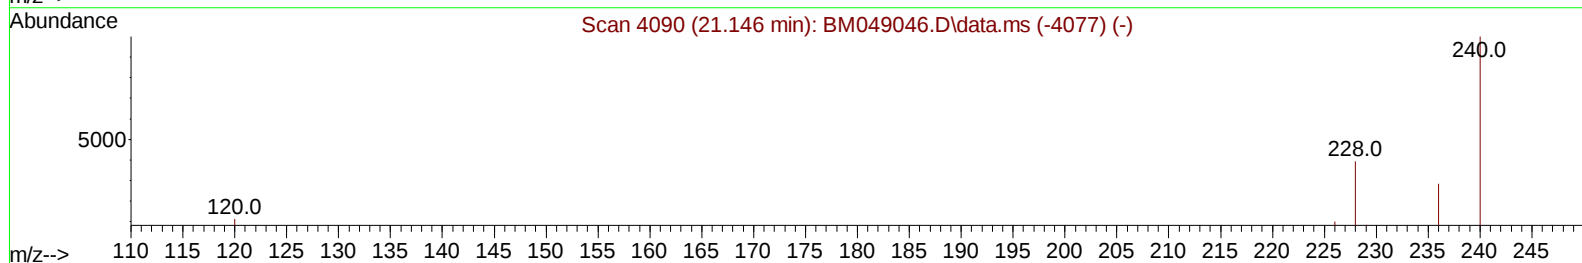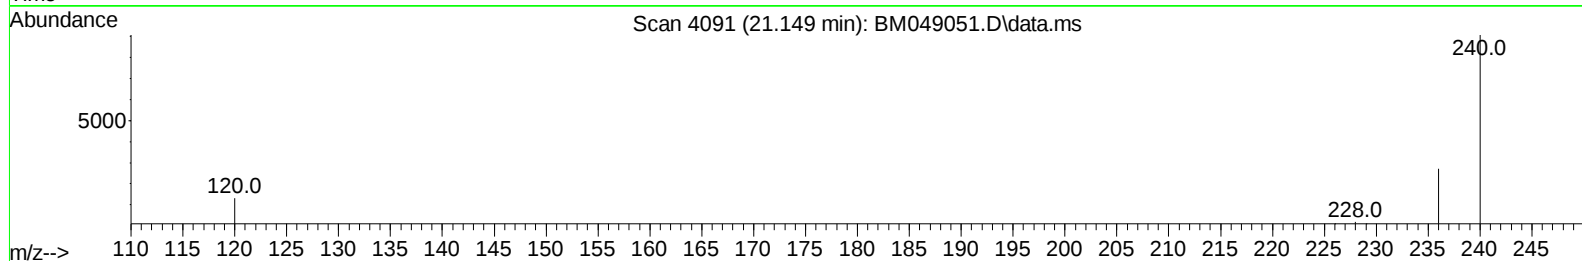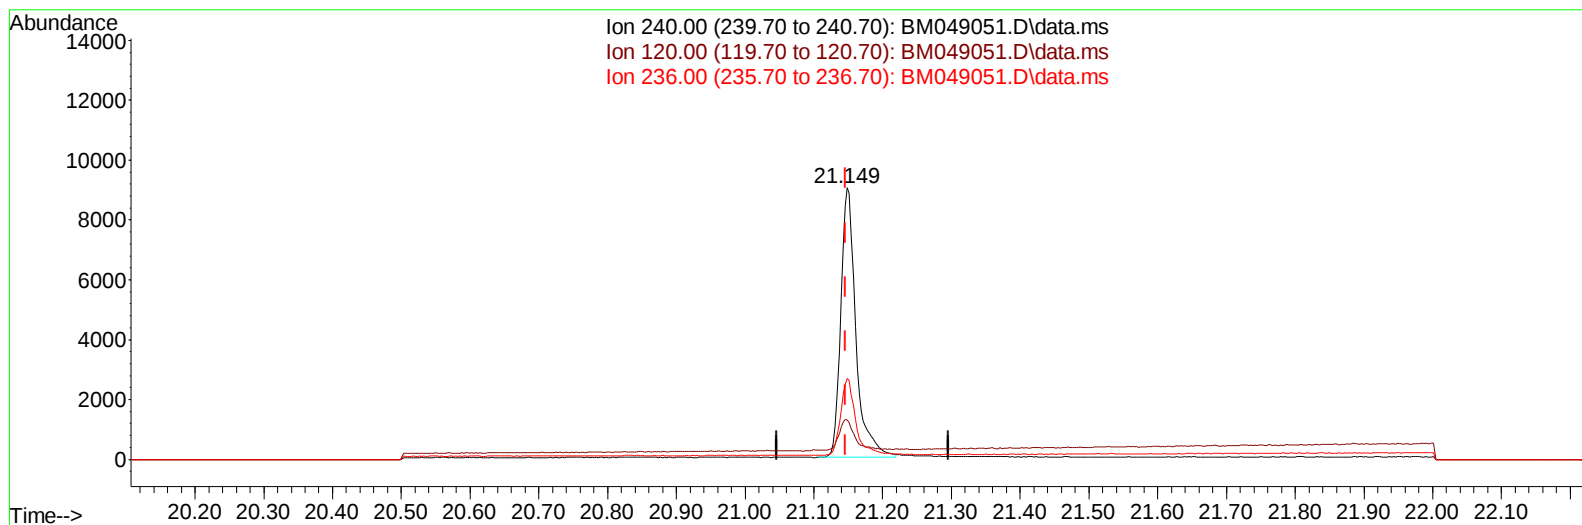

TIC: BM049051.D\data.ms

(17) Chrysene-d12




21.149min (+ 0.002) 0.40 ng/ul m

response 13729

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	14.54
236.00	29.80	29.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

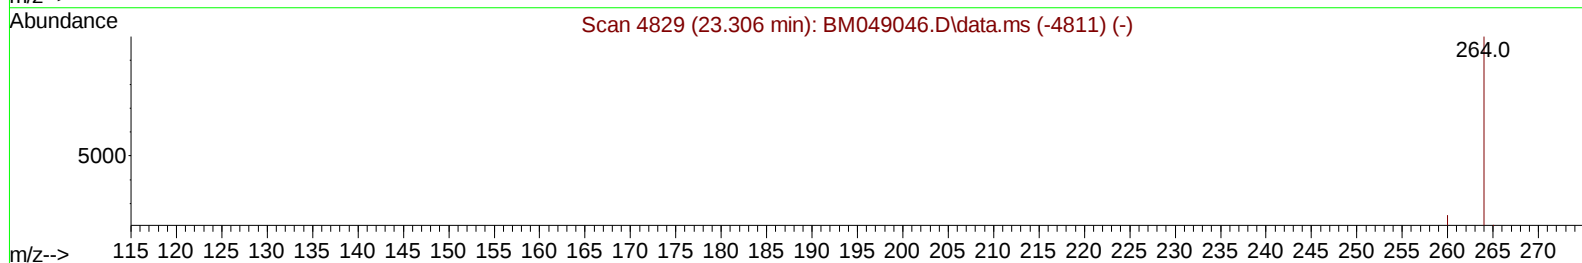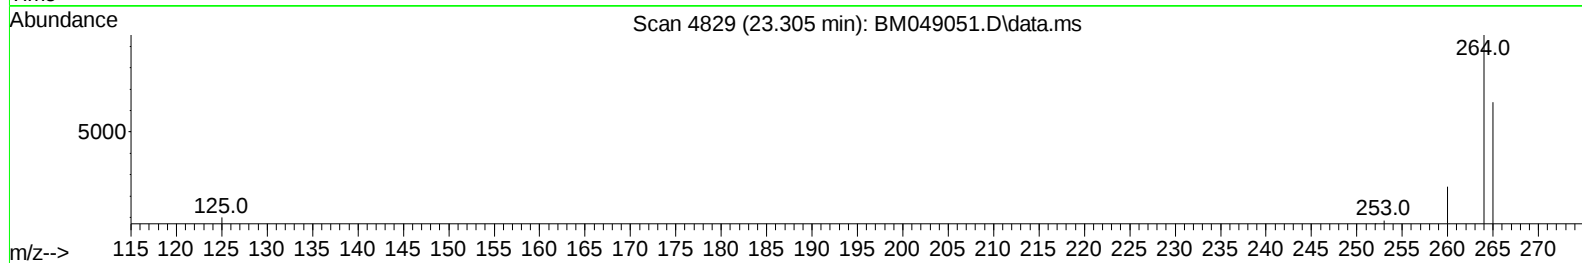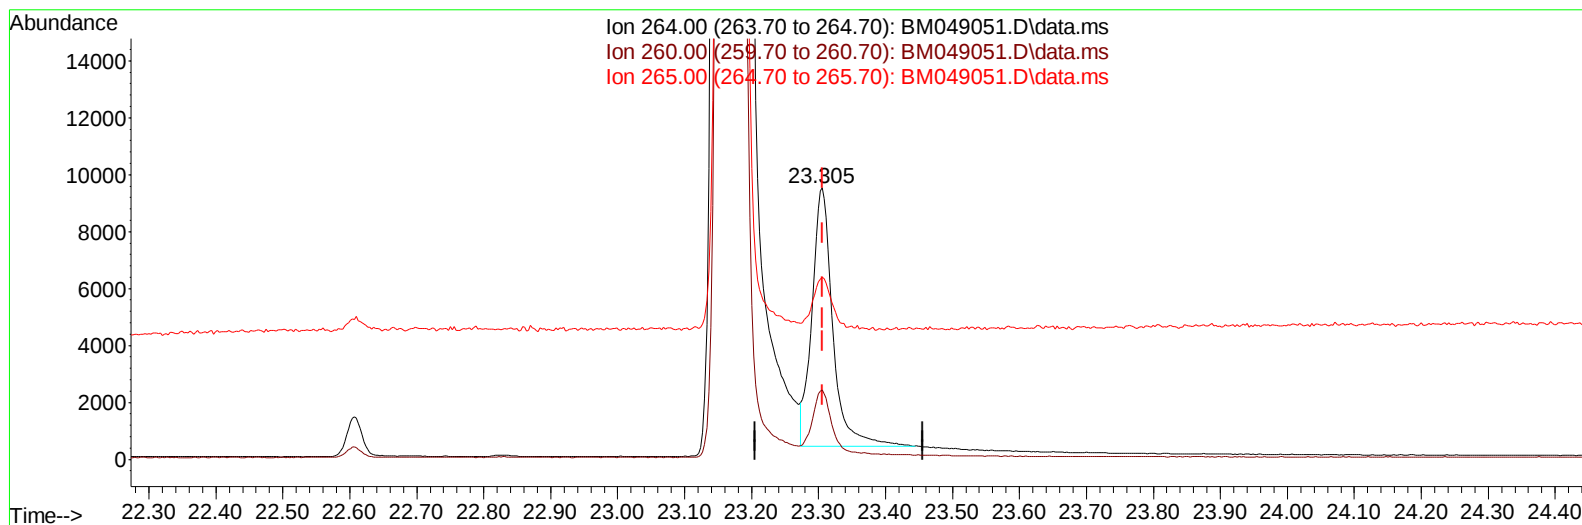

TIC: BM049051.D\data.ms

(23) Perylene-d12 (I)




23.305min (-0.000) 0.40 ng/u1

response 19678

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.50
265.00	78.30	67.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

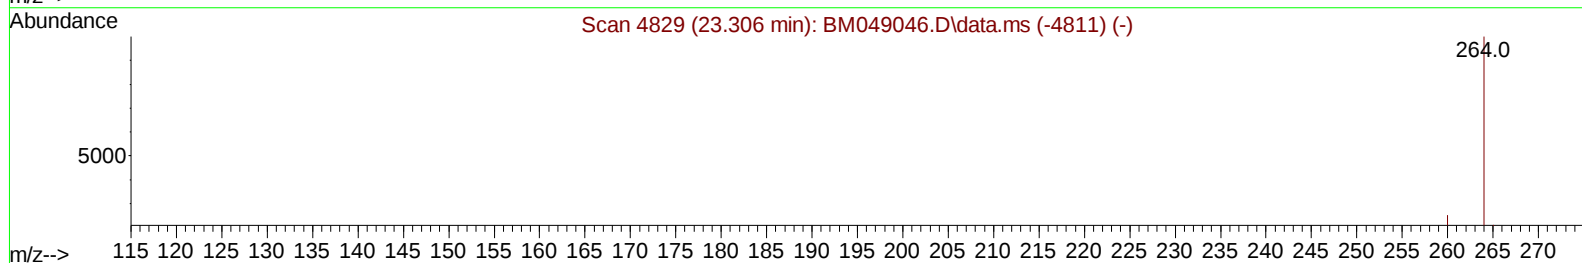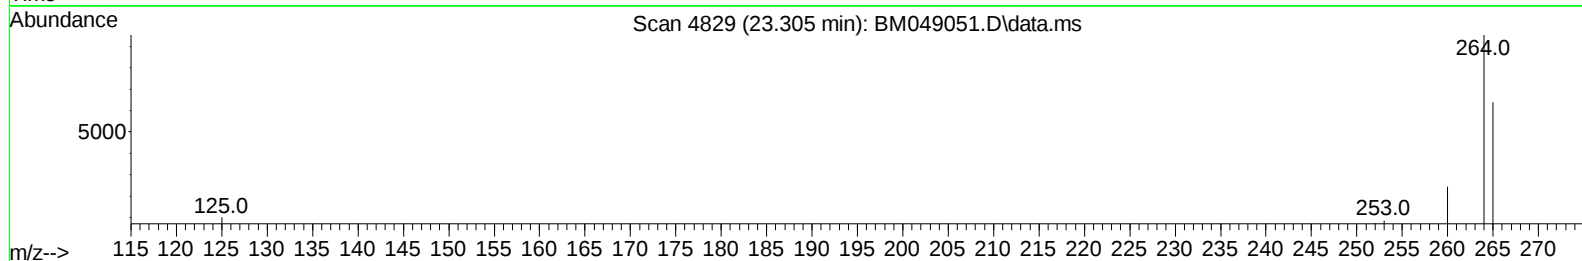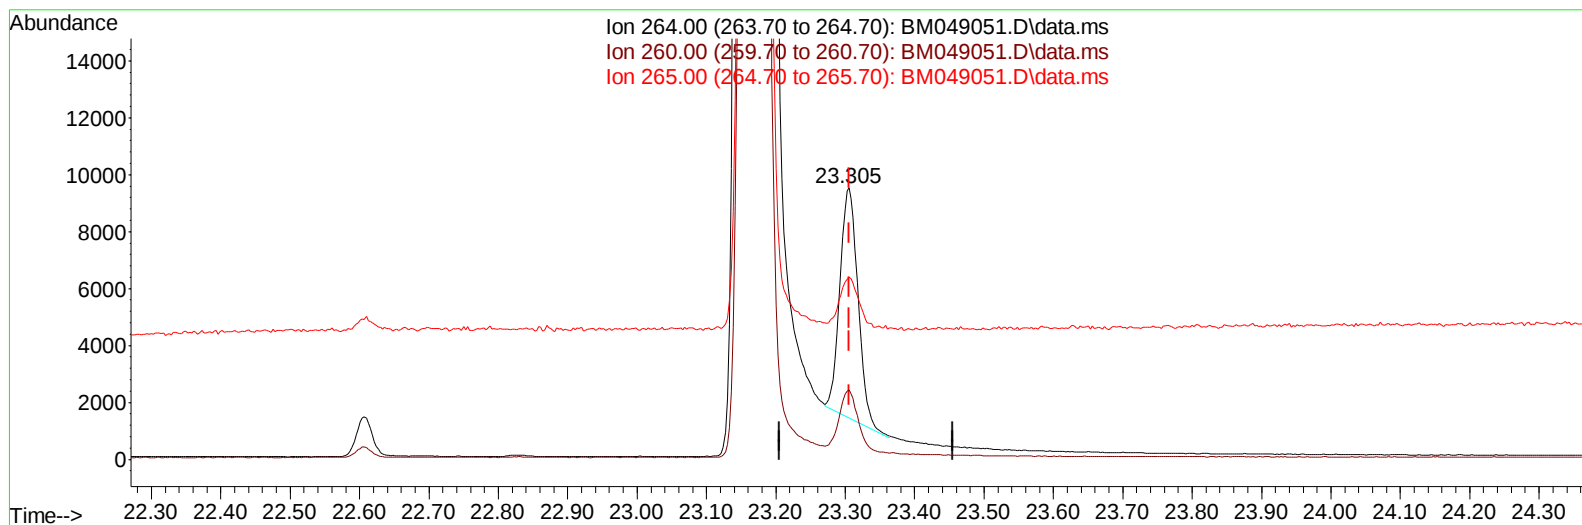

TIC: BM049051.D\data.ms

(23) Perylene-d12 (I)

23.305min (-0.000) 0.40 ng/ul m

response 14563

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.50
265.00	78.30	67.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
 Data File : BM049051.D
 Acq On : 18 Dec 2024 16:10
 Operator : RC/JU
 Sample : PB165622BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.564	152	5413	0.400	ng/ul	0.00
4) Naphthalene-d8	10.326	136	15445	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.201	164	8307	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.947	188	17983m	0.400	ng/ul	0.00
17) Chrysene-d12	21.149	240	13729m	0.400	ng/ul	0.00
23) Perylene-d12	23.305	264	14563m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.147	96	36168	5.794	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.932	152	6292	0.303	ng/ul	0.00
18) Fluoranthene-d10	18.983	212	12710	0.326	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049051.D
Acq On : 18 Dec 2024 16:10
Operator : RC/JU
Sample : PB165622BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Dec 18 16:39:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

