
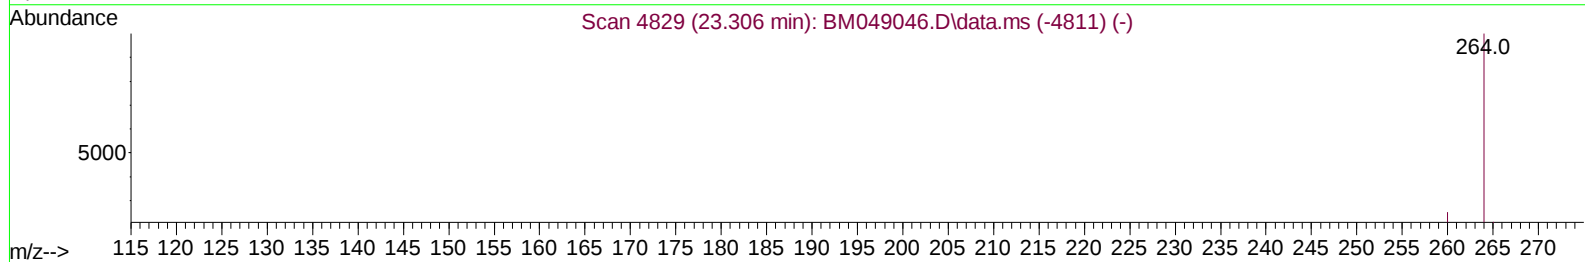
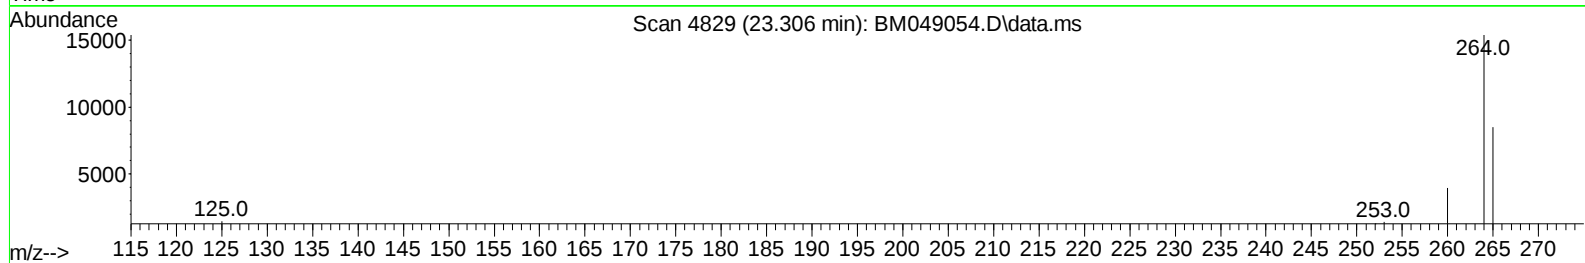


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

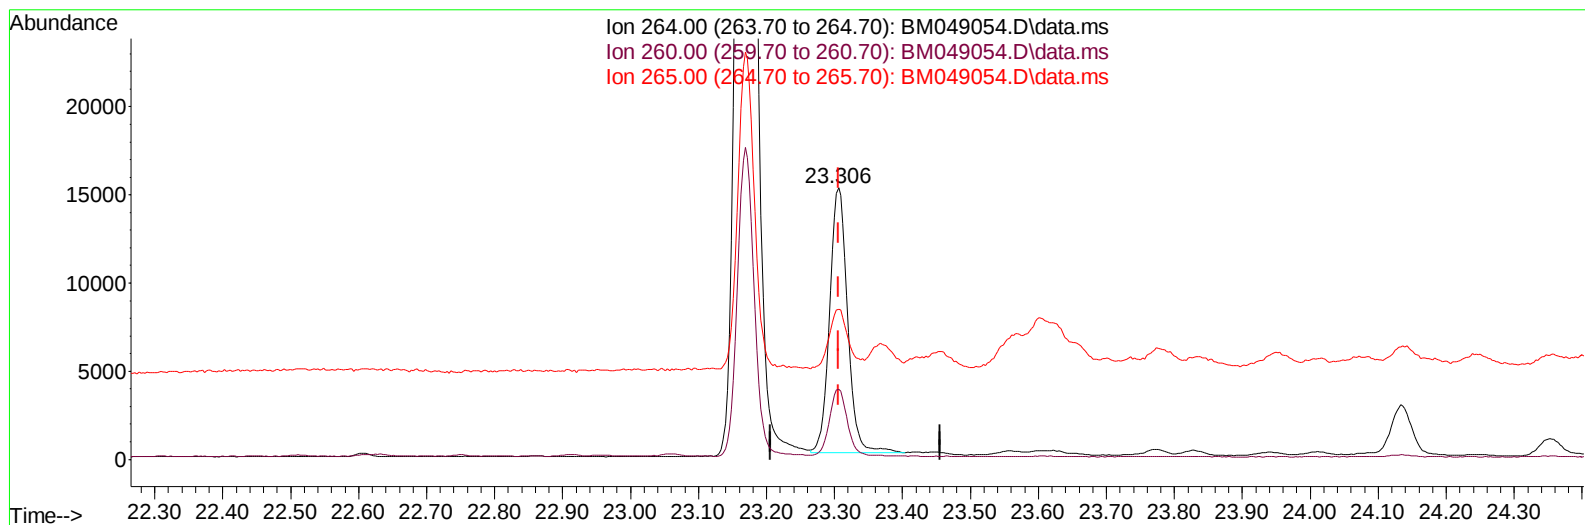

TIC: BM049054.D\data.ms

(23) Perylene-d12 (I)




23.306min (+ 0.000) 0.40 ng/ul

response 27603

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.75
265.00	78.30	55.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

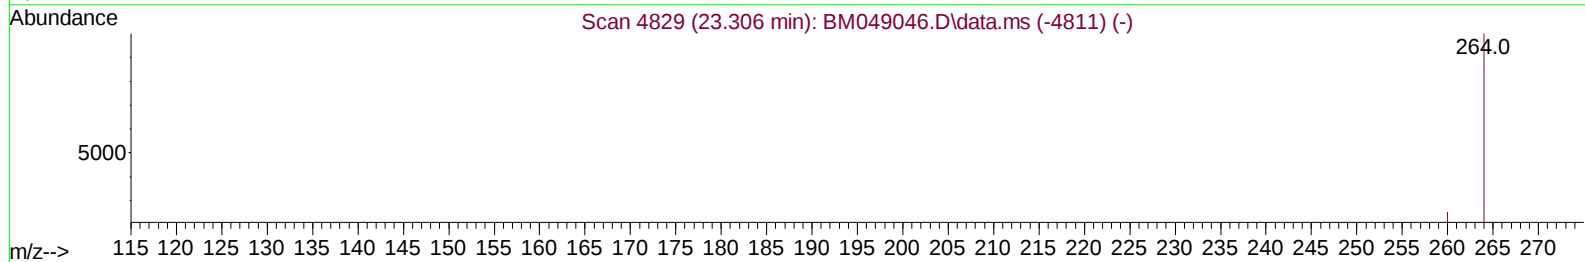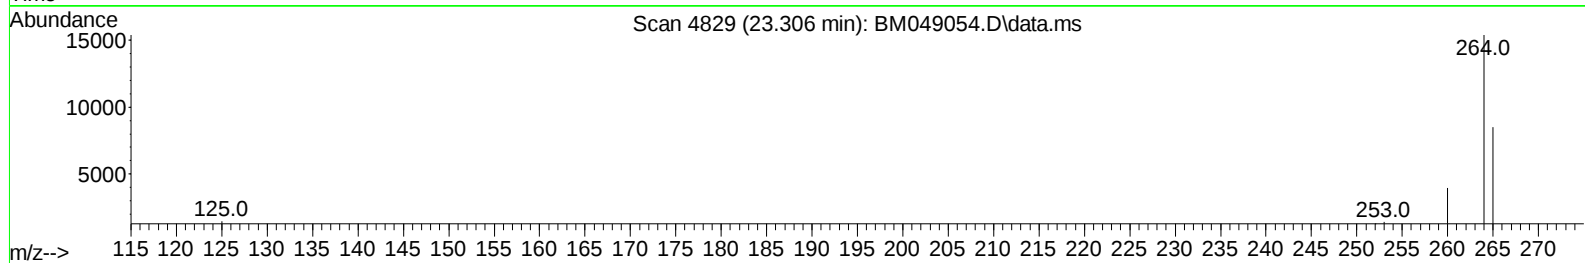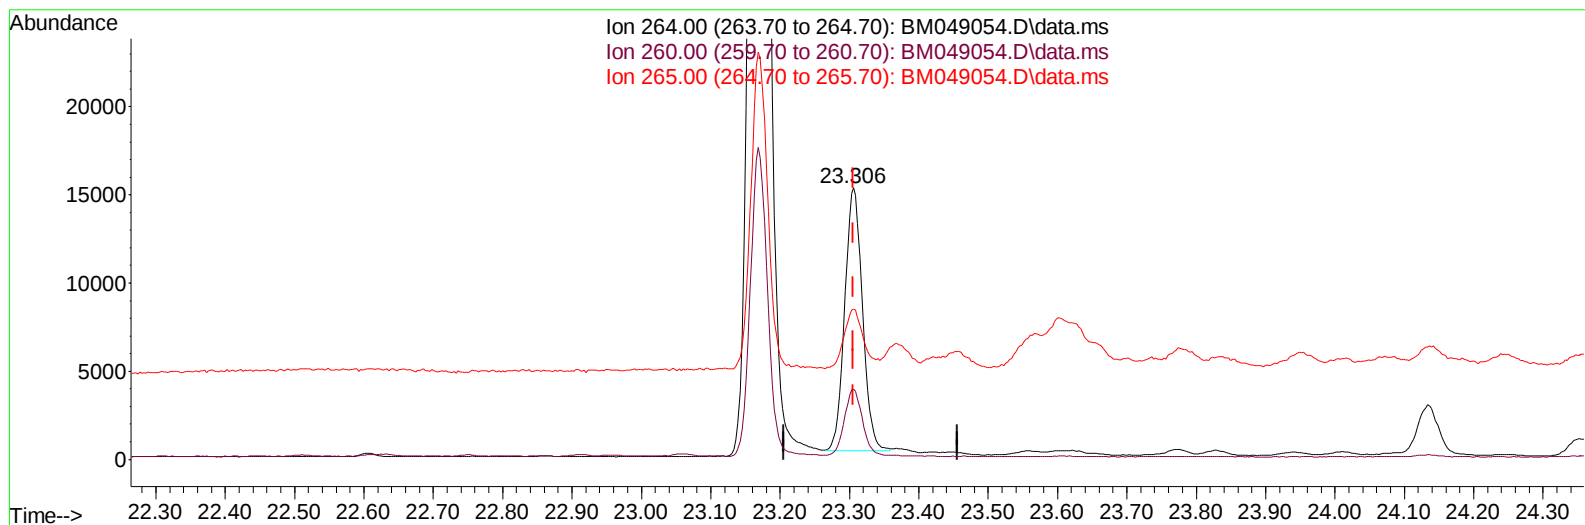

TIC: BM049054.D\data.ms

(23) Perylene-d12 (I)




23.306min (+ 0.000) 0.40 ng/ul m

response 26524

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.75
265.00	78.30	55.33#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

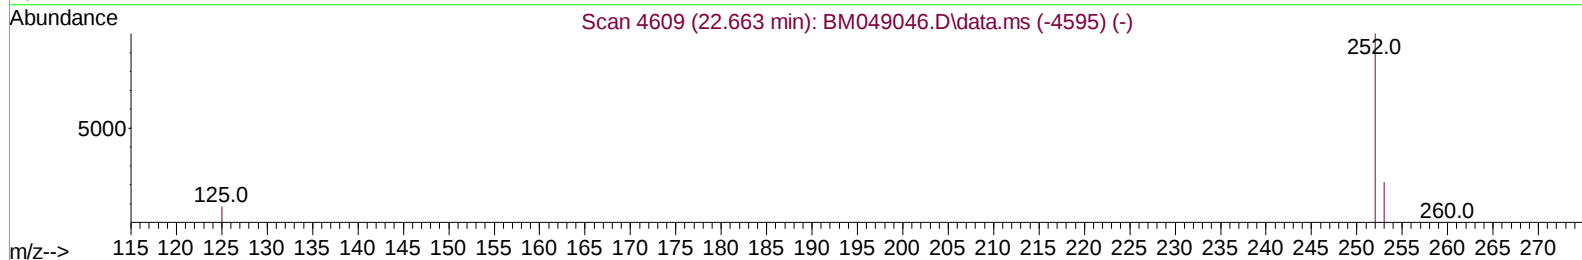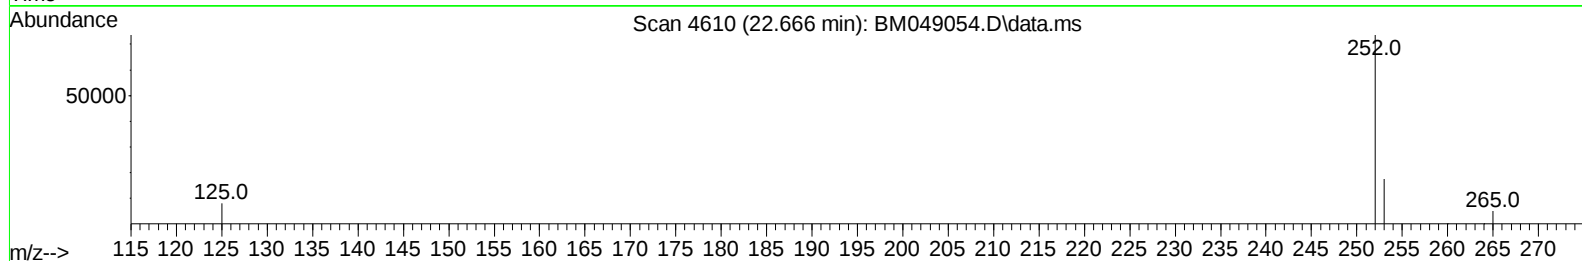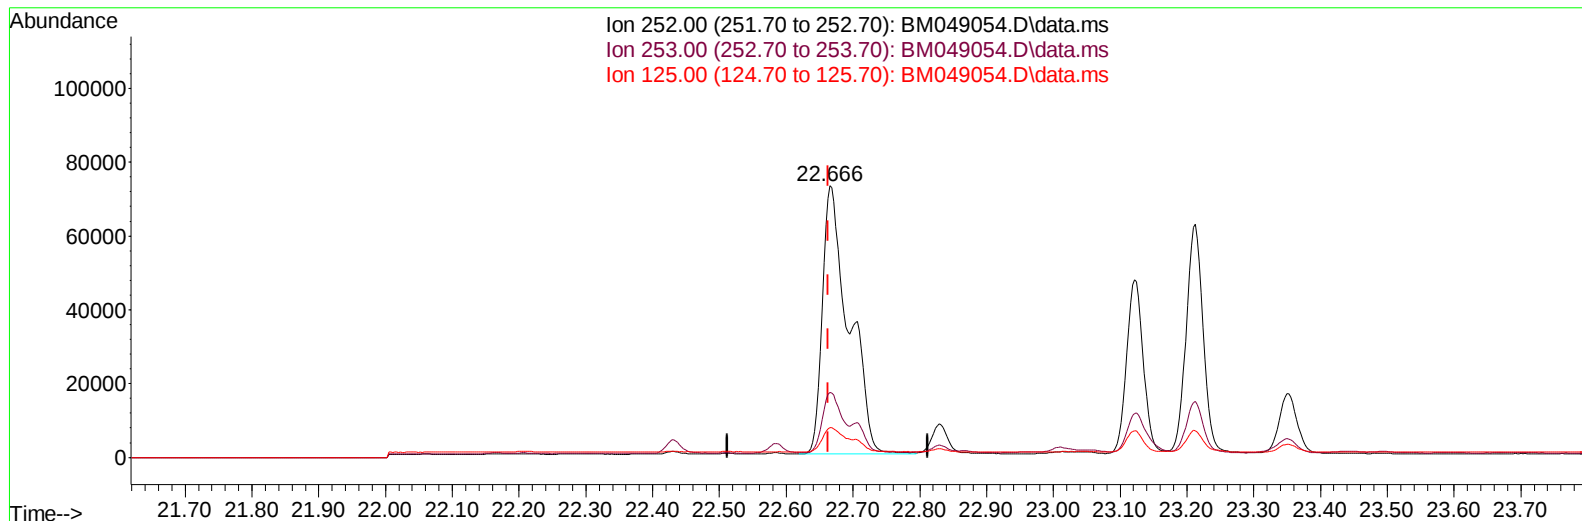

TIC: BM049054.D\data.ms

(24) Benzo(b)fluoranthene




22.666min (+ 0.003) 2.36 ng/u1

response 200023

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.30	23.98
125.00	15.40	10.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

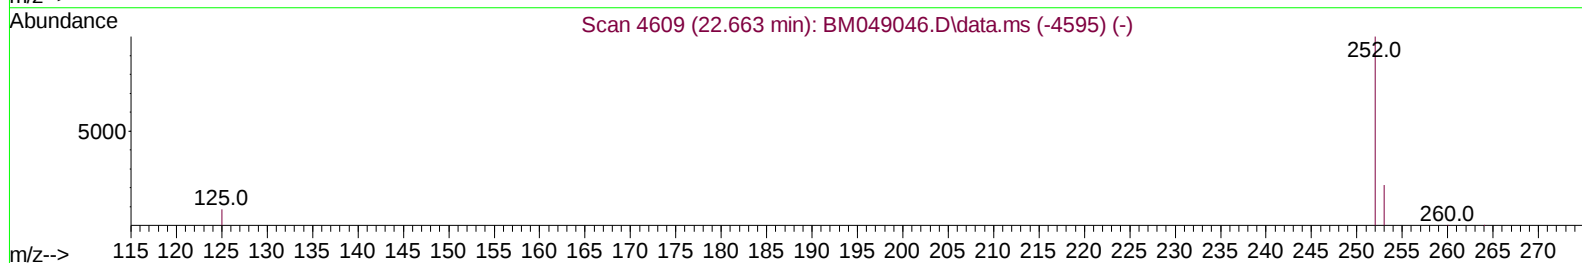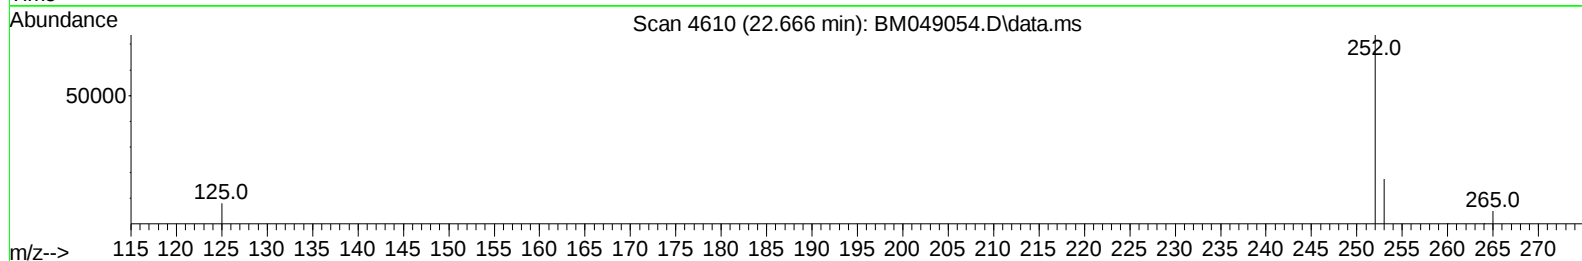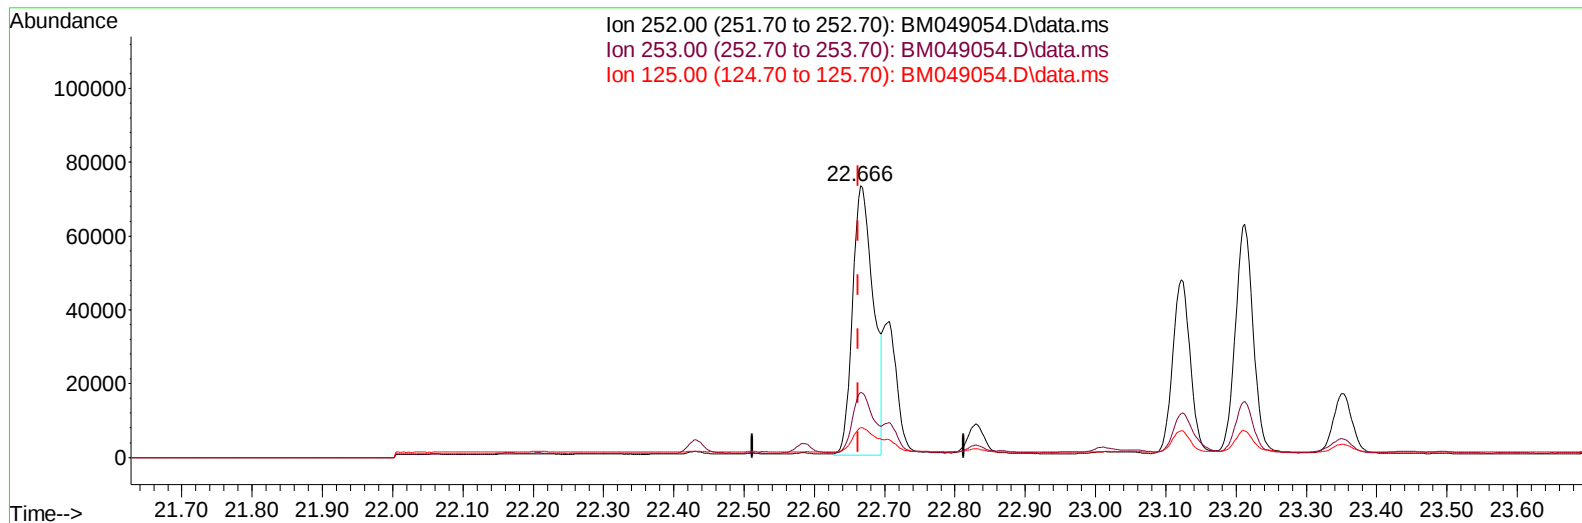

TIC: BM049054.D\data.ms

(24) Benzo(b)fluoranthene




22.666min (+ 0.003) 1.77 ng/u1 m

response 150287

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.30	23.98
125.00	15.40	10.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

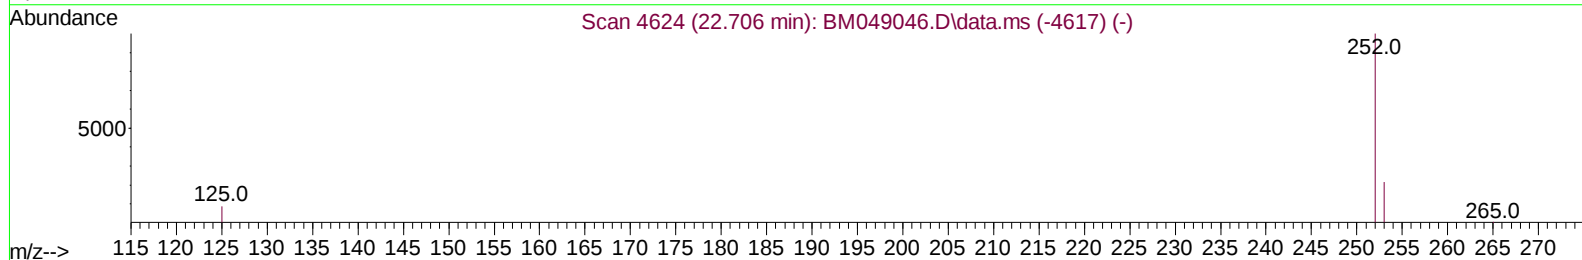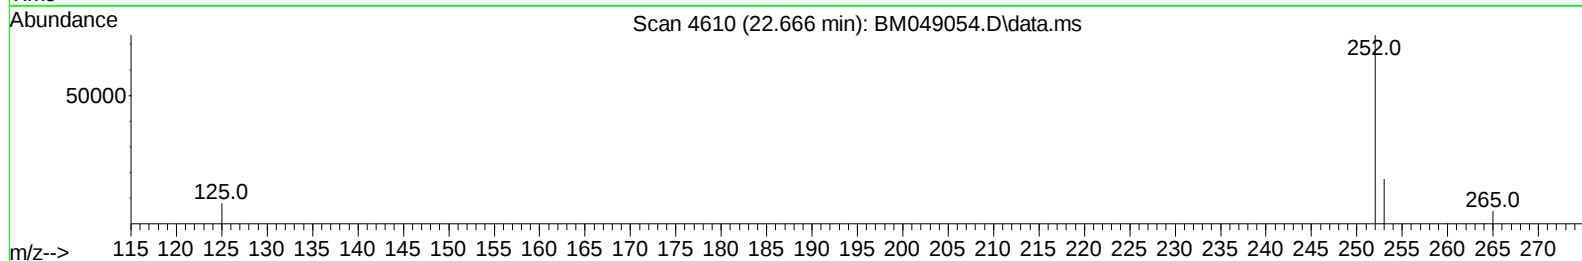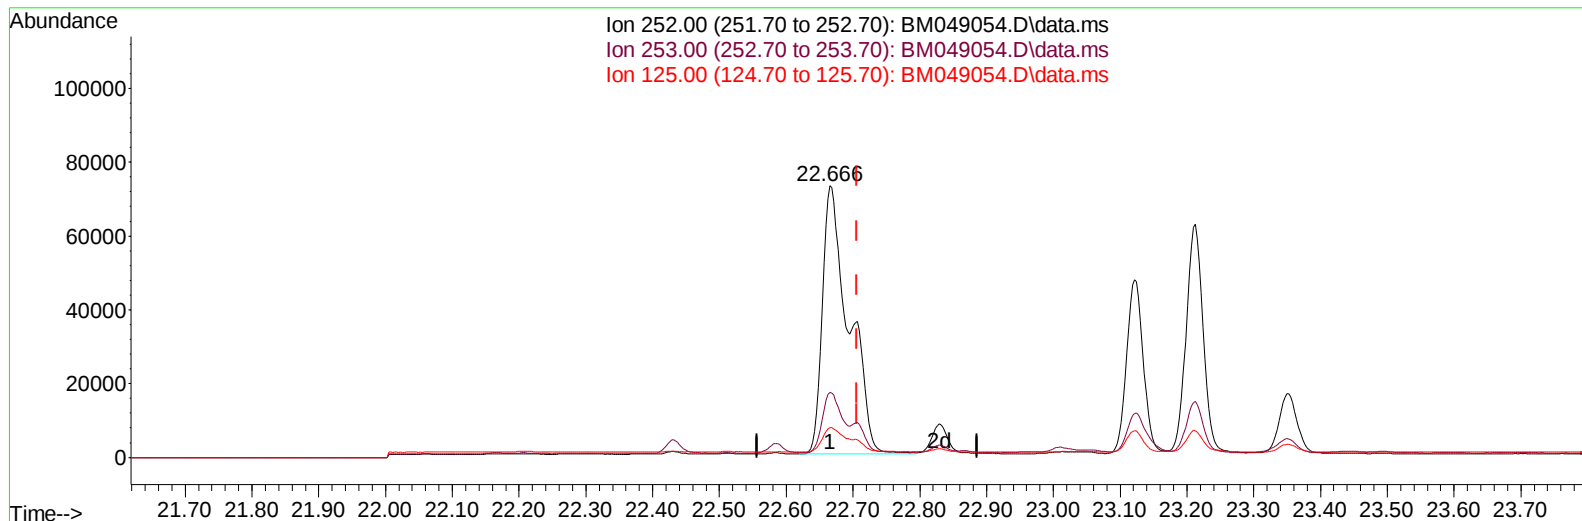

TIC: BM049054.D\data.ms

(25) Benzo(k)fluoranthene




22.666min (-0.041) 2.15 ng/u1

response 200023

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.60	23.98
125.00	15.70	10.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

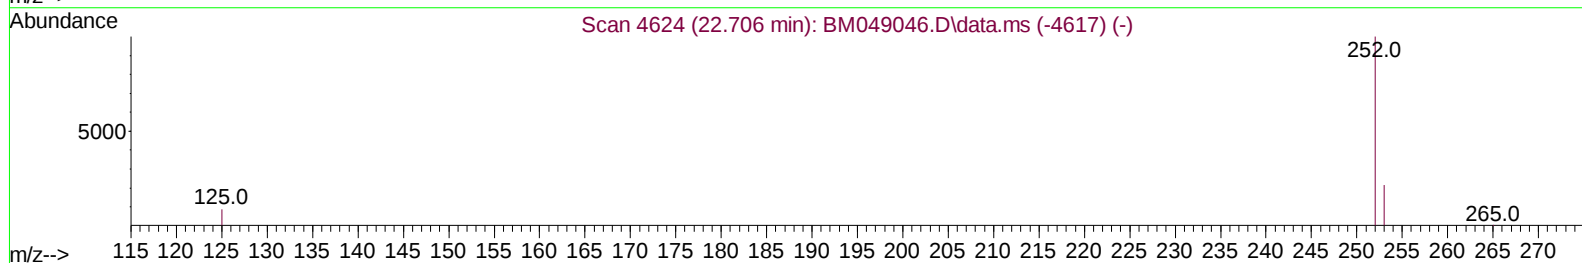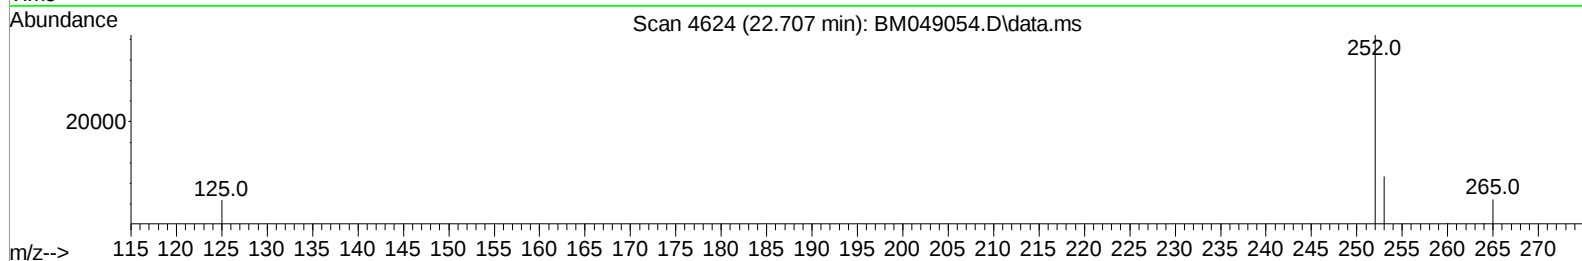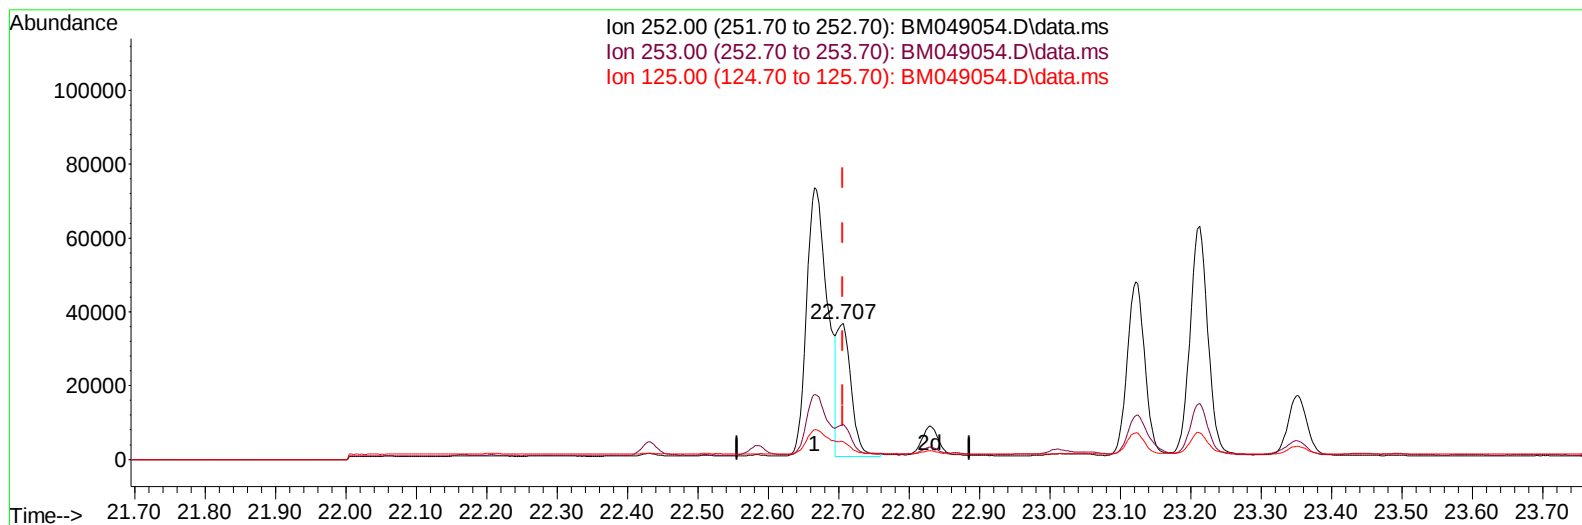

TIC: BM049054.D\data.ms

(25) Benzo(k)fluoranthene




22.707min (+ 0.000) 0.54 ng/u1 m

response 50085

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.60	25.50
125.00	15.70	12.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

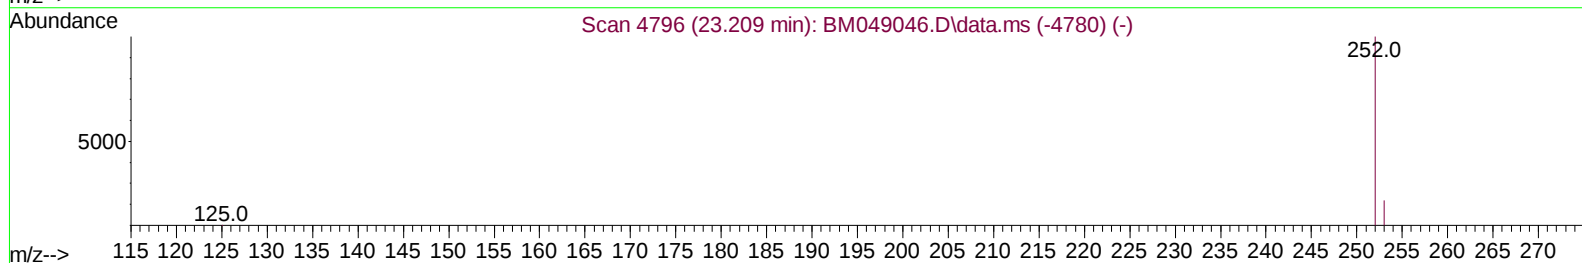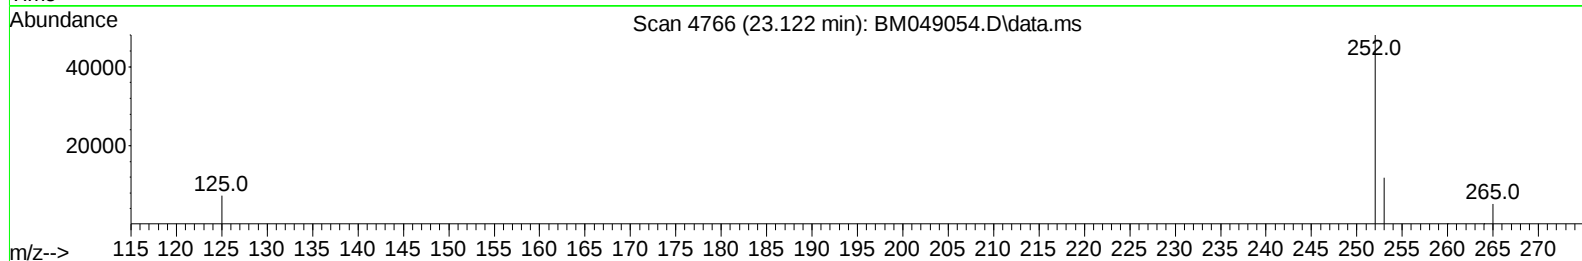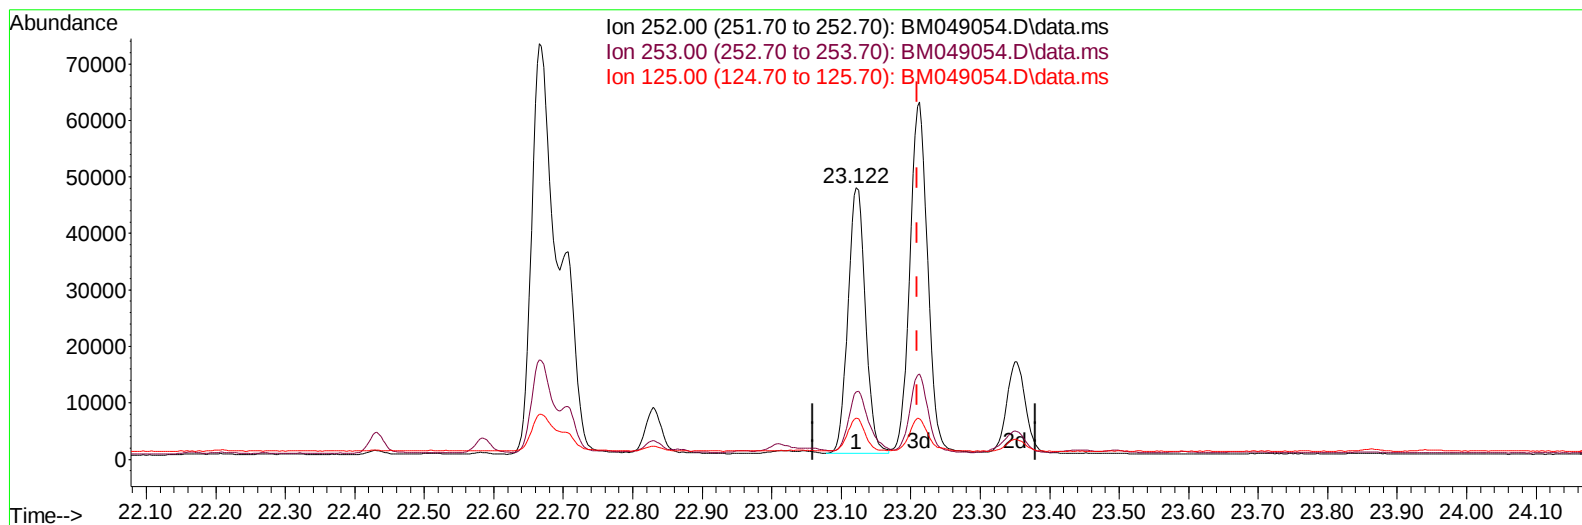

TIC: BM049054.D\data.ms

(26) Benzo(a)pyrene (C)




23.122min (-0.088) 1.01 ng/u1

response 82302

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.00	24.85
125.00	18.50	15.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

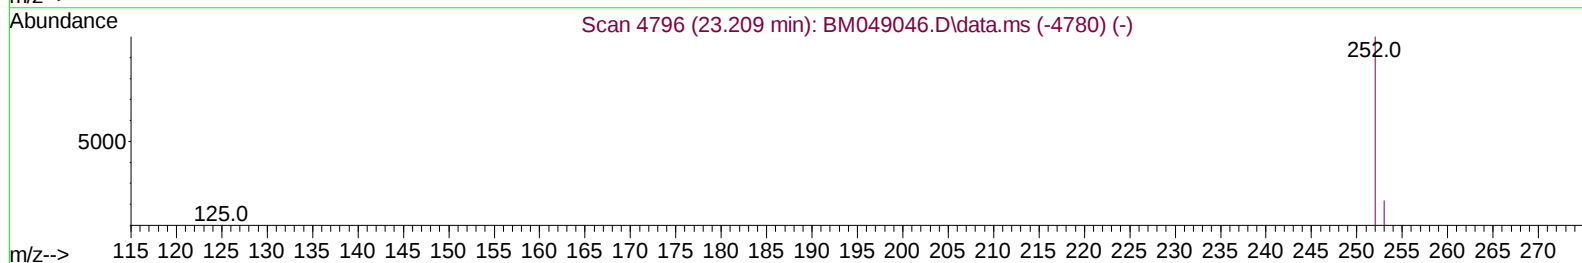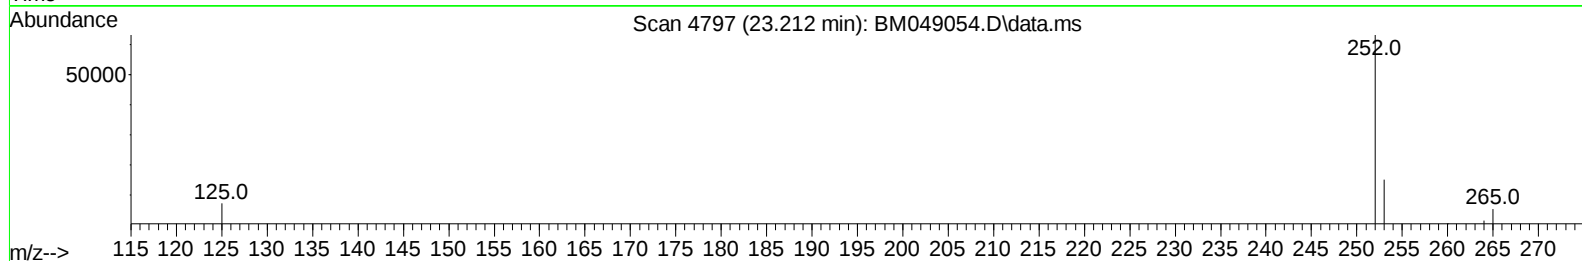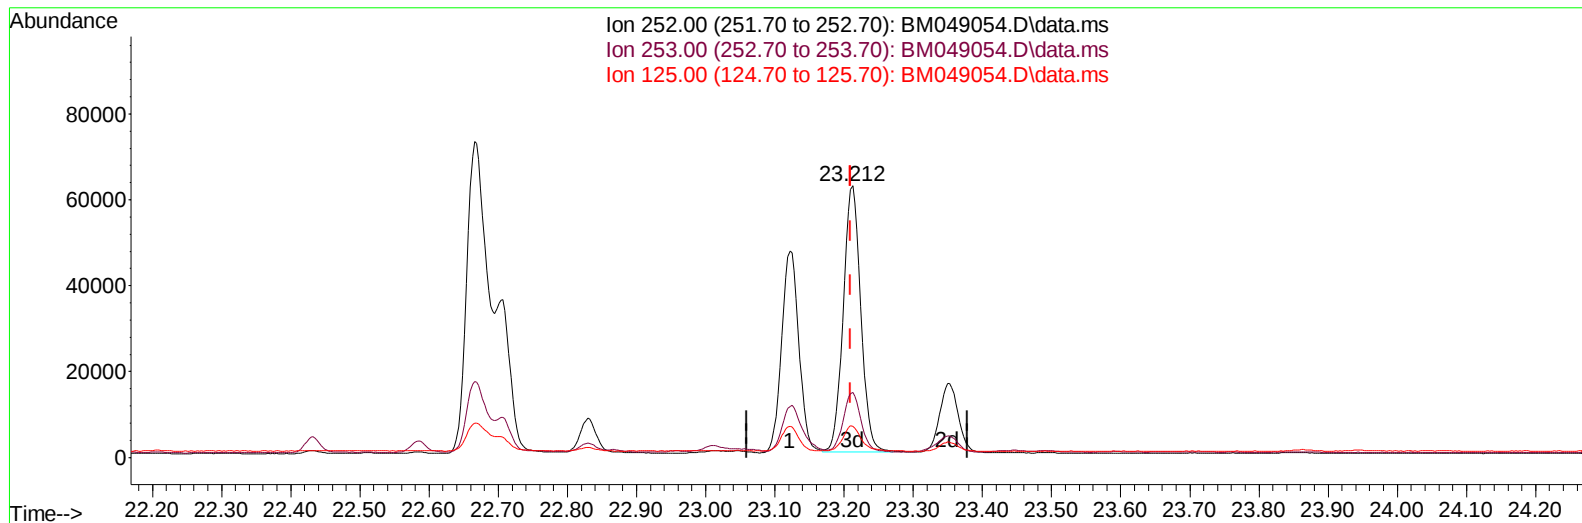

TIC: BM049054.D\data.ms

(26) Benzo(a)pyrene (C)

23.212min (+ 0.003) 1.34 ng/ul m

response 109041

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.00	24.02
125.00	18.50	11.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
 Data File : BM049054.D
 Acq On : 18 Dec 2024 18:01
 Operator : RC/JU
 Sample : P5155-16DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.565	152	8247	0.400	ng/ul	0.00
4) Naphthalene-d8	10.330	136	24930	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.200	164	14373	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	30017	0.400	ng/ul	0.00
17) Chrysene-d12	21.146	240	25389	0.400	ng/ul	0.00
23) Perylene-d12	23.306	264	26524m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.151	96	5230	0.550	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	1124	0.034	ng/ul	0.00
18) Fluoranthene-d10	18.982	212	2142	0.030	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.374	128	19329	0.310	ng/ul	99
7) 2-Methylnaphthalene	12.002	142	5328	0.135	ng/ul	97
8) 1-Methylnaphthalene	12.222	142	2133	0.053	ng/ul	98
10) Acenaphthylene	13.918	152	2840	0.048	ng/ul#	90
11) Acenaphthene	14.260	153	1579	0.036	ng/ul	95
12) Fluorene	15.255	166	1873	0.038	ng/ul#	91
15) Phenanthrene	16.988	178	29016	0.370	ng/ul	100
16) Anthracene	17.077	178	5241	0.073	ng/ul#	94
19) Fluoranthene	19.010	202	62478	0.681	ng/ul	99
20) Pyrene	19.373	202	72614	0.742	ng/ul	99
21) Benzo(a)anthracene	21.132	228	60326	0.683	ng/ul	99
22) Chrysene	21.184	228	77204	0.815	ng/ul	97
24) Benzo(b)fluoranthene	22.666	252	150287m	1.774	ng/ul	
25) Benzo(k)fluoranthene	22.707	252	50085m	0.539	ng/ul	
26) Benzo(a)pyrene	23.212	252	109041m	1.342	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.444	276	97328	0.846	ng/ul#	92
28) Dibenzo(a,h)anthracene	25.451	278	20875	0.234	ng/ul	95
29) Benzo(g,h,i)perylene	26.098	276	110017	1.190	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121824\
Data File : BM049054.D
Acq On : 18 Dec 2024 18:01
Operator : RC/JU
Sample : P5155-16DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 19 01:35:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

