

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121918\
 Data File : BM018302.D
 Acq On : 19 Dec 2018 18:34
 Operator : JU/SJ
 Sample : J6465-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EB01_0-2

Quant Time: Dec 20 01:07:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	85749	20.00	ng	-0.02
21) Naphthalene-d8	10.25	136	318722	20.00	ng	-0.02
39) Acenaphthene-d10	14.14	164	164647	20.00	ng	-0.02
64) Phenanthrene-d10	16.91	188	344127	20.00	ng	-0.01
76) Chrysene-d12	21.13	240	370524	20.00	ng	-0.01
87) Perylene-d12	23.29	264	422000	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	607804	118.41	ng	0.00
7) Phenol-d6	6.69	99	790946	110.86	ng	-0.02
23) Nitrobenzene-d5	8.65	82	501308	80.68	ng	-0.02
42) 2,4,6-Tribromophenol	15.65	330	245484	101.58	ng	-0.02
45) 2-Fluorobiphenyl	12.75	172	914486	71.94	ng	-0.02
79) Terphenyl-d14	19.56	244	1130850	69.03	ng	-0.01
Target Compounds						
10) Phenol	6.71	94	41064	5.435	ng	85
50) Dimethylphthalate	13.62	163	63829	4.663	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121918\
Data File : BM018302.D
Acq On : 19 Dec 2018 18:34
Operator : JU/SJ
Sample : J6465-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EB01_0-2

Quant Time: Dec 20 01:07:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

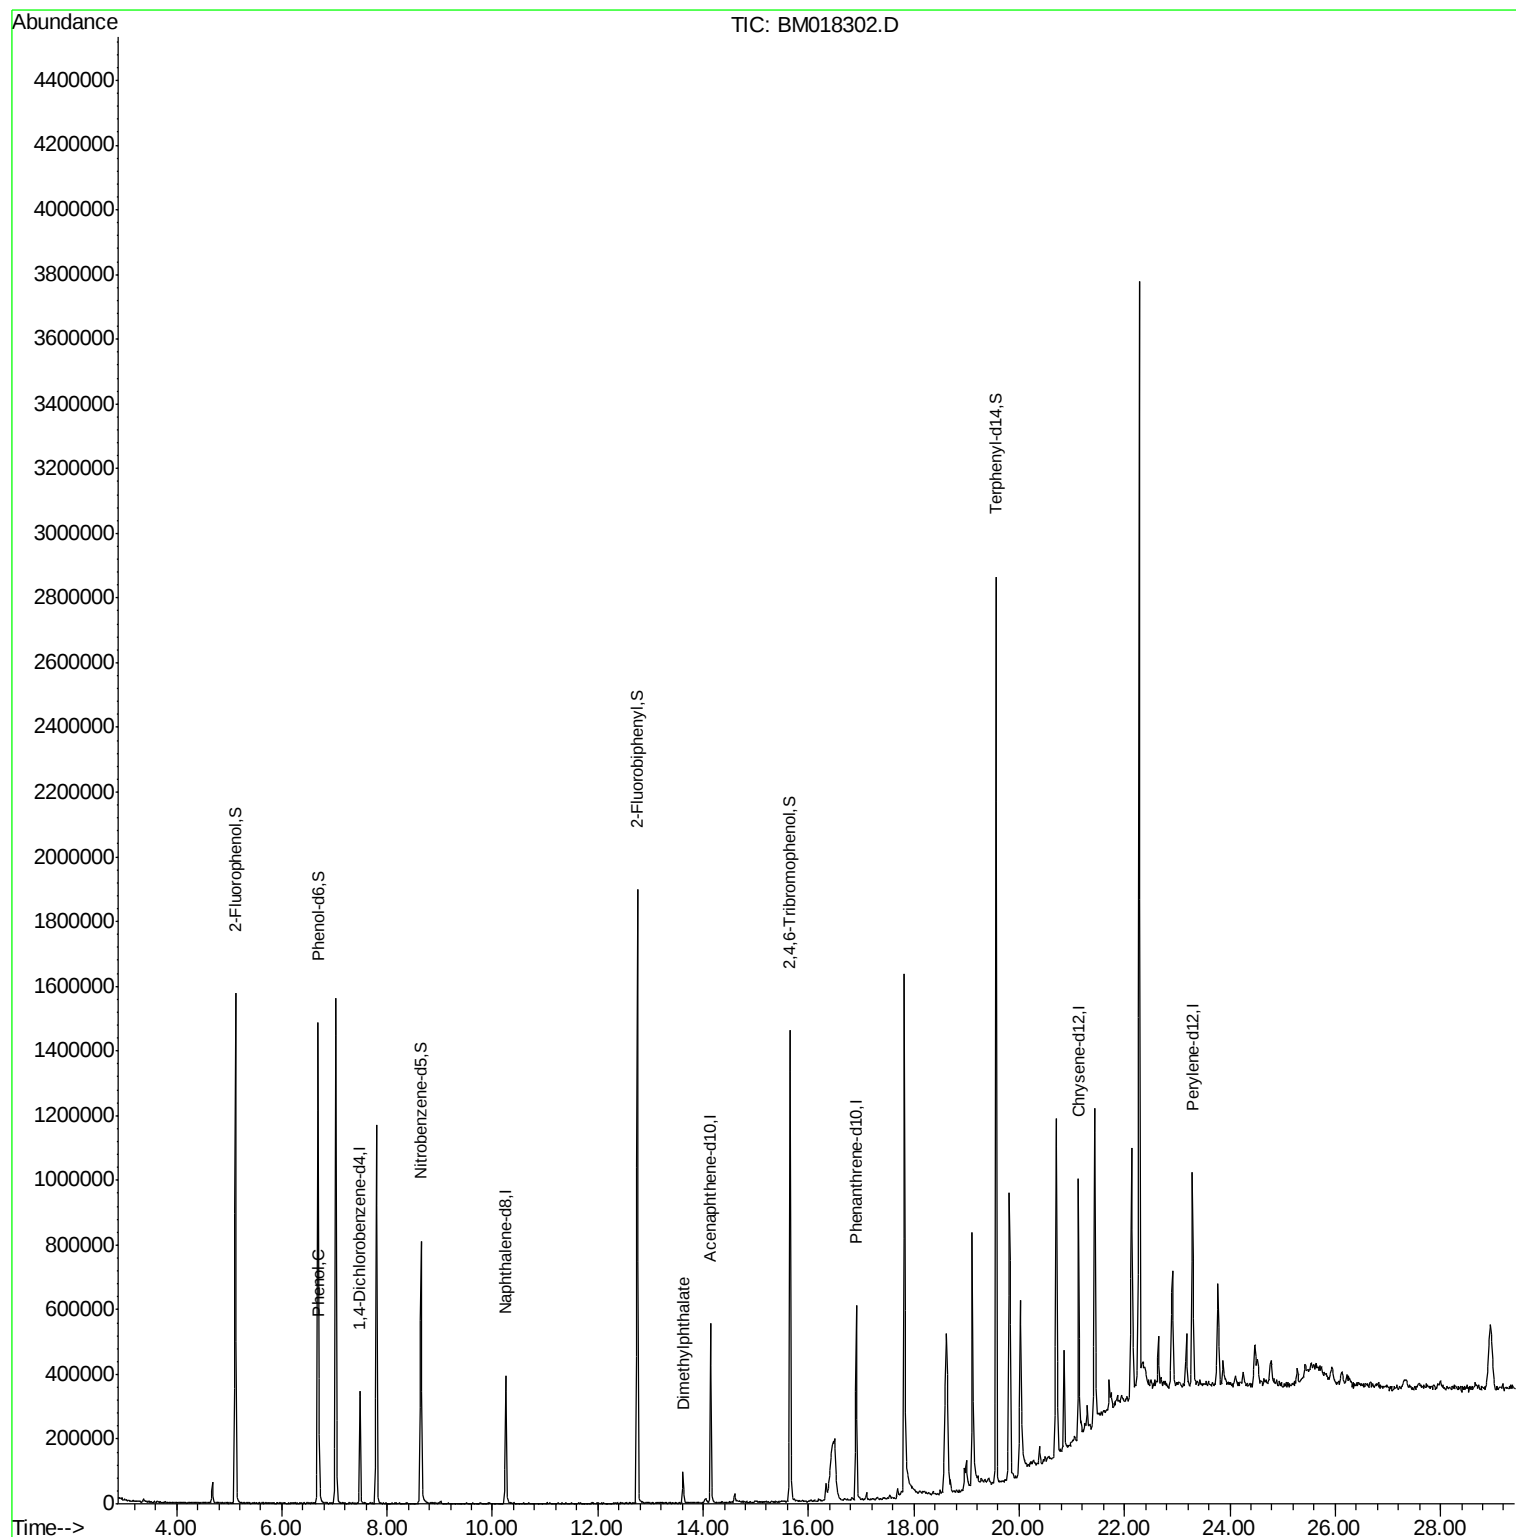

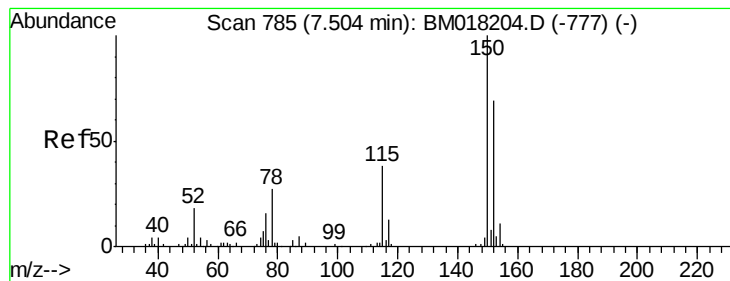


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 782
Delta R.T. -0.02 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Instrument :
BNA_M
ClientSampleId :
EB01_0-2

Tgt Ion:152 Resp: 85749
Ion Ratio Lower Upper
152 100
150 154.3 116.1 174.1
115 64.5 44.6 67.0

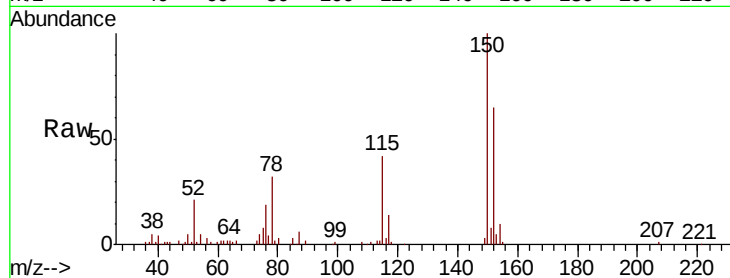


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

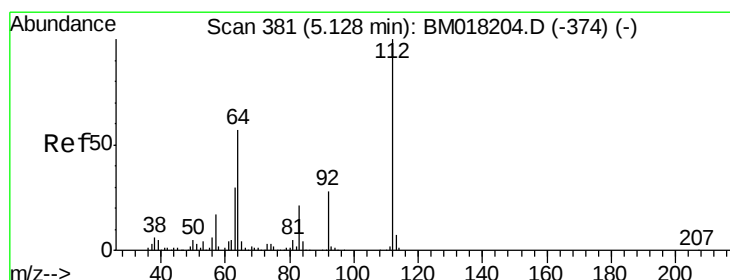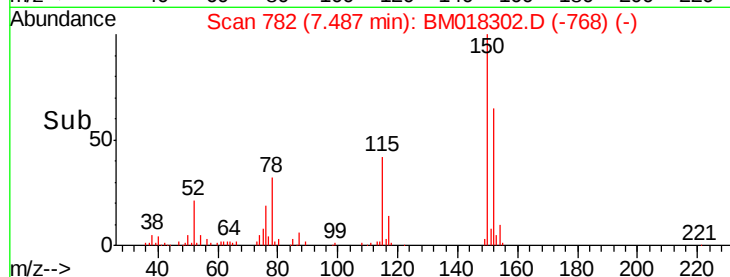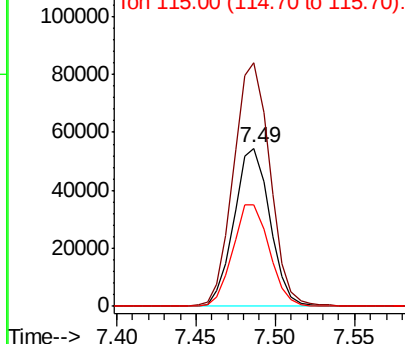



#5




2-Fluorophenol
Concen: 118.407 ng
RT: 5.12 min Scan# 380
Delta R.T. -0.01 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Tgt Ion:112 Resp: 607804
Ion Ratio Lower Upper
112 100
64 60.1 45.4 68.2
63 33.1 24.0 36.0

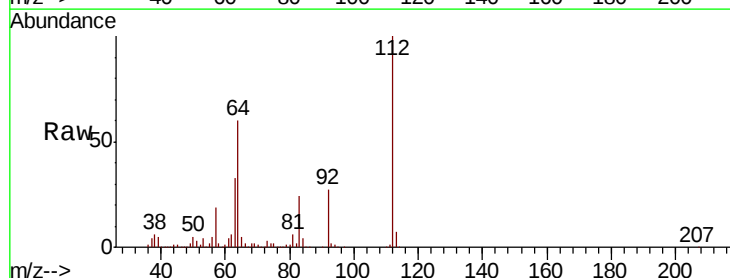

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

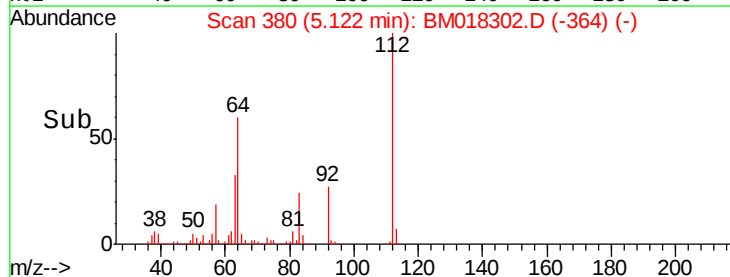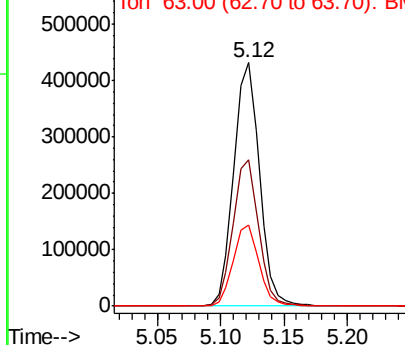

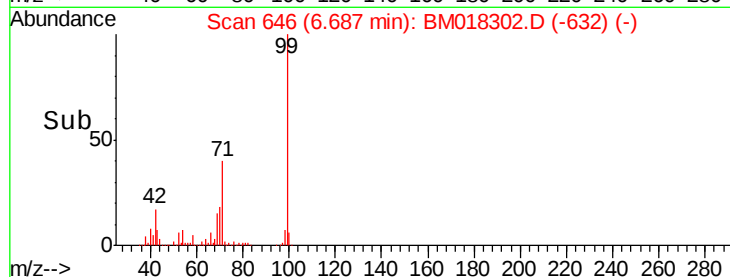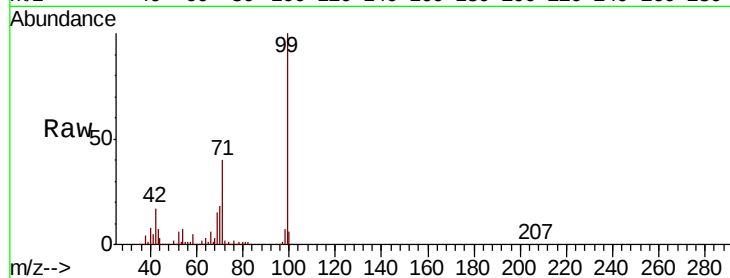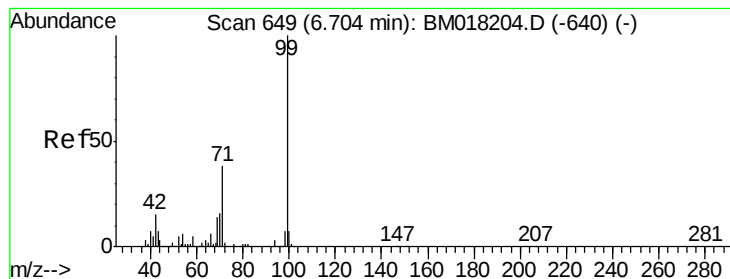

#7

Phenol-d6

Concen: 110.859 ng

RT: 6.69 min Scan# 646

Delta R.T. -0.02 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34

Instrument :

BNA_M

ClientSampleId :

EB01_0-2





Tgt Ion: 99 Resp: 790946

Ion Ratio Lower Upper

99 100

42 16.8 12.3 18.5

71 40.4 30.2 45.2

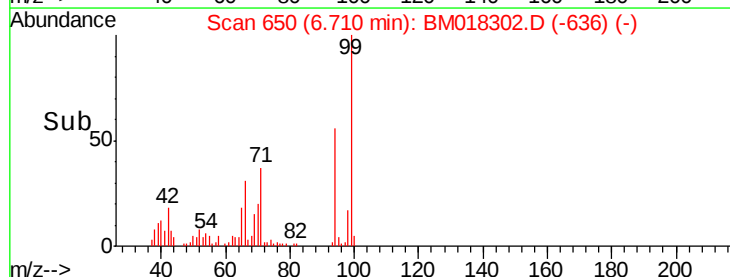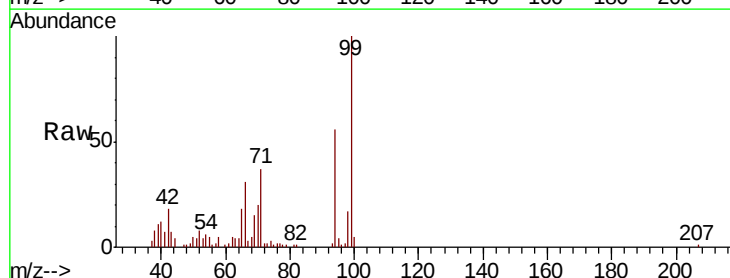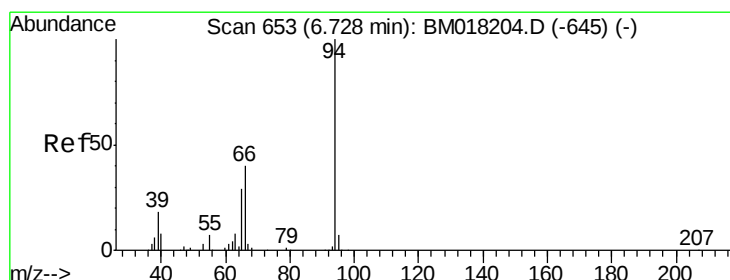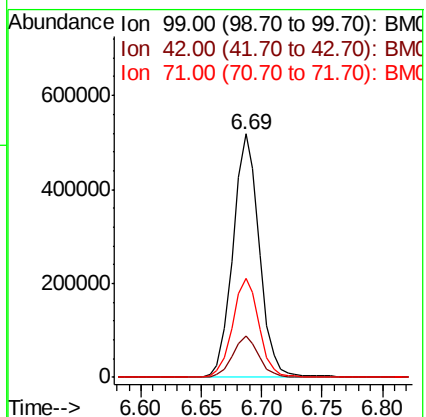

#10

Phenol

Concen: 5.435 ng

RT: 6.71 min Scan# 650

Delta R.T. -0.02 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34


Tgt Ion: 94 Resp: 41064


Ion Ratio Lower Upper

94 100

65 32.6 9.5 49.5

66 55.2 21.3 61.3

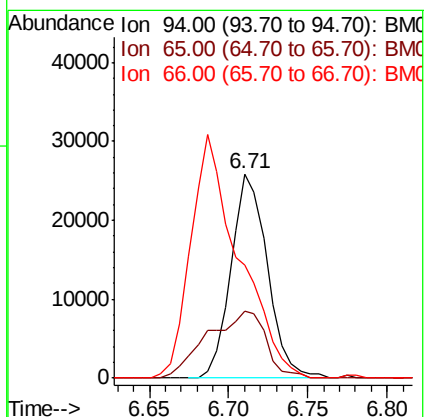


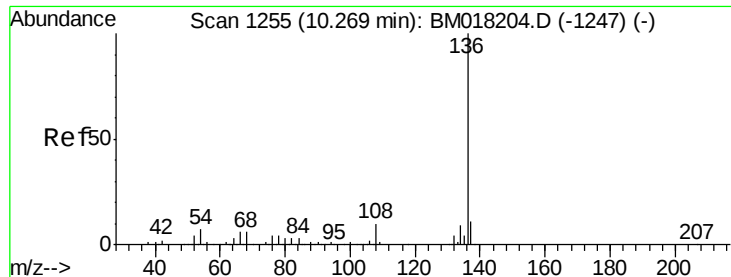




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.25 min Scan# 1252
Delta R.T. -0.02 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Instrument :
BNA_M
ClientSampleId :
EB01_0-2

Tgt Ion:	136	Resp:	318722
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.2	13.8
54	6.6	5.2	7.8
68	5.7	5.0	7.6

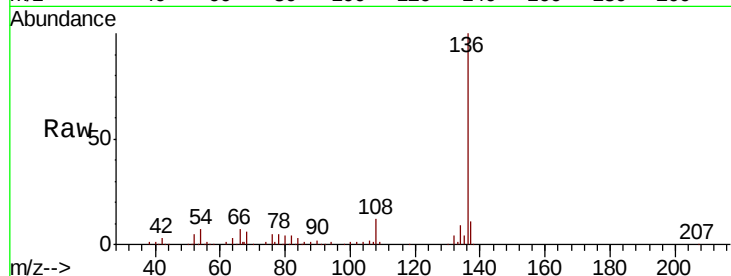


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BM
Ion 68.00 (67.70 to 68.70): BM

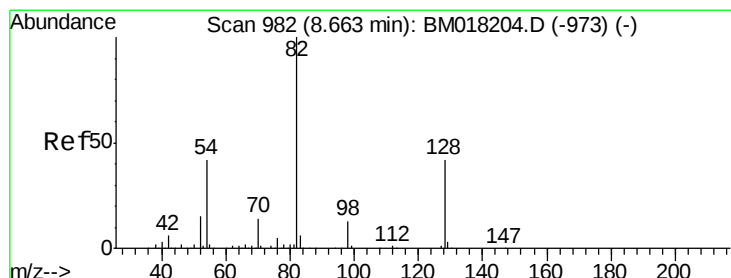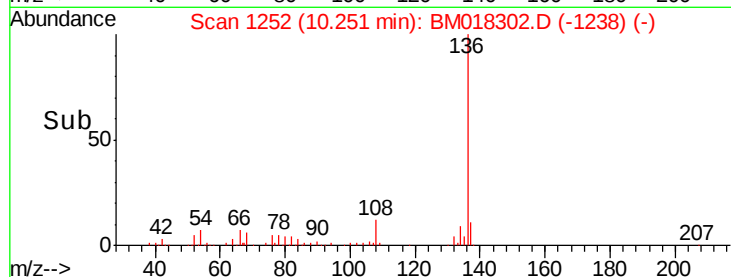
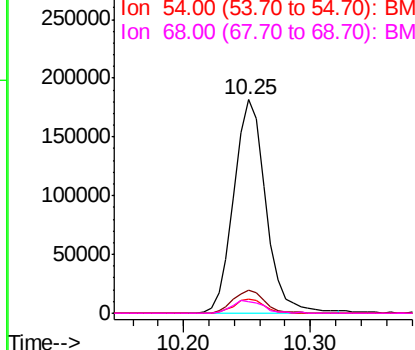



#23
Nitrobenzene-d5
Concen: 80.678 ng
RT: 8.65 min Scan# 979
Delta R.T. -0.02 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Tgt Ion:	82	Resp:	501308
Ion	Ratio	Lower	Upper
82	100		
128	37.3	33.4	50.2
54	42.0	33.4	50.2

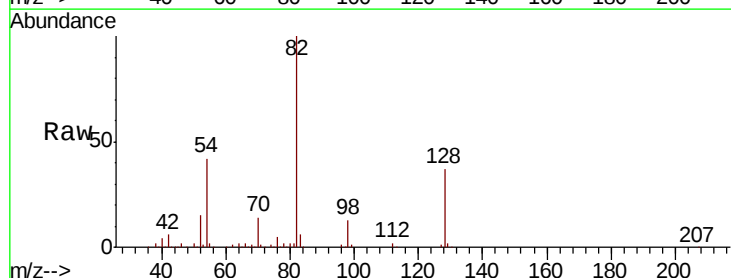

Abundance Ion 82.00 (81.70 to 82.70): BM
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BM

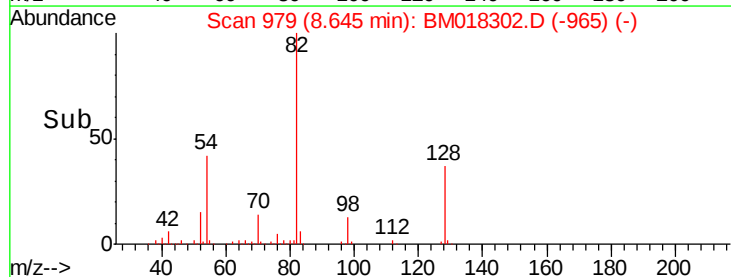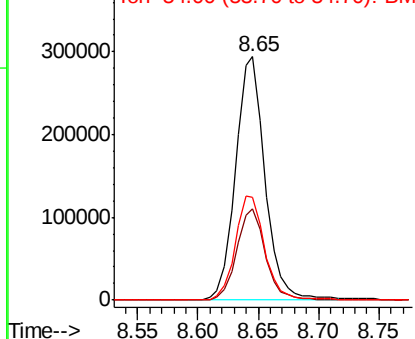

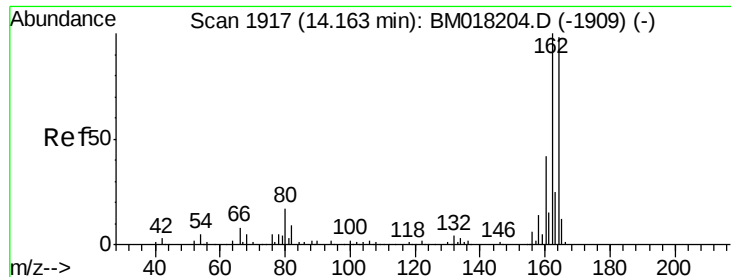

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.14 min Scan# 1914

Delta R.T. -0.02 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34

Instrument :

BNA_M

ClientSampleId :

EB01_0-2


Tgt Ion:164 Resp: 164647

Ion Ratio Lower Upper

164 100

162 108.3 81.8 122.6




160 45.8 34.6 51.8

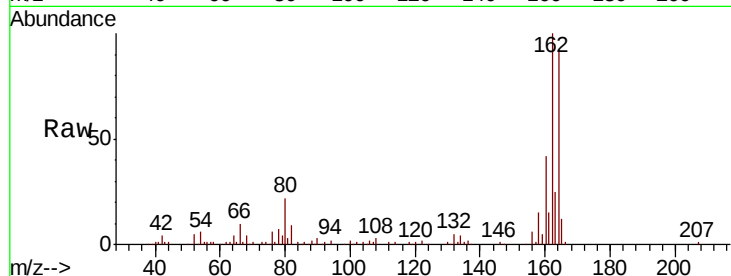

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

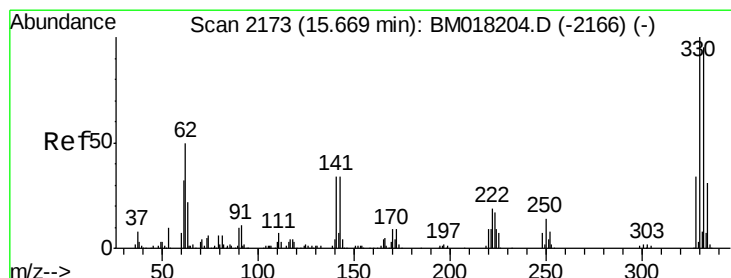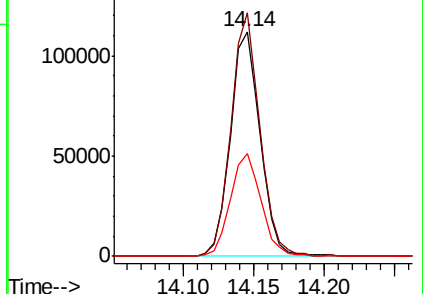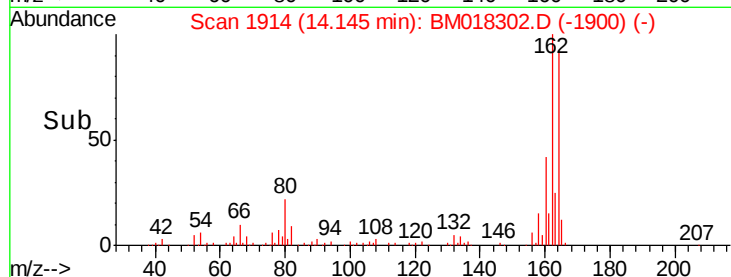

#42

2,4,6-Tribromophenol

Concen: 101.584 ng

RT: 15.65 min Scan# 2170

Delta R.T. -0.02 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34


Tgt Ion:330 Resp: 245484

Ion Ratio Lower Upper

330 100

332 97.5 78.6 118.0



141 39.5 27.1 40.7

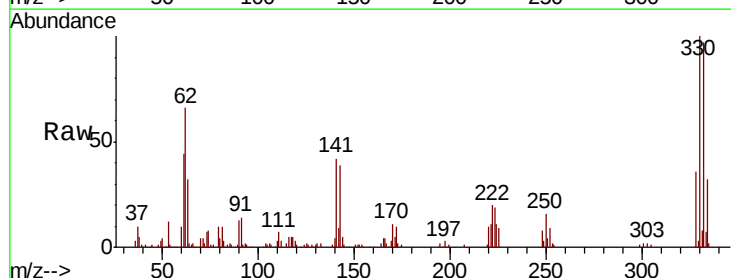


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



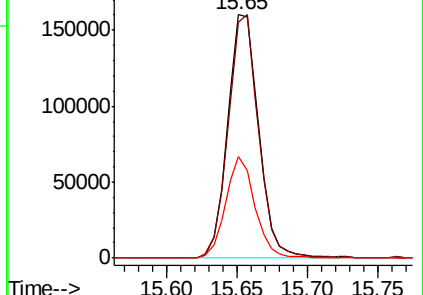
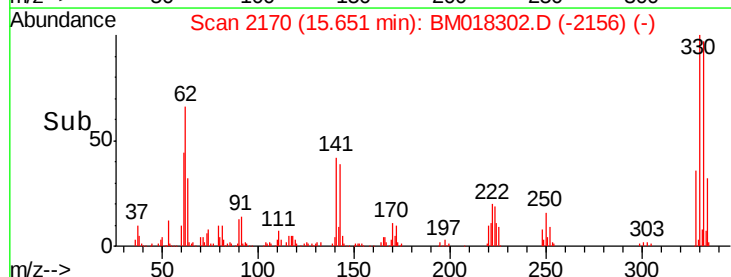


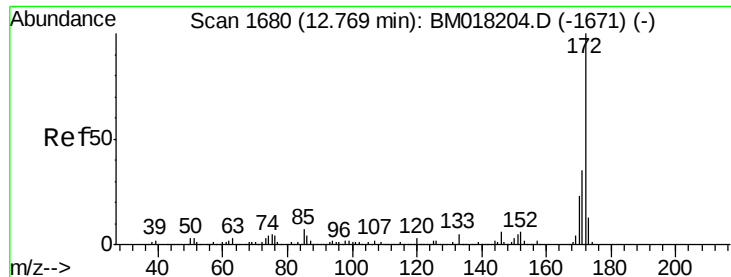

#45
2-Fluorobiphenyl
Concen: 71.940 ng
RT: 12.75 min Scan# 1677
Delta R.T. -0.02 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34




Instrument :
BNA_M
ClientSampleId :
EB01_0-2


Tgt Ion:172 Resp: 914486
Ion Ratio Lower Upper
172 100
171 34.0 28.3 42.5
170 22.4 18.1 27.1

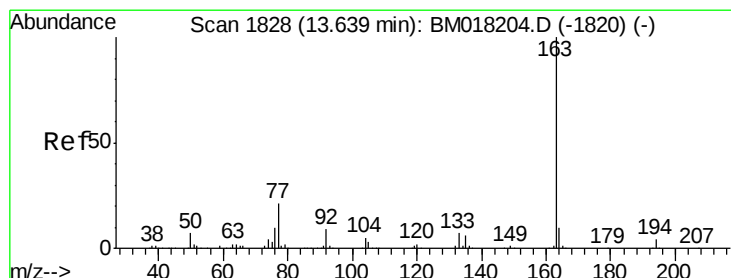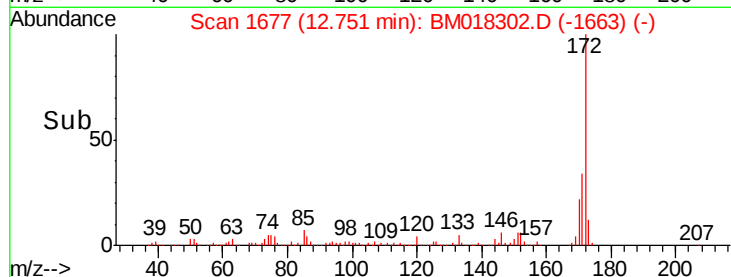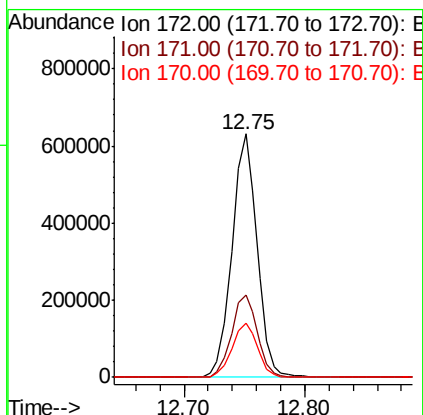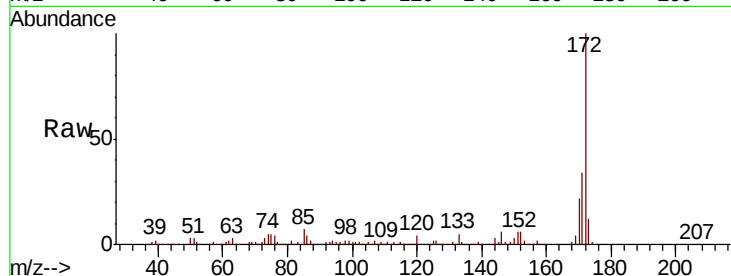

#50
Dimethylphthalate
Concen: 4.663 ng
RT: 13.62 min Scan# 1825
Delta R.T. -0.02 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Tgt Ion:163 Resp: 63829
Ion Ratio Lower Upper
163 100
194 3.7 3.1 4.7
164 9.0 7.9 11.9

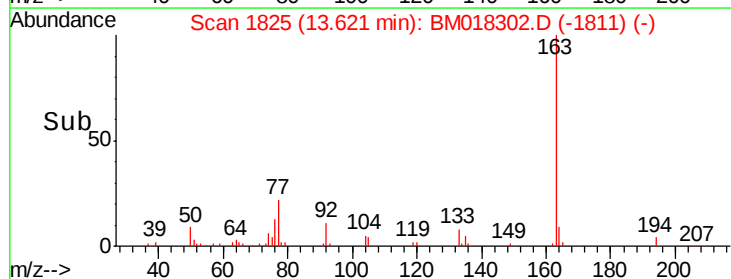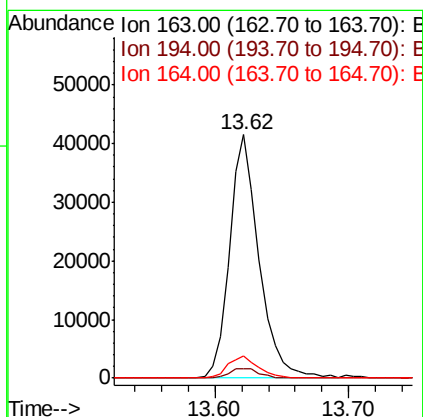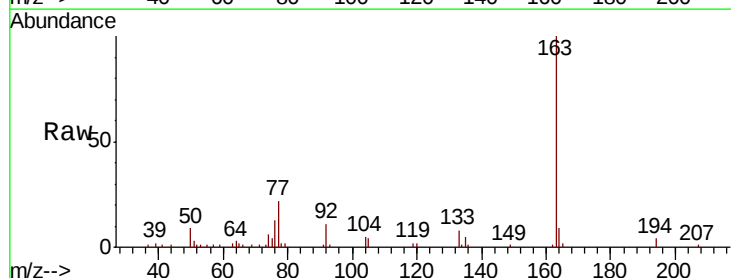


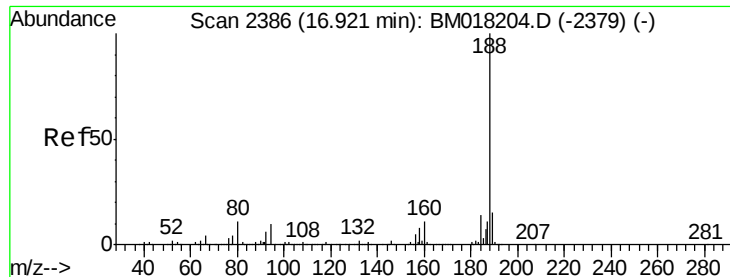




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.91 min Scan# 2384
Delta R.T. -0.01 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Instrument :
BNA_M
ClientSampleId :
EB01_0-2

Tgt Ion:188 Resp: 344127
Ion Ratio Lower Upper
188 100
94 9.2 8.0 12.0
80 9.5 9.0 13.6

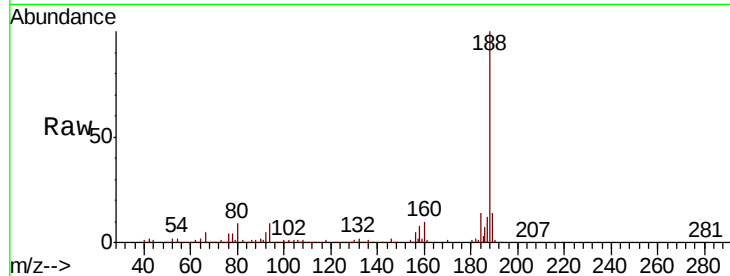


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

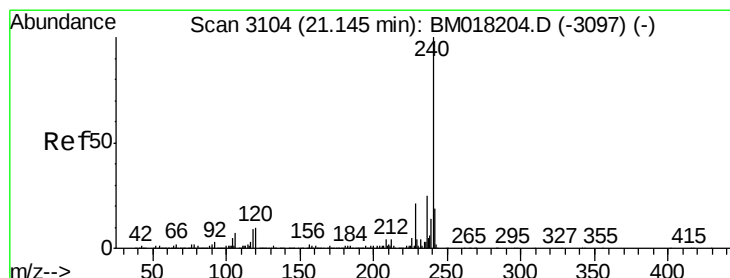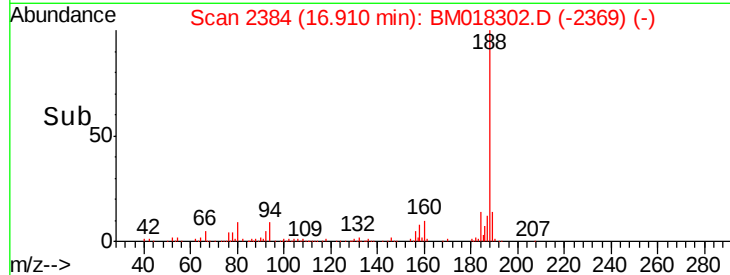
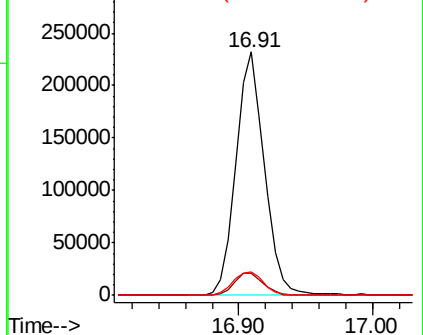



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.13 min Scan# 3102
Delta R.T. -0.01 min
Lab File: BM018302.D
Acq: 19 Dec 2018 18:34

Tgt Ion:240 Resp: 370524
Ion Ratio Lower Upper
240 100
120 9.6 8.2 12.2
236 25.5 20.3 30.5

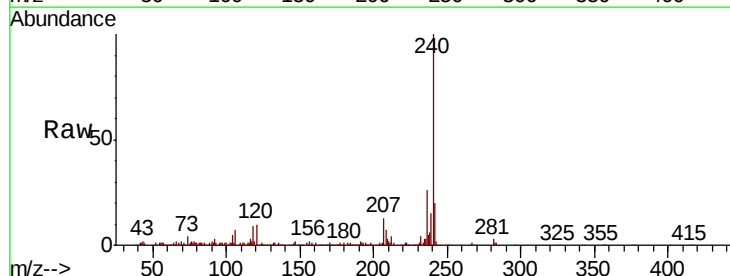

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

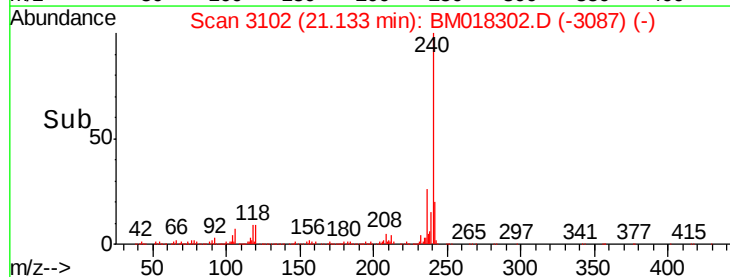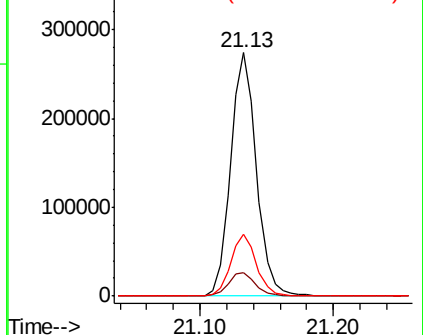

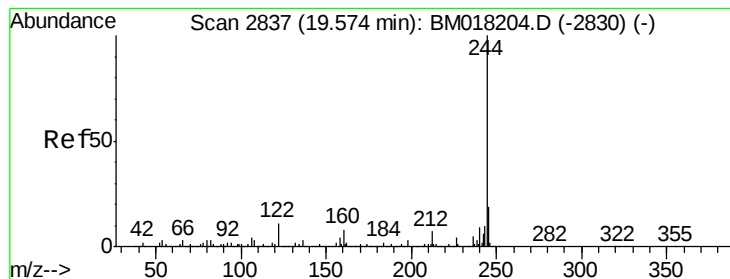

#79

Terphenyl-d14

Concen: 69.026 ng

RT: 19.56 min Scan# 2835

Delta R.T. -0.01 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34

Instrument :

BNA_M

ClientSampleId :

EB01_0-2


Tgt Ion:244 Resp: 1130850

Ion Ratio Lower Upper

244 100

212 7.3 5.8 8.8




122 9.9 9.0 13.6

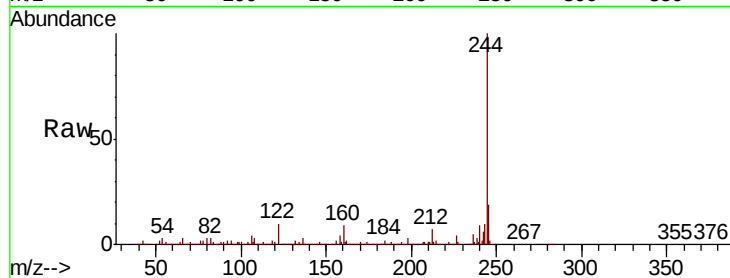

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

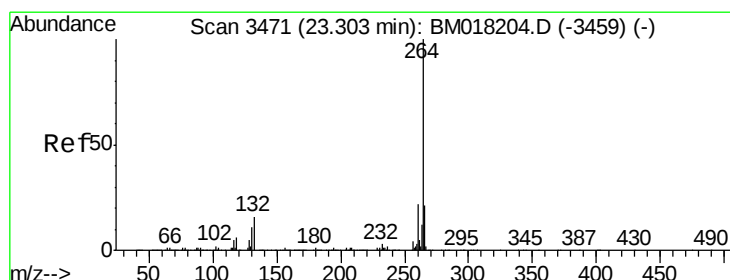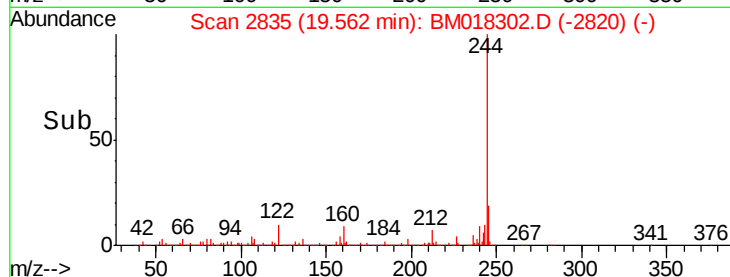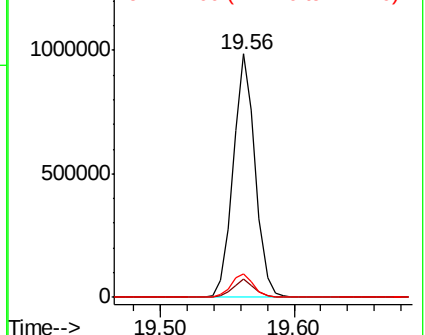

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.29 min Scan# 3469

Delta R.T. -0.01 min

Lab File: BM018302.D

Acq: 19 Dec 2018 18:34


Tgt Ion:264 Resp: 422000

Ion Ratio Lower Upper

264 100

260 22.9 17.5 26.3

265 22.1 17.3 25.9

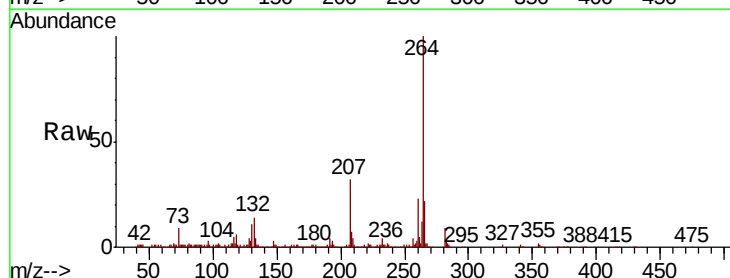

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

