

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121918\
 Data File : BM018303.D
 Acq On : 19 Dec 2018 19:11
 Operator : JU/SJ
 Sample : J6477-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-A1

Quant Time: Dec 20 01:07:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	90943	20.00	ng	-0.02
21) Naphthalene-d8	10.25	136	333795	20.00	ng	-0.02
39) Acenaphthene-d10	14.15	164	172679	20.00	ng	-0.02
64) Phenanthrene-d10	16.91	188	348221	20.00	ng	-0.01
76) Chrysene-d12	21.13	240	353079	20.00	ng	-0.01
87) Perylene-d12	23.29	264	395040	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	823245	151.22	ng	0.00
7) Phenol-d6	6.69	99	1076955	142.32	ng	-0.02
23) Nitrobenzene-d5	8.65	82	681454	104.72	ng	-0.02
42) 2,4,6-Tribromophenol	15.65	330	319349	126.00	ng	-0.02
45) 2-Fluorobiphenyl	12.75	172	1240358	93.04	ng	-0.02
79) Terphenyl-d14	19.56	244	1498305	95.97	ng	-0.01
Target Compounds						
10) Phenol	6.72	94	78695	9.820	ng	94
15) Benzyl Alcohol	7.80	79	13190	2.139	ng	# 45
50) Dimethylphthalate	13.62	163	85692	5.969	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121918\
Data File : BM018303.D
Acq On : 19 Dec 2018 19:11
Operator : JU/SJ
Sample : J6477-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-A1

Quant Time: Dec 20 01:07:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

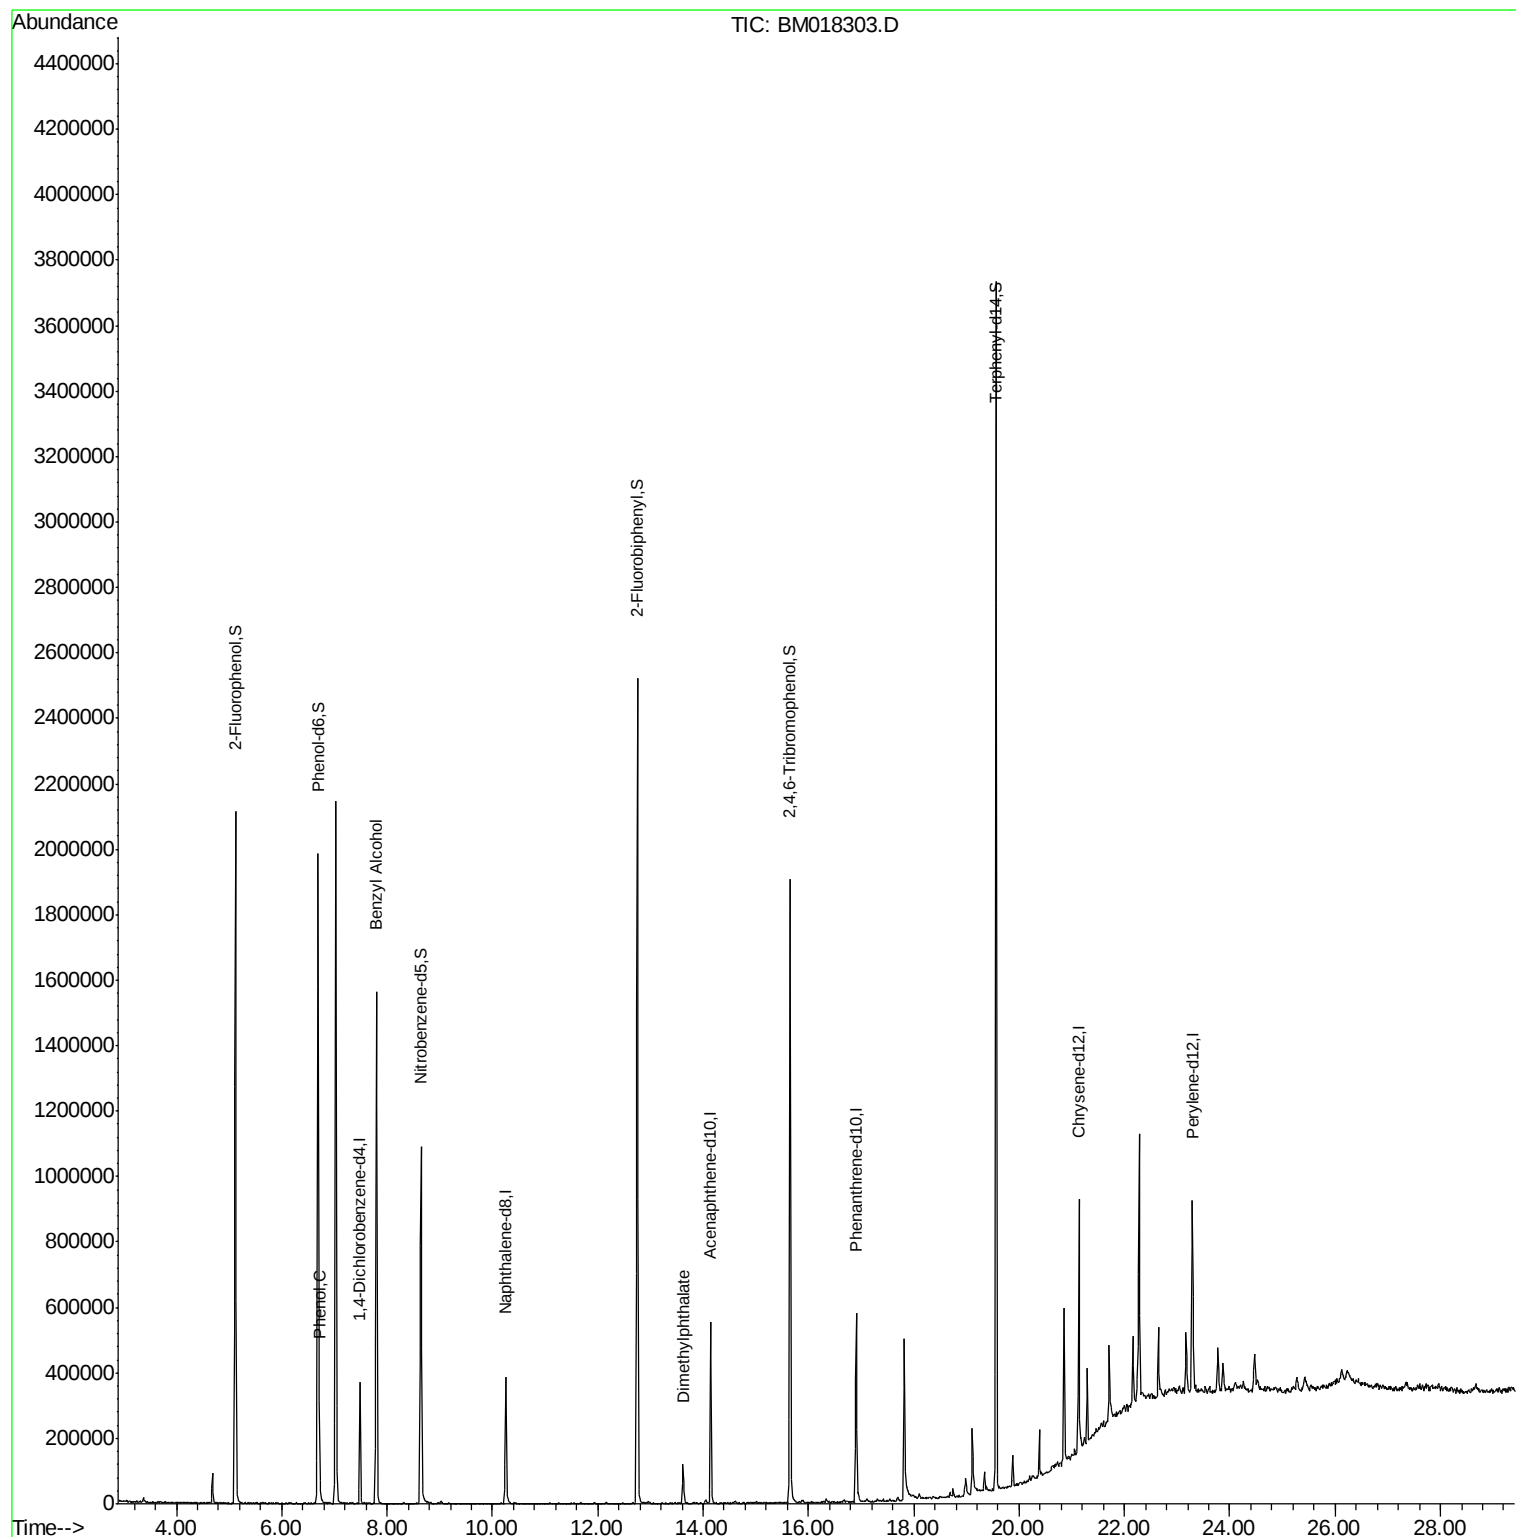




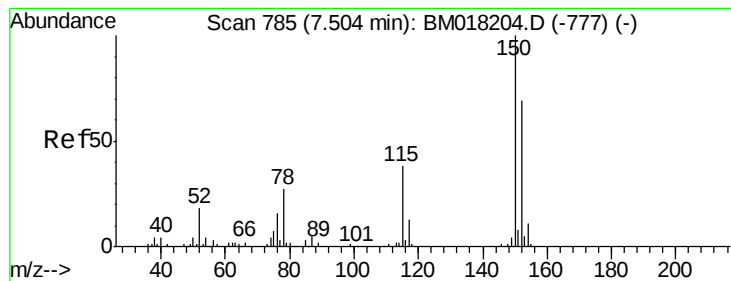


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.49 min Scan# 782
Delta R.T. -0.02 min
Lab File: BM018303.D
Acq: 19 Dec 2018 19:11

Instrument :
BNA_M
ClientSampleId :
SB-A1




Tgt Ion:152 Resp: 90943
Ion Ratio Lower Upper
152 100
150 163.0 116.1 174.1
115 66.0 44.6 67.0

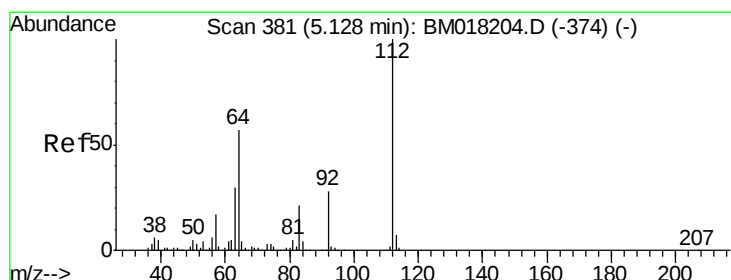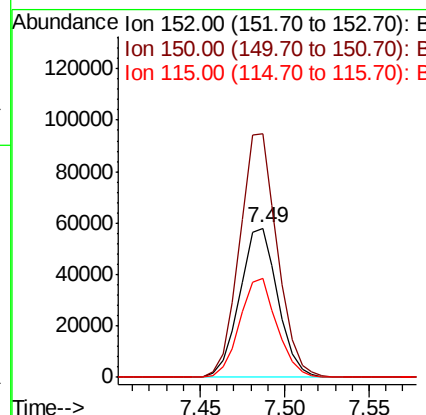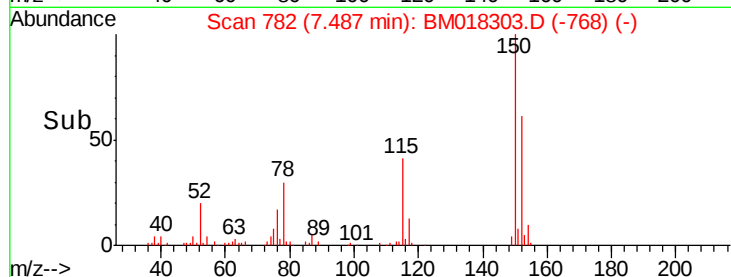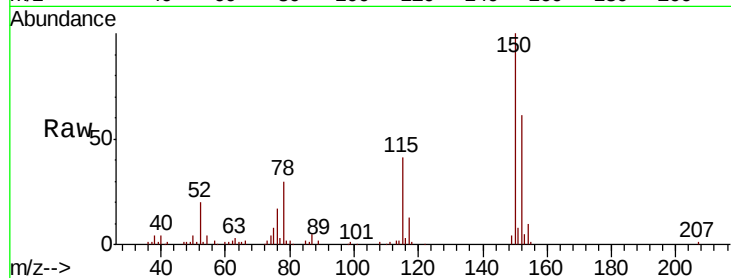

#5

2-Fluorophenol
Concen: 151.218 ng
RT: 5.12 min Scan# 380
Delta R.T. -0.01 min
Lab File: BM018303.D
Acq: 19 Dec 2018 19:11

Tgt Ion:112 Resp: 823245
Ion Ratio Lower Upper
112 100
64 58.3 45.4 68.2
63 32.3 24.0 36.0

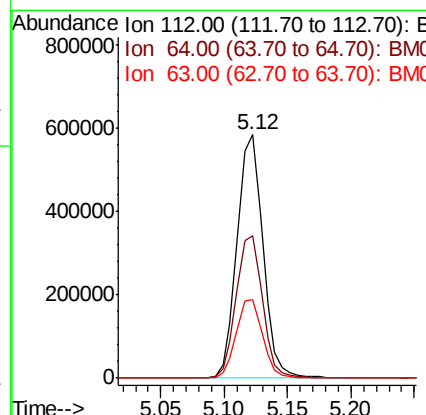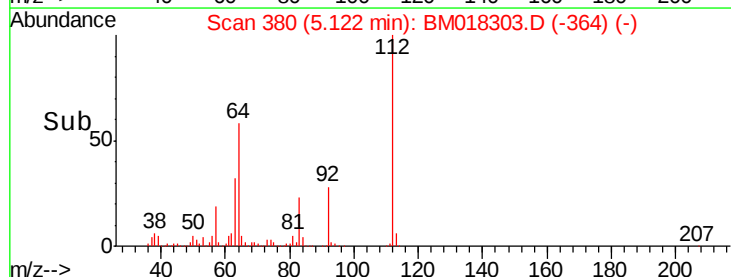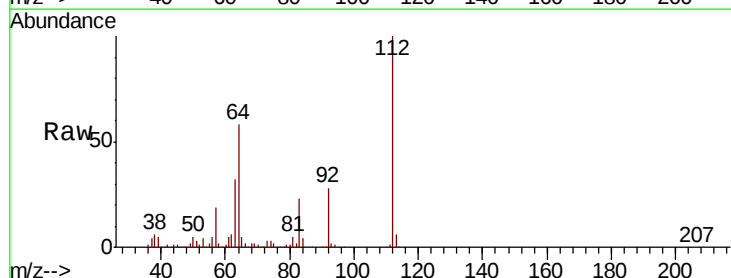



#7

Phenol-d6

Concen: 142.325 ng

RT: 6.69 min Scan# 646

Delta R.T. -0.02 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11

Instrument :

BNA_M

ClientSampleId :

SB-A1


Tgt Ion: 99 Resp: 1076955

Ion Ratio Lower Upper

99 100

42 16.3 12.3 18.5




71 40.0 30.2 45.2



Abundance Ion 99.00 (98.70 to 99.70): BM018303.D (-632) (-)

Ion 42.00 (41.70 to 42.70): BM018303.D (-632) (-)

Ion 71.00 (70.70 to 71.70): BM018303.D (-632) (-)

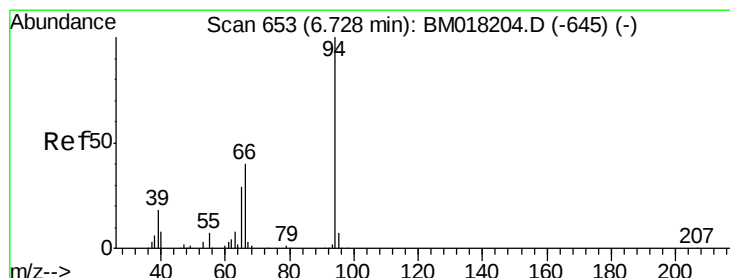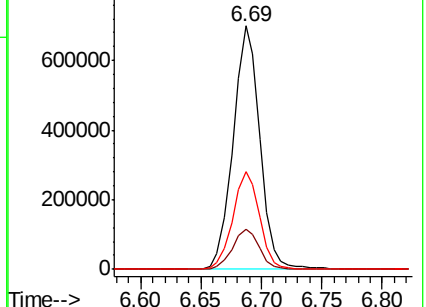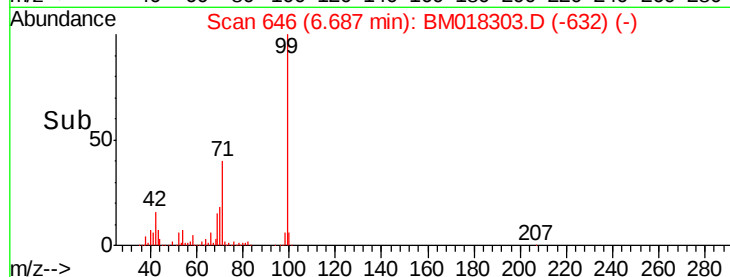

#10

Phenol

Concen: 9.820 ng

RT: 6.72 min Scan# 651

Delta R.T. -0.01 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11


Tgt Ion: 94 Resp: 78695

Ion Ratio Lower Upper

94 100

65 27.2 9.5 49.5



66 46.2 21.3 61.3




Abundance Ion 94.00 (93.70 to 94.70): BM018303.D (-636) (-)

Ion 65.00 (64.70 to 65.70): BM018303.D (-636) (-)

Ion 66.00 (65.70 to 66.70): BM018303.D (-636) (-)

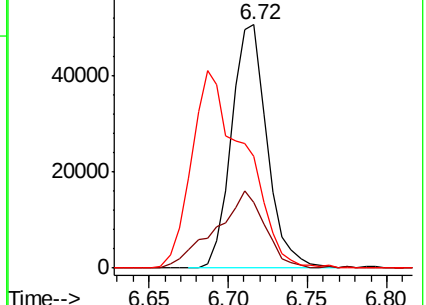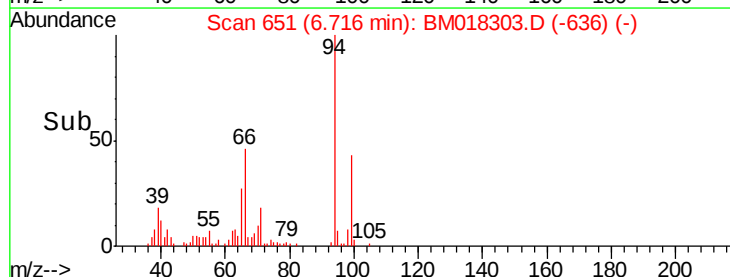

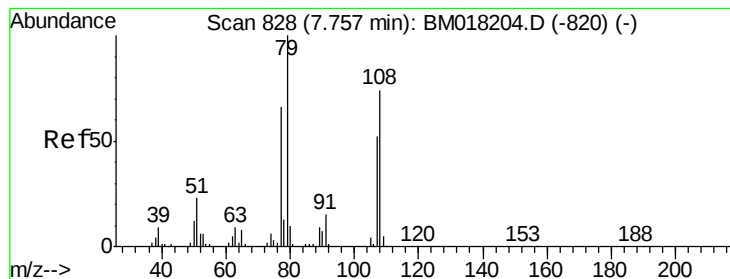

#15

Benzyl Alcohol

Concen: 2.139 ng

RT: 7.80 min Scan# 835

Delta R.T. 0.04 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11

Instrument :

BNA_M

ClientSampleId :

SB-A1


Tgt Ion: 79 Resp: 13190

Ion Ratio Lower Upper

79 100

108 43.3 59.3 88.9#




77 126.3 53.0 79.4#



Abundance Ion 79.00 (78.70 to 79.70): BM018204.D (-820) (-)

Ion 108.00 (107.70 to 108.70): BM018204.D (-820) (-)

Ion 77.00 (76.70 to 77.70): BM018204.D (-820) (-)

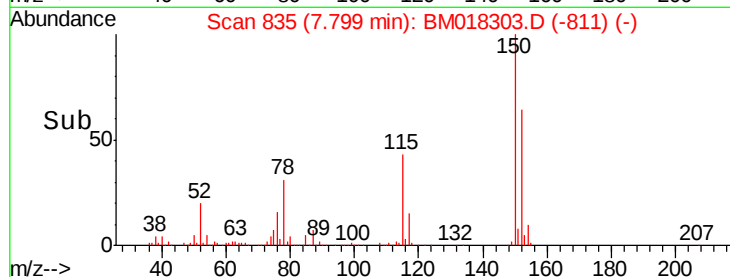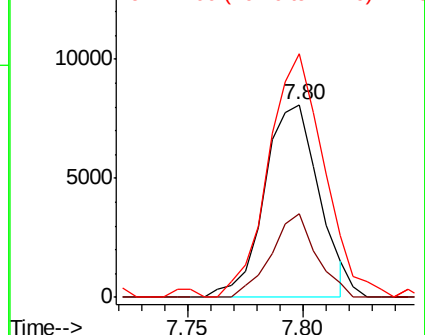

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.25 min Scan# 1252

Delta R.T. -0.02 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11

Tgt Ion: 136 Resp: 333795


Ion Ratio Lower Upper

136 100

137 10.7 9.2 13.8

54 6.3 5.2 7.8

68 6.9 5.0 7.6






Abundance Ion 136.00 (135.70 to 136.70): BM018204.D (-1247) (-)

Ion 137.00 (136.70 to 137.70): BM018204.D (-1247) (-)

Ion 54.00 (53.70 to 54.70): BM018204.D (-1247) (-)

Ion 68.00 (67.70 to 68.70): BM018204.D (-1247) (-)



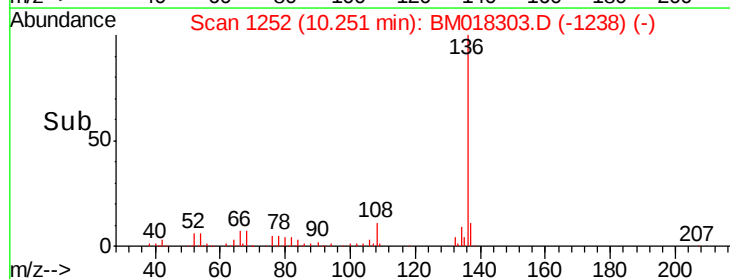
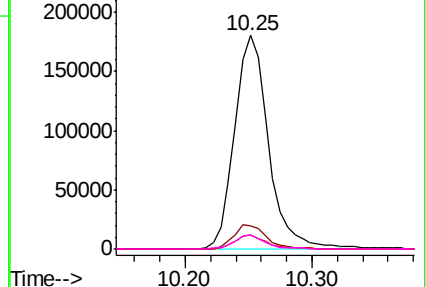


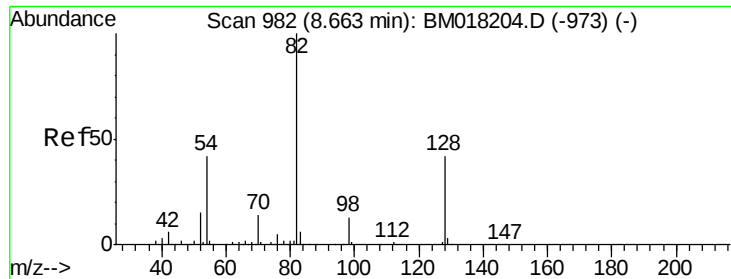

#23
 Nitrobenzene-d5
 Concen: 104.718 ng
 RT: 8.65 min Scan# 979
 Delta R.T. -0.02 min
 Lab File: BM018303.D
 Acq: 19 Dec 2018 19:11




Instrument :
 BNA_M
 ClientSampleId :
 SB-A1


Tgt Ion	Ratio	Lower	Upper
82	100		
128	38.5	33.4	50.2
54	42.2	33.4	50.2

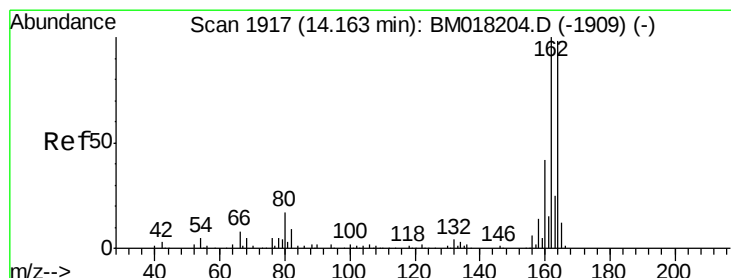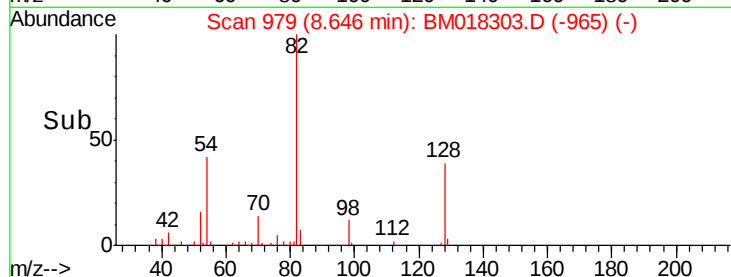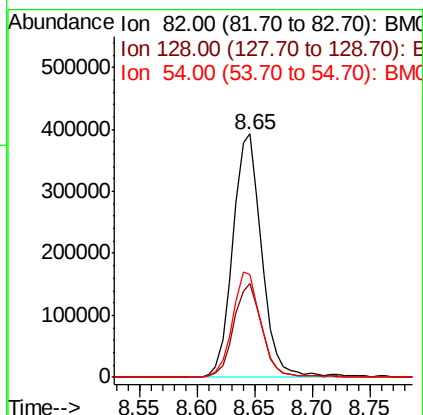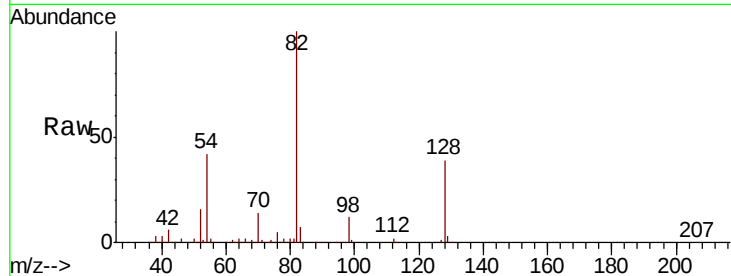

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.15 min Scan# 1914
 Delta R.T. -0.02 min
 Lab File: BM018303.D
 Acq: 19 Dec 2018 19:11

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.2	81.8	122.6
160	45.6	34.6	51.8

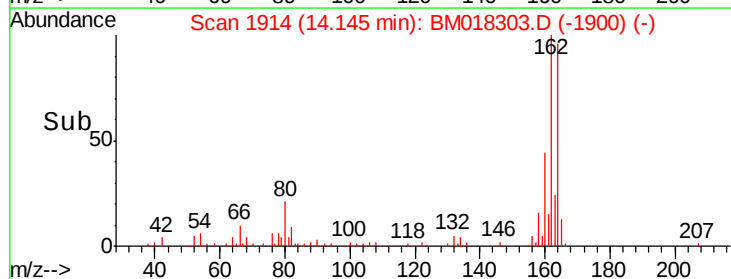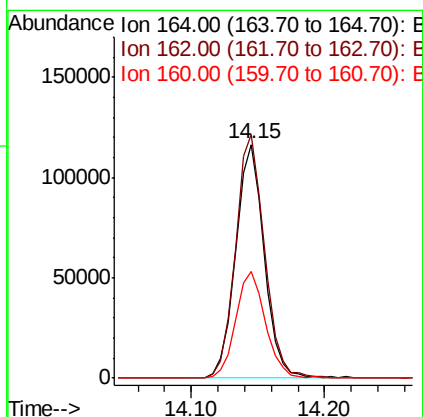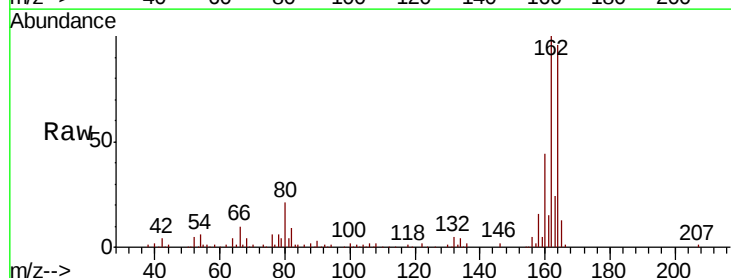

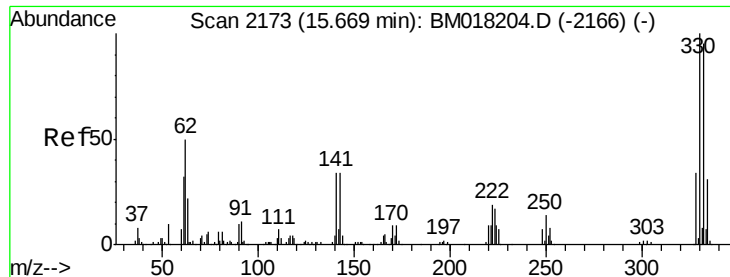

#42

2,4,6-Tribromophenol

Concen: 126.003 ng

RT: 15.65 min Scan# 2170

Delta R.T. -0.02 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11

Instrument :

BNA_M

ClientSampleId :

SB-A1


Tgt Ion:330 Resp: 319349

Ion Ratio Lower Upper

330 100

332 98.0 78.6 118.0

141 39.8 27.1 40.7



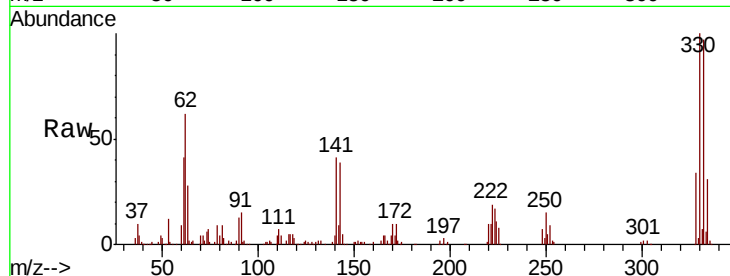


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

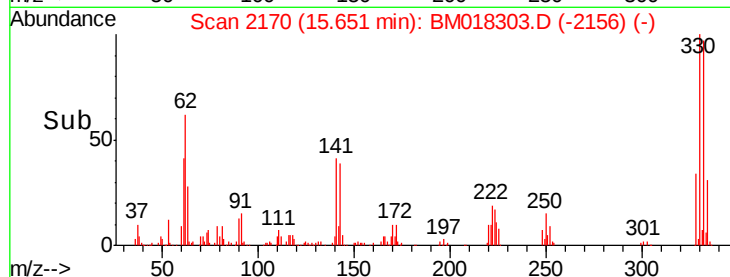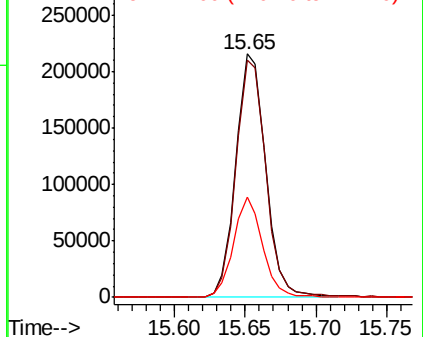

#45

2-Fluorobiphenyl

Concen: 93.037 ng

RT: 12.75 min Scan# 1677

Delta R.T. -0.02 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11


Tgt Ion:172 Resp: 1240358

Ion Ratio Lower Upper

172 100

171 35.1 28.3 42.5

170 22.8 18.1 27.1






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

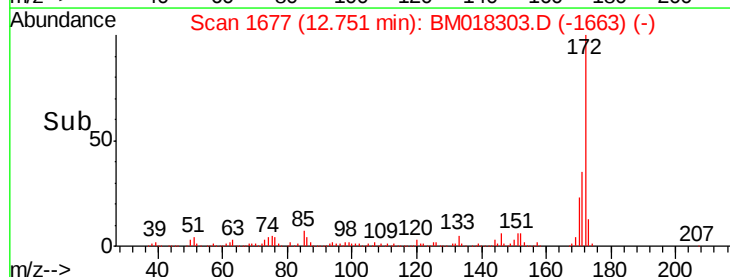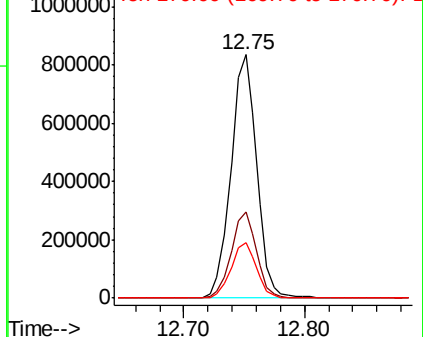

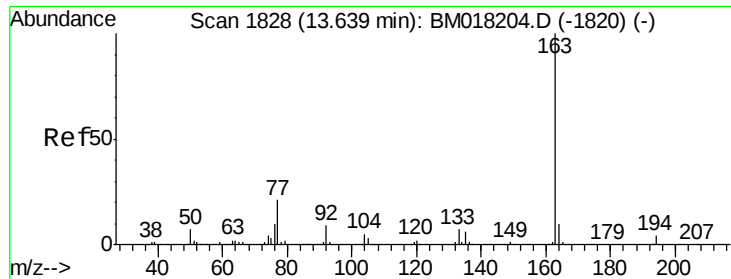

#50

Dimethylphthalate

Concen: 5.969 ng

RT: 13.62 min Scan# 1825

Delta R.T. -0.02 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11

Instrument :

BNA_M

ClientSampleId :

SB-A1


Tgt Ion:163 Resp: 85692

Ion Ratio Lower Upper

163 100

194 4.3 3.1 4.7




164 9.3 7.9 11.9

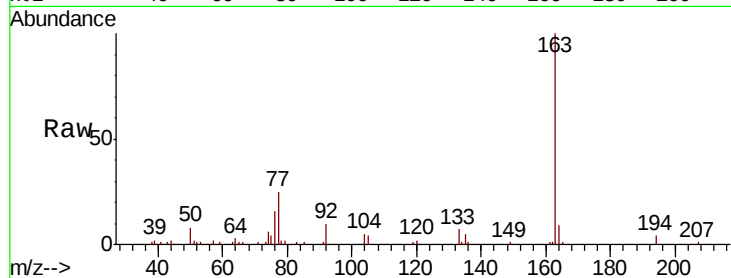

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

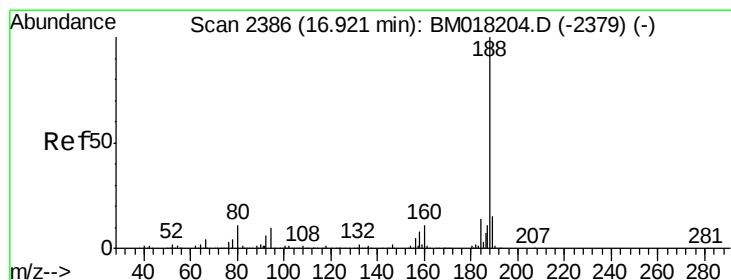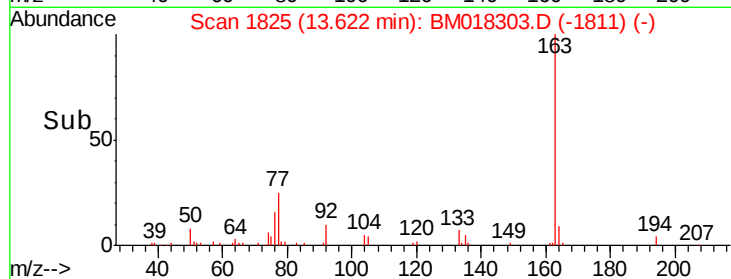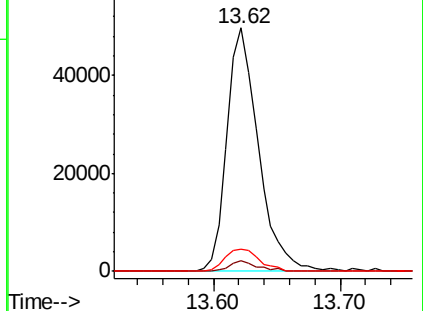

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.91 min Scan# 2384

Delta R.T. -0.01 min

Lab File: BM018303.D

Acq: 19 Dec 2018 19:11


Tgt Ion:188 Resp: 348221

Ion Ratio Lower Upper

188 100

94 8.1 8.0 12.0



80 9.4 9.0 13.6

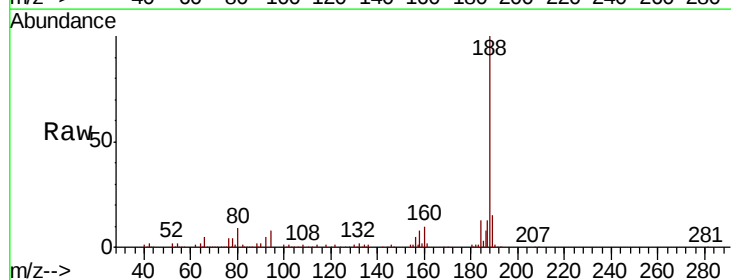


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0



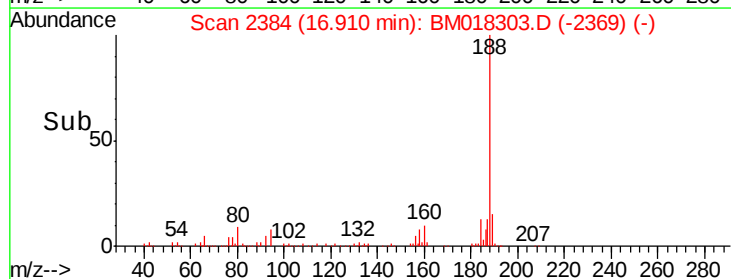
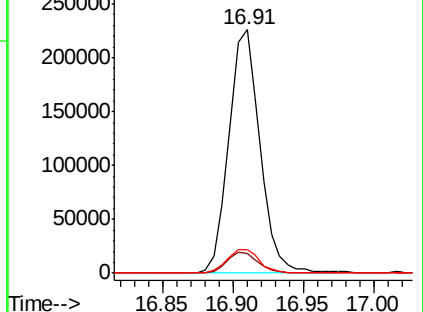


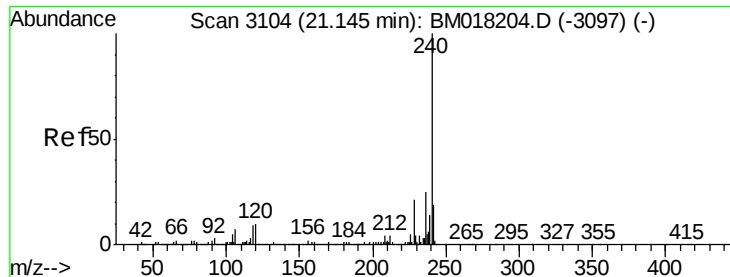

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.13 min Scan# 3102
Delta R.T. -0.01 min
Lab File: BM018303.D
Acq: 19 Dec 2018 19:11




Instrument :
BNA_M
ClientSampleId :
SB-A1


Tgt Ion	Ratio	Lower	Upper
240	100		
120	8.5	8.2	12.2
236	25.2	20.3	30.5

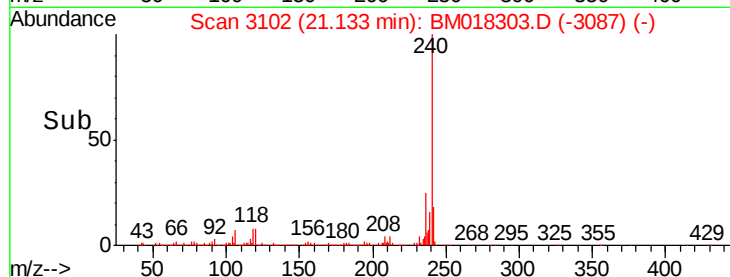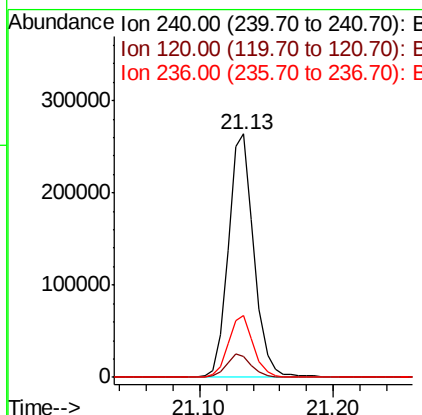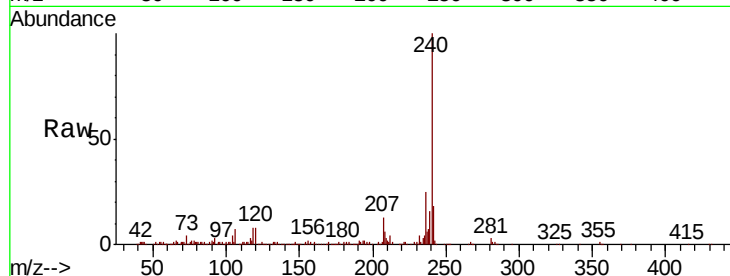

#79
Terphenyl-d14
Concen: 95.974 ng
RT: 19.56 min Scan# 2835
Delta R.T. -0.01 min
Lab File: BM018303.D
Acq: 19 Dec 2018 19:11

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.0	5.8	8.8
122	9.8	9.0	13.6

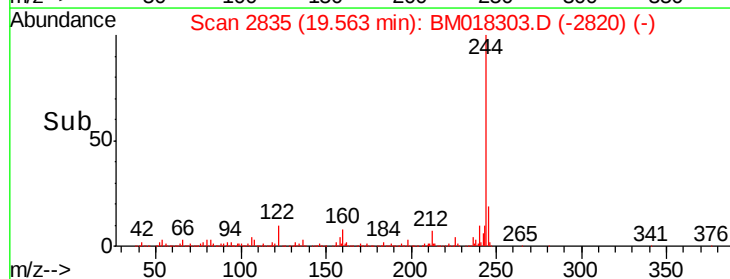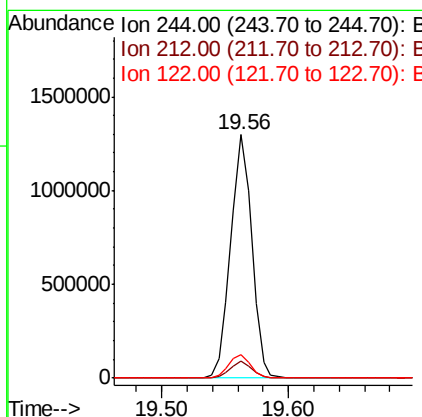

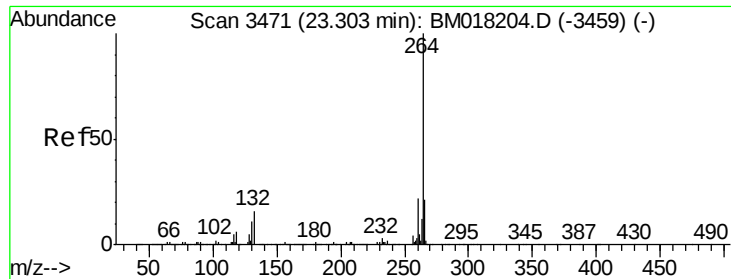

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.29 min Scan# 3469
Delta R.T. -0.01 min
Lab File: BM018303.D
Acq: 19 Dec 2018 19:11

Instrument :
BNA_M
ClientSampleId :
SB-A1

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.7	17.5	26.3
265	21.6	17.3	25.9

