


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121918\
 Data File : BM018289.D
 Acq On : 19 Dec 2018 08:47
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

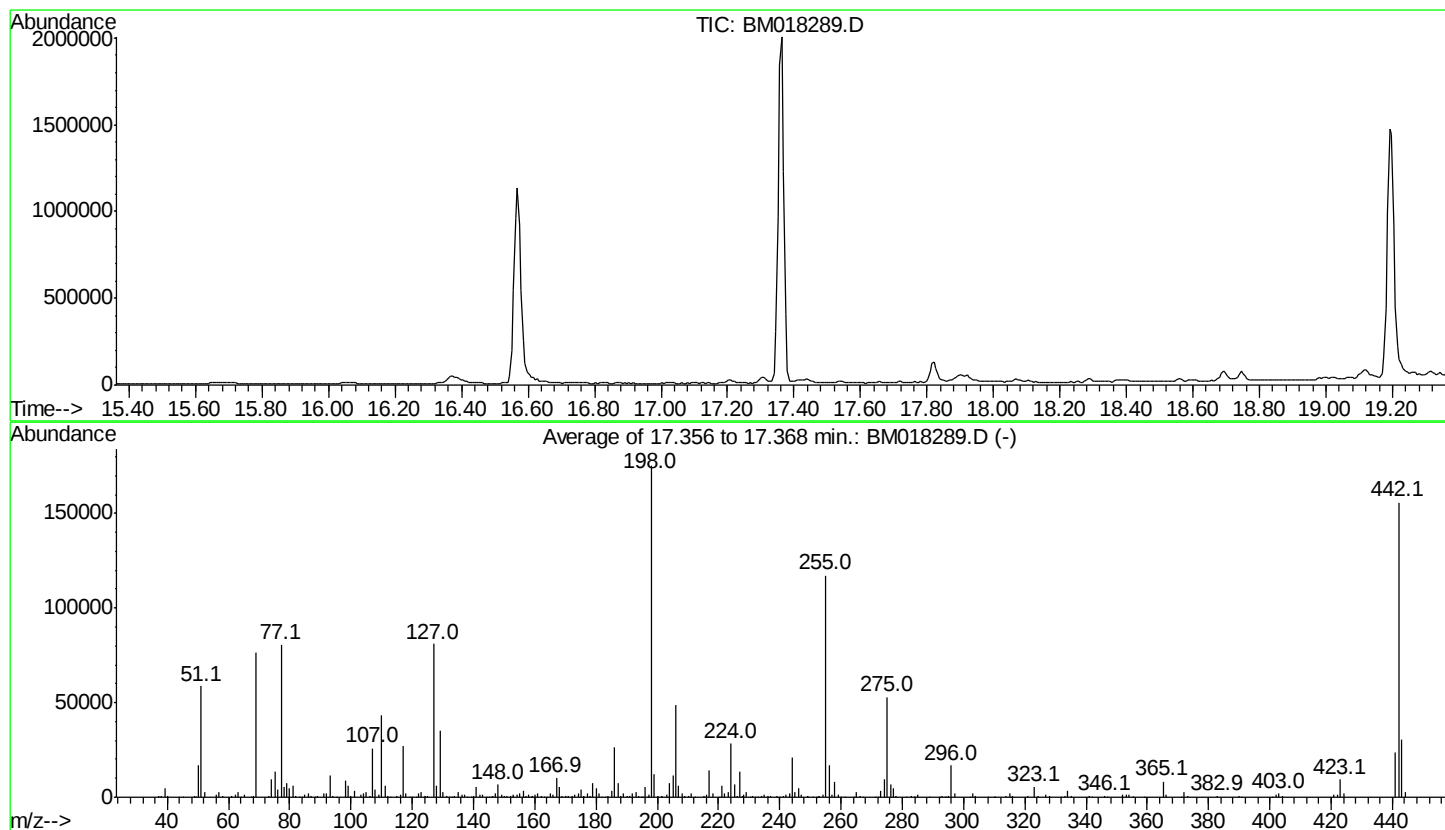

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	58624	PASS
68	69	0.00	2	1.3	1034	PASS
69	198	0.00	100	43.7	76659	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	80949	PASS
197	198	0.00	2	0.7	1175	PASS
198	198	100	100	100.0	175250	PASS
199	198	5	9	6.9	12134	PASS
275	198	10	60	30.2	52944	PASS
365	198	1	100	4.8	8447	PASS
441	198	0.01	100	13.7	23989	PASS
442	198	50	100	88.9	155797	PASS
443	442	15	24	19.7	30632	PASS