
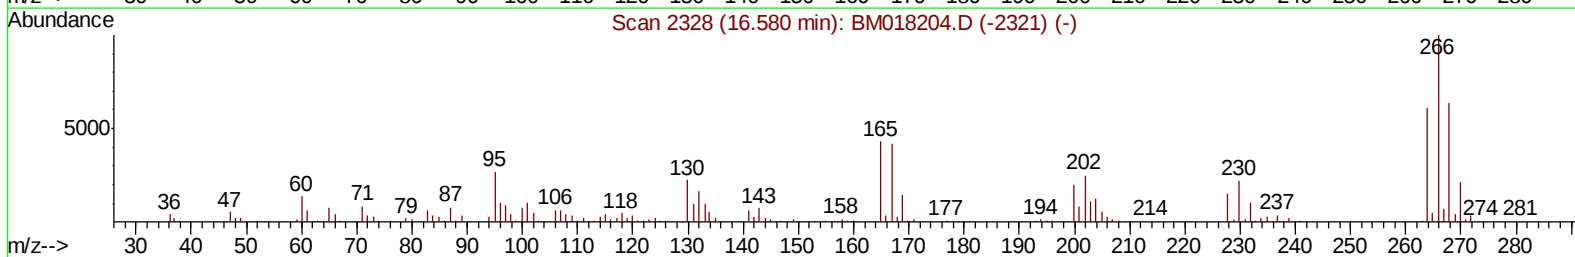
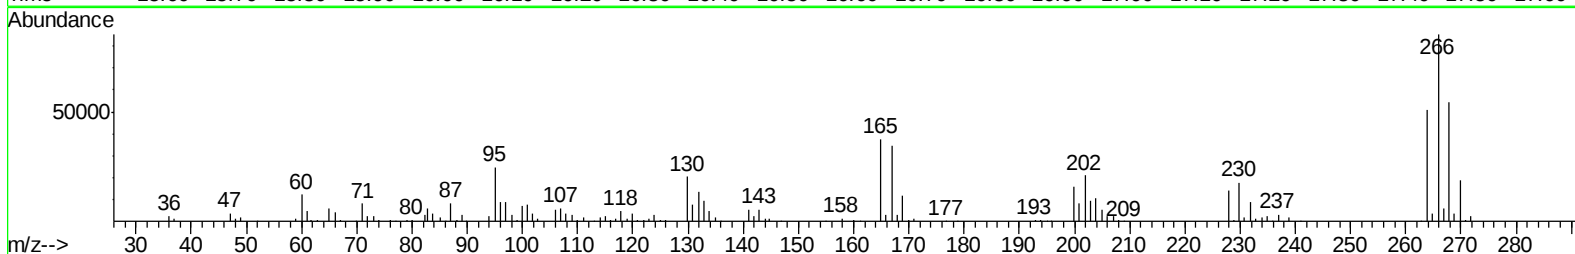


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122018\
Data File : BM018330.D
Acq On : 20 Dec 2018 14:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 01:20:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 21:39:37 2018
Response via : Initial Calibration

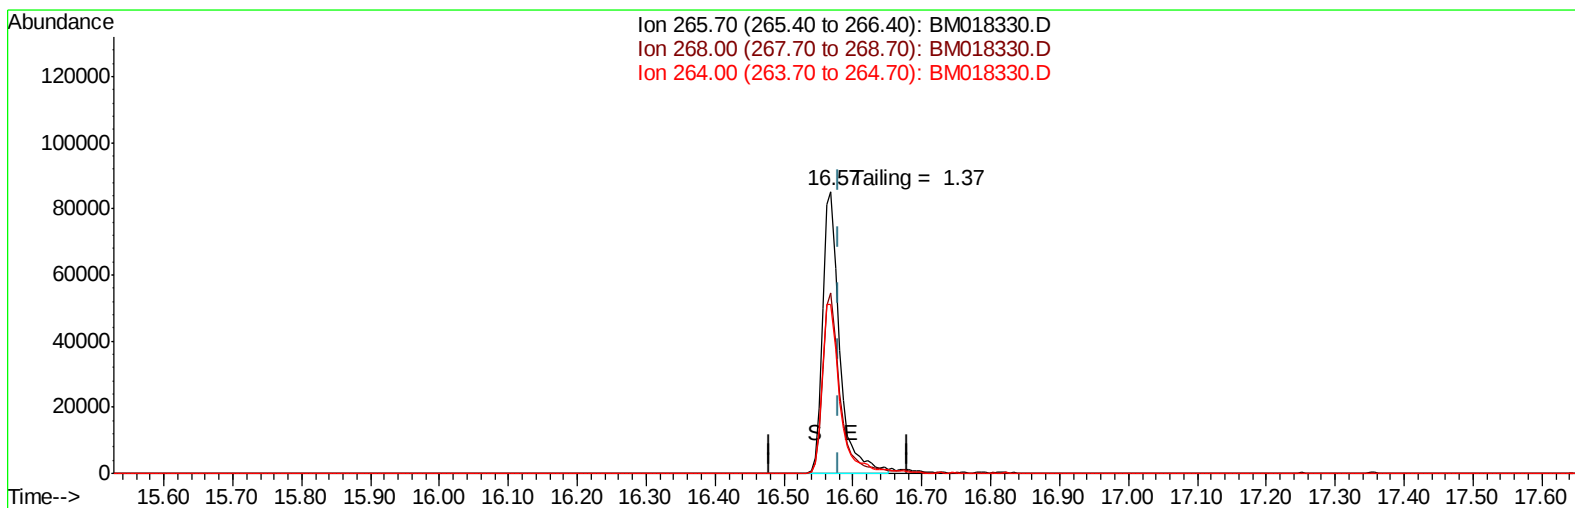

TIC: BM018330.D

(70) Pentachlorophenol (C)




16.568min (-0.012) 0.00ng

response 145368

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.02
264.00	61.20	59.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122018\
 Data File : BM018330.D
 Acq On : 20 Dec 2018 14:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 21 01:20:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 21:39:37 2018
 Response via : Initial Calibration

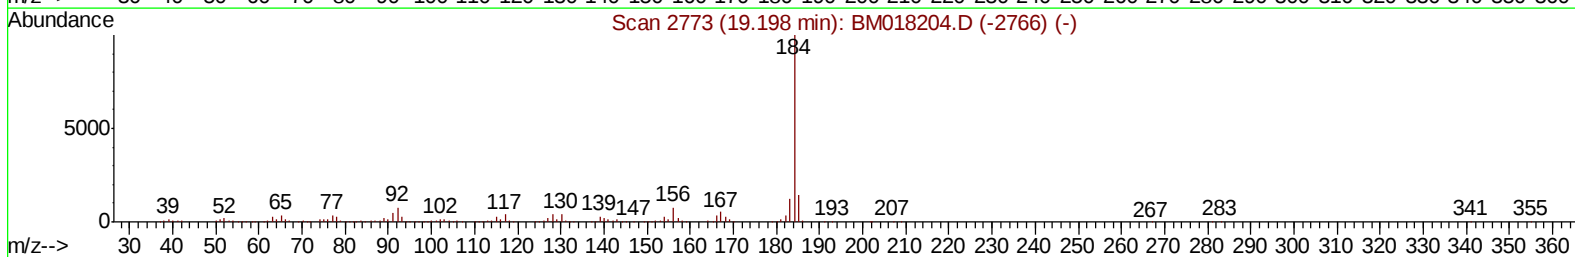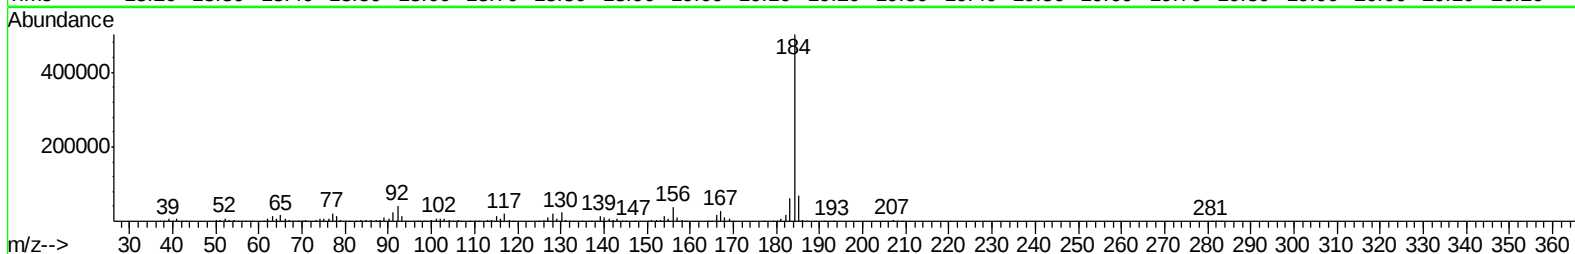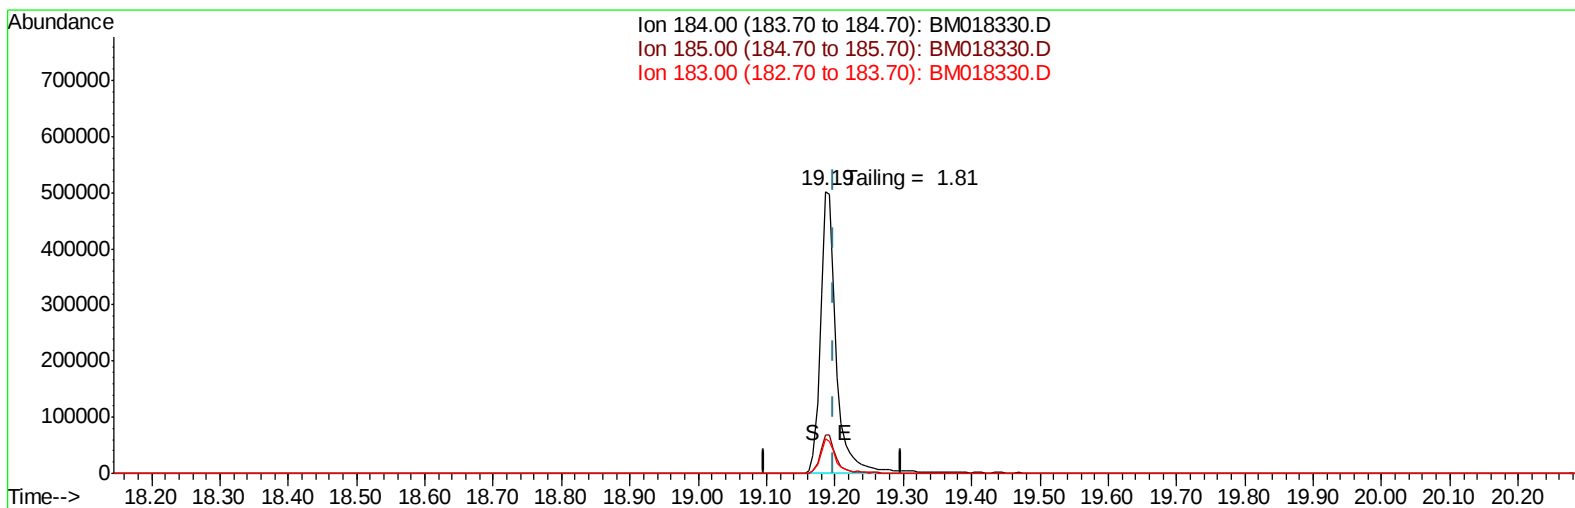

TIC: BM018330.D

(77) Benzidine

19.186min (-0.012) 13493.76ng

response 810273

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.71
183.00	12.10	12.16
0.00	0.00	0.00