


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122118\
 Data File : BM018350.D
 Acq On : 21 Dec 2018 08:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

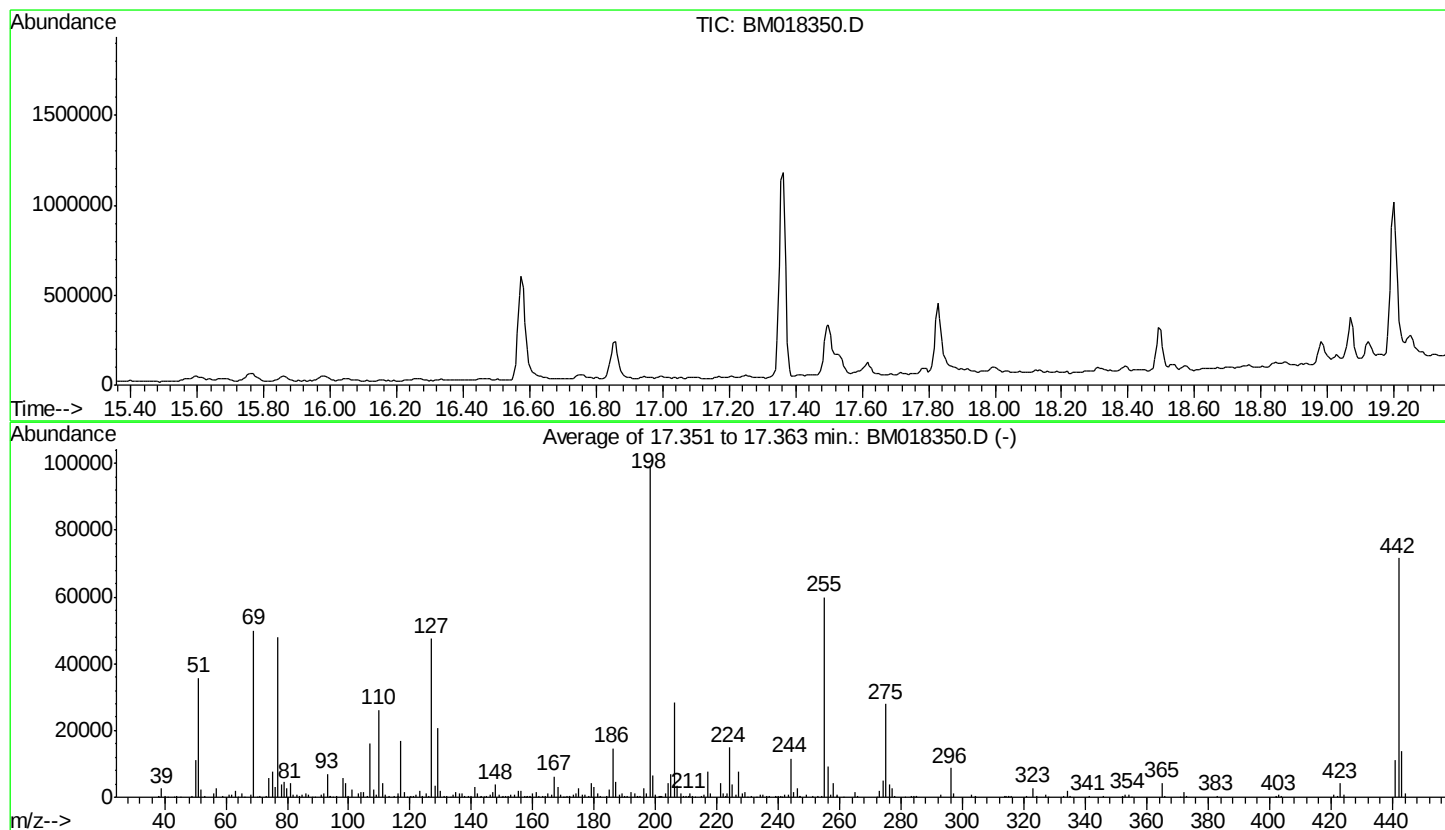

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	35826	PASS
68	69	0.00	2	1.9	933	PASS
69	198	0.00	100	50.3	50003	PASS
70	69	0.00	2	0.1	36	PASS
127	198	10	80	47.7	47418	PASS
197	198	0.00	2	1.1	1081	PASS
198	198	100	100	100.0	99317	PASS
199	198	5	9	6.6	6532	PASS
275	198	10	60	28.0	27850	PASS
365	198	1	100	4.4	4375	PASS
441	198	0.01	100	11.2	11155	PASS
442	198	50	100	72.0	71517	PASS
443	442	15	24	19.3	13787	PASS