


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122118\
 Data File : BM018361.D
 Acq On : 21 Dec 2018 16:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

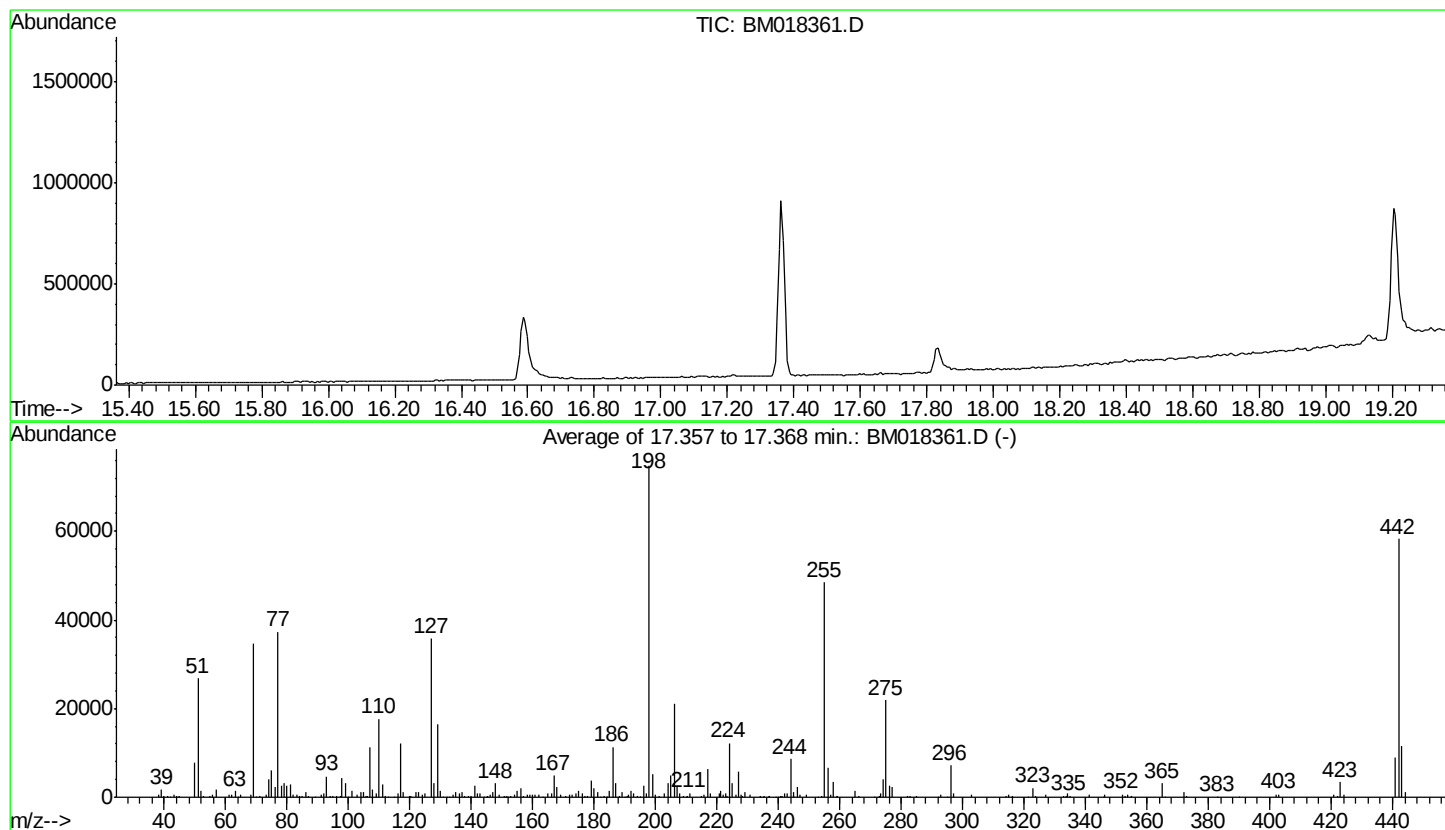

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	26800	PASS
68	69	0.00	2	1.5	515	PASS
69	198	0.00	100	46.5	34769	PASS
70	69	0.00	2	0.2	62	PASS
127	198	10	80	47.8	35757	PASS
197	198	0.00	2	1.1	838	PASS
198	198	100	100	100.0	74826	PASS
199	198	5	9	7.0	5239	PASS
275	198	10	60	29.3	21888	PASS
365	198	1	100	4.2	3151	PASS
441	198	0.01	100	12.2	9097	PASS
442	198	50	100	77.9	58280	PASS
443	442	15	24	19.8	11520	PASS