


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122118\
 Data File : BM018379.D
 Acq On : 22 Dec 2018 10:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM121518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 15 21:39:37 2018

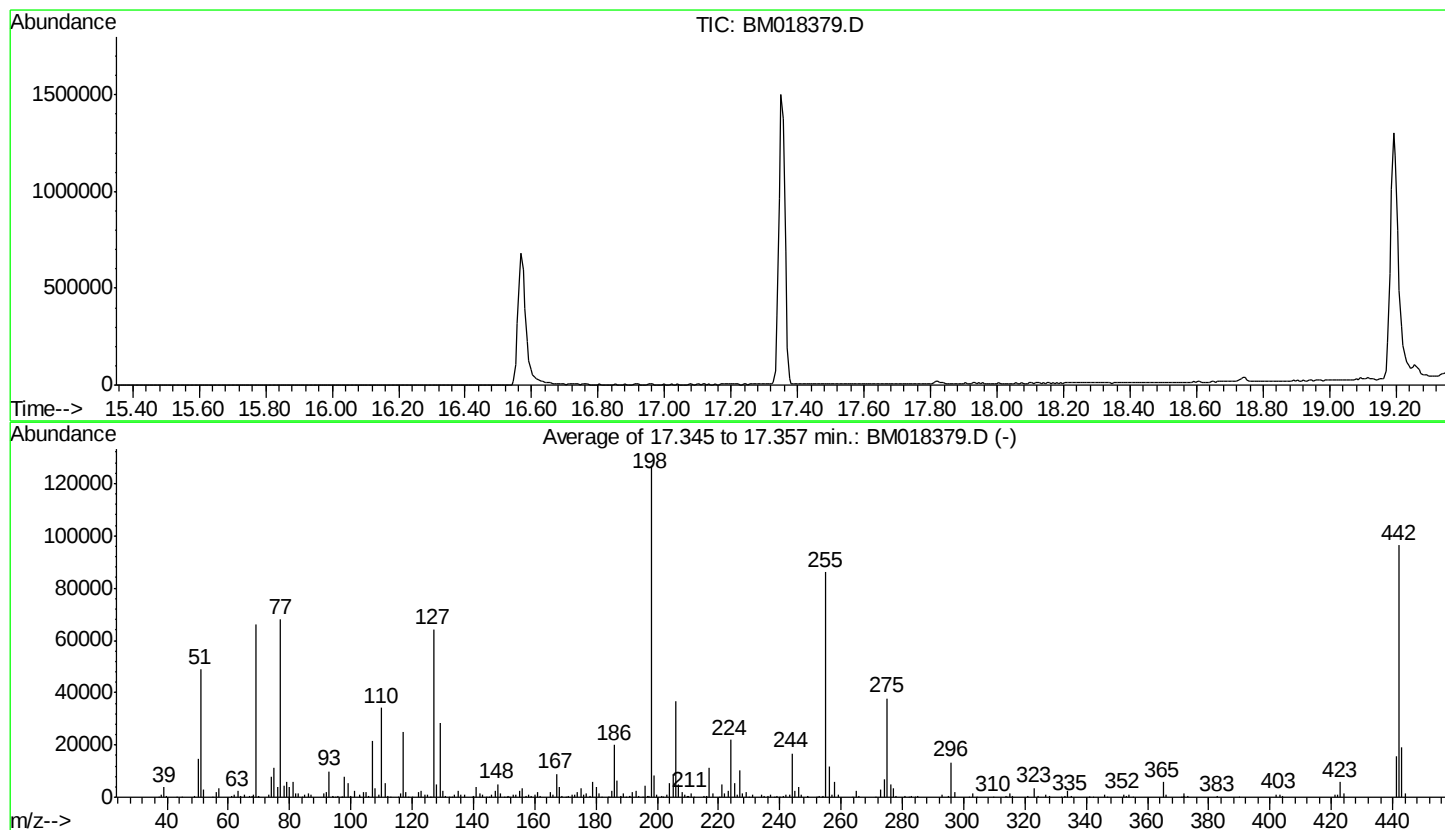

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	48848	PASS
68	69	0.00	2	1.2	774	PASS
69	198	0.00	100	52.2	66253	PASS
70	69	0.00	2	0.7	478	PASS
127	198	10	80	50.5	64072	PASS
197	198	0.00	2	0.4	551	PASS
198	198	100	100	100.0	126850	PASS
199	198	5	9	6.5	8236	PASS
275	198	10	60	29.9	37922	PASS
365	198	1	100	4.6	5848	PASS
441	198	0.01	100	12.2	15481	PASS
442	198	50	100	76.0	96370	PASS
443	442	15	24	19.8	19118	PASS