
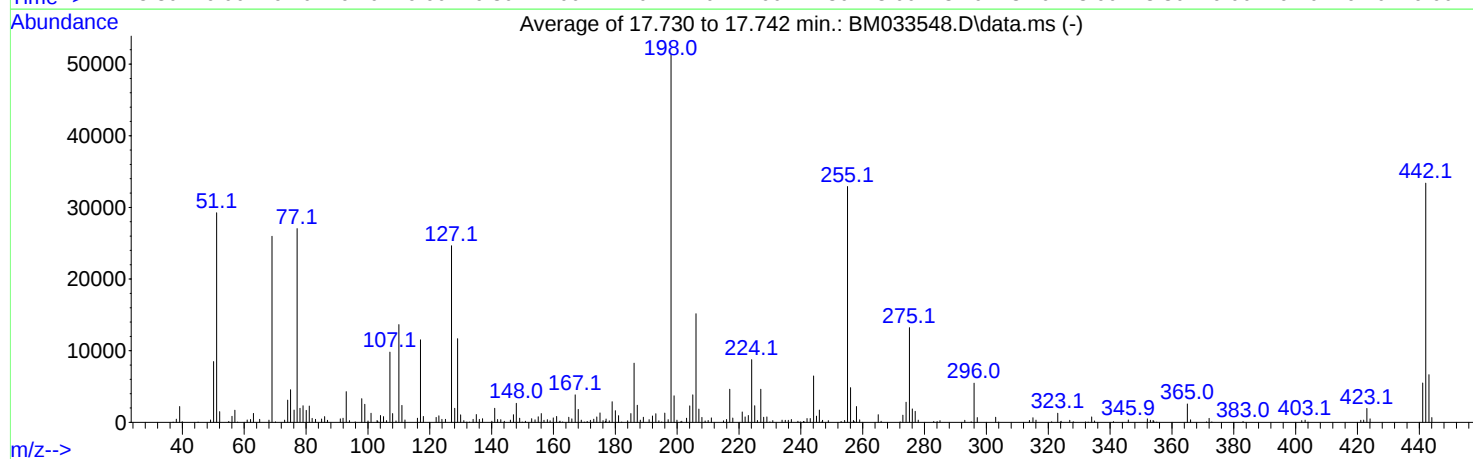


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122121\
 Data File : BM033548.D
 Acq On : 21 Dec 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 21 16:25:49 2021

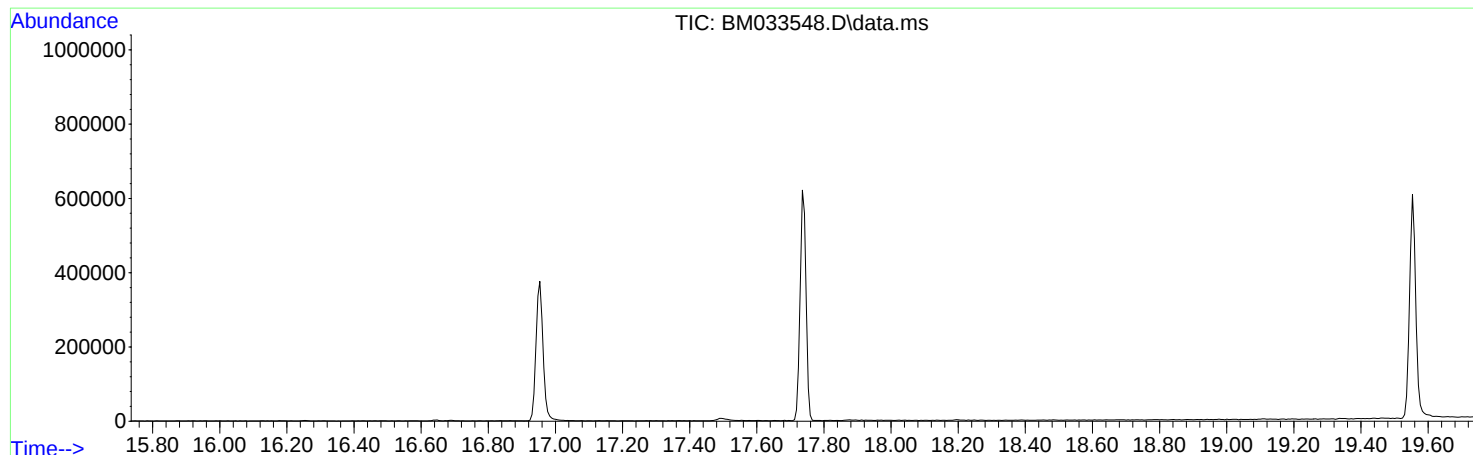




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	29256	PASS
68	69	0.00	2	1.2	316	PASS
69	198	0.00	100	50.6	25979	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	48.0	24648	PASS
197	198	0.00	2	0.7	380	PASS
198	198	100	100	100.0	51339	PASS
199	198	5	9	7.2	3701	PASS
275	198	10	60	25.8	13226	PASS
365	198	1	100	5.0	2571	PASS
441	198	0.01	100	10.7	5505	PASS
442	442	50	100	100.0	33392	PASS
443	442	15	24	19.9	6660	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122121\
Data File : BM033548.D
Acq On : 21 Dec 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 21 13:56:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 13:51:44 2021
Response via : Initial Calibration

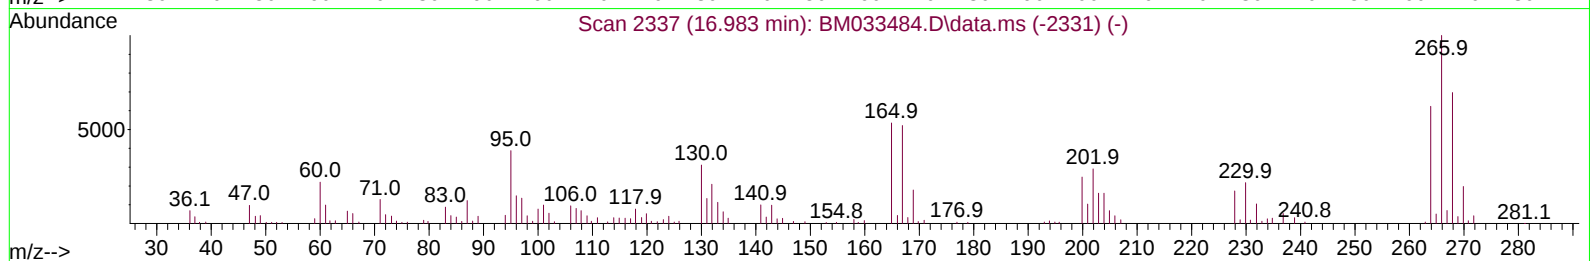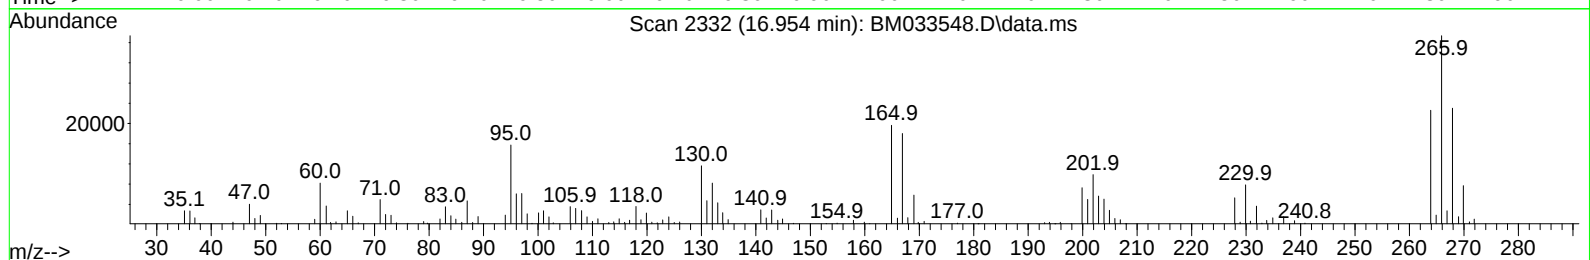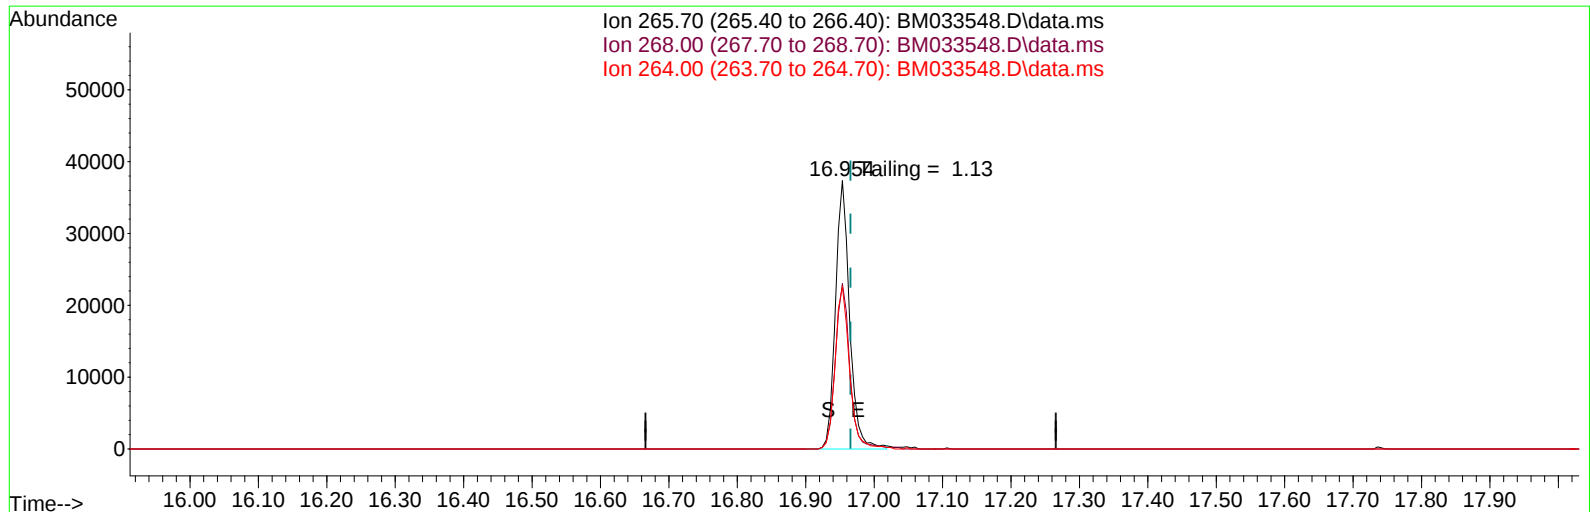

TIC: BM033548.D\data.ms

(70) Pentachlorophenol (C)

16.954min (-0.012) 0.00 ng




response 53830

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	61.63
264.00	61.40	60.51
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122121\  
Data File : BM033548.D  
Acq On    : 21 Dec 2021  10:34  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 21 13:56:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM122121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 21 13:51:44 2021
Response via : Initial Calibration

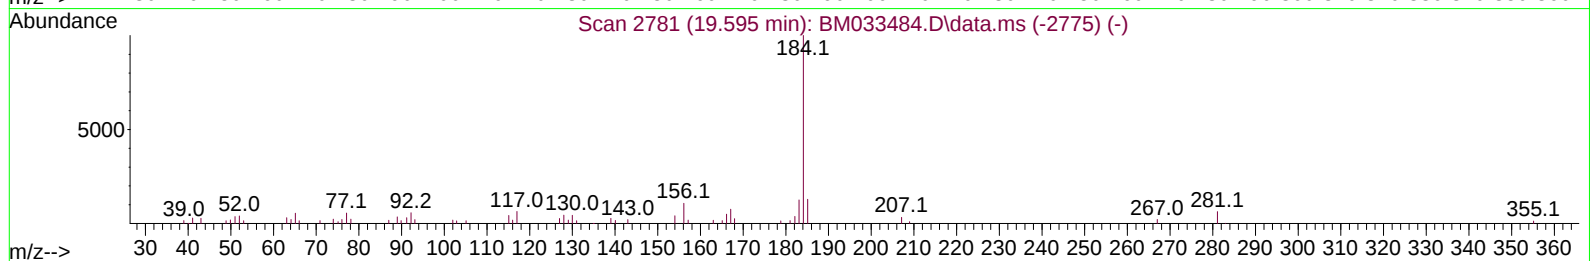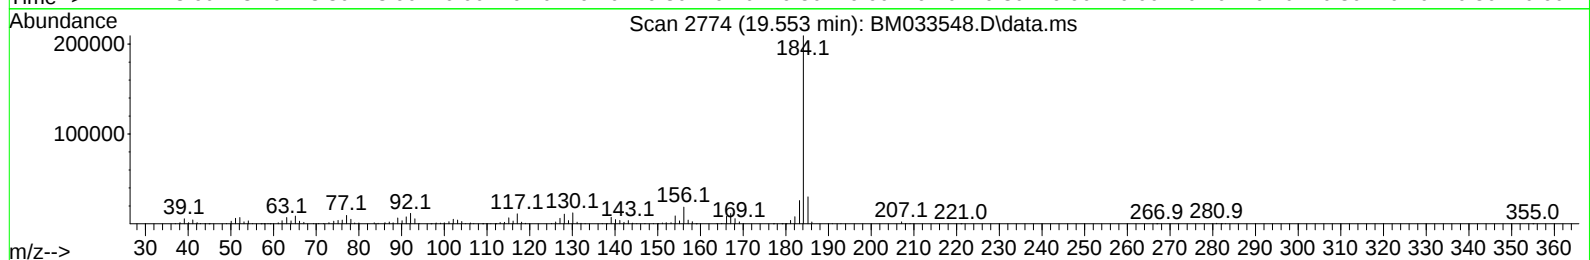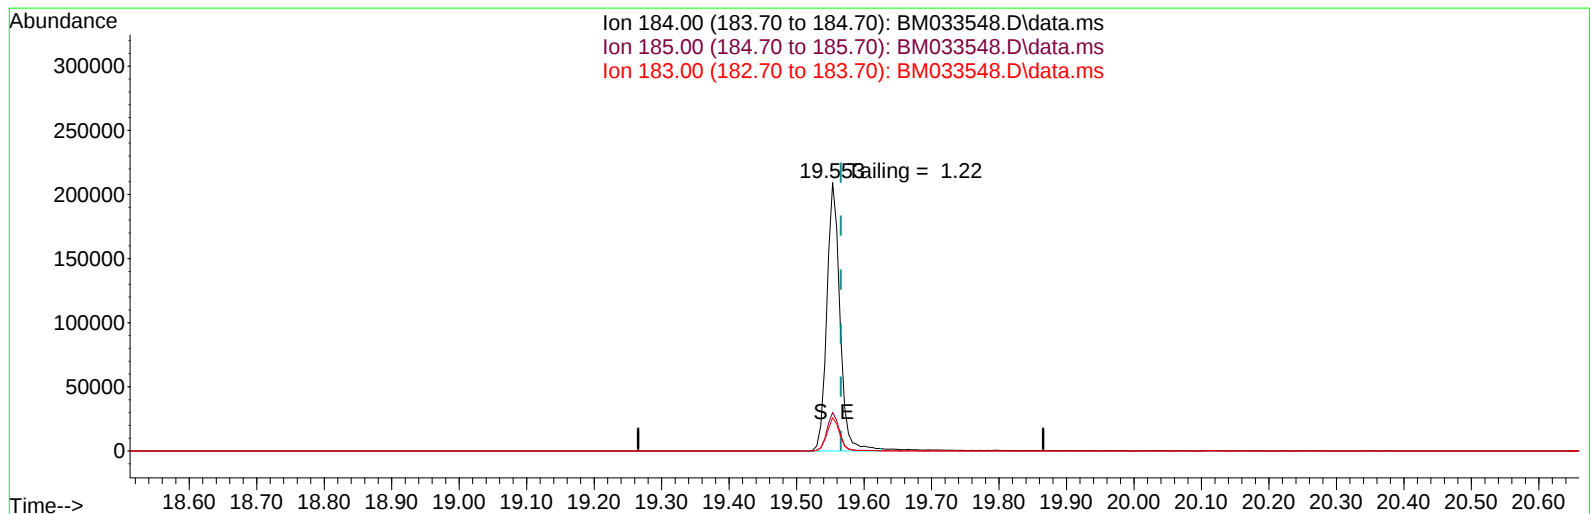

TIC: BM033548.D\data.ms

(77) Benzidine

19.553min (-0.012) 0.00 ng

response **284591**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.37
183.00	12.10	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2021	BNA_M	<u>BM033548.D</u>
Compound Name	Response	Retention Time
DDT	183283	20.77
DDD	849	20.38
DDE	0	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
849	184132	0.46