

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033574.D
 Acq On : 22 Dec 2021 13:51
 Operator : CG/JU
 Sample : PB141312BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 22 14:39:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	352	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.720	136	898	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.557	164	570	0.400	ng/ul	0.00
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.32
17) Chrysene-d12	21.504	240	1348	0.400	ng/ul	# 0.01
23) Perylene-d12	23.887	264	1725	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	2265	7.537	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152	515	0.429	ng/ul	0.01
18) Fluoranthene-d10	19.334	212	1550	0.497	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.693	202	306	0.071	ng/ul#	1
26) Benzo(a)pyrene	23.720	252	556	0.110	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
Data File : BM033574.D
Acq On : 22 Dec 2021 13:51
Operator : CG/JU
Sample : PB141312BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 22 14:39:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 12:43:31 2021
Response via : Initial Calibration




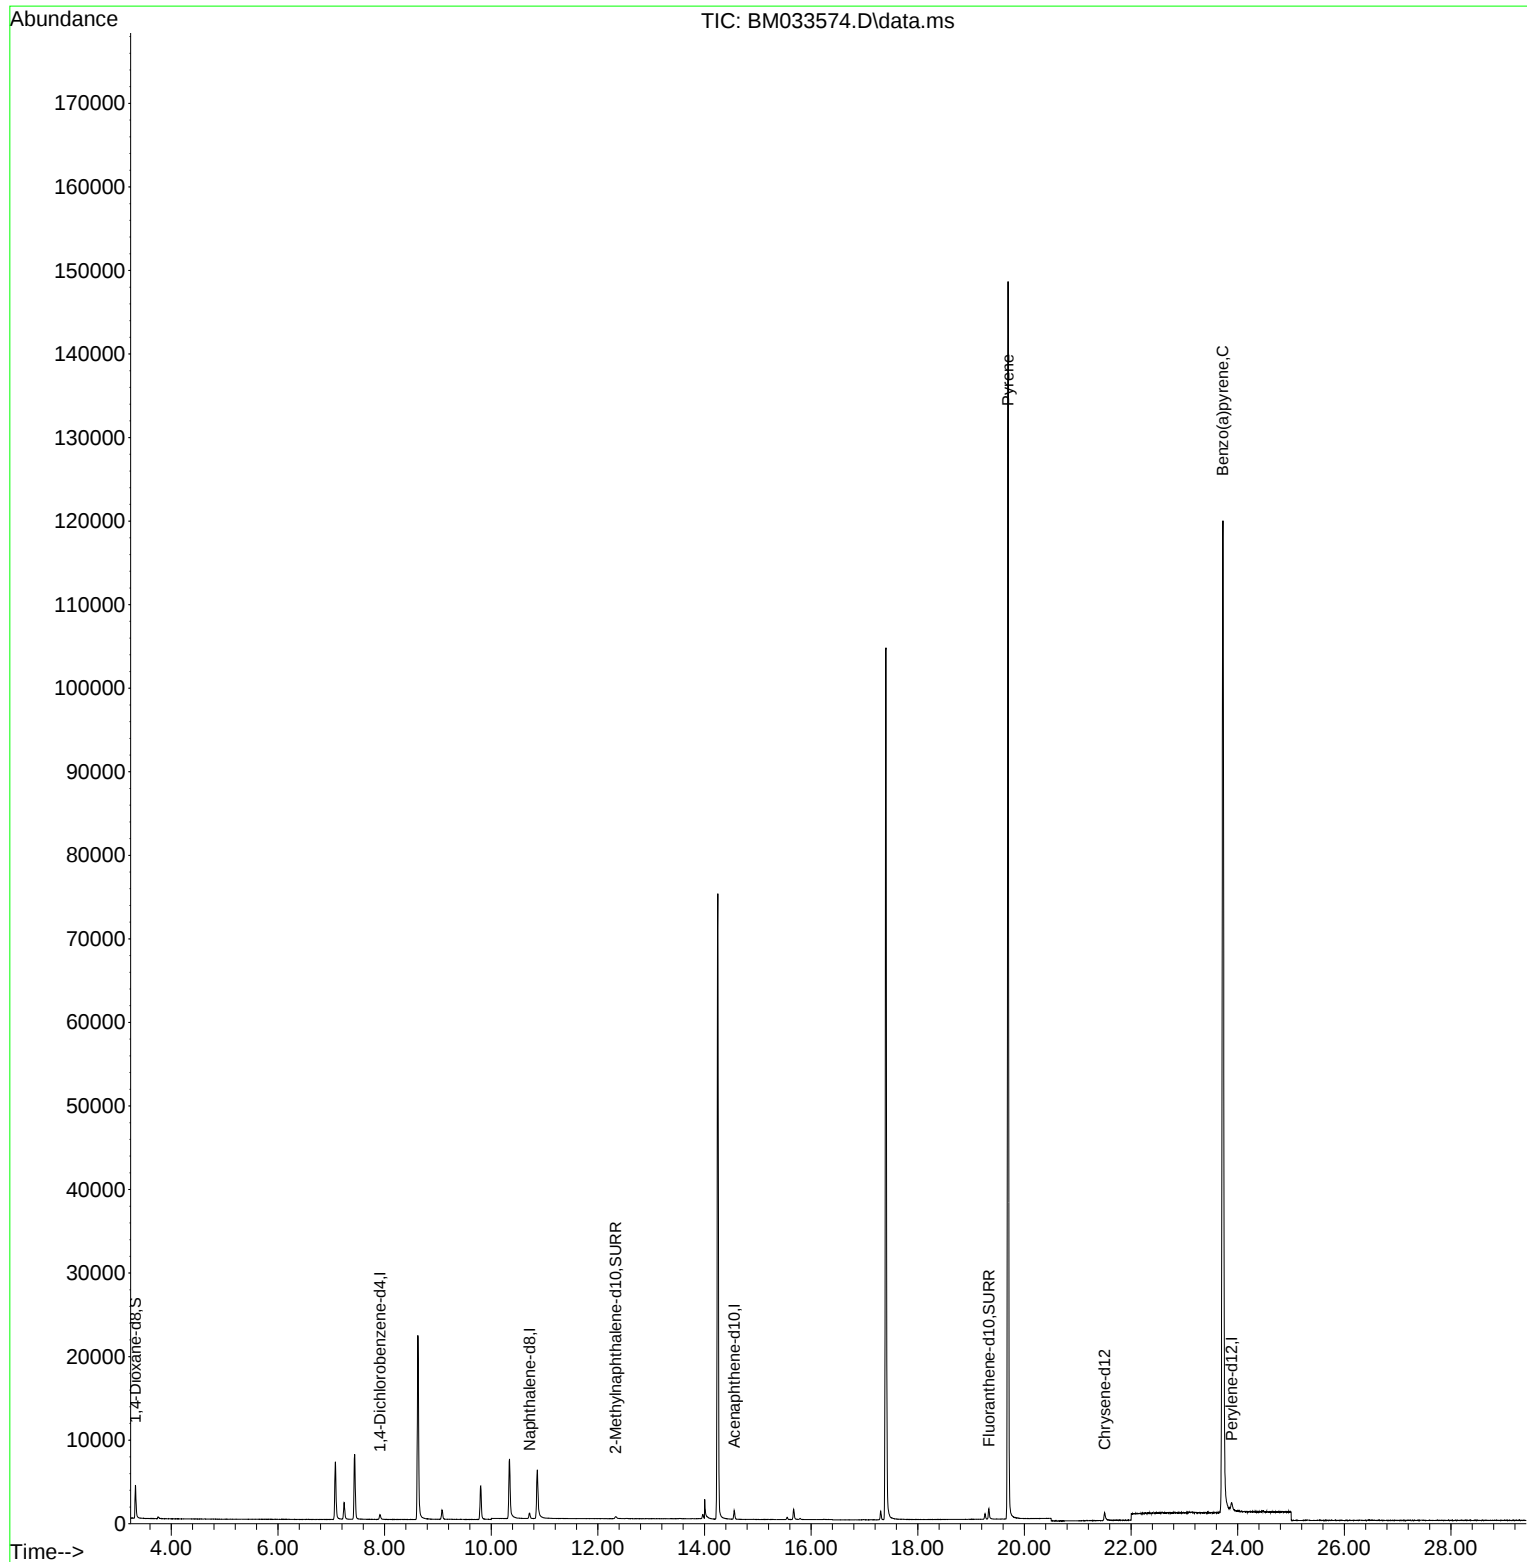


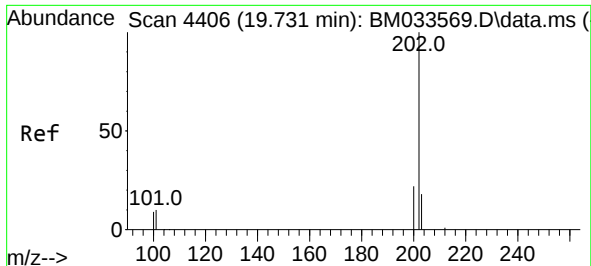

#20
Pyrene
Concen: 0.071 ng/ul
RT: 19.693 min Scan# 41
Delta R.T. -0.038 min
Lab File: BM033574.D
Acq: 22 Dec 2021 13:51

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 306
Ion Ratio Lower Upper
202 100
101 238.7 9.3 13.9#
100 1831.7 7.8 11.6#

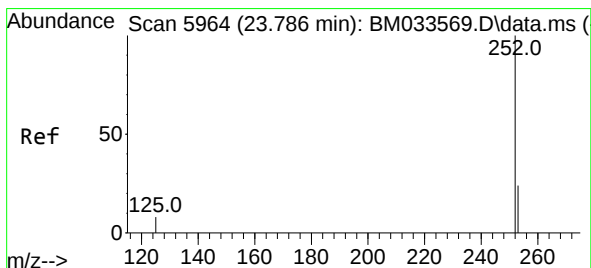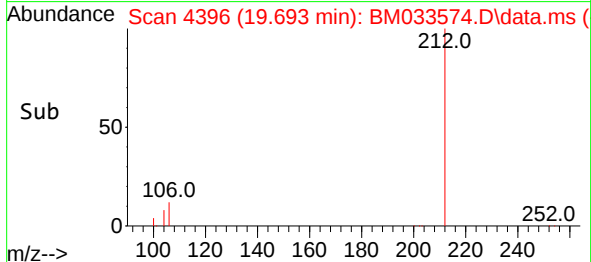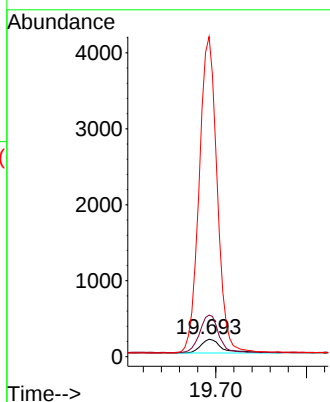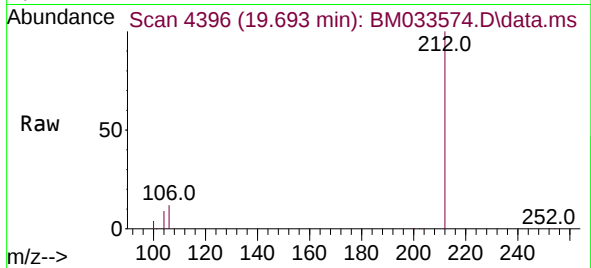

#26
Benzo(a)pyrene
Concen: 0.110 ng/ul
RT: 23.720 min Scan# 5937
Delta R.T. -0.065 min
Lab File: BM033574.D
Acq: 22 Dec 2021 13:51

Tgt Ion:252 Resp: 556
Ion Ratio Lower Upper
252 100
253 76.7 32.0 48.0#
125 61.2 14.5 21.7#

