




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033588.D
 Acq On : 22 Dec 2021 22:52
 Operator : CG/JU
 Sample : M5090-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG3C2

Manual IntegrationsAPPROVED

Quant Time: Dec 23 01:34:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2021
 Supervised By :mohammad ahmed 12/29/2021

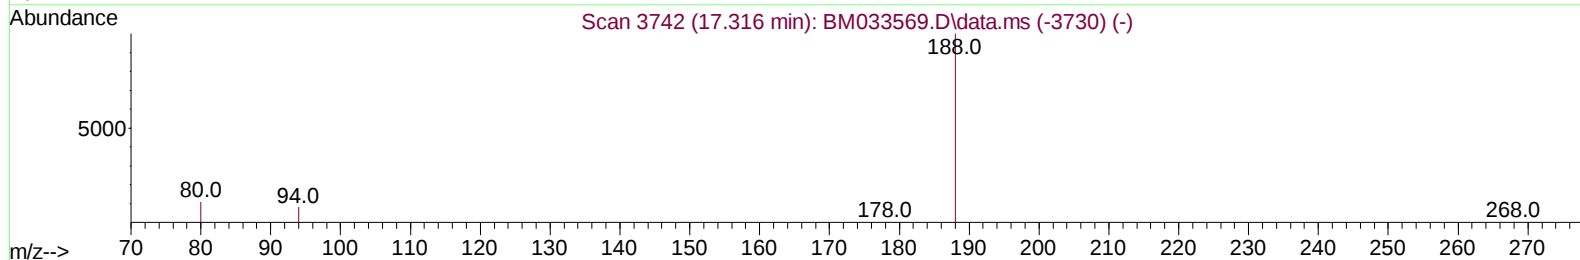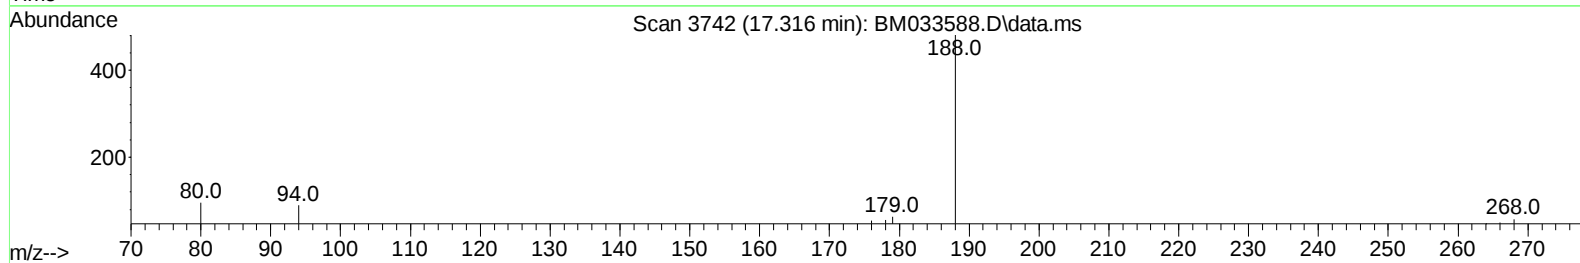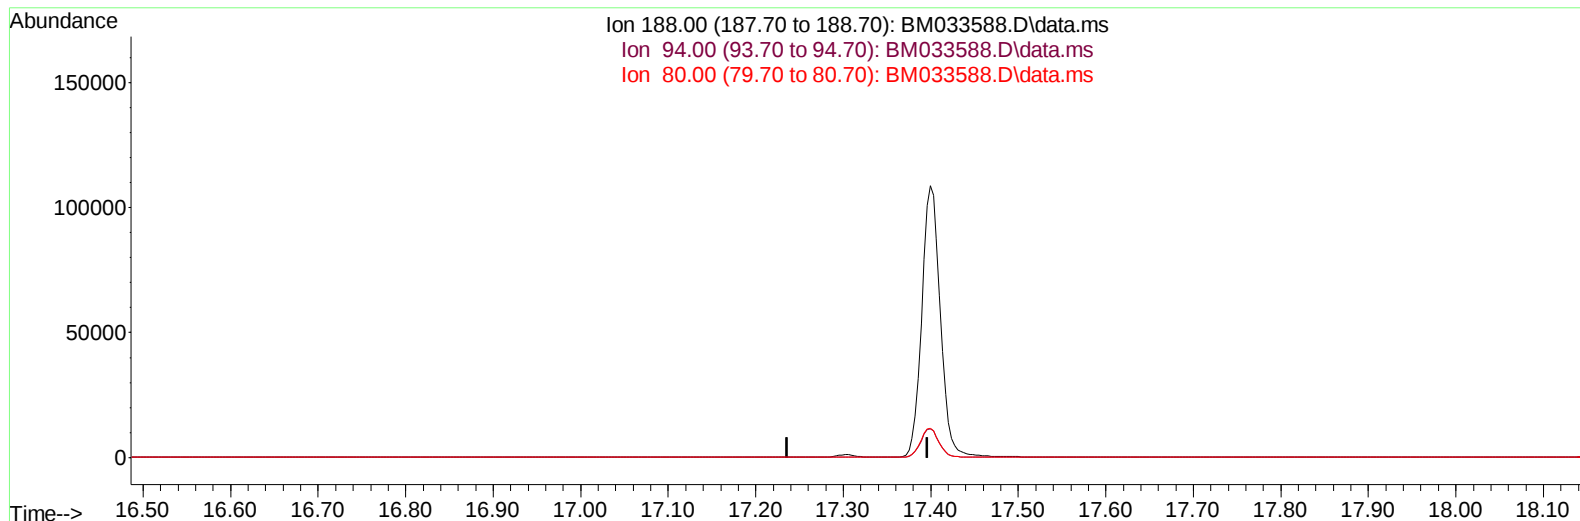

TIC: BM033588.D\data.ms

(13) Phenanthrene-d10 (I)

17.316min (-17.316) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.30	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033588.D
 Acq On : 22 Dec 2021 22:52
 Operator : CG/JU
 Sample : M5090-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG3C2

Manual IntegrationsAPPROVED

Quant Time: Dec 23 01:34:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2021
 Supervised By :mohammad ahmed 12/29/2021

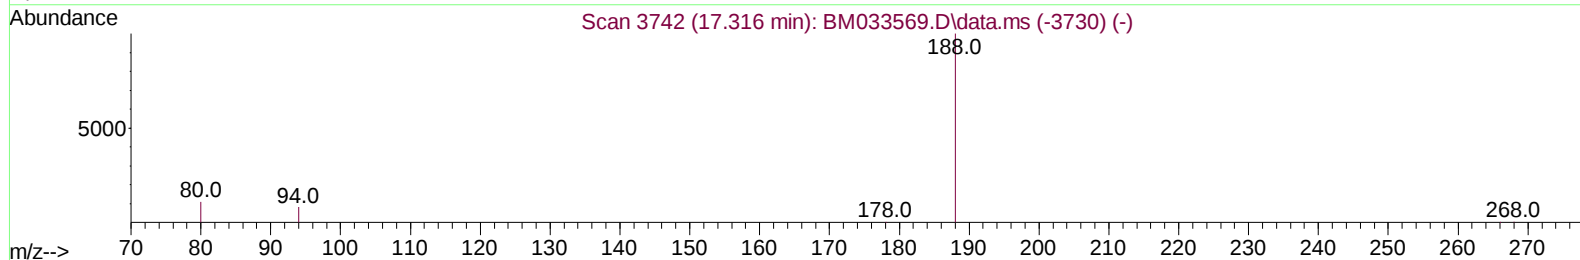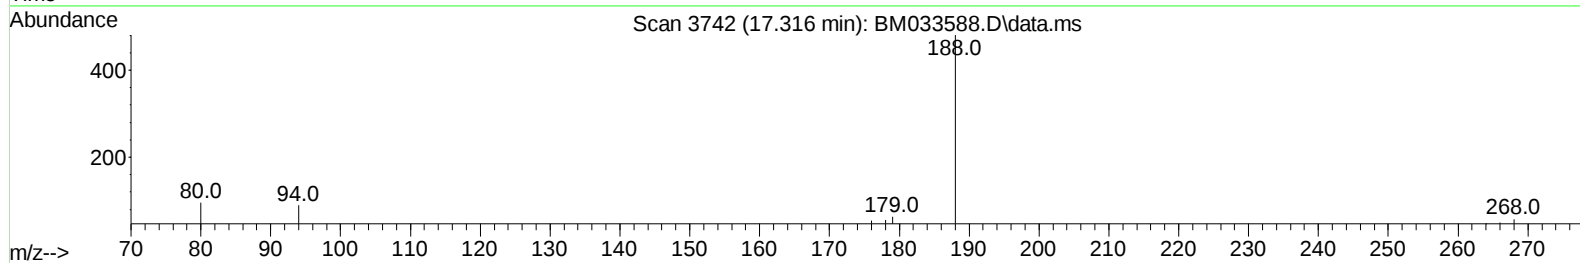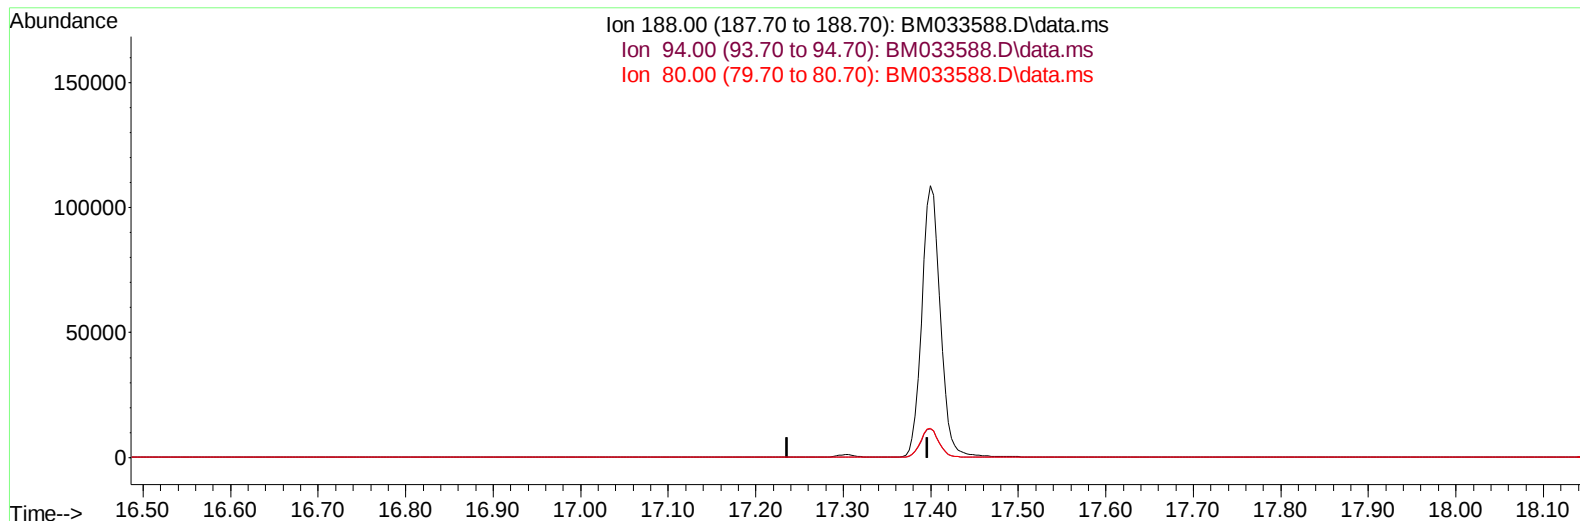

TIC: BM033588.D\data.ms

(13) Phenanthrene-d10 (I)

17.316min (-17.316) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	13.30	0.00#
80.00	15.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033588.D
 Acq On : 22 Dec 2021 22:52
 Operator : CG/JU
 Sample : M5090-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG3C2

Manual IntegrationsAPPROVED

Quant Time: Dec 23 01:34:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2021
 Supervised By :mohammad ahmed 12/29/2021

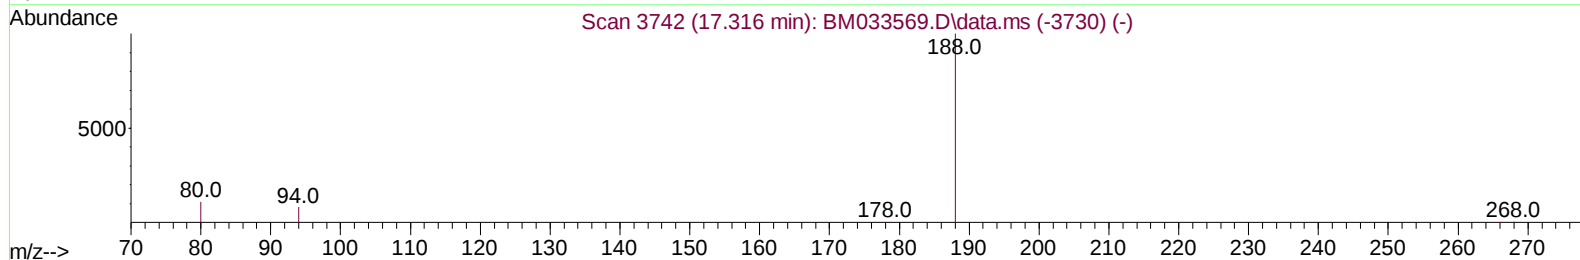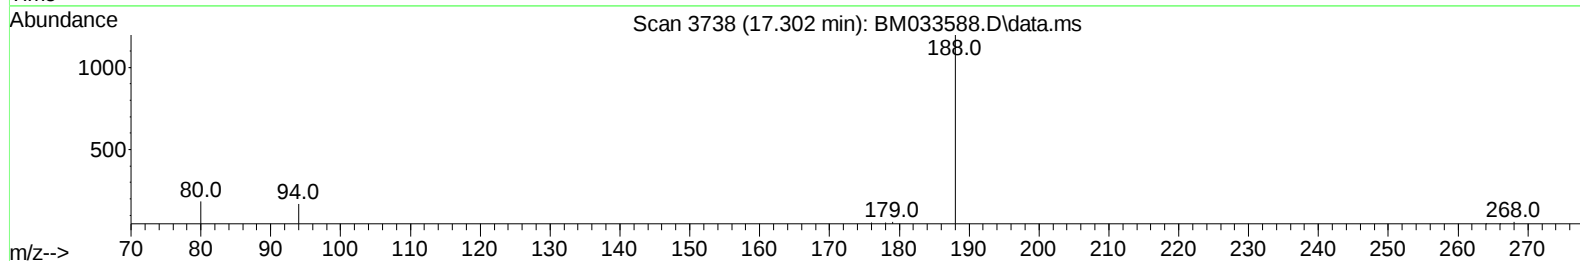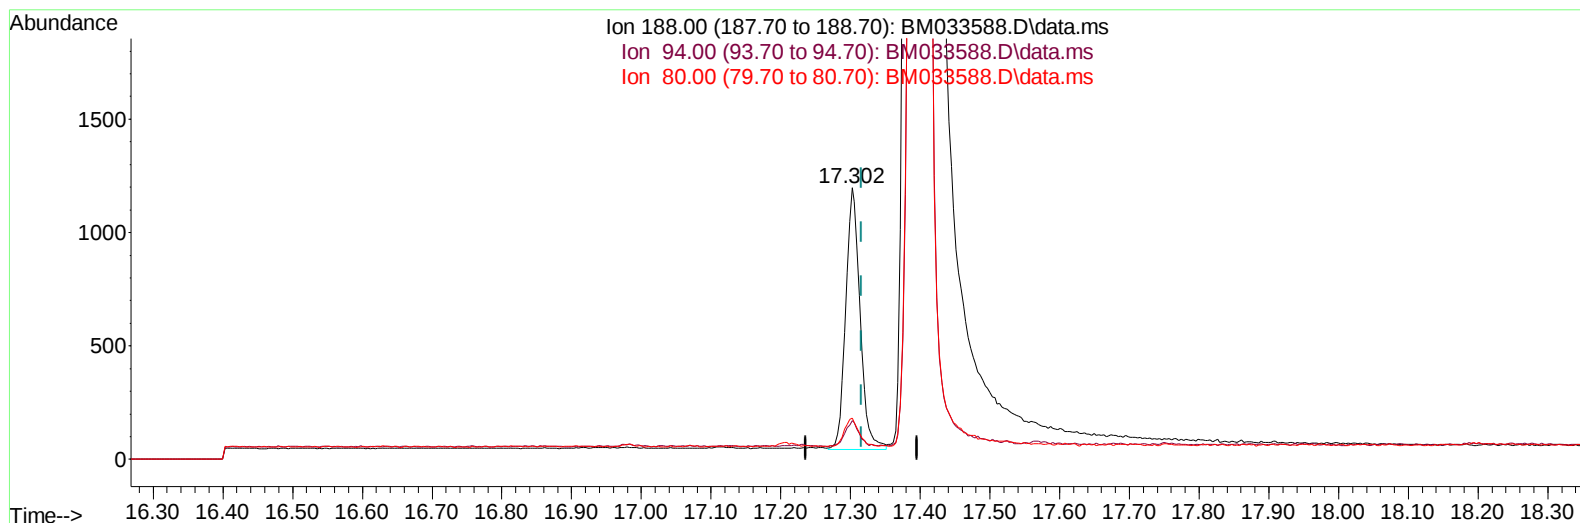

TIC: BM033588.D\data.ms

(13) Phenanthrene-d10 (I)

17.302min (-0.014) 0.40 ng/ul m

response 1641

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.30	14.20
80.00	15.50	15.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033588.D
 Acq On : 22 Dec 2021 22:52
 Operator : CG/JU
 Sample : M5090-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG3C2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/23/2021
 Supervised By :mohammad ahmed 12/29/2021

Quant Time: Dec 23 01:34:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.915	152		429	0.400	ng/ul	0.00
4) Naphthalene-d8	10.720	136		1139	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.557	164		744	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.302	188		1641m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.490	240		1919	0.400	ng/ul	# 0.00
23) Perylene-d12	23.878	264		2423	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.330	96		1927	5.262	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.335	152		509	0.334	ng/ul	0.01
18) Fluoranthene-d10	19.330	212		1980	0.446	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
Data File : BM033588.D
Acq On : 22 Dec 2021 22:52
Operator : CG/JU
Sample : M5090-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG3C2

Manual IntegrationsAPPROVED

Quant Time: Dec 23 01:34:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 12:43:31 2021
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/23/2021
Supervised By :mohammad ahmed 12/29/2021

