

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
 Data File : BM033603.D
 Acq On : 23 Dec 2021 08:25
 Operator : CG/JU
 Sample : M5090-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG3C7

Quant Time: Dec 23 09:12:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 12:43:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	453	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.716	136	1187	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.553	164	791	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.299	188	1848	0.400	ng/ul	-0.02
17) Chrysene-d12	21.485	240	2234	0.400	ng/ul	# 0.00
23) Perylene-d12	23.868	264	2633	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	1651	4.269	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	504	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.327	212	2168	0.420	ng/ul	0.00
Target Compounds						Qvalue
15) Phenanthrene	17.340	178	189	0.032	ng/ul#	47

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122221\
Data File : BM033603.D
Acq On : 23 Dec 2021 08:25
Operator : CG/JU
Sample : M5090-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG3C7

Quant Time: Dec 23 09:12:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM122221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 12:43:31 2021
Response via : Initial Calibration

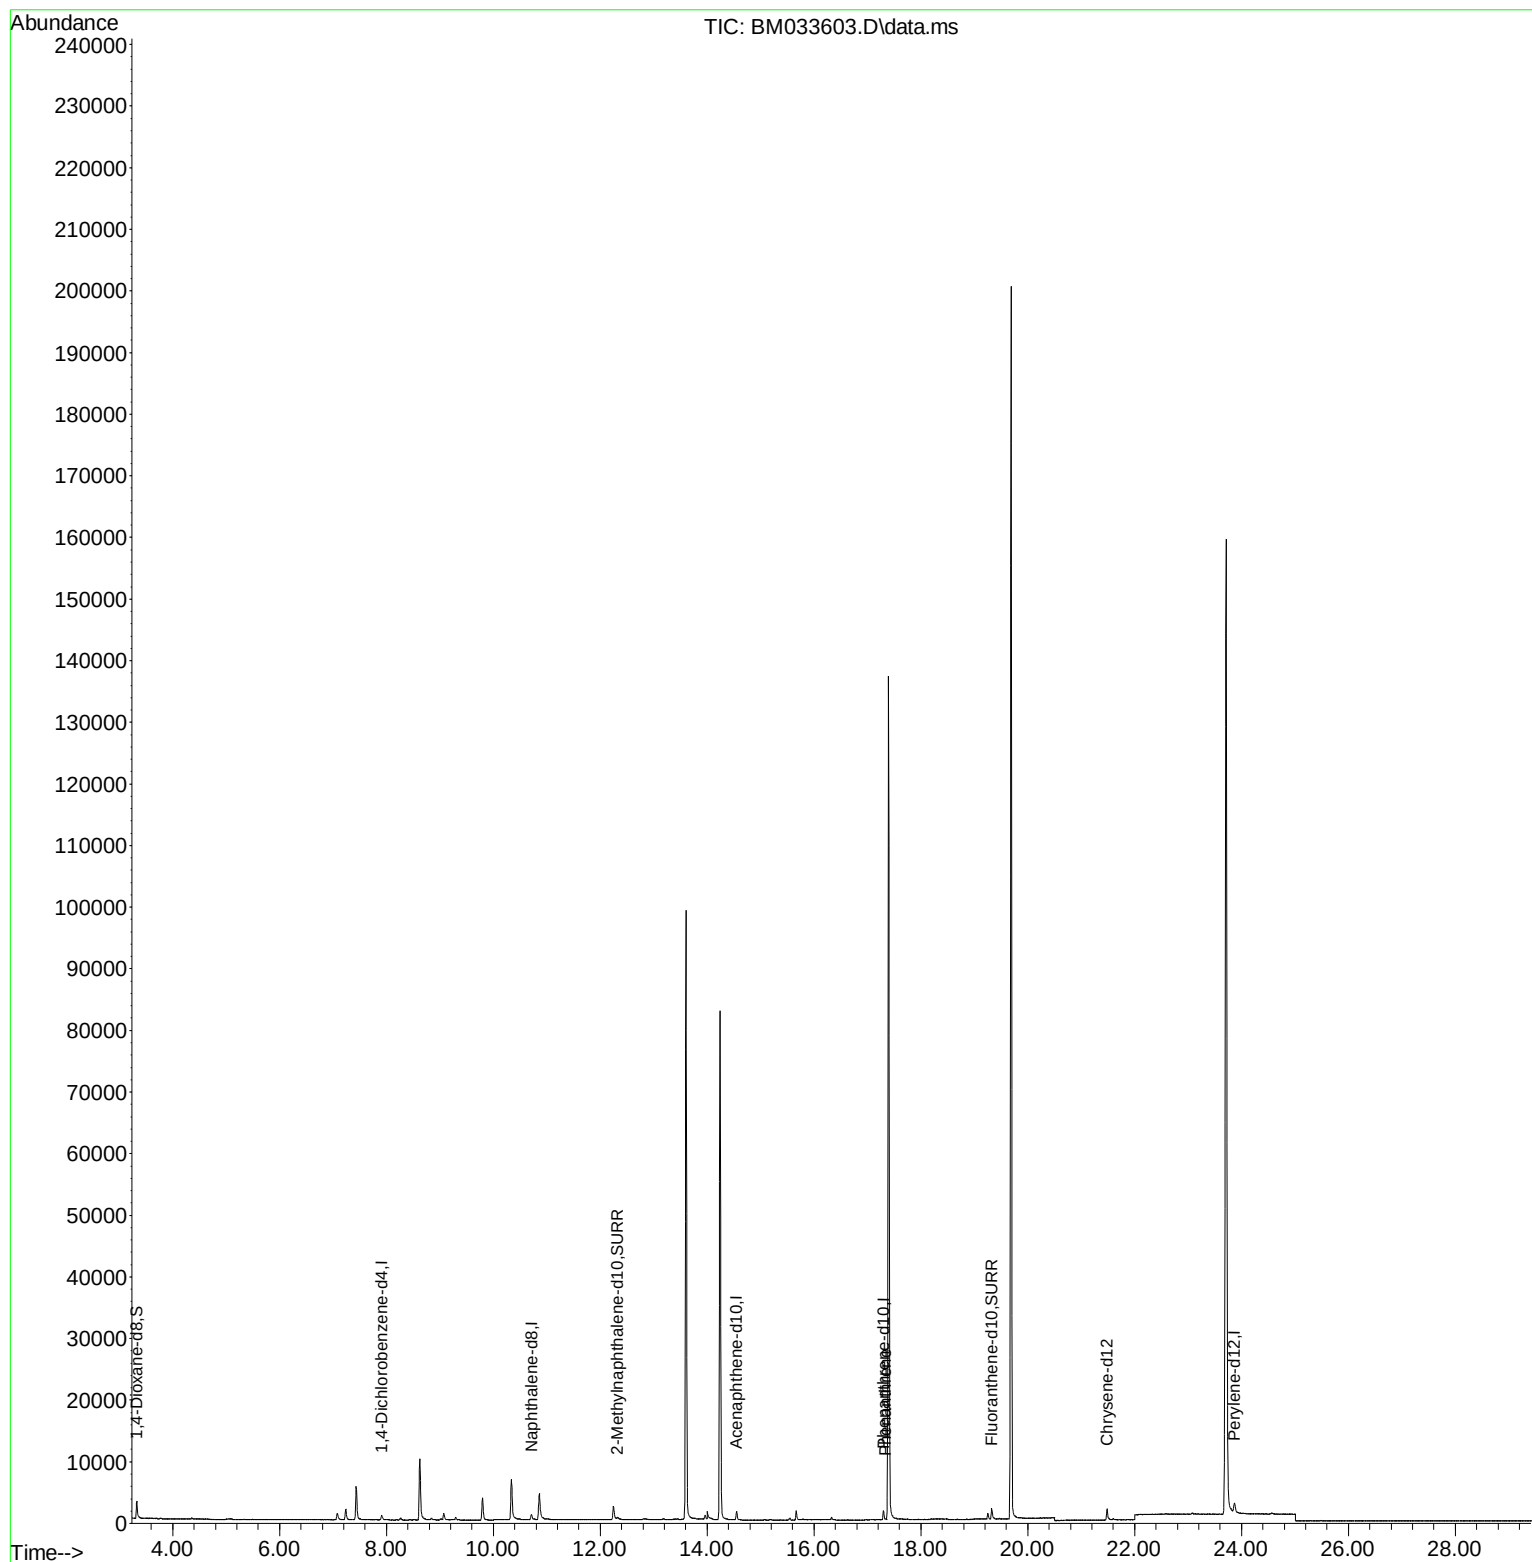



Abundance Scan 3756 (17.365 min): BM033594.D\data.ms (-3745) (-)

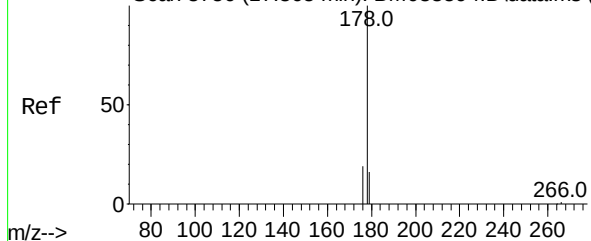

Phenanthrene
Concen: 0.032 ng/ul
RT: 17.340 min Scan# 1
Delta R.T. -0.017 min
Lab File: BM033603.D
Acq: 23 Dec 2021 08:25

Instrument :
BNA_M
ClientSampleId :
BG3C7

Tgt Ion:	178	Resp:	189
Ion	Ratio	Lower	Upper
178	100		
179	44.8	15.0	22.6#
176	45.9	17.9	26.9#

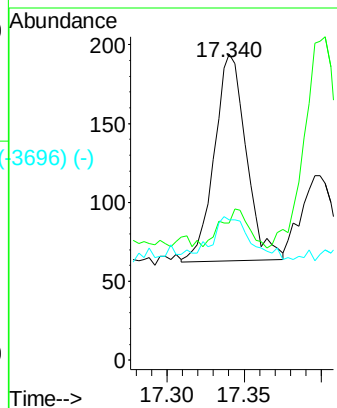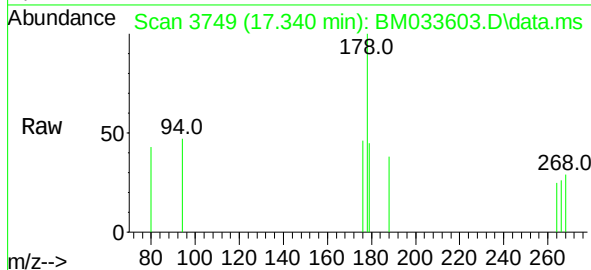

Abundance Scan 3749 (17.340 min): BM033603.D\data.ms (-3696) (-)

