

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122223\
 Data File : BM043552.D
 Acq On : 23 Dec 2023 00:25
 Operator : MA/JU
 Sample : 05927-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3J3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/25/2023
 Supervised By :mohammad ahmed 12/28/2023

Quant Time: Dec 23 02:15:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	6247	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	19252	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.606	164	9316	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	18506m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	10996m	0.400	ng/ul	0.00
23) Perylene-d12	23.939	264	15433	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.377	96	17447	2.210	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	7343	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	12278	0.313	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.414	88	685	0.087	ng/ul#	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122223\
Data File : BM043552.D
Acq On : 23 Dec 2023 00:25
Operator : MA/JU
Sample : 05927-02
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH3J3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/25/2023
Supervised By :mohammad ahmed 12/28/2023


Quant Time: Dec 23 02:15:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

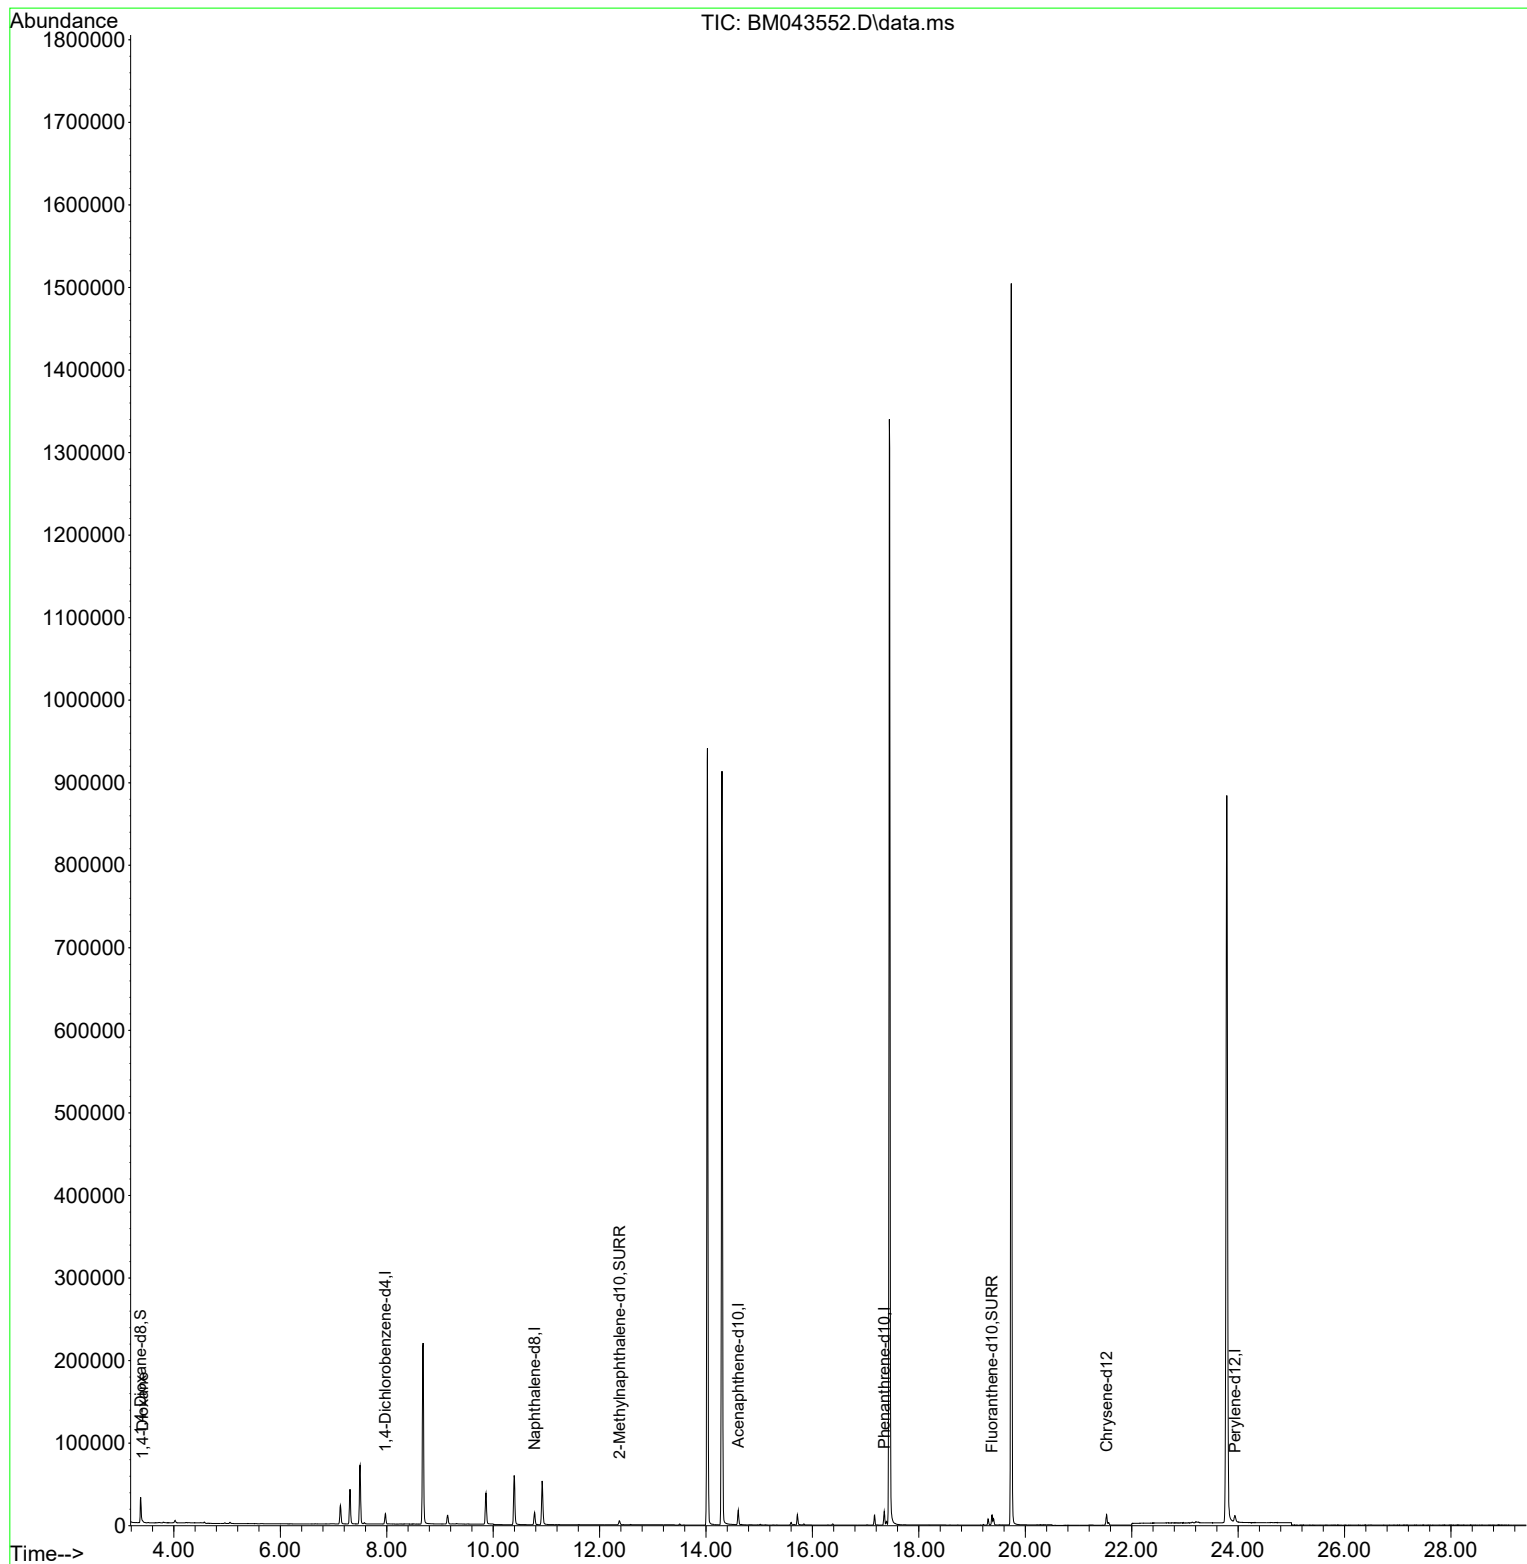

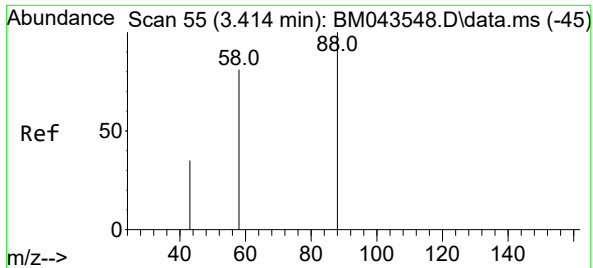

#2
 1,4-Dioxane
 Concen: 0.087 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM043552.D
 Acq: 23 Dec 2023 00:25

Instrument :
 BNA_M
 ClientSampleId :
 BH3J3

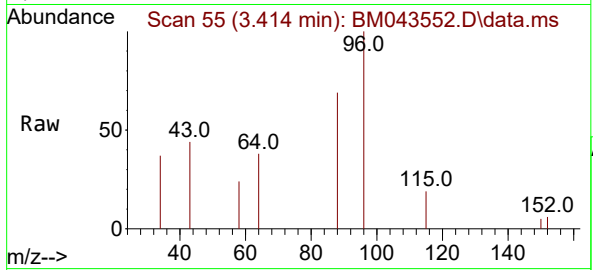

Tgt Ion: 88 Resp: 68

Ion	Ratio	Lower	Upper
88	100		
43	64.0	27.9	41.9
58	35.4	43.4	65.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/25/2023
 Supervised By :mohammad ahmed 12/28/2023

