

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122223\
 Data File : BM043559.D
 Acq On : 23 Dec 2023 04:38
 Operator : MA/JU
 Sample : 05927-10
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3C9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2023
 Supervised By :mohammad ahmed 12/28/2023

Quant Time: Dec 25 00:23:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	6216	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	19599	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.606	164	9397	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	19038m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	10386m	0.400	ng/ul	0.00
23) Perylene-d12	23.942	264	13143m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	19206	2.445	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	8334	0.300	ng/ul	-0.01
18) Fluoranthene-d10	19.376	212	13205m	0.356	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	1986	0.252	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122223\
Data File : BM043559.D
Acq On : 23 Dec 2023 04:38
Operator : MA/JU
Sample : 05927-10
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3C9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :mohammad ahmed 12/28/2023

Quant Time: Dec 25 00:23:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

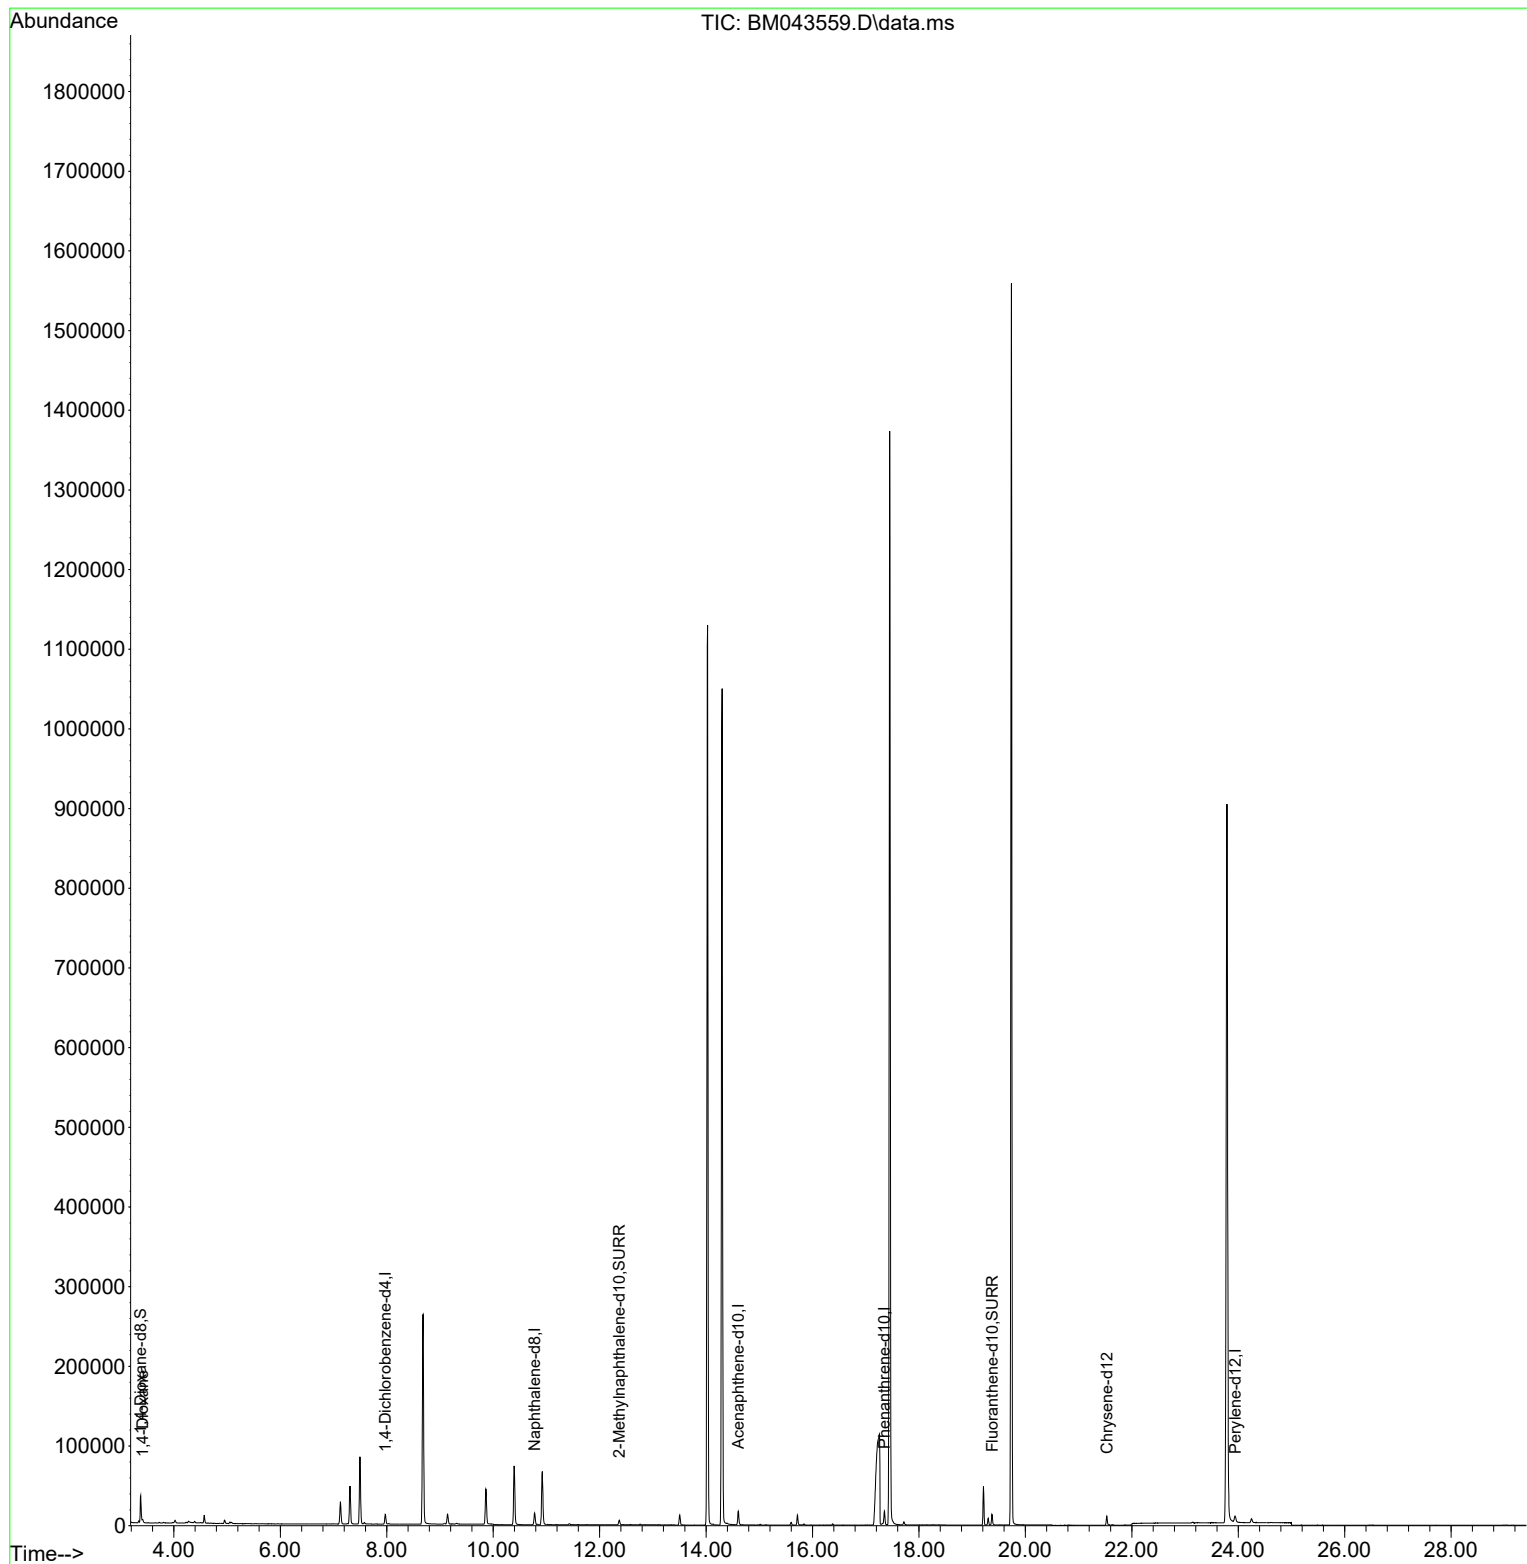


Abundance Scan 55 (3.414 min): BM043548.D\data.ms (-45)

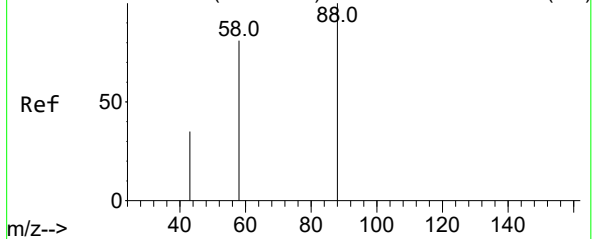

#2
1,4-Dioxane
Concen: 0.252 ng/ul
RT: 3.414 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM043559.D
Acq: 23 Dec 2023 04:38

Instrument :
BNA_M
ClientSampleId :
BH3C9

Abundance Scan 55 (3.414 min): BM043559.D\data.ms

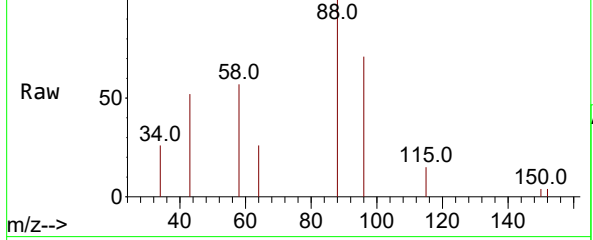

Tgt Ion: 88	Resp: 1980
Ion Ratio	Lower Upper
88	100
43	52.3 27.9 41.9
58	56.8 43.4 65.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :mohammad ahmed 12/28/2023

Abundance Scan 55 (3.414 min): BM043559.D\data.ms (-42)

