
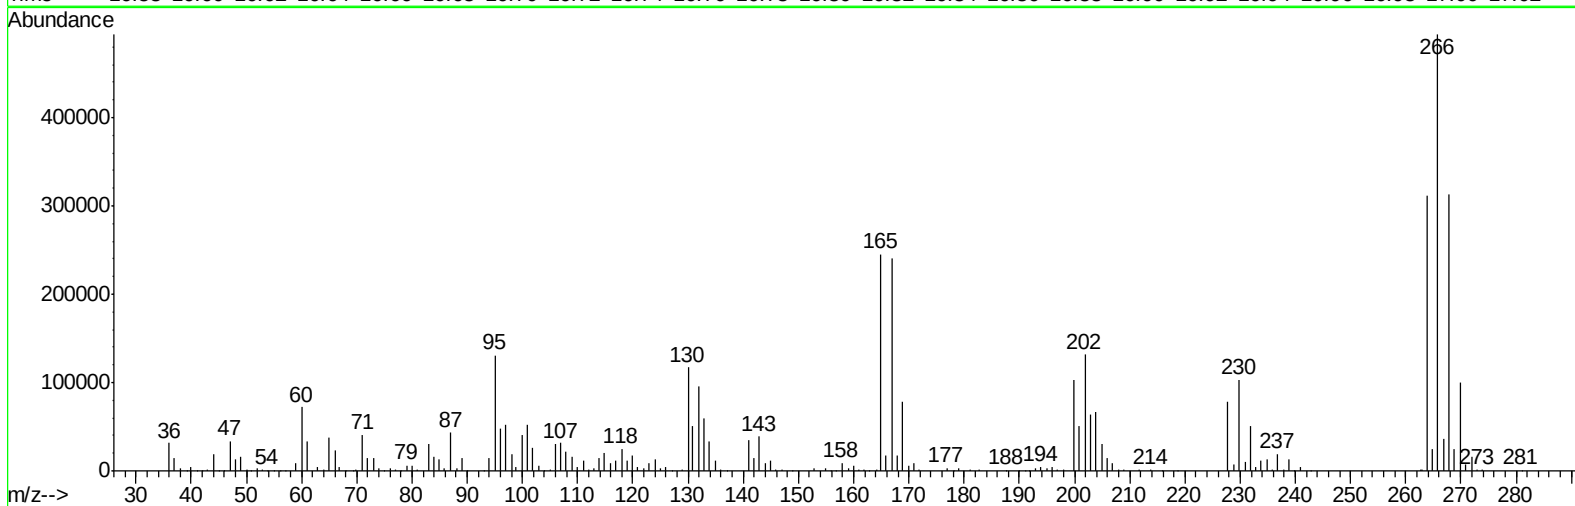


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM122718\
Data File : BM018396.D
Acq On : 27 Dec 2018 15:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:39:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 27 14:18:47 2018
Response via : Initial Calibration

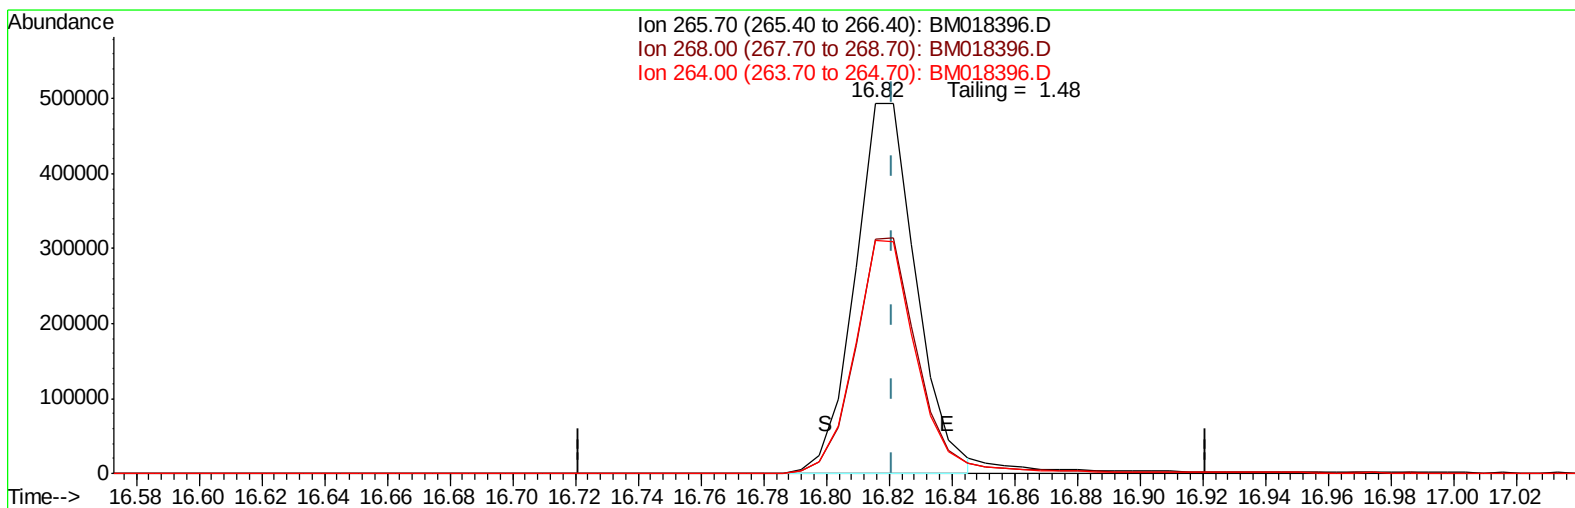

TIC: BM018396.D

(70) Pentachlorophenol (C)



16.815min (-0.006) 861677.51ng

response 687975

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.44
264.00	62.60	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM122718\
 Data File : BM018396.D
 Acq On : 27 Dec 2018 15:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:39:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 27 14:18:47 2018
 Response via : Initial Calibration

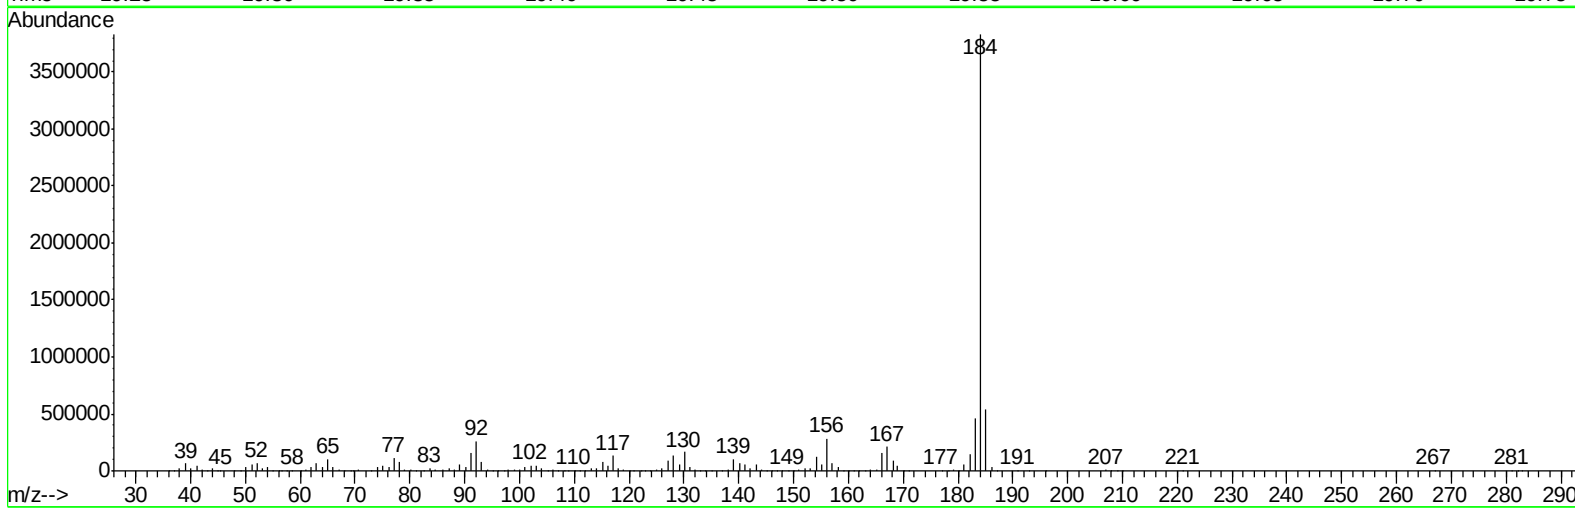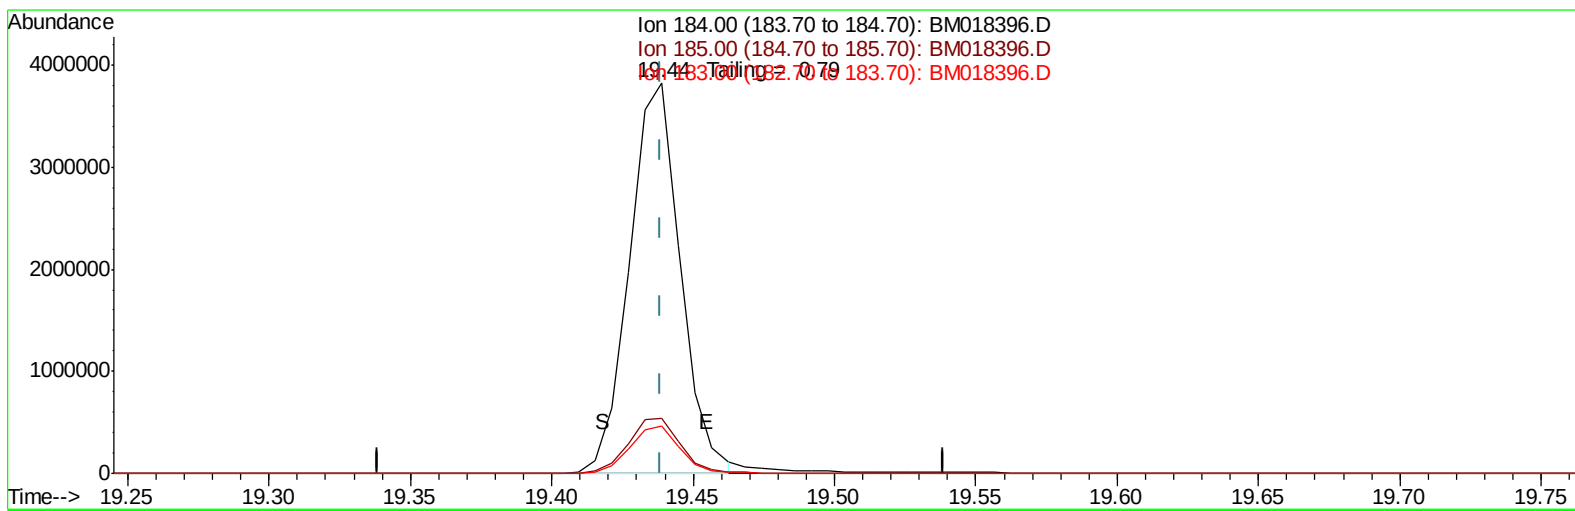

TIC: BM018396.D

(77) Benzidine

19.439min (+0.000) 0.00ng

response 4871772

Ion	Exp%	Act%
184.00	100	100
185.00	14.20	14.20
183.00	11.90	12.07
0.00	0.00	0.00