

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018405.D
 Acq On : 27 Dec 2018 20:29
 Operator : JU/SJ
 Sample : PB116035BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB116035BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	25	28	38	rVB2	272344	404323	3.71%	0.901%
2	5.357	415	420	427	rBV	373690	553678	5.08%	1.234%
3	6.934	683	688	697	rVB	306258	506767	4.65%	1.130%
4	7.781	826	832	840	rVB	996221	1548989	14.22%	3.453%
5	8.945	1023	1030	1037	rBV	874051	1484432	13.63%	3.310%
6	9.316	1089	1093	1100	rVB2	95260	145245	1.33%	0.324%
7	10.575	1300	1307	1314	rBV	1467718	2390339	21.95%	5.329%
8	13.045	1720	1727	1734	rBV	2850754	4087024	37.53%	9.112%
9	14.427	1956	1962	1970	rVB2	2398226	3567380	32.76%	7.953%
10	15.916	2209	2215	2222	rBV	1308566	1792518	16.46%	3.996%
11	17.174	2422	2429	2437	rBV	3393352	4519982	41.51%	10.077%
12	19.809	2871	2877	2884	rBV	9289385	10889597	100.00%	24.278%
13	21.286	3124	3128	3132	rBV	119689	153183	1.41%	0.342%
14	21.368	3137	3142	3153	rVV	4964522	5976224	54.88%	13.324%
15	22.968	3410	3414	3420	rVB	99480	149782	1.38%	0.334%
16	23.556	3510	3514	3522	rVB	139609	227875	2.09%	0.508%
17	23.662	3525	3532	3542	rVB2	3284650	6218854	57.11%	13.865%
18	24.227	3624	3628	3635	rVB3	128360	236862	2.18%	0.528%


Sum of corrected areas: 44853054

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018405.D
Acq On : 27 Dec 2018 20:29
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

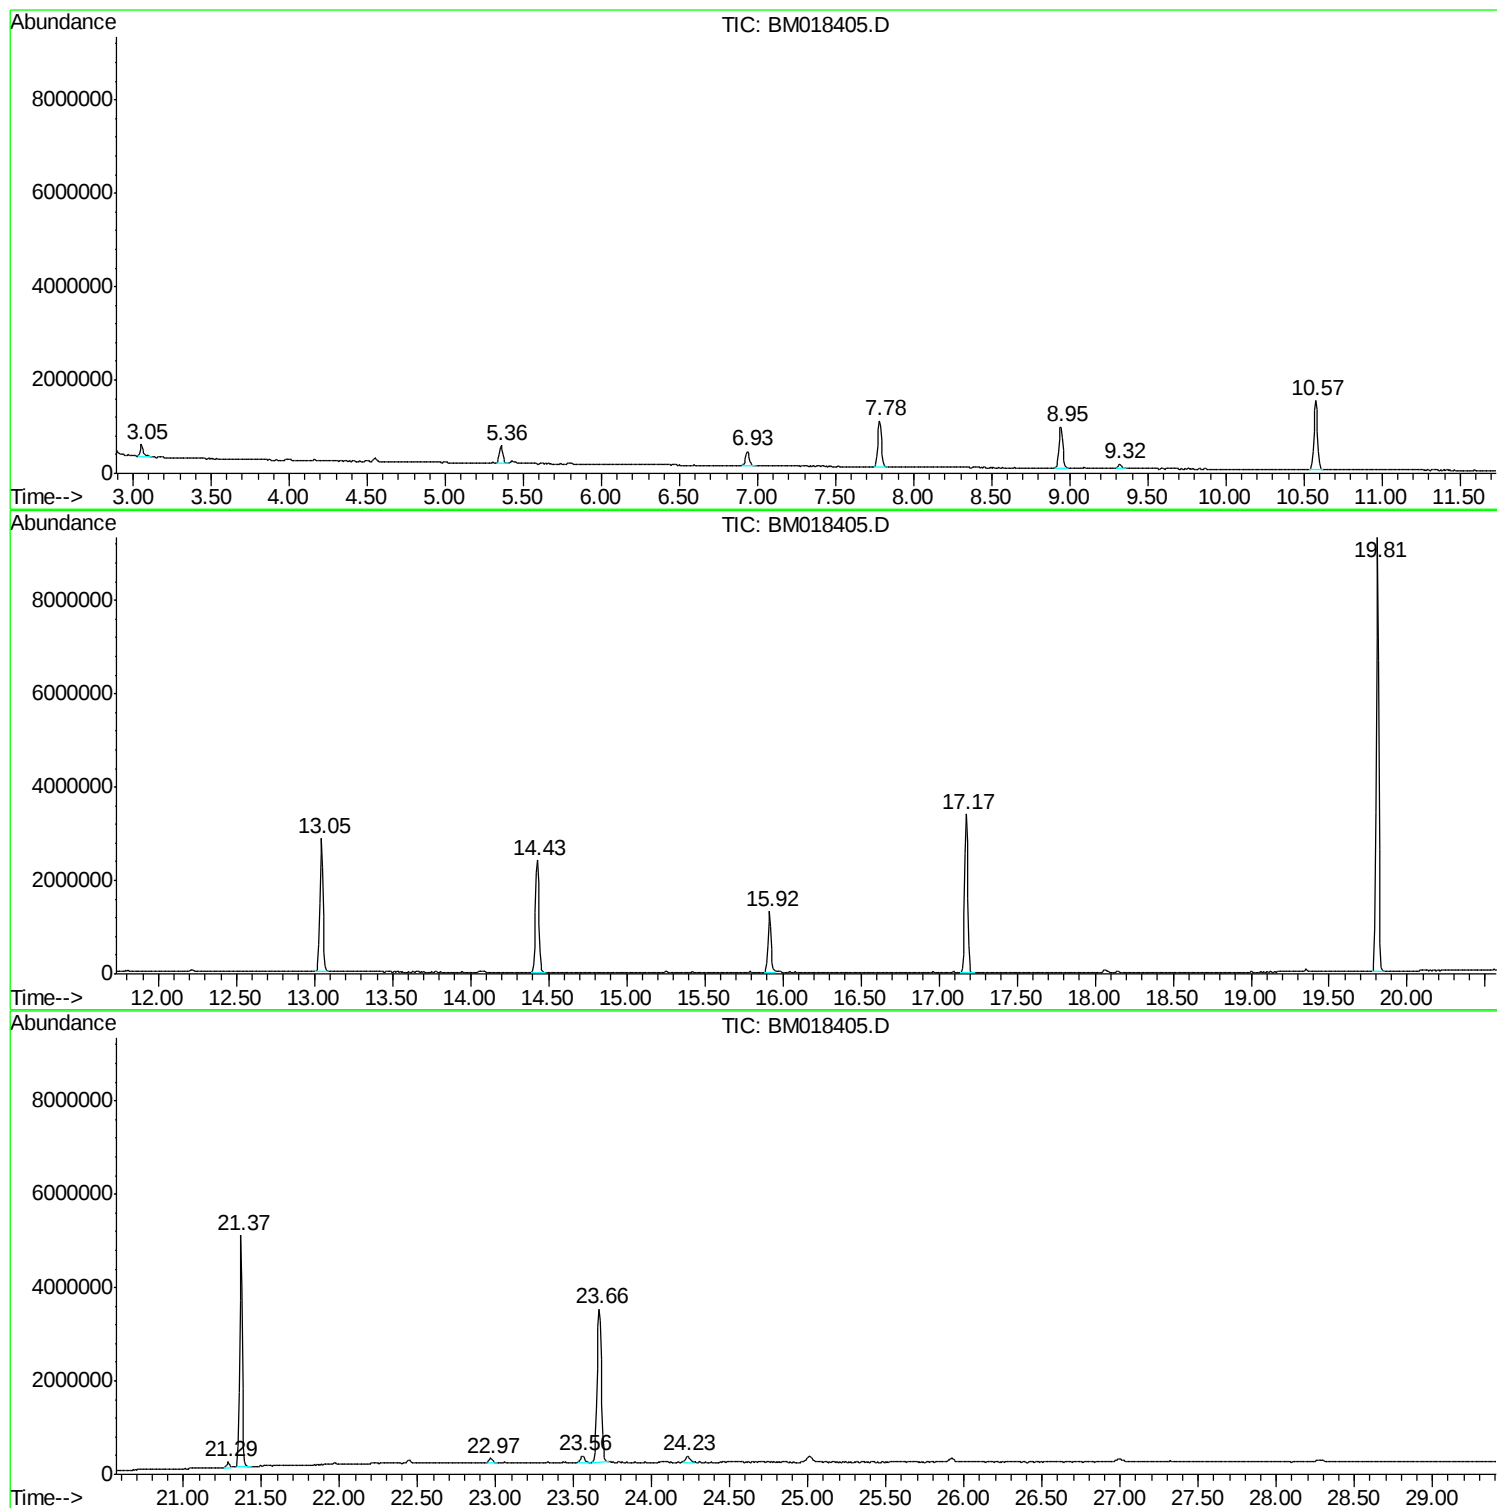

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018405.D
Acq On : 27 Dec 2018 20:29
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Furan, tetrahydro-2-(methox... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.05	5.22 ng	404323	1,4-Dichlorobenzene-d4	7.78

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Furan, tetrahydro-2-(methoxymeth...	116	C6H12O2	019354-27-9	72
2		3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	64
3		Butane, 2-bromo-2-methyl-	150	C5H11Br	000507-36-8	59
4		3-Penten-2-ol	86	C5H10O	001569-50-2	56
5		Butanoyl chloride	106	C4H7ClO	000141-75-3	53

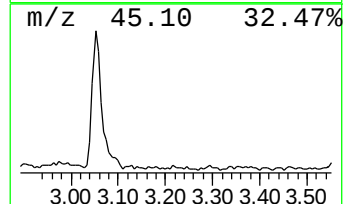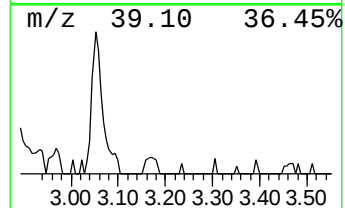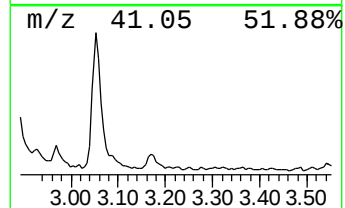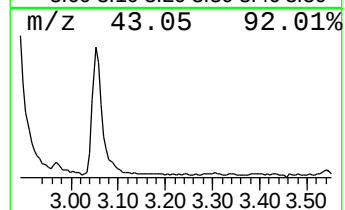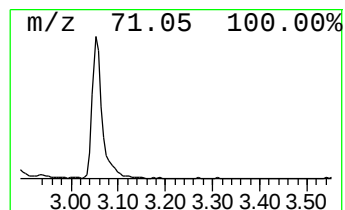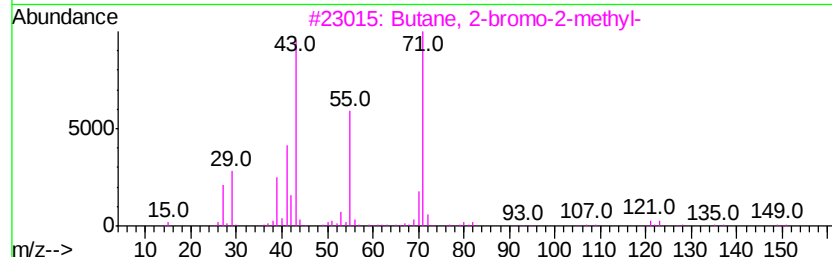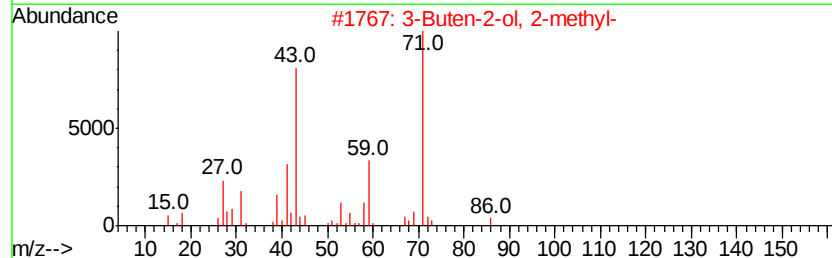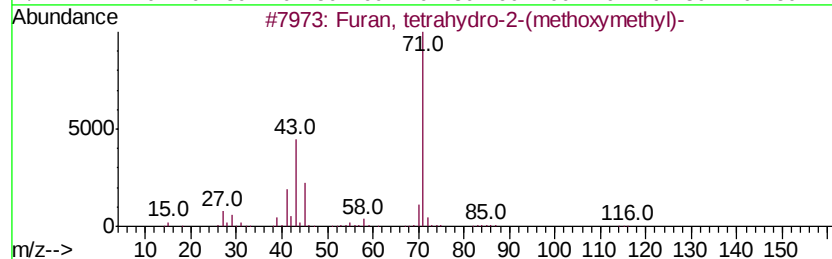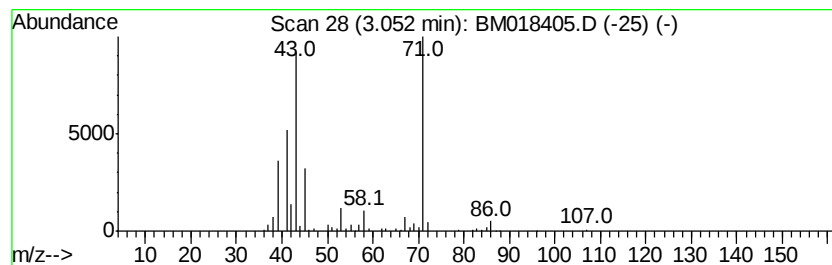

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122718\
Data File : BM018405.D
Acq On : 27 Dec 2018 20:29
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Furan, tetrahydro...	3.05	5.2	ng	404323	1	7.78	1548990	20.0