

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018406.D
 Acq On : 27 Dec 2018 21:05
 Operator : JU/SJ
 Sample : PB116035BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB116035BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	25	28	41	rVB	351469	518180	4.69%	0.997%
2	5.357	415	420	427	rVB	489857	732751	6.63%	1.410%
3	6.934	683	688	697	rVB	404362	632549	5.72%	1.217%
4	7.781	826	832	840	rVB	1222624	1885033	17.05%	3.627%
5	8.945	1023	1030	1039	rBV	932956	1525033	13.79%	2.934%
6	9.316	1088	1093	1101	rVB2	91629	145511	1.32%	0.280%
7	10.575	1300	1307	1314	rVB	1794229	2872850	25.99%	5.527%
8	13.045	1720	1727	1735	rVB	3027350	4389663	39.71%	8.445%
9	14.068	1893	1901	1908	rBV2	83190	140167	1.27%	0.270%
10	14.427	1955	1962	1969	rBV2	2785884	4180725	37.82%	8.043%
11	15.915	2209	2215	2221	rBV	2012032	2755485	24.92%	5.301%
12	15.968	2221	2224	2233	rVB	156227	230922	2.09%	0.444%
13	17.174	2419	2429	2439	rBV	3802860	5141443	46.51%	9.892%
14	18.062	2576	2580	2585	rBV	156140	199328	1.80%	0.383%
15	19.350	2794	2799	2806	rBV3	174275	242322	2.19%	0.466%
16	19.498	2818	2824	2832	rBV7	54111	111588	1.01%	0.215%
17	19.809	2871	2877	2885	rVB	8481781	11055529	100.00%	21.270%
18	20.121	2925	2930	2940	rBV6	67456	158928	1.44%	0.306%
19	21.086	3090	3094	3103	rVB6	151421	212552	1.92%	0.409%
20	21.280	3124	3127	3132	rBV	108267	156571	1.42%	0.301%
21	21.368	3136	3142	3156	rVV	5014863	6711448	60.71%	12.912%
22	21.968	3241	3244	3250	rVB	148338	209514	1.90%	0.403%
23	22.439	3321	3324	3329	rVB3	103164	127383	1.15%	0.245%
24	22.962	3410	3413	3420	rVB2	153426	218636	1.98%	0.421%
25	23.550	3509	3513	3519	rVB3	180028	304973	2.76%	0.587%
26	23.656	3524	3531	3543	rVB2	3349624	6371866	57.64%	12.259%
27	24.227	3623	3628	3635	rBV2	175602	342435	3.10%	0.659%
28	25.003	3756	3760	3772	rVB2	182110	404932	3.66%	0.779%


Sum of corrected areas: 51978317

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018406.D
Acq On : 27 Dec 2018 21:05
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

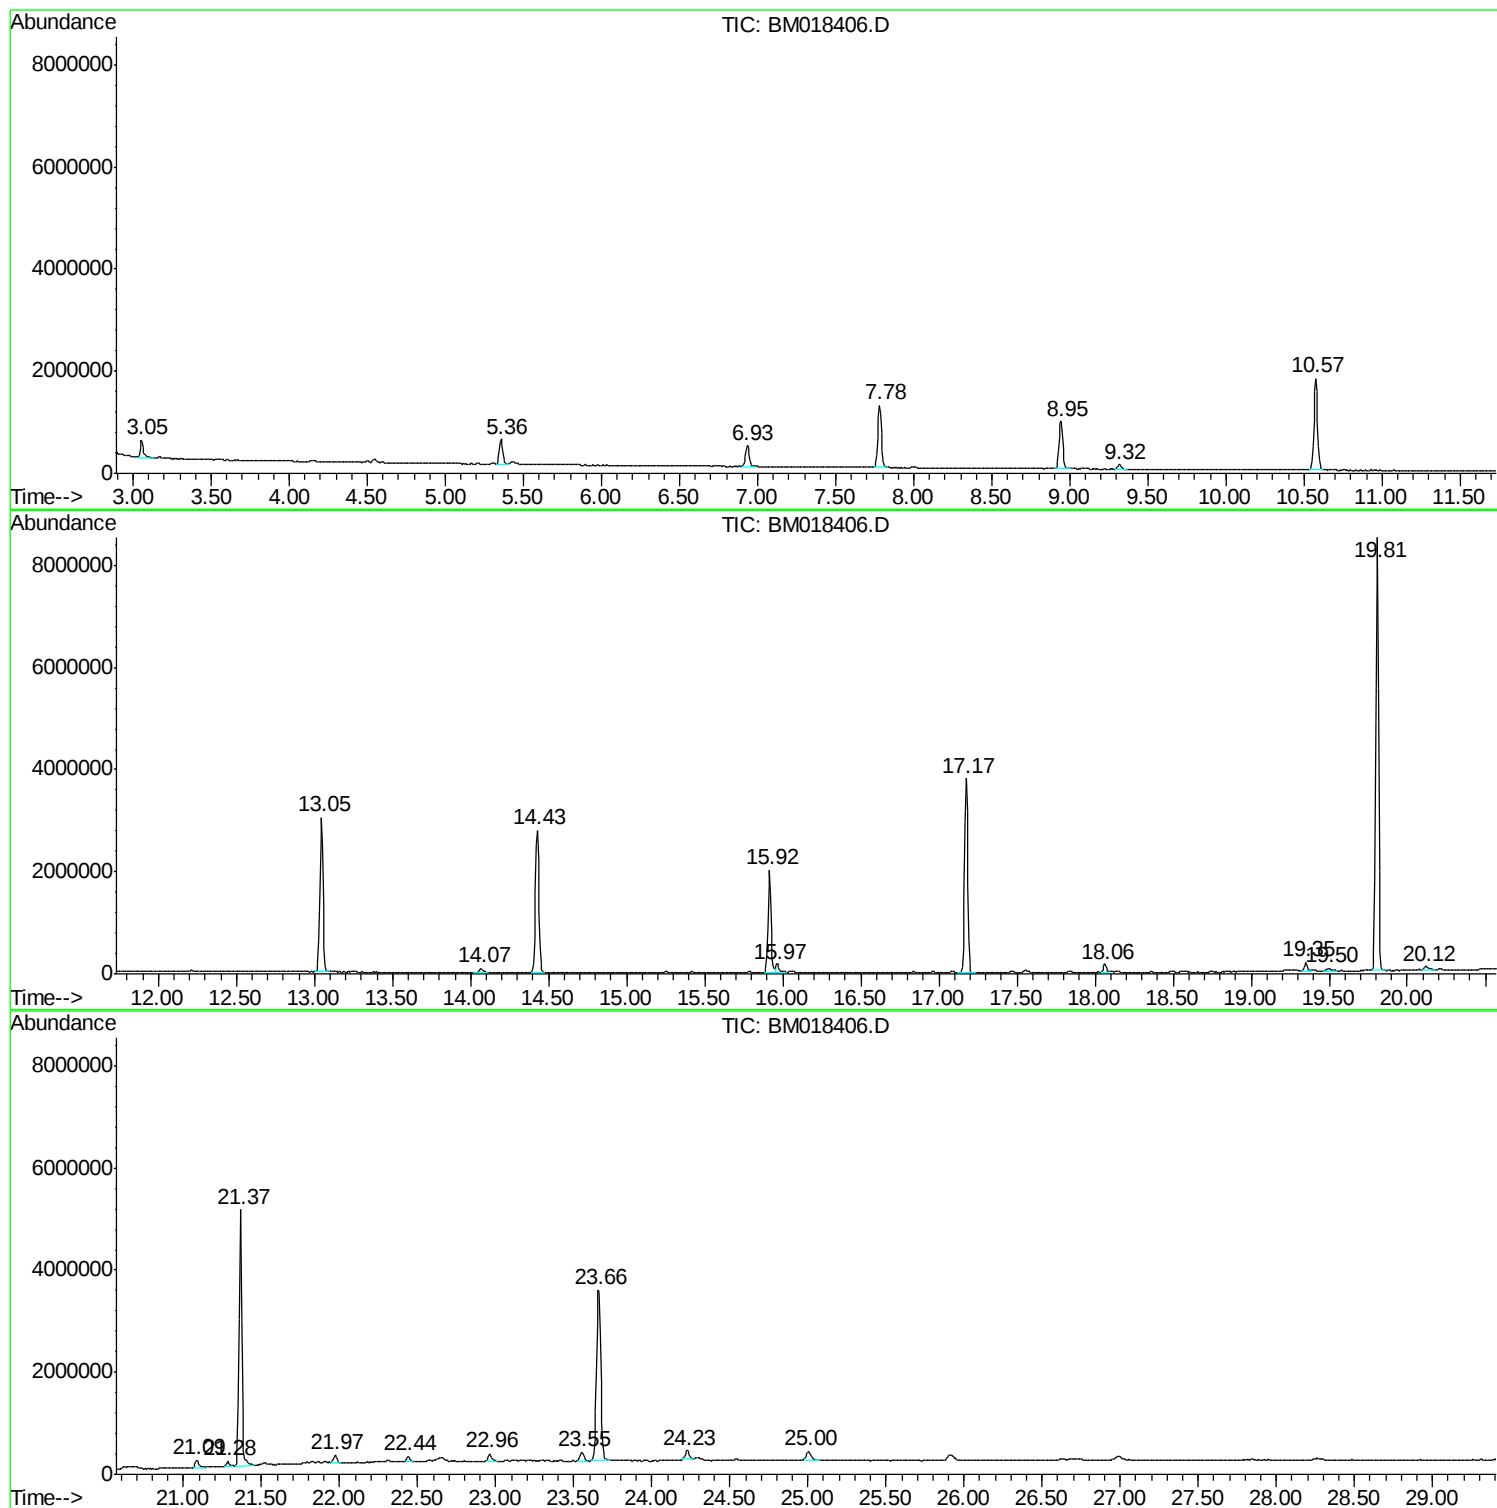

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018406.D
Acq On : 27 Dec 2018 21:05
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Penten-2-ol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.05	5.50 ng	518180	1,4-Dichlorobenzene-d4	7.78

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Penten-2-ol	86	C5H10O	001569-50-2	72
2			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	52
3			Acetic acid, (1,2-dimethyl-1-propenyl) ester	128	C7H12O2	003814-41-3	50
4			1,6-Heptadien-4-ol	112	C7H12O	002883-45-6	45
5			2-Furanmethanol, tetrahydro-, ac...	144	C7H12O3	000637-64-9	43

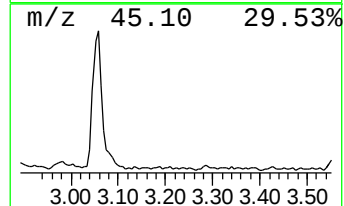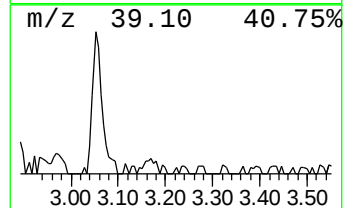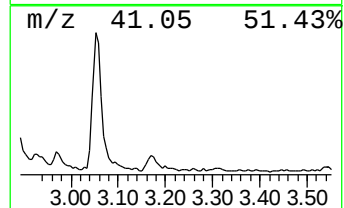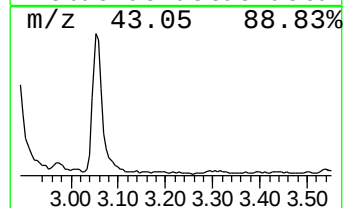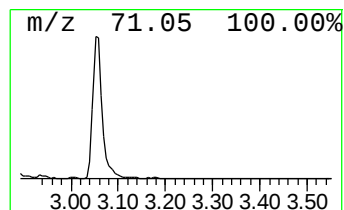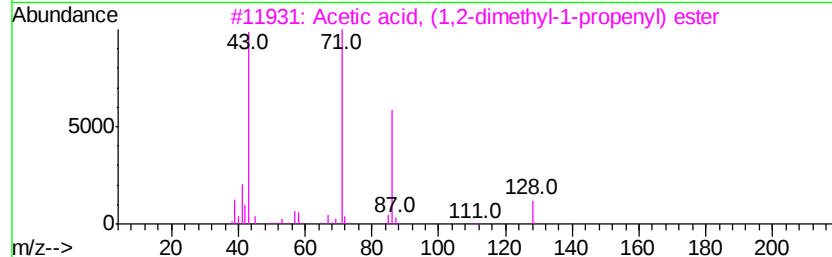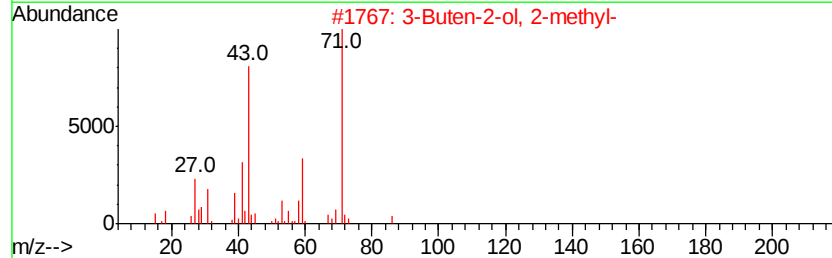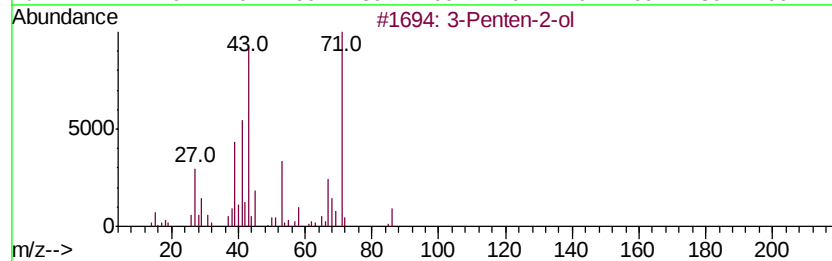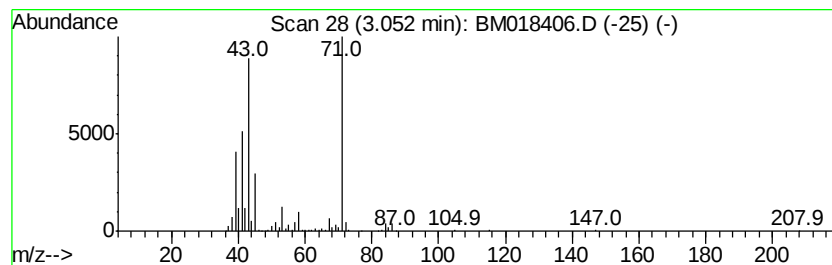

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122718\
Data File : BM018406.D
Acq On : 27 Dec 2018 21:05
Operator : JU/SJ
Sample : PB116035BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB116035BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Penten-2-ol	3.05	5.5	ng	518180	1	7.78	1885030	20.0