

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018410.D
 Acq On : 27 Dec 2018 23:28
 Operator : JU/SJ
 Sample : J6572-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 381204157-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	415	420	426	rBV	269742	404729	3.52%	0.760%
2	6.934	683	688	698	rVB	266934	424346	3.69%	0.797%
3	7.781	826	832	839	rVB	1417865	2180495	18.97%	4.093%
4	8.940	1023	1029	1036	rBV	551933	925790	8.06%	1.738%
5	10.575	1300	1307	1317	rVB	2072879	3428893	29.83%	6.437%
6	13.045	1720	1727	1735	rVB	2123022	3139835	27.32%	5.894%
7	14.427	1954	1962	1971	rBV2	3233134	4974677	43.28%	9.338%
8	15.916	2209	2215	2222	rBV	1914040	2708654	23.57%	5.085%
9	17.174	2423	2429	2441	rBV2	4293616	6047952	52.62%	11.353%
10	18.062	2575	2580	2585	rBV3	101515	161056	1.40%	0.302%
11	18.139	2585	2593	2599	rVB4	88438	168006	1.46%	0.315%
12	19.168	2763	2768	2775	rBV3	84969	139891	1.22%	0.263%
13	19.345	2794	2798	2804	rBV2	113796	158603	1.38%	0.298%
14	19.680	2851	2855	2866	rBV7	54731	127655	1.11%	0.240%
15	19.804	2870	2876	2886	rVB	9328791	11492970	100.00%	21.574%
16	21.362	3136	3141	3153	rBV	6195900	7647721	66.54%	14.356%
17	22.433	3320	3323	3329	rVB	113017	142627	1.24%	0.268%
18	22.956	3408	3412	3421	rVB	158377	241027	2.10%	0.452%
19	23.544	3508	3512	3519	rVB	197223	339427	2.95%	0.637%
20	23.656	3523	3531	3543	rVB	3907464	7580547	65.96%	14.230%
21	24.215	3622	3626	3634	rVB3	191215	365053	3.18%	0.685%
22	24.991	3753	3758	3767	rVB2	208843	472058	4.11%	0.886%


Sum of corrected areas: 53272012

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018410.D
Acq On : 27 Dec 2018 23:28
Operator : JU/SJ
Sample : J6572-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
381204157-6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

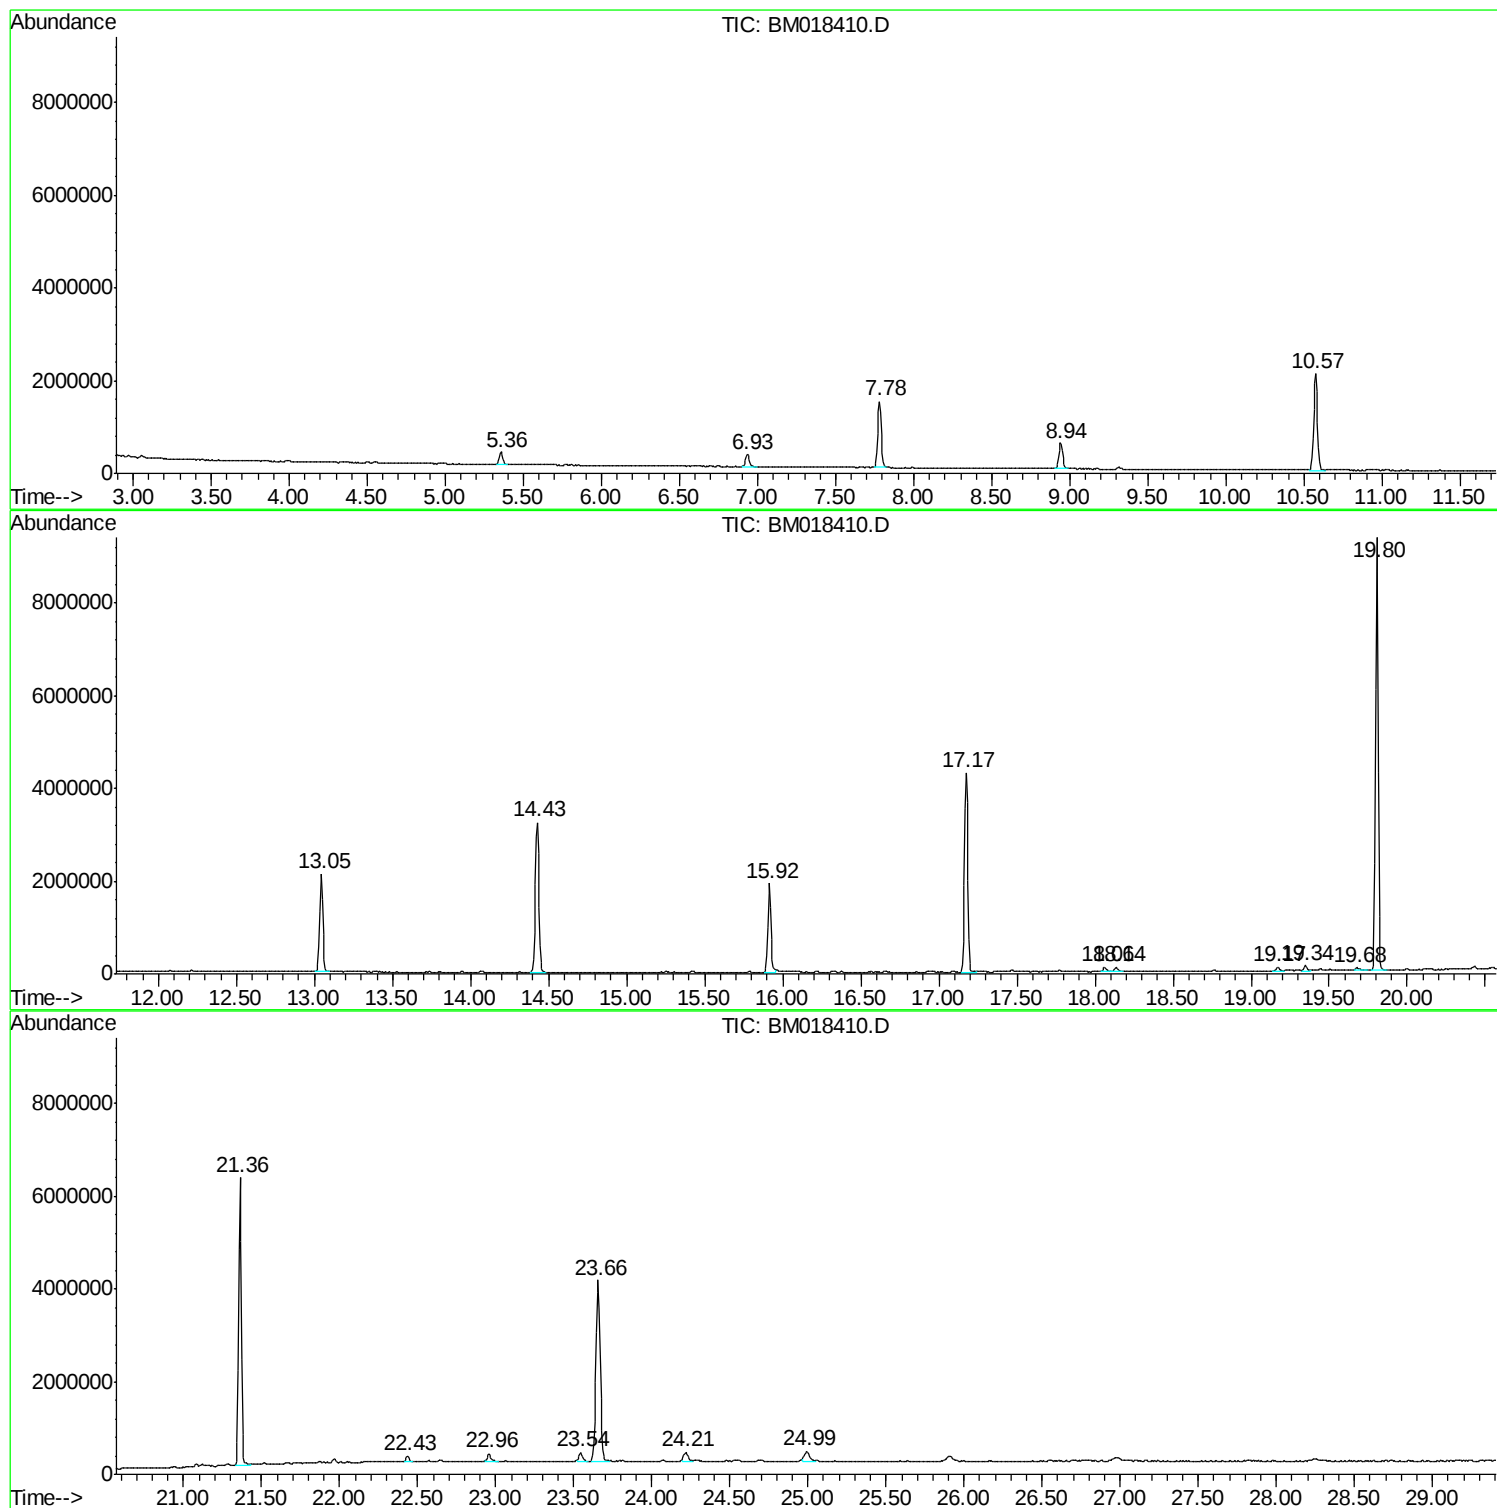

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122718\
Data_File : BM018410.D
Acq_On : 27 Dec 2018 23:288
Operator : JU/SJJ
Sample : J6572-022
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
381204157-6

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
