

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018412.D
 Acq On : 28 Dec 2018 00:40
 Operator : JU/SJ
 Sample : J6572-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 381205140-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	415	420	425	rVB	249530	357504	3.18%	0.621%
2	6.934	684	688	700	rVB	222484	378804	3.37%	0.658%
3	7.781	825	832	840	rVB	1617523	2473901	22.00%	4.299%
4	8.939	1023	1029	1039	rVB	467561	779556	6.93%	1.355%
5	10.575	1298	1307	1315	rBV	2331728	3901800	34.69%	6.780%
6	13.045	1719	1727	1736	rVB	1799673	2594135	23.07%	4.508%
7	14.063	1892	1900	1908	rBV3	114488	190268	1.69%	0.331%
8	14.427	1954	1962	1970	rBV2	3619574	5520511	49.09%	9.593%
9	15.915	2209	2215	2220	rBV	2176458	2996235	26.64%	5.206%
10	15.962	2220	2223	2228	rVB2	135390	192468	1.71%	0.334%
11	16.939	2384	2389	2397	rBV6	86244	196030	1.74%	0.341%
12	17.174	2423	2429	2438	rVB	4885256	6667705	59.29%	11.586%
13	18.062	2576	2580	2590	rBV	250457	435800	3.88%	0.757%
14	19.350	2795	2799	2809	rBV2	196978	326112	2.90%	0.567%
15	19.803	2871	2876	2884	rVB	9337955	11246283	100.00%	19.542%
16	21.362	3136	3141	3155	rBV	7225899	8575370	76.25%	14.901%
17	21.962	3240	3243	3250	rVB3	102996	143248	1.27%	0.249%
18	22.433	3320	3323	3330	rVB2	155518	211836	1.88%	0.368%
19	22.956	3408	3412	3418	rVB	221790	314618	2.80%	0.547%
20	23.544	3507	3512	3519	rVB	270011	484970	4.31%	0.843%
21	23.656	3523	3531	3541	rVB	4596487	8476214	75.37%	14.729%
22	24.215	3621	3626	3633	rVB	240313	469530	4.17%	0.816%
23	24.991	3753	3758	3769	rVB2	250997	615395	5.47%	1.069%


Sum of corrected areas: 57548293

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
Data File : BM018412.D
Acq On : 28 Dec 2018 00:40
Operator : JU/SJ
Sample : J6572-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
381205140-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM122718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

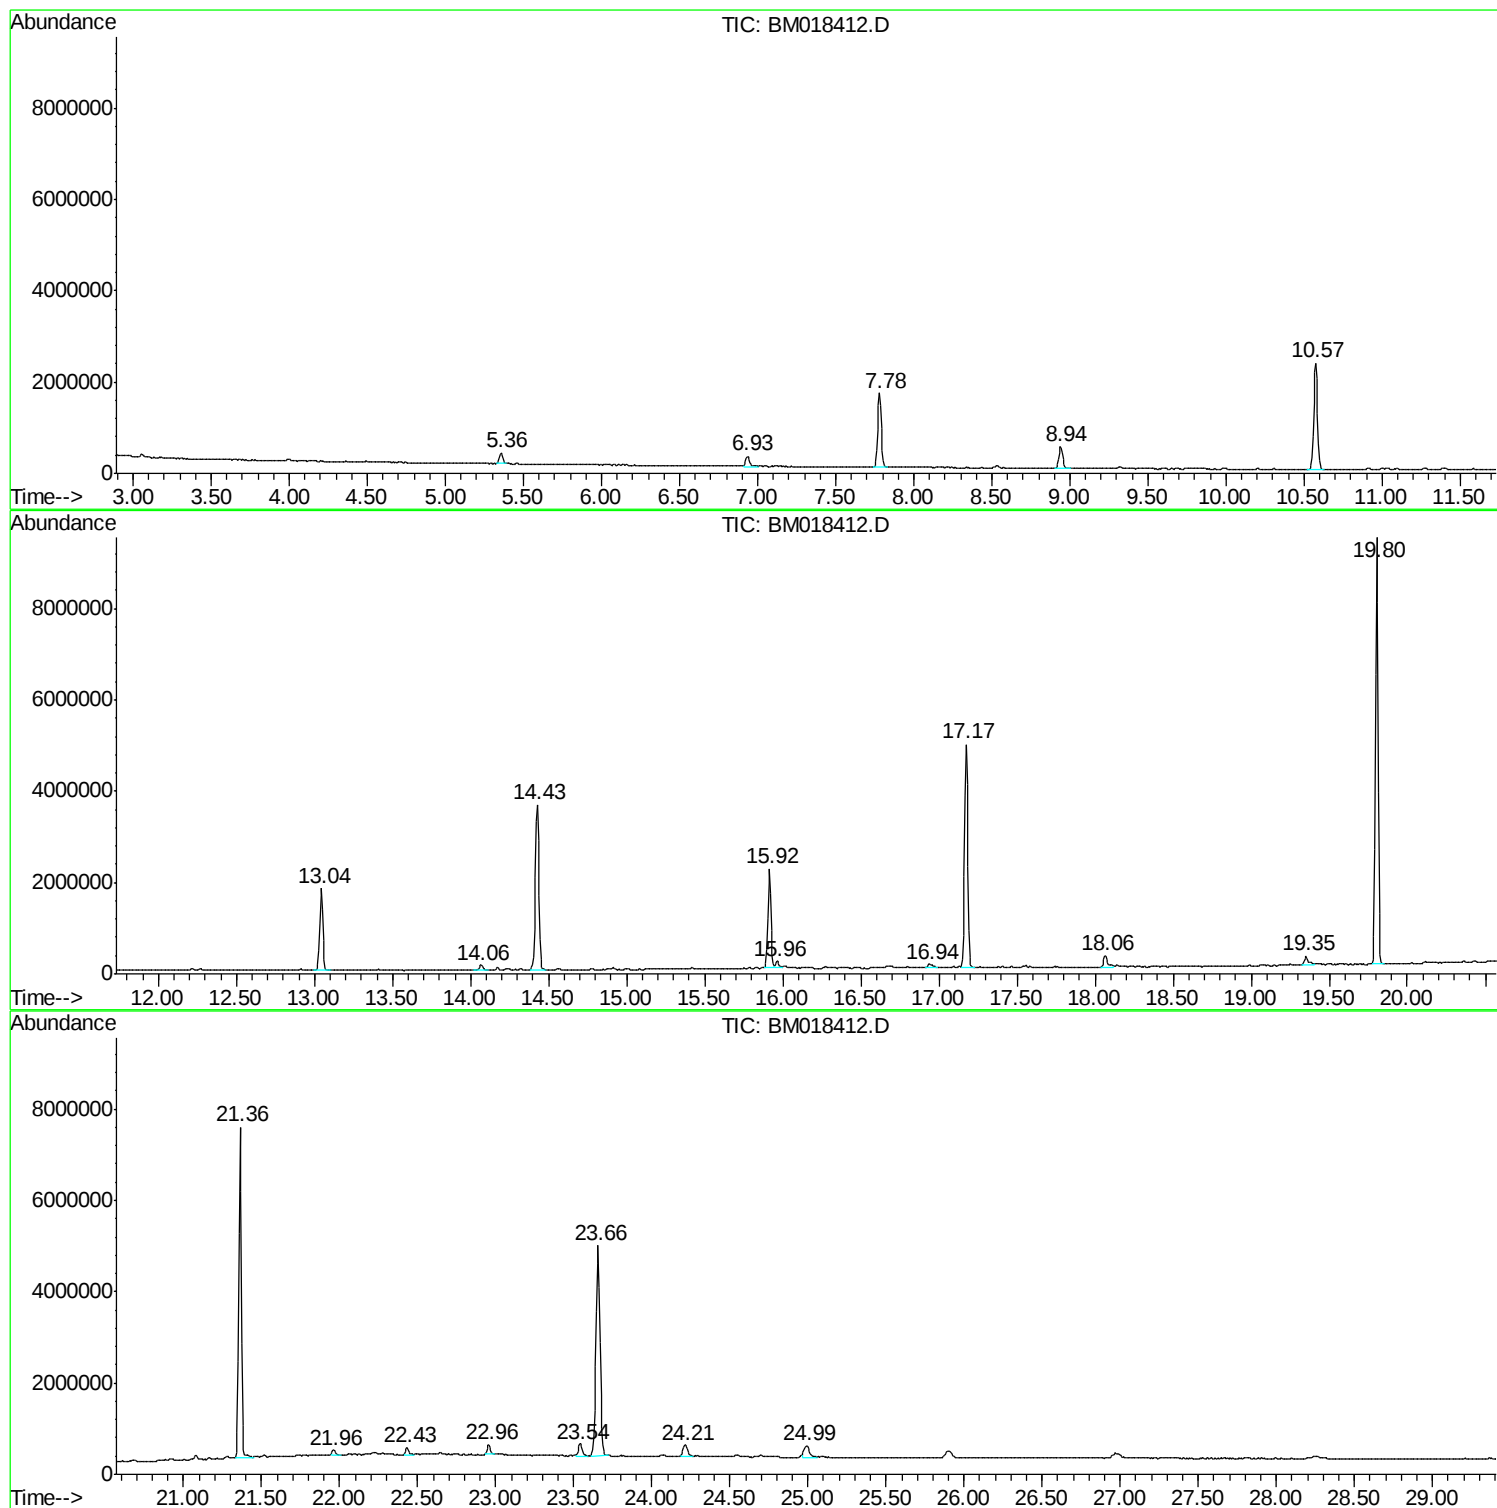

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122718\
Data_File : BM018412.D
Acq_On : 28-Dec-2018 00:400
Operator : JU/SJJ
Sample : J6572-066
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
381205140-3

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
