


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018396.D
 Acq On : 27 Dec 2018 15:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 27 14:18:47 2018

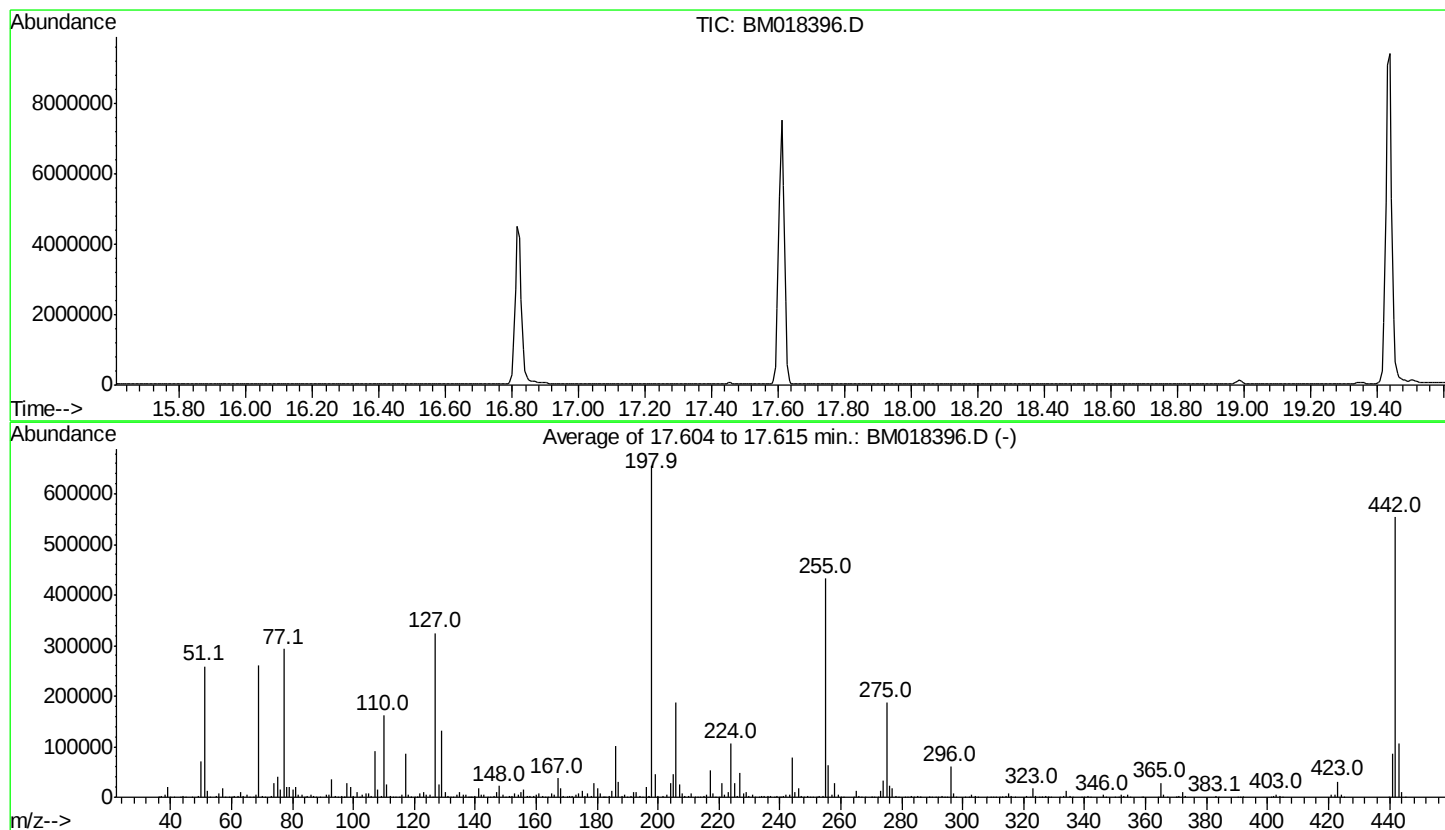

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	258773	PASS
68	69	0.00	2	1.8	4578	PASS
69	198	0.00	100	39.6	259904	PASS
70	69	0.00	2	0.7	1752	PASS
127	198	10	80	49.5	324842	PASS
197	198	0.00	2	0.4	2700	PASS
198	198	100	100	100.0	656021	PASS
199	198	5	9	7.0	45701	PASS
275	198	10	60	28.5	186645	PASS
365	198	1	100	4.3	28370	PASS
441	198	0.01	100	13.3	87269	PASS
442	198	50	100	84.4	553792	PASS
443	442	15	24	19.3	106605	PASS